

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060819\
 Data File : VV011333.D
 Acq On : 08 Jun 2019 22:10
 Operator : SY/MD
 Sample : K3276-11
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8E7

Quant Time: Jun 09 00:47:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Jun 09 00:10:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	140267	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	128304	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	49744	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	43650	4.11	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.20%
7) Chloroethane-d5	1.56	69	36361	4.12	ug/L	0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.40%
11) 1,1-Dichloroethene-d2	2.12	63	71229	3.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.00%
20) 2-Butanone-d5	3.95	46	115224	48.15	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.30%
24) Chloroform-d	4.40	84	86511	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
26) 1,2-Dichloroethane-d4	5.08	65	48763	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.40%
32) Benzene-d6	5.09	84	174905	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.20%
36) 1,2-Dichloropropane-d6	6.12	67	53937	4.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.20%
41) Toluene-d8	7.36	98	153178	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.00%
43) trans-1,3-Dichloropropene-	7.67	79	15965	3.54	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.80%
46) 2-Hexanone-d5	8.14	63	85990	45.16	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.32%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	34206	4.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	47333	4.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	8860	5.522 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060819\
Data File : VV011333.D
Acq On : 08 Jun 2019 22:10
Operator : SY/MD
Sample : K3276-11
Misc : 25ML/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB8E7

Quant Time: Jun 09 00:47:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Jun 09 00:10:13 2019
Response via : Initial Calibration

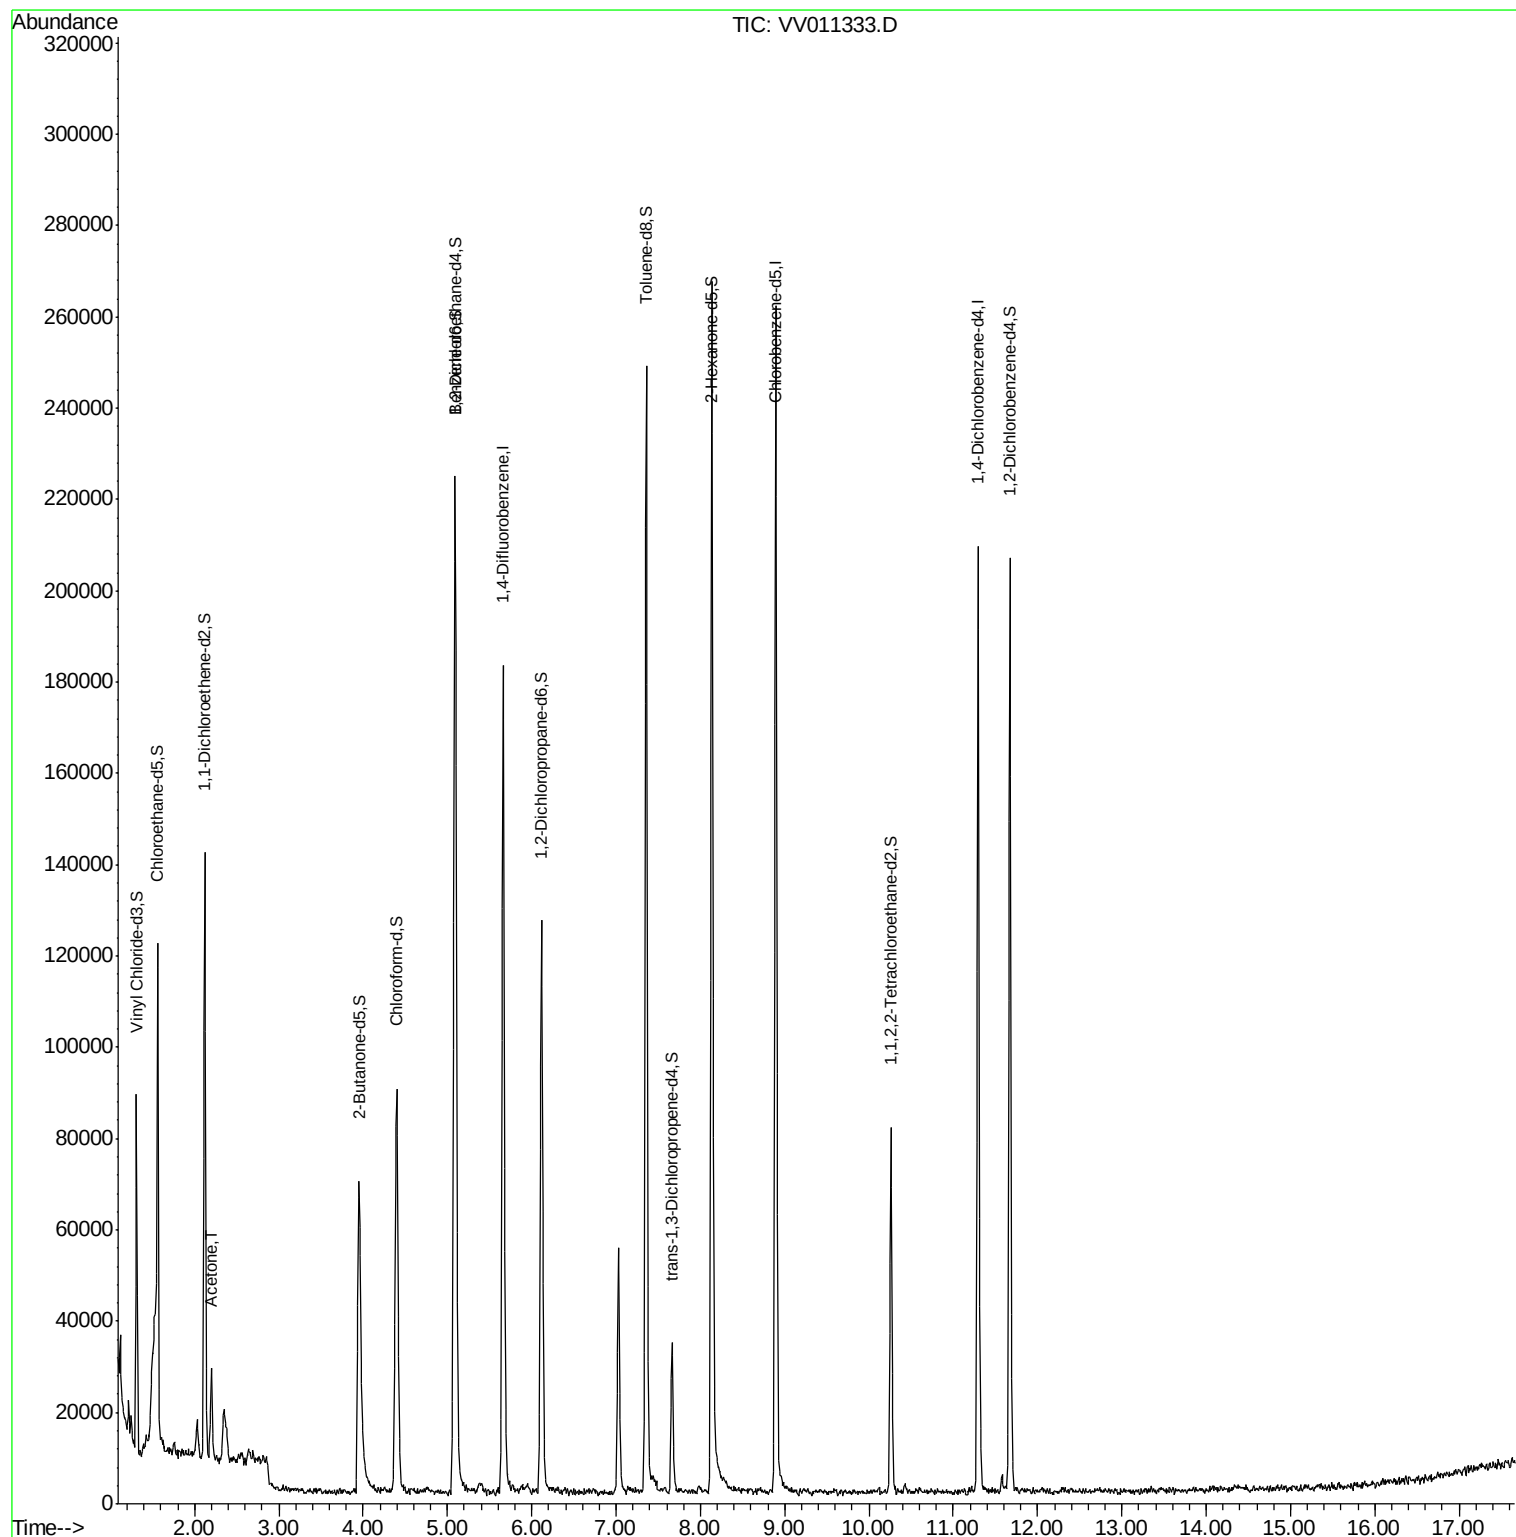

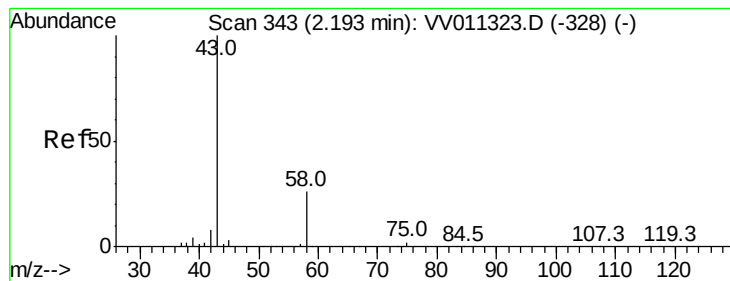

#13

Acetone

Concen: 5.522 ug/L

RT: 2.20 min Scan# 345

Delta R.T. 0.01 min

Lab File: VV011333.D

Acq: 08 Jun 2019 22:10

Instrument :
MSVOA_V
ClientSampleId :
DB8E7

Tot Ion: 43 Resp: 8860

Ion Ratio Lower Upper

43 100

58 35.1 0.0 55.2

