

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060819\
 Data File : VV011334.D
 Acq On : 08 Jun 2019 22:38
 Operator : SY/MD
 Sample : K3276-12
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8E8

Quant Time: Jun 09 00:51:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Jun 09 00:10:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	130975	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	120559	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	49305	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	39620	3.99	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.80%
7) Chloroethane-d5	1.55	69	33611	4.07	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.40%
11) 1,1-Dichloroethene-d2	2.12	63	67175	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	3.94	46	107787	48.24	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.48%
24) Chloroform-d	4.40	84	80718	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	5.08	65	46141	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
32) Benzene-d6	5.09	84	163117	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.12	67	50467	4.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.80%
41) Toluene-d8	7.36	98	144267	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
43) trans-1,3-Dichloropropene-	7.66	79	14095	3.33	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.60%
46) 2-Hexanone-d5	8.13	63	84507	47.23	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.46%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	33963	4.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	48111	4.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	6769	4.518 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060819\
Data File : VV011334.D
Acq On : 08 Jun 2019 22:38
Operator : SY/MD
Sample : K3276-12
Misc : 25ML/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB8E8

Quant Time: Jun 09 00:51:26 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Jun 09 00:10:13 2019
Response via : Initial Calibration

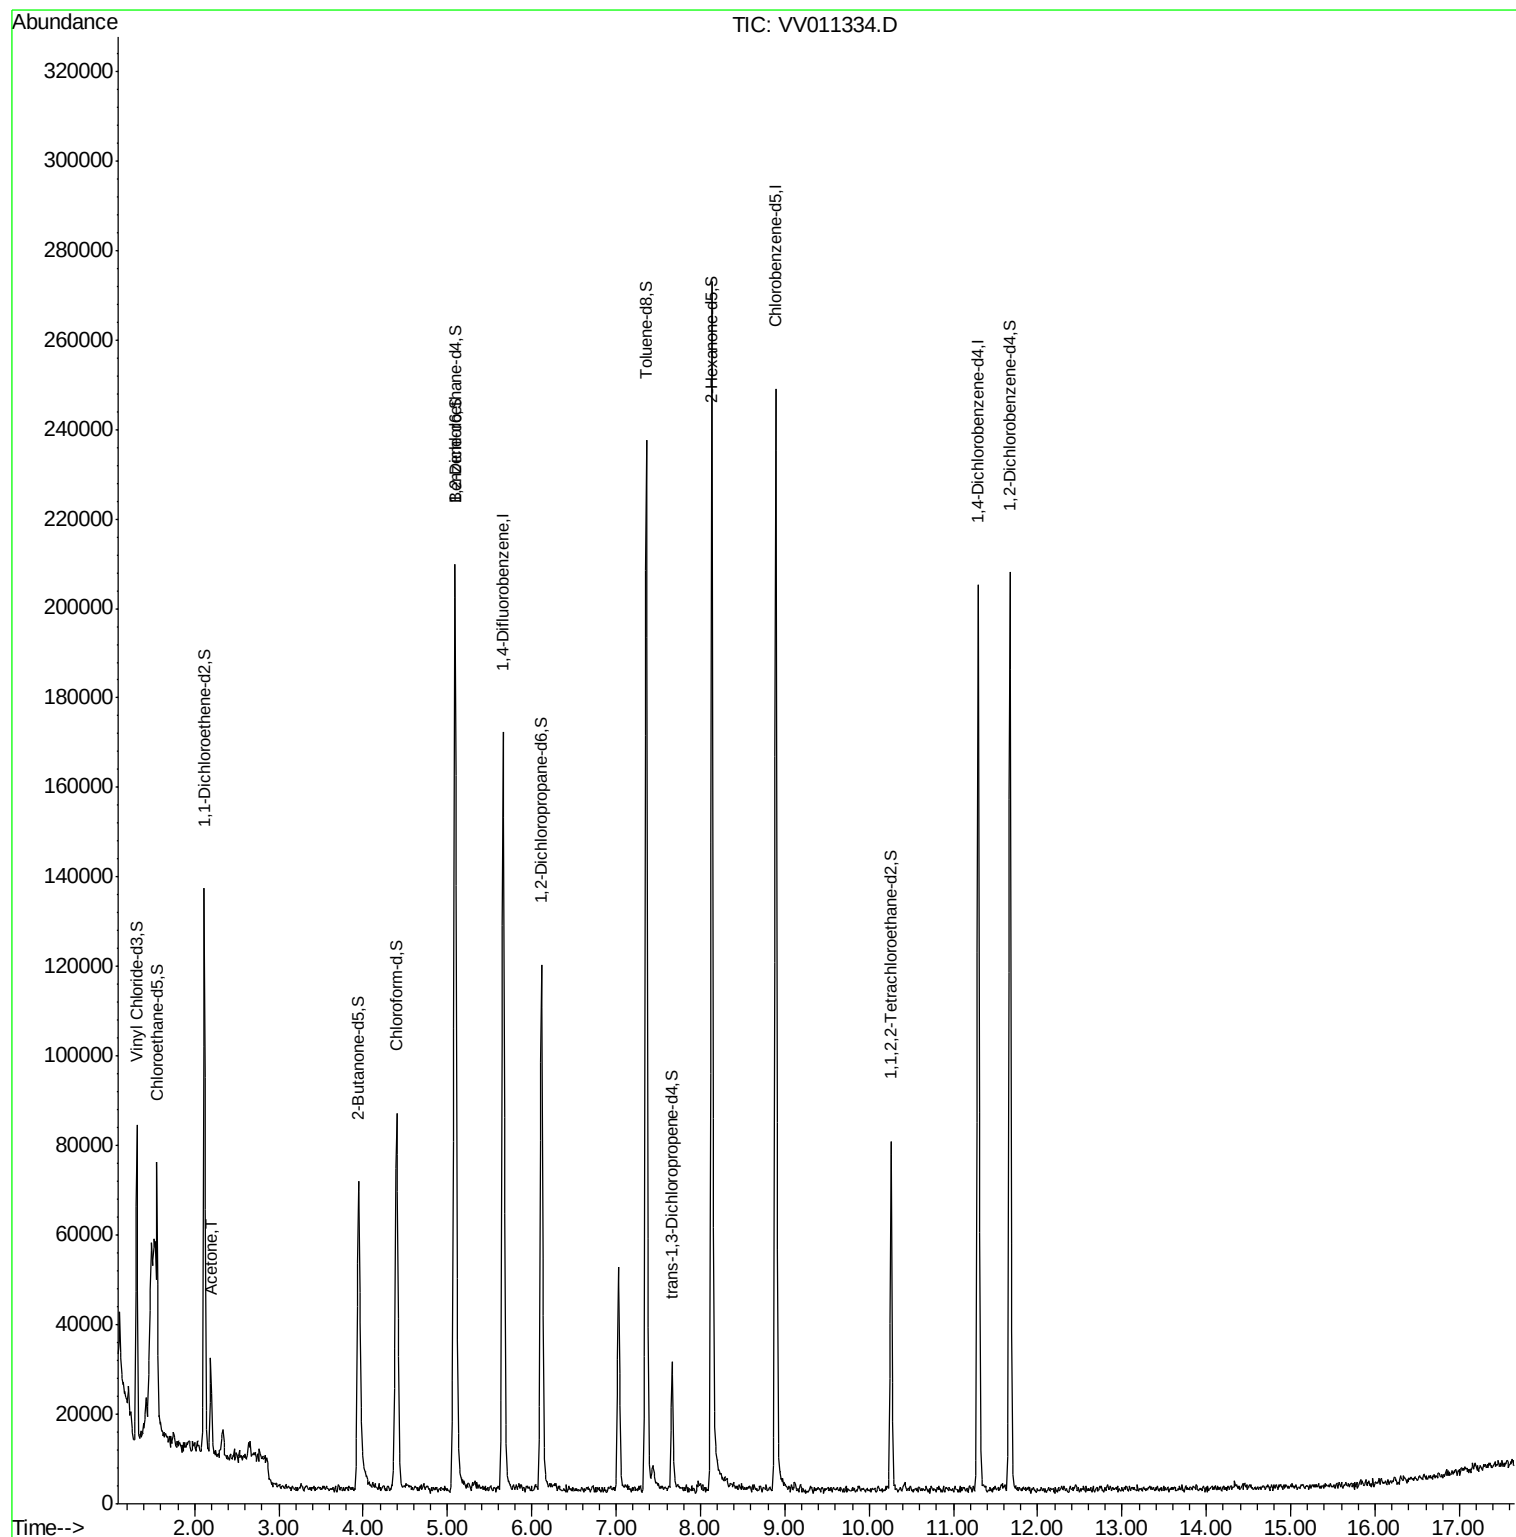

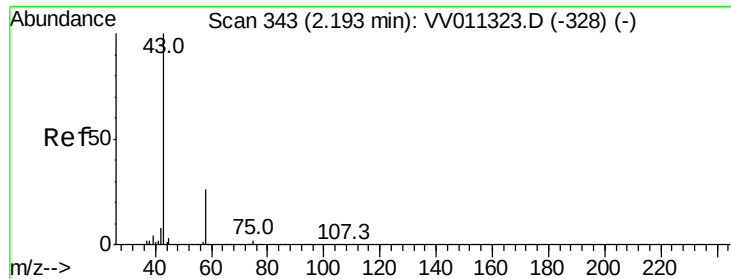

#13

Acetone

Concen: 4.518 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.00 min

Lab File: VV011334.D

Acq: 08 Jun 2019 22:38

Instrument :
MSVOA_V
ClientSampleId :
DB8E8

Tot Ion: 43 Resp: 6769

Ion Ratio Lower Upper

43 100

58 31.6 0.0 55.2

