

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060819\
 Data File : VV011336.D
 Acq On : 09 Jun 2019 00:02
 Operator : SY/MD
 Sample : K3276-18
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8F4

Quant Time: Jun 09 00:59:57 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Jun 09 00:10:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	143839	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	128791	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	50165	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	43302	3.97	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.40%
7) Chloroethane-d5	1.57	69	37550	4.14	ug/L	0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.80%
11) 1,1-Dichloroethene-d2	2.12	63	71925	3.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.00%
20) 2-Butanone-d5	3.95	46	114052	46.48	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.96%
24) Chloroform-d	4.40	84	86910	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.60%
26) 1,2-Dichloroethane-d4	5.08	65	51339	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
32) Benzene-d6	5.09	84	178263	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
36) 1,2-Dichloropropane-d6	6.12	67	54070	4.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.20%
41) Toluene-d8	7.36	98	157027	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
43) trans-1,3-Dichloropropene-	7.66	79	15914	3.52	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.40%
46) 2-Hexanone-d5	8.14	63	85798	44.89	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.78%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35296	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	48203	4.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	8510	5.173 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060819\
Data File : VV011336.D
Acq On : 09 Jun 2019 00:02
Operator : SY/MD
Sample : K3276-18
Misc : 25ML/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB8F4

Quant Time: Jun 09 00:59:57 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Jun 09 00:10:13 2019
Response via : Initial Calibration

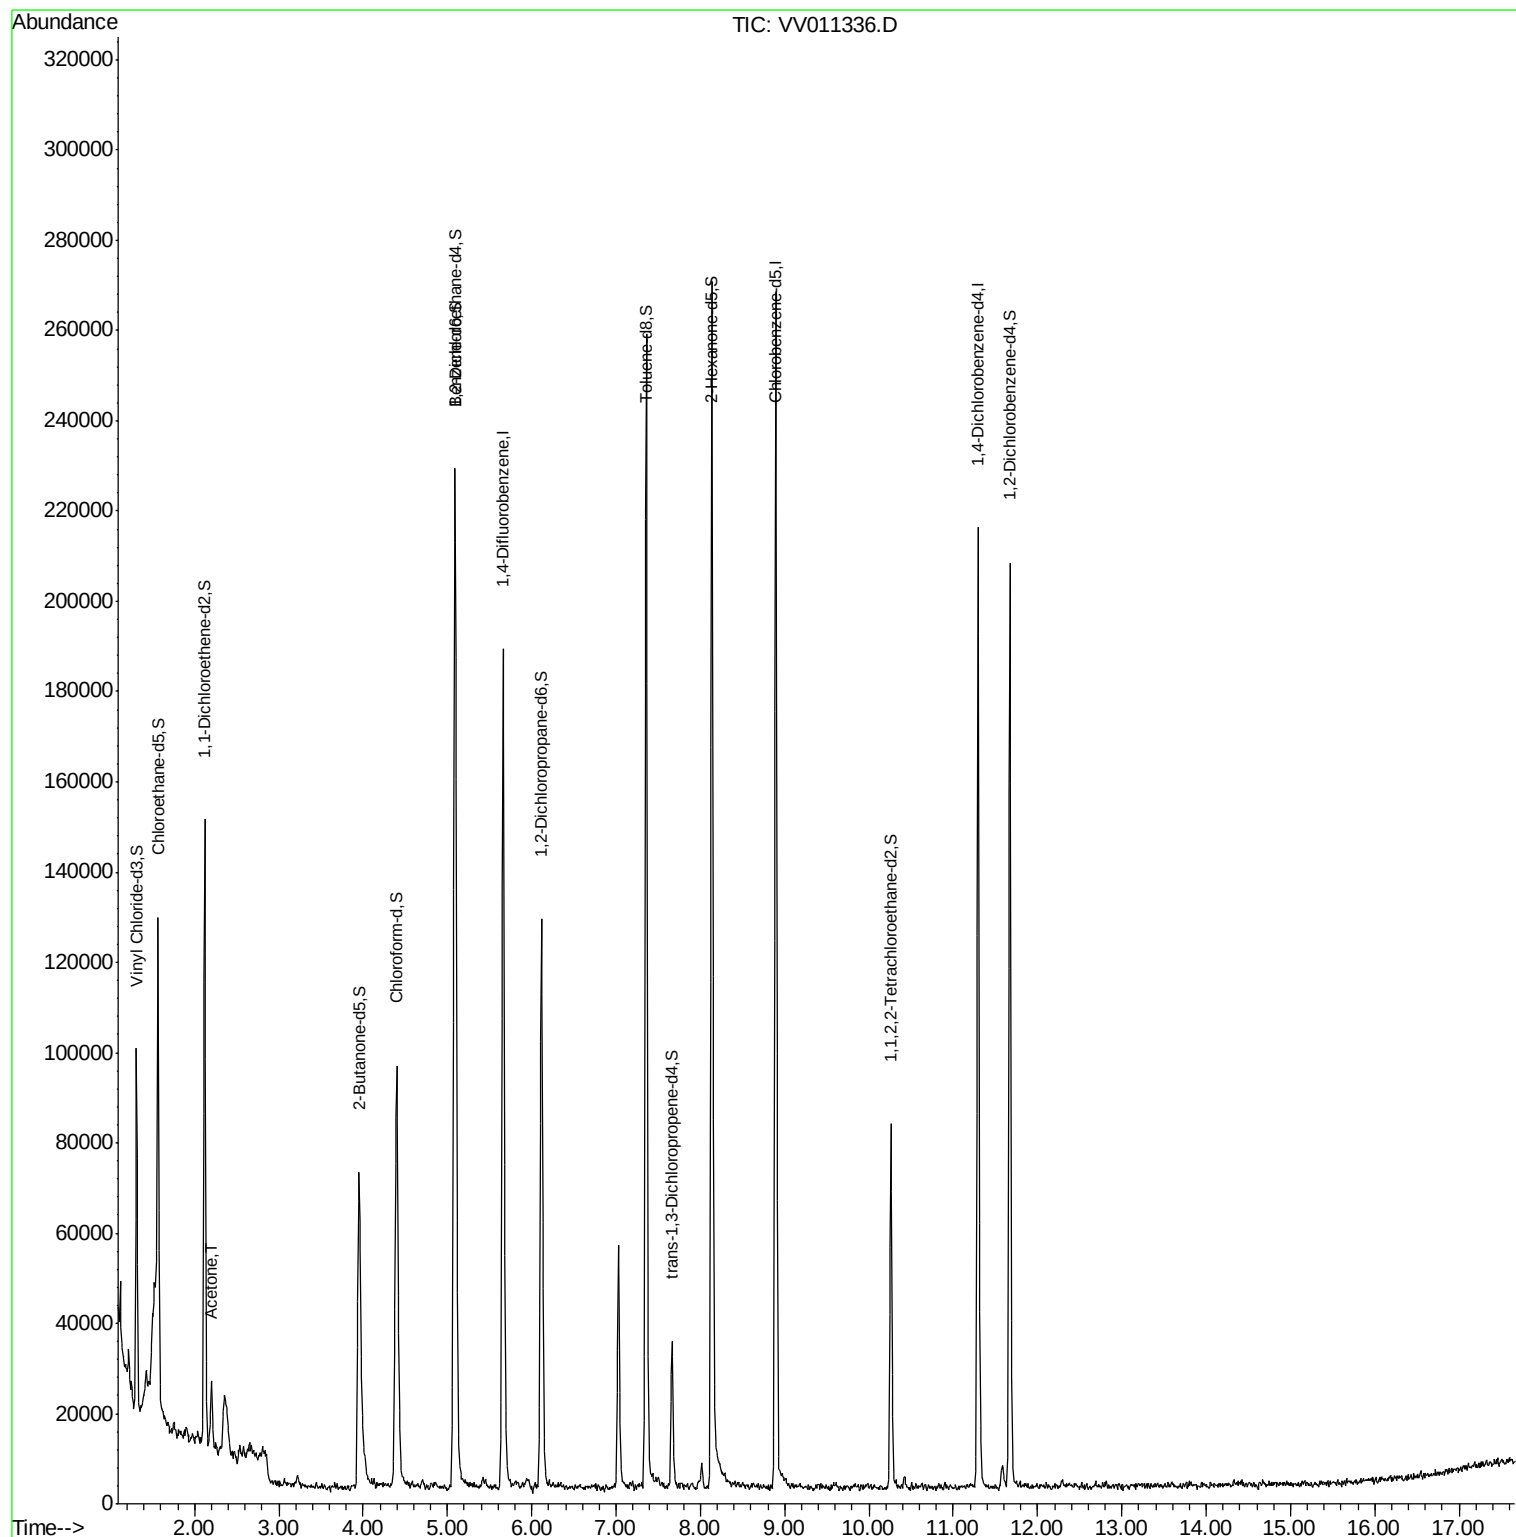

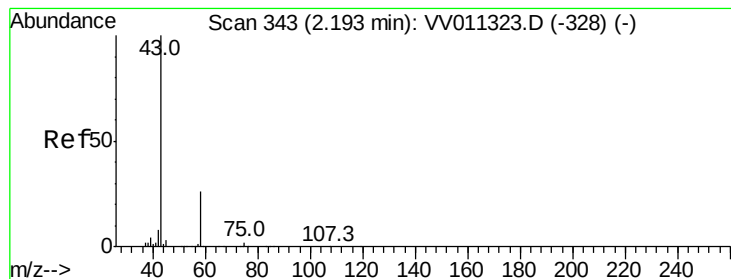

#13
 Acetone
 Concen: 5.173 ug/L
 RT: 2.20 min Scan# 346
 Delta R.T. 0.01 min
 Lab File: VV011336.D
 Acq: 09 Jun 2019 00:02

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8F4

Tot Ion: 43 Resp: 8510
 Ion Ratio Lower Upper
 43 100
 58 31.9 0.0 55.2

