


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV060819\
 Data File : VV011322.D
 Acq On : 08 Jun 2019 16:00
 Operator : SY/MD
 Sample : BFB45
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB45

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jun 10 06:50:13 2019

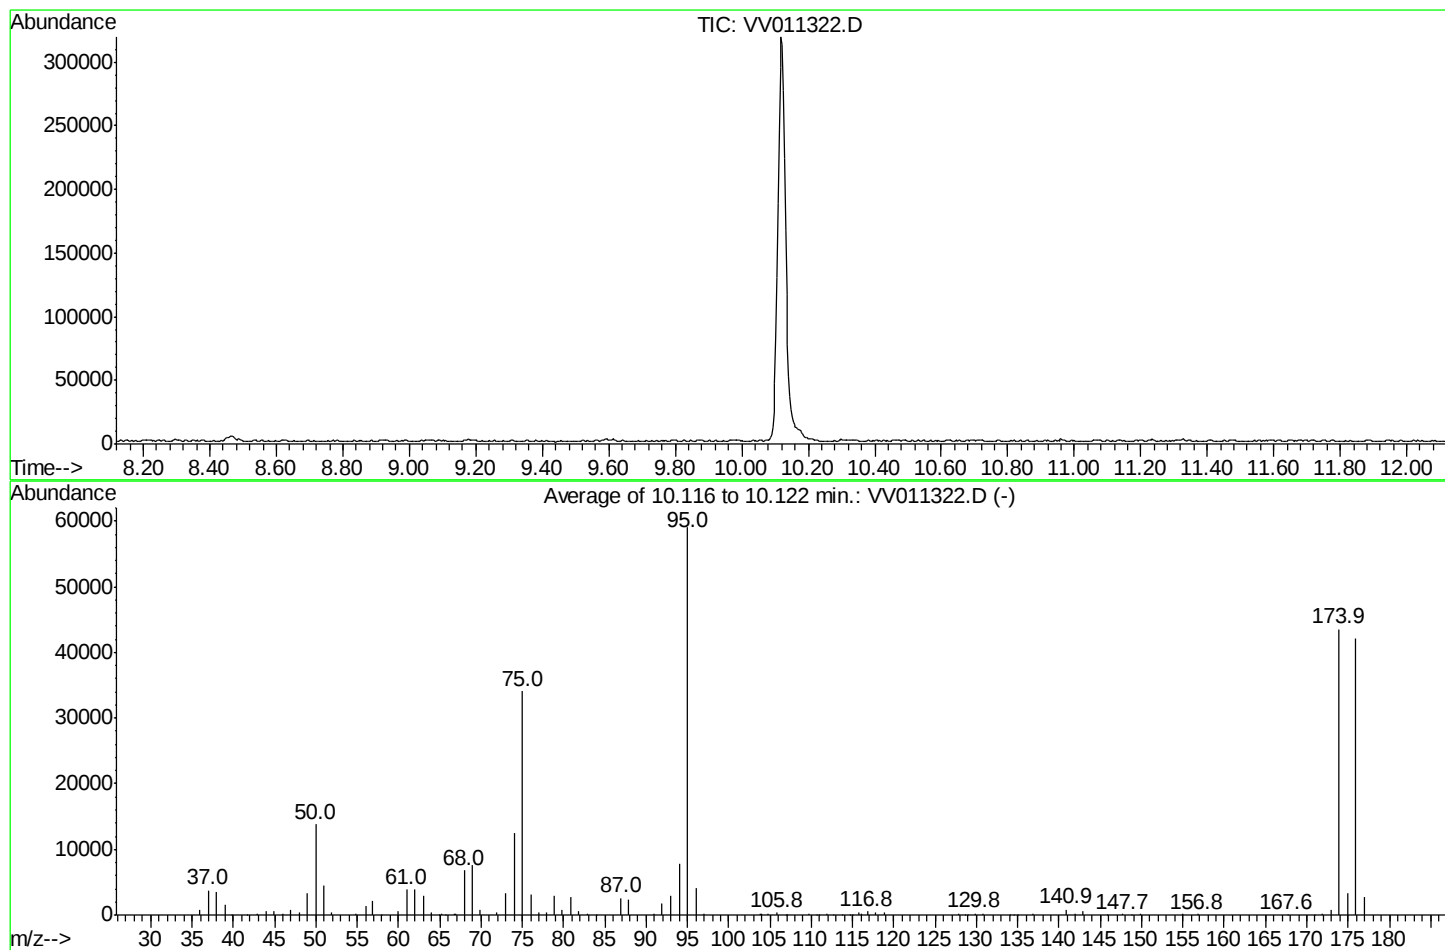

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	13811	PASS
75	95	30	80	57.8	34114	PASS
95	95	100	100	100.0	59066	PASS
96	95	5	9	6.9	4067	PASS
173	174	0.00	2	1.9	839	PASS
174	95	50	120	73.8	43592	PASS
175	174	5	9	7.6	3305	PASS
176	174	95	101	96.6	42109	PASS
177	176	5	9	6.3	2660	PASS

m/z	Abundance
36.00	161.0
37.10	129.0
38.00	114.0
38.70	142.0
39.80	458.0
40.90	131.0
41.60	114.0
42.10	134.0
44.00	444.0
44.80	113.0
46.60	130.0
53.00	129.0
54.90	121.0
57.90	144.0
78.90	103.0
91.10	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
35.90	832.0
37.00	3755.0
38.00	3394.0
39.00	1517.0
39.90	546.0
41.60	112.0
42.90	135.0
43.90	891.0
45.00	732.0
46.10	140.0
47.00	961.0
48.00	463.0
49.00	3356.0
50.00	13456.0
51.00	4477.0
51.90	305.0
55.00	318.0
56.00	1386.0
56.90	2034.0
58.00	211.0
60.00	639.0
61.00	3694.0
62.00	3792.0
63.00	2760.0
64.00	307.0
65.10	260.0
66.70	240.0
67.00	218.0
68.00	6731.0
69.00	7277.0
69.90	620.0
72.00	421.0
73.00	3269.0
74.00	12115.0
75.00	32640.0
76.00	3147.0
76.90	420.0
77.90	307.0
78.90	2850.0
79.90	722.0
80.90	2508.0
81.80	732.0
83.00	104.0
84.00	101.0
86.90	2489.0
87.90	2246.0
90.90	394.0
91.90	1809.0
92.90	2834.0
94.00	7614.0
95.00	56056.0
96.00	4019.0
96.90	139.0
103.80	317.0
104.70	140.0
105.90	340.0
106.90	119.0
109.80	115.0
111.00	155.0
115.00	102.0
115.70	321.0
116.10	285.0
116.80	530.0
117.80	325.0
118.80	483.0
127.90	236.0
128.60	102.0
129.80	286.0
130.80	155.0
136.80	173.0
140.90	773.0
142.00	217.0
142.90	622.0
147.70	195.0
148.80	107.0
149.90	112.0
154.90	110.0
156.70	144.0
171.10	104.0
171.80	256.0
173.00	755.0
173.90	41544.0
174.90	3146.0
175.90	38544.0
176.90	2575.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
35.90	911.0
37.00	3941.0
38.00	3691.0
39.00	1630.0
39.90	560.0
41.60	148.0
42.90	134.0
43.90	967.0
45.00	757.0
46.00	159.0
47.00	899.0
48.00	438.0
49.00	3490.0
50.00	14275.0
51.00	4649.0
51.90	329.0
55.00	336.0
56.00	1491.0
56.90	2198.0
58.00	214.0
60.00	655.0
61.00	3891.0
62.00	3994.0
63.00	3084.0
64.00	341.0
65.20	226.0
65.70	105.0
66.80	264.0
67.90	7020.0
69.00	7912.0
69.90	709.0
71.90	487.0
73.00	3424.0
74.00	12945.0
75.00	35296.0
76.00	3105.0
77.00	419.0
77.90	383.0
78.90	3084.0
79.80	753.0
80.90	2752.0
81.80	706.0
82.90	143.0
86.90	2669.0
87.90	2434.0
90.90	418.0
91.90	1860.0
93.00	2893.0
94.00	8025.0
95.00	61088.0
96.00	4152.0
96.90	136.0
103.80	362.0
104.70	181.0
105.80	392.0
106.80	124.0
109.70	126.0
111.00	154.0
111.80	138.0
112.70	123.0
113.80	102.0
115.00	101.0
115.70	348.0
116.10	263.0
116.80	565.0
117.80	354.0
118.80	502.0
127.90	214.0
128.90	135.0
129.80	308.0
130.80	192.0
134.00	114.0
134.50	110.0
136.90	180.0
140.90	840.0
142.00	204.0
142.90	689.0
147.70	157.0
149.90	127.0
154.90	143.0
156.80	145.0
171.80	288.0
173.00	855.0
173.90	45000.0
174.90	3377.0
175.90	43592.0
176.90	2729.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45

m/z	Abundance
35.90	882.0
37.00	3874.0
38.00	3594.0
39.00	1590.0
39.90	576.0
41.10	108.0
41.60	162.0
42.90	137.0
44.00	960.0
45.00	727.0
46.00	163.0
47.00	765.0
47.90	408.0
49.00	3236.0
50.00	13702.0
51.00	4339.0
52.00	270.0
54.90	318.0
56.00	1378.0
56.90	2211.0
58.00	186.0
59.90	680.0
61.00	3888.0
62.00	3728.0
63.00	3061.0
63.90	293.0
64.90	159.0
65.20	169.0
65.80	131.0
66.90	286.0
67.90	6670.0
69.00	7532.0
69.90	758.0
71.90	553.0
73.00	3291.0
74.00	12500.0
75.00	34408.0
76.00	2840.0
77.00	395.0
77.90	430.0
78.90	2952.0
79.80	750.0
80.90	2716.0
81.90	607.0
82.90	156.0
87.00	2482.0
87.90	2499.0
90.90	369.0
91.90	1788.0
93.00	2830.0
94.00	7806.0
95.00	60056.0
96.00	4031.0
97.00	113.0
104.00	365.0
104.70	182.0
105.80	435.0
107.10	101.0
109.70	111.0
110.60	151.0
111.80	188.0
112.70	147.0
114.70	101.0
115.70	298.0
116.80	583.0
117.70	320.0
118.90	462.0
127.80	197.0
128.90	145.0
129.90	282.0
130.80	176.0
134.00	119.0
134.90	127.0
136.80	168.0
140.90	808.0
142.00	145.0
142.90	684.0
145.80	132.0
147.70	120.0
149.80	105.0
154.90	148.0
156.80	140.0
167.60	103.0
170.90	101.0
171.90	280.0
173.00	907.0
173.90	44232.0
174.90	3392.0
175.90	44192.0
176.90	2678.0

Instrument :
MSVOA_V
ClientSampleId :
BFB45