


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016692.D
Acq On : 09 Jun 2020 04:30
Operator : SY/MD
Sample : L2901-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 49 Sample Multiplier: 1

Quant Time: Jun 09 05:50:05 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 09 03:40:57 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
Client Sampled :
ETTR3

Manual Integrations
APPROVED

MMDadoda
6/10/2020 11:39:15 AM

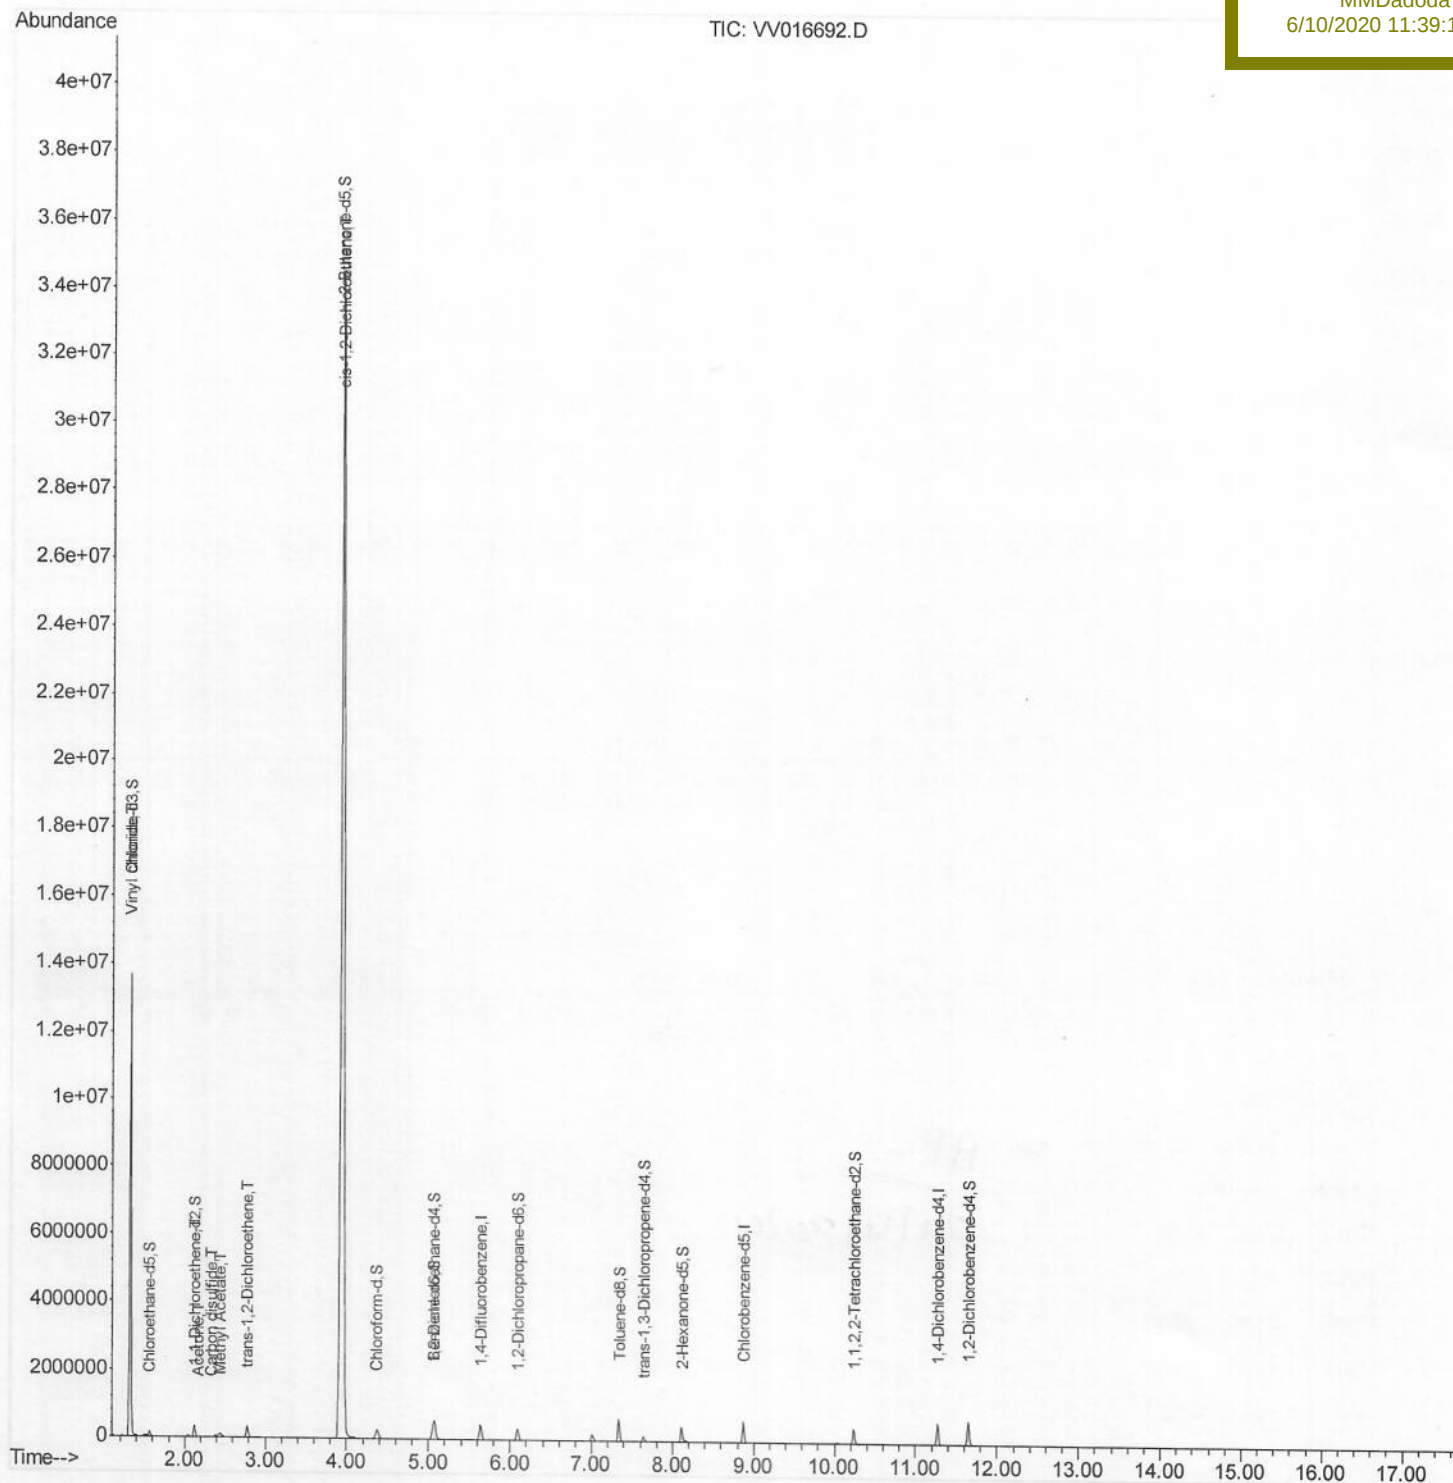

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016692.D
 Acq On : 09 Jun 2020 04:30
 Operator : SY/MD
 Sample : L2901-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Quant Time: Jun 09 05:42:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 09 03:40:57 2020
 Response via : Initial Calibration

Instrument :
 MSVOA_V
ClientSampleId :
 ETTR3

Manual Integrations
APPROVED

MMDadoda
 6/10/2020 11:39:15 AM

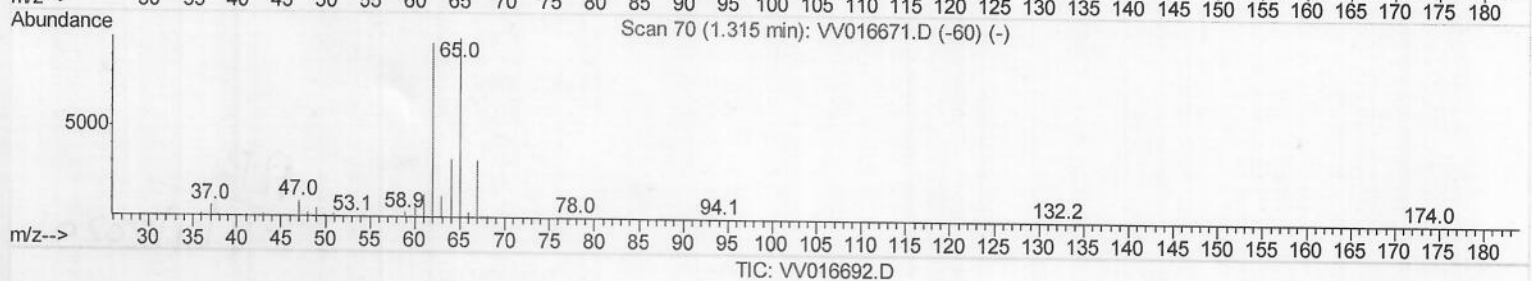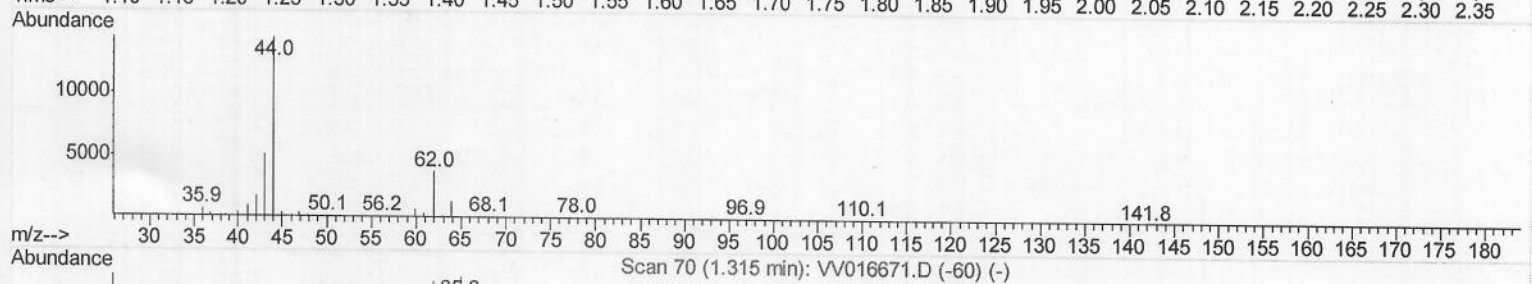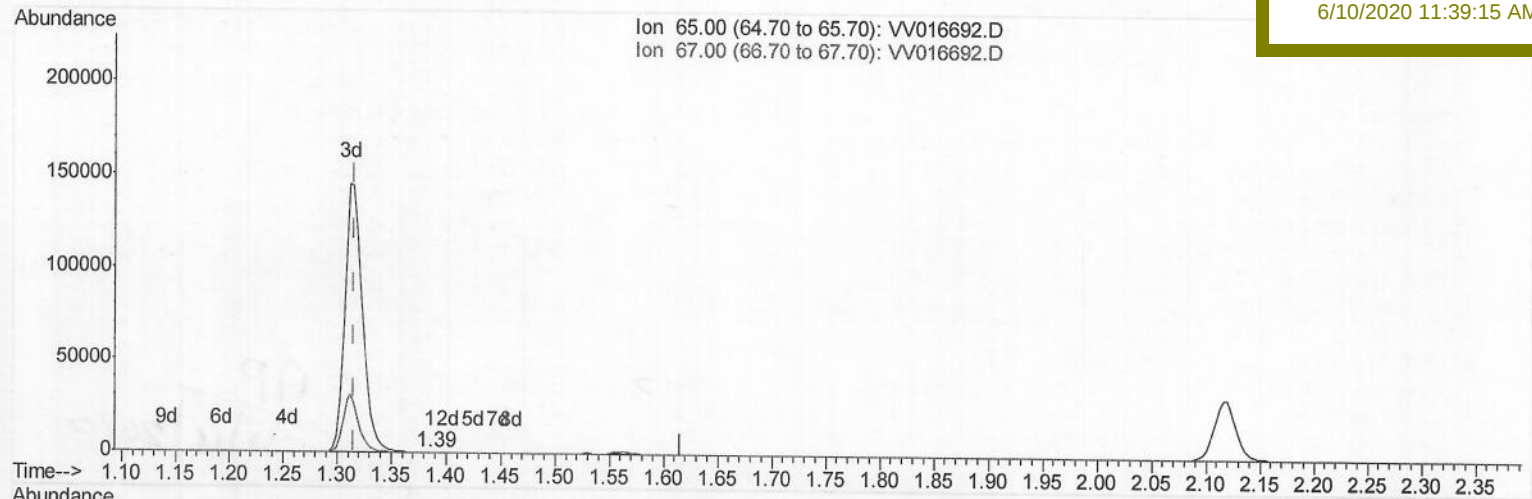

(4) Vinyl Chloride-d3 (S)

1.386min (+0.071) 0.05ug/L

response 117

Ion	Exp%	Act%
65.00	100	100
67.00	31.40	35.90
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\

Data File : VV016692.D

Acq On : 09 Jun 2020 04:30

Operator : SY/MD

Sample : L2901-03

Misc : 5.0mL/MSVOA V/WATER

ALS Vial : 49 Sample Multiplier: 1

Quant Time: Jun 09 05:42:03 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA V\METHOD\SOMVLM060820WMA.M

Quant Title : VOC Analysis

QLast Update : Tue Jun 09 03:40:57 2020

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampleId :




ETTR3

Manual Integrations

APPROVED

MMDadoda

6/10/2020 11:39:15 AM

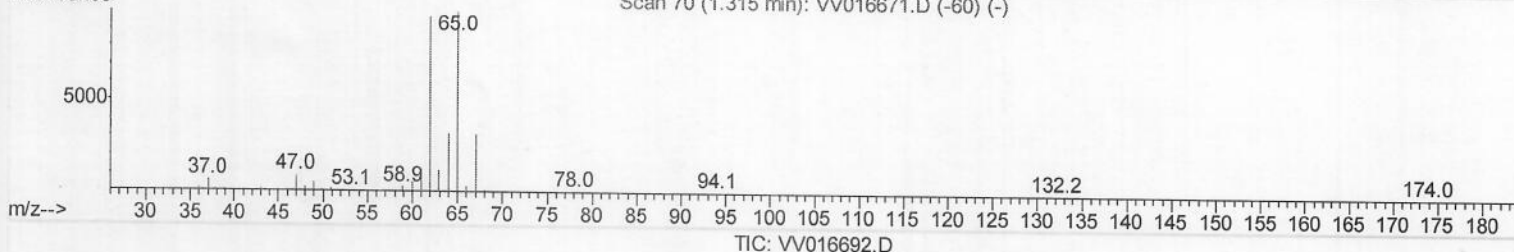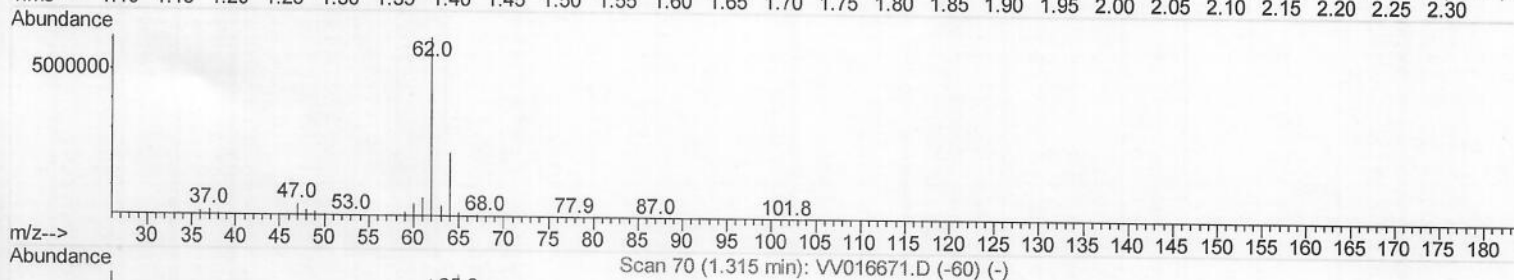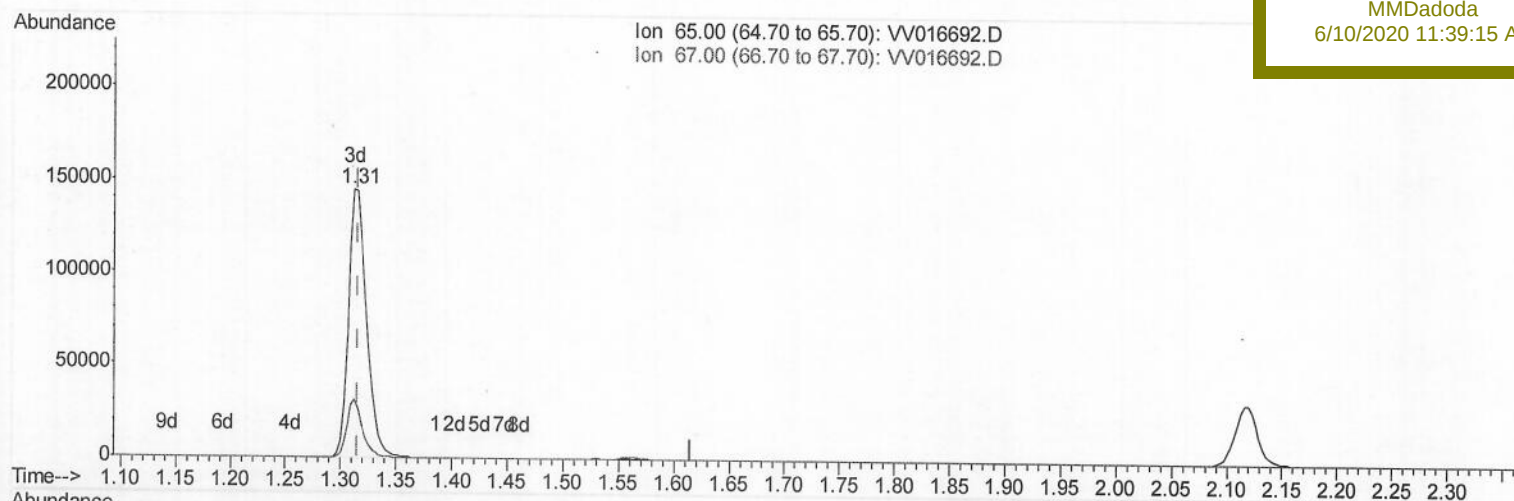

(4) Vinyl Chloride-d3 (S)

1.312min (-0.003) 68.00ug/L m

response 164462

> MD
6/10/20

Ion	Exp%	Act%
65.00	100	100
67.00	31.40	0.03#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016692.D
Acq On : 09 Jun 2020 04:30
Operator : SY/MD
Sample : L2901-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 49 Sample Multiplier: 1

Quant Time: Jun 09 05:42:03 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 09 03:40:57 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
ETTR3

Manual Integrations
APPROVED

MMDadoda
6/10/2020 11:39:15 AM

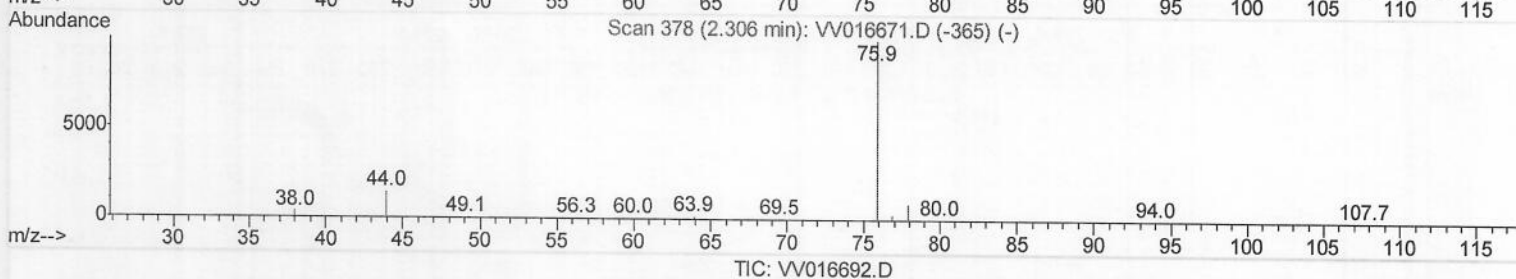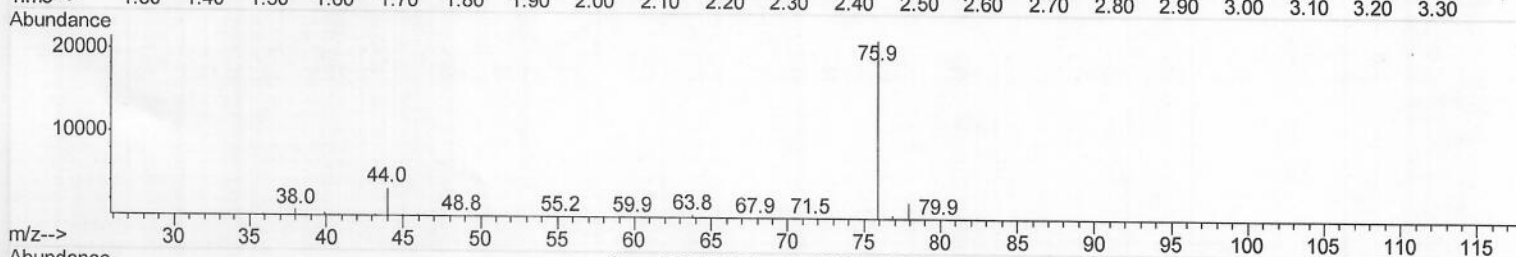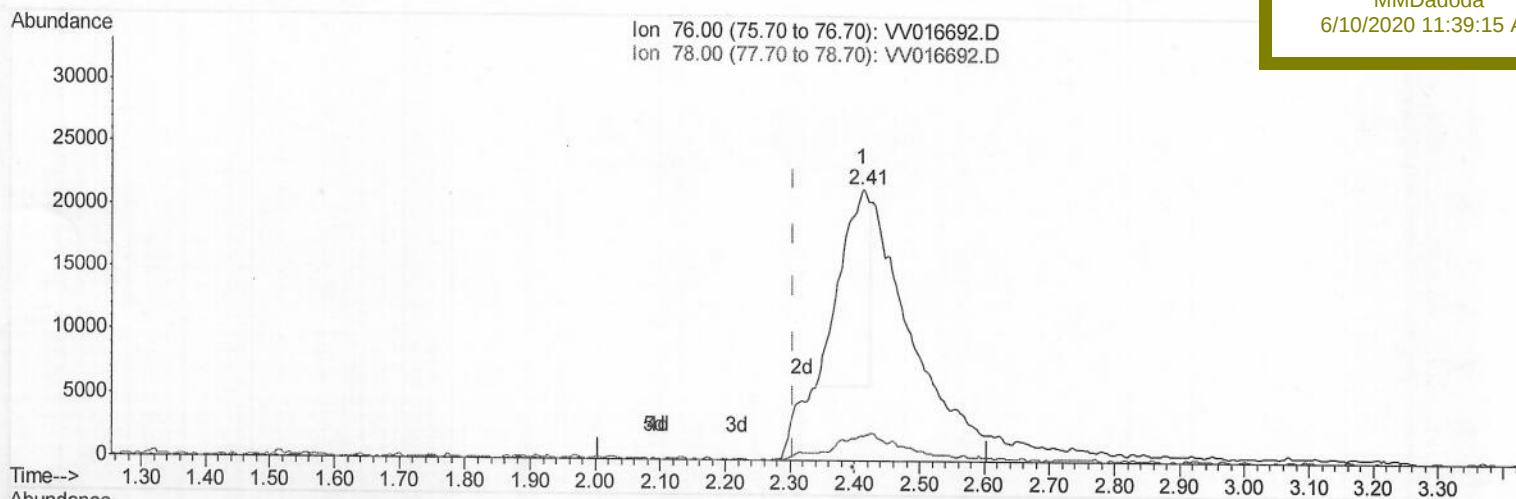

(14) Carbon disulfide (T)

2.412min (+0.106) 7.96ug/L

response 49022

Ion	Exp%	Act%
76.00	100	100
78.00	9.20	9.07
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\

Data File : VV016692.D

Acq On : 09 Jun 2020 04:30

Operator : SY/MD

Sample : L2901-03

Misc : 5.0mL/MSVOA V/WATER

ALS Vial : 49 Sample Multiplier: 1

Quant Time: Jun 09 05:42:03 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M

Quant Title : VOC Analysis

QLast Update : Tue Jun 09 03:40:57 2020

Response via : Initial Calibration

Instrument :

MSVOA_V

ClientSampleId :




ETTR3

Manual Integrations

APPROVED

MMDadoda

6/10/2020 11:39:15 AM

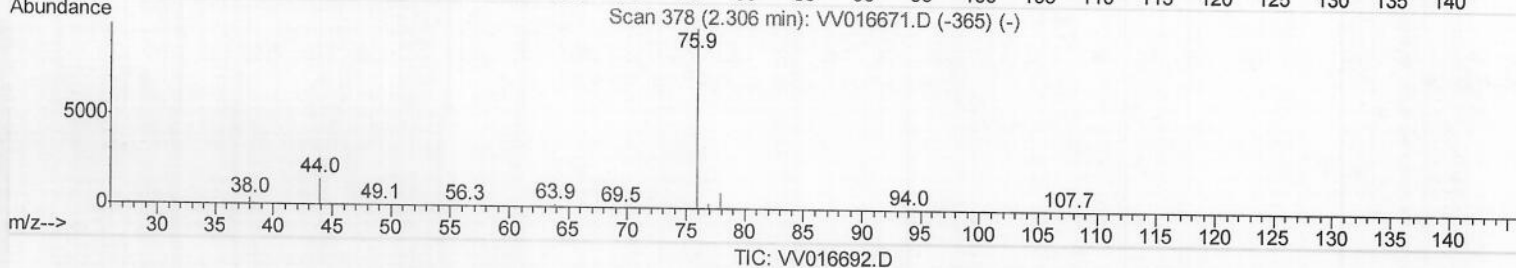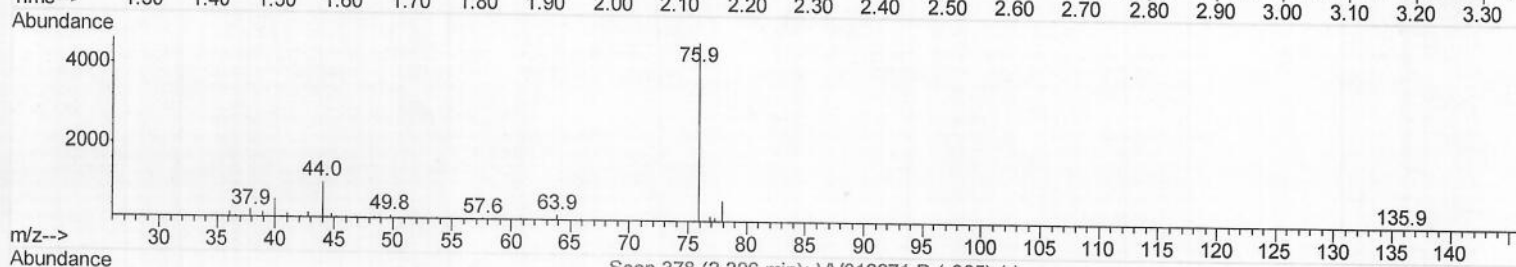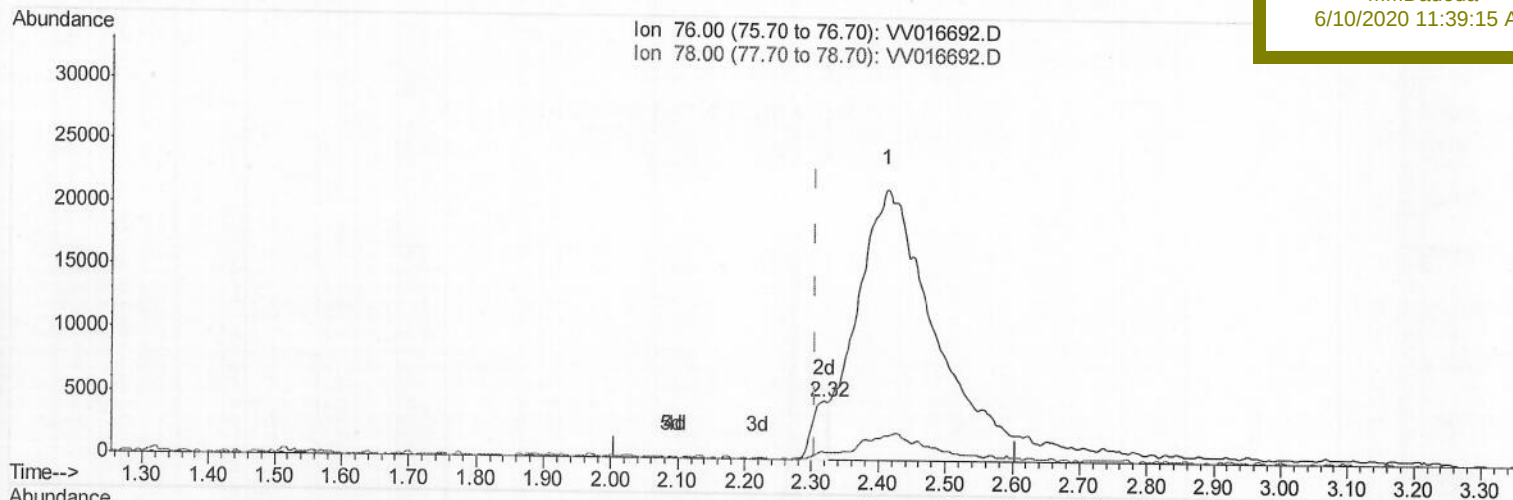

(14) Carbon disulfide (T)

2.319min (+0.013) 1.28ug/L m

response 7911

Ion	Exp%	Act%
76.00	100	100
78.00	9.20	13.29#
0.00	0.00	0.00
0.00	0.00	0.00

> MD
6/10/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016692.D
 Acq On : 09 Jun 2020 04:30
 Operator : SY/MD
 Sample : L2901-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR3

Quant Time: Jun 09 05:50:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 09 03:40:57 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 6/10/2020 11:39:15 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	342735	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	322266	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	152685	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	164462m	68.00	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	136.00%#
7) Chloroethane-d5	1.56	69	57670	39.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.48%
11) 1,1-Dichloroethene-d2	2.12	63	159433	39.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.52%
21) 2-Butanone-d5	3.92	46	213339	119.19	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	119.19%
24) Chloroform-d	4.38	84	232494	47.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.56%
26) 1,2-Dichloroethane-d4	5.05	65	167810	50.17	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.34%
32) Benzene-d6	5.07	84	449652	48.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.80%
36) 1,2-Dichloropropane-d6	6.09	67	140978	48.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.36%
41) Toluene-d8	7.34	98	407926	47.85	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.70%
43) trans-1,3-Dichloropropene-	7.64	79	67408	44.69	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.38%
47) 2-Hexanone-d5	8.11	63	144272	114.28	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	114.28%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	197812	51.60	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.20%
64) 1,2-Dichlorobenzene-d4	11.65	152	170201	52.23	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.46%

> MD
 6/10/20

Target Compounds

					Ovalue
5) Vinyl chloride	1.32	62	8764558	3586.687 ug/L	92
12) 1,1-Dichloroethene	2.13	96	29572	17.384 ug/L #	43
13) Acetone	2.18	43	4714	3.997 ug/L	88
14) Carbon disulfide	2.32	76	7911m	1.284 ug/L	98
15) Methyl Acetate	2.44	43	86786	33.016 ug/L	98
17) trans-1,2-Dichloroethene	2.78	96	113073	48.752 ug/L	98
20) cis-1,2-Dichloroethene	3.94	96	19571402	7740.175 ug/L	86

> MD
 6/10/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed