

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016660.D
 Acq On : 08 Jun 2020 15:26
 Operator : SY/MD
 Sample : L2862-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	213040	217416	13.57%	1.812%
2	1.557	138	145	158	rVB	133046	163120	10.18%	1.359%
3	2.116	308	319	334	rBV	320597	468718	29.26%	3.906%
4	2.389	401	404	407	rBV4	1630	1220	0.08%	0.010%
5	2.511	432	442	444	rBV10	3183	4264	0.27%	0.036%
6	2.730	506	510	511	rBV3	1310	697	0.04%	0.006%
7	2.820	537	538	542	rBV5	1121	784	0.05%	0.007%
8	2.872	551	554	557	rBV4	1336	745	0.05%	0.006%
9	3.061	609	613	614	rBV4	1041	715	0.04%	0.006%
10	3.132	631	635	636	rBV4	1931	1180	0.07%	0.010%
11	3.161	641	644	647	rBV4	1386	1036	0.06%	0.009%
12	3.277	678	680	683	rVB3	1381	795	0.05%	0.007%
13	3.322	692	694	697	rBV4	1151	727	0.05%	0.006%
14	3.563	767	769	772	rBV3	1407	1064	0.07%	0.009%
15	3.618	783	786	790	rVB5	1260	1094	0.07%	0.009%
16	3.650	793	796	797	rBV3	1105	702	0.04%	0.006%
17	3.685	802	807	811	rBV7	2163	2081	0.13%	0.017%
18	3.894	860	872	902	rBV2	126271	342061	21.35%	2.850%
19	4.373	1006	1021	1044	rBV	257404	619721	38.68%	5.164%
20	4.656	1107	1109	1113	rBV4	1463	1037	0.06%	0.009%
21	4.688	1116	1119	1123	rBV5	1769	1577	0.10%	0.013%
22	4.714	1123	1127	1129	rBV5	1551	1168	0.07%	0.010%
23	4.897	1180	1184	1189	rBV6	1528	1335	0.08%	0.011%
24	5.068	1220	1237	1260	rVV2	626492	1602099	100.00%	13.350%
25	5.309	1309	1312	1314	rBV4	1739	977	0.06%	0.008%
26	5.470	1359	1362	1364	rBV4	1112	686	0.04%	0.006%
27	5.515	1372	1376	1378	rBV4	1472	1192	0.07%	0.010%
28	5.640	1402	1415	1442	rBV	452124	915831	57.16%	7.632%
29	6.032	1536	1537	1542	rBV5	1176	746	0.05%	0.006%
30	6.093	1542	1556	1584	rVV	358209	729299	45.52%	6.077%
31	6.576	1703	1706	1708	rBV3	1935	1031	0.06%	0.009%
32	6.643	1723	1727	1731	rBV7	2307	2358	0.15%	0.020%
33	6.659	1731	1732	1735	rBV3	1198	751	0.05%	0.006%
34	6.868	1794	1797	1802	rVB5	1573	1315	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016660.D
 Acq On : 08 Jun 2020 15:26
 Operator : SY/MD
 Sample : L2862-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.939	1817	1819	1822	rVB3	1679	839	0.05%	0.007%
36	6.958	1822	1825	1827	rBV3	1391	955	0.06%	0.008%
37	7.006	1827	1840	1859	rBV	211549	375799	23.46%	3.132%
38	7.338	1931	1943	1963	rBV	746964	1273210	79.47%	10.610%
39	7.640	2025	2037	2053	rBV	148533	253140	15.80%	2.109%
40	7.859	2102	2105	2109	rBV5	1235	902	0.06%	0.008%
41	7.891	2112	2115	2117	rBV4	988	846	0.05%	0.007%
42	7.984	2138	2144	2149	rBV9	1396	1661	0.10%	0.014%
43	8.106	2172	2182	2217	rVV	411907	767770	47.92%	6.398%
44	8.431	2279	2283	2285	rBV4	2499	2188	0.14%	0.018%
45	8.502	2303	2305	2309	rVB4	1395	775	0.05%	0.006%
46	8.527	2309	2313	2316	rBV6	1709	1210	0.08%	0.010%
47	8.823	2402	2405	2407	rVB4	1441	708	0.04%	0.006%
48	8.871	2407	2420	2447	rBV	679538	1110414	69.31%	9.253%
49	9.039	2470	2472	2476	rBV5	1527	1242	0.08%	0.010%
50	9.103	2485	2492	2494	rBV8	2083	2098	0.13%	0.017%
51	9.151	2505	2507	2509	rBV2	1263	694	0.04%	0.006%
52	9.289	2545	2550	2553	rBV7	2049	1715	0.11%	0.014%
53	9.431	2592	2594	2596	rBV3	1649	832	0.05%	0.007%
54	9.518	2619	2621	2622	rBV2	1647	719	0.04%	0.006%
55	9.579	2636	2640	2643	rBV5	2486	1928	0.12%	0.016%
56	9.649	2659	2662	2663	rBV3	1480	724	0.05%	0.006%
57	9.711	2675	2681	2683	rBV7	1301	1459	0.09%	0.012%
58	9.897	2735	2739	2744	rBV6	1580	1643	0.10%	0.014%
59	9.936	2747	2751	2754	rBV5	1320	1395	0.09%	0.012%
60	10.042	2781	2784	2789	rBV5	1683	1416	0.09%	0.012%
61	10.093	2795	2800	2801	rBV5	1264	900	0.06%	0.007%
62	10.238	2832	2845	2861	rBV	472560	735618	45.92%	6.130%
63	10.392	2890	2893	2896	rBV4	1570	1556	0.10%	0.013%
64	10.675	2979	2981	2984	rVV3	1334	896	0.06%	0.007%
65	10.720	2992	2995	2998	rVB5	1763	850	0.05%	0.007%
66	10.749	3001	3004	3008	rBV4	1287	953	0.06%	0.008%
67	10.820	3023	3026	3028	rBV3	1930	1194	0.07%	0.010%
68	10.874	3034	3043	3045	rBV8	2704	3294	0.21%	0.027%
69	10.939	3057	3063	3068	rBV7	2197	2757	0.17%	0.023%
70	10.977	3074	3075	3080	rVB5	1837	1041	0.06%	0.009%
71	11.010	3080	3085	3087	rBV4	1581	1427	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016660.D
 Acq On : 08 Jun 2020 15:26
 Operator : SY/MD
 Sample : L2862-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.048	3095	3097	3102	rVB6	1785	1279	0.08%	0.011%
73	11.270	3155	3166	3182	rBV	703845	1081301	67.49%	9.010%
74	11.498	3234	3237	3245	rVB7	1963	2064	0.13%	0.017%
75	11.646	3271	3283	3302	rVV	776210	1240306	77.42%	10.335%
76	11.945	3372	3376	3380	rBV7	1542	1210	0.08%	0.010%
77	12.026	3398	3401	3403	rBV3	1582	812	0.05%	0.007%
78	12.061	3408	3412	3415	rBV6	1545	1193	0.07%	0.010%
79	12.090	3419	3421	3423	rBV3	1119	709	0.04%	0.006%
80	12.360	3503	3505	3511	rVB6	2170	1927	0.12%	0.016%
81	12.392	3511	3515	3518	rBV6	2310	1900	0.12%	0.016%
82	12.627	3585	3588	3593	rVB8	1590	1255	0.08%	0.010%
83	12.788	3635	3638	3642	rVB5	1295	1131	0.07%	0.009%
84	12.826	3647	3650	3653	rBV6	1412	1129	0.07%	0.009%
85	12.868	3660	3663	3664	rBV2	1018	714	0.04%	0.006%
86	12.961	3690	3692	3697	rBV5	1050	1031	0.06%	0.009%
87	13.029	3708	3713	3715	rBV5	1704	1938	0.12%	0.016%
88	13.090	3727	3732	3735	rBV7	1605	1349	0.08%	0.011%
89	13.527	3864	3868	3870	rBV4	2204	1695	0.11%	0.014%
90	13.932	3991	3994	3996	rBV3	1318	796	0.05%	0.007%
91	14.009	4015	4018	4024	rBV7	1557	1370	0.09%	0.011%
92	14.051	4029	4031	4033	rBV3	1239	685	0.04%	0.006%
93	14.273	4096	4100	4101	rBV4	1149	846	0.05%	0.007%
94	14.402	4137	4140	4142	rBV2	1634	767	0.05%	0.006%
95	14.614	4201	4206	4211	rBV8	1444	1664	0.10%	0.014%
96	14.820	4267	4270	4271	rBV3	1708	1053	0.07%	0.009%
97	14.900	4293	4295	4296	rBV2	1605	702	0.04%	0.006%
98	14.993	4320	4324	4326	rBV4	1899	1394	0.09%	0.012%
99	15.013	4328	4330	4336	rVB5	2004	1224	0.08%	0.010%
100	15.193	4381	4386	4387	rBV4	1128	813	0.05%	0.007%


Sum of corrected areas: 12000567

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016660.D
Acq On : 08 Jun 2020 15:26
Operator : SY/MD
Sample : L2862-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

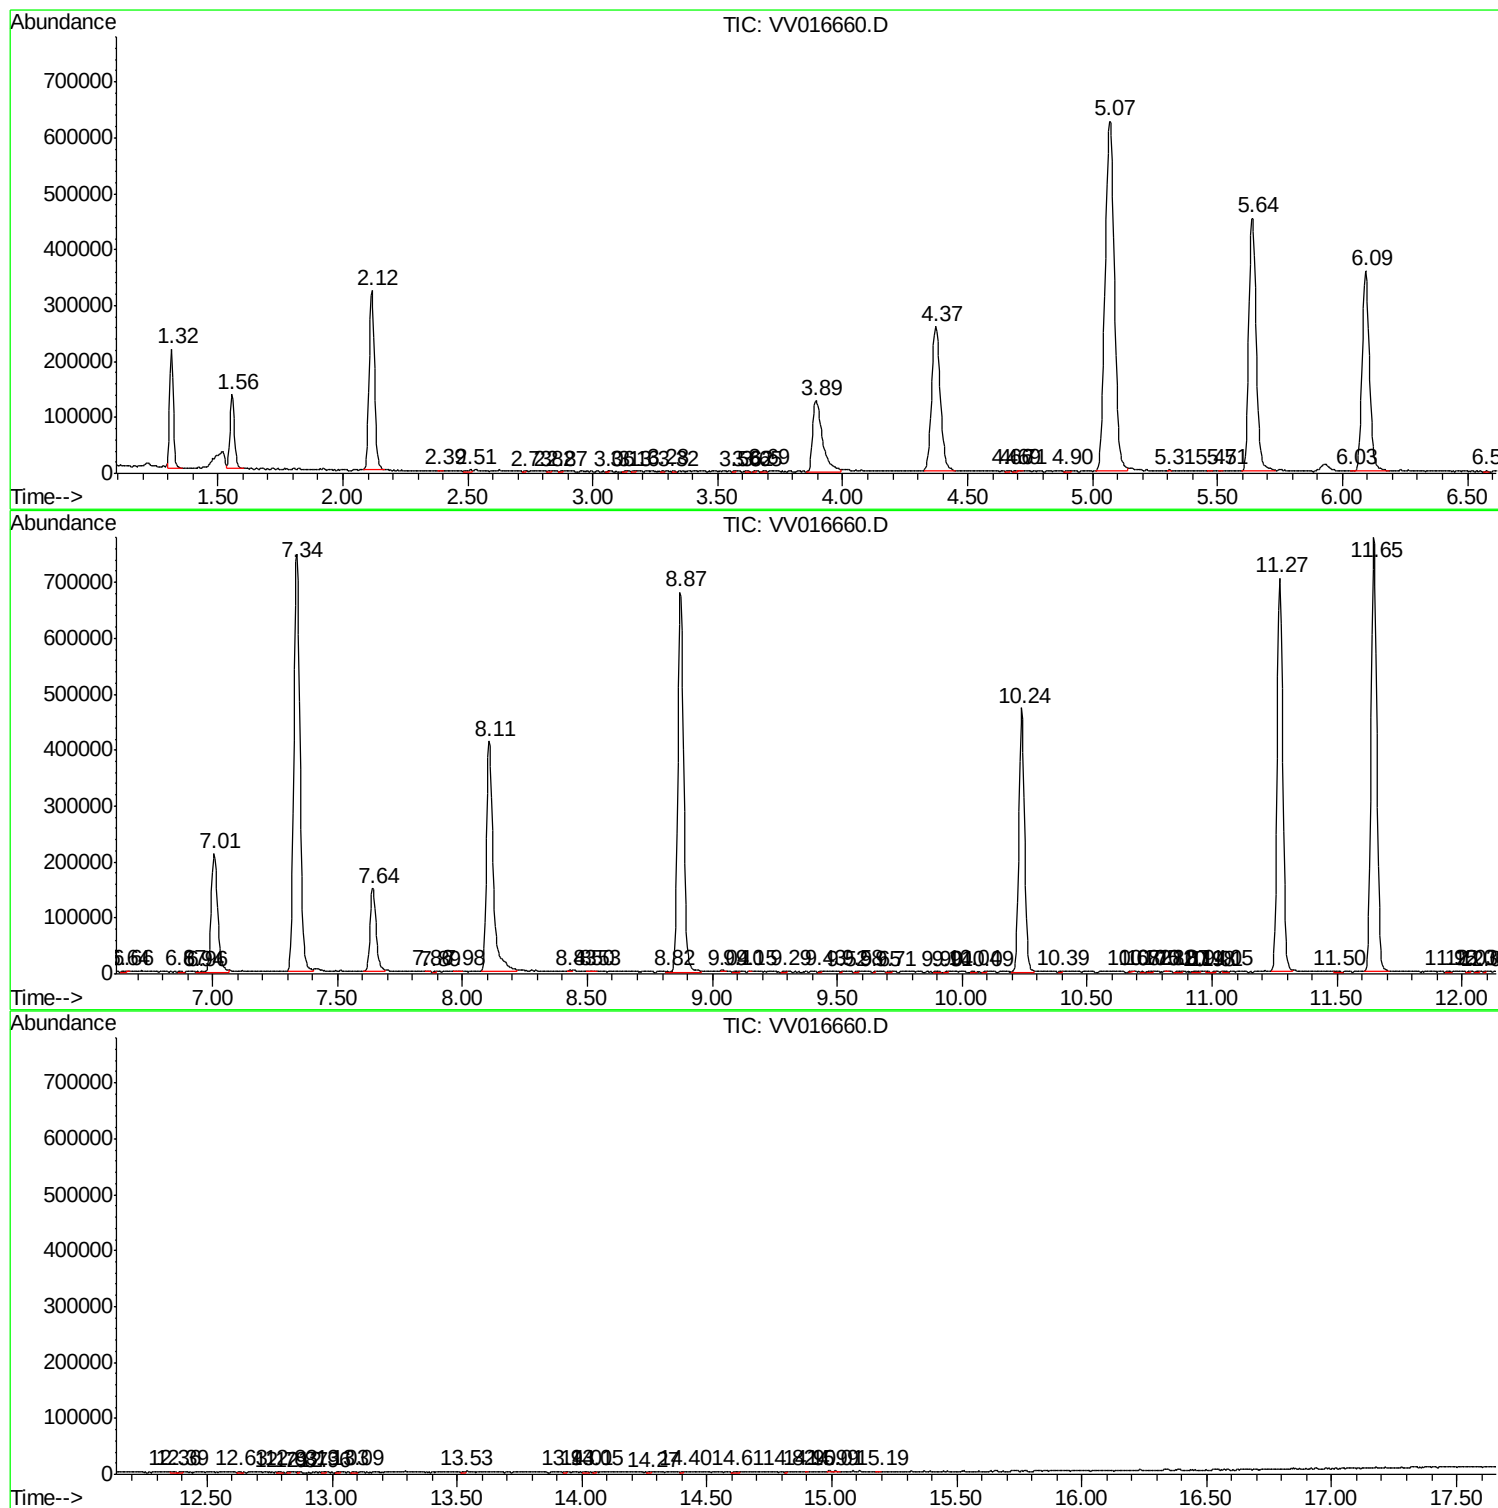

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016660.D
Acq On : 08 Jun 2020 15:26
Operator : SY/MD
Sample : L2862-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016660.D
Acq On : 08 Jun 2020 15:26
Operator : SY/MD
Sample : L2862-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc