

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016664.D
 Acq On : 08 Jun 2020 17:01
 Operator : SY/MD
 Sample : L2861-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	81	rVB	189044	190489	13.02%	1.713%
2	1.560	139	146	156	rVB	118534	142275	9.72%	1.280%
3	2.116	310	319	332	rBV	288244	415704	28.41%	3.739%
4	2.270	365	367	369	rVB2	1934	724	0.05%	0.007%
5	2.286	369	372	373	rBV2	1846	1128	0.08%	0.010%
6	2.672	490	492	495	rBV3	1666	953	0.07%	0.009%
7	2.717	504	506	508	rVB2	1509	641	0.04%	0.006%
8	2.936	570	574	575	rBV3	1464	1021	0.07%	0.009%
9	3.155	640	642	644	rBV4	1423	750	0.05%	0.007%
10	3.290	681	684	686	rBV4	1803	929	0.06%	0.008%
11	3.338	697	699	702	rBV3	1079	698	0.05%	0.006%
12	3.383	709	713	714	rBV4	1316	925	0.06%	0.008%
13	3.421	721	725	729	rBV8	1263	983	0.07%	0.009%
14	3.492	742	747	749	rBV4	944	939	0.06%	0.008%
15	3.692	806	809	812	rBV4	1717	1269	0.09%	0.011%
16	3.765	828	832	834	rBV3	1036	671	0.05%	0.006%
17	3.833	850	853	856	rVB5	1793	1395	0.10%	0.013%
18	3.894	862	872	900	rBV	114159	307263	21.00%	2.764%
19	4.290	993	995	997	rBV3	1586	773	0.05%	0.007%
20	4.373	1005	1021	1041	rBV	242007	603553	41.25%	5.429%
21	4.576	1082	1084	1087	rBV3	1564	1019	0.07%	0.009%
22	4.949	1198	1200	1205	rVB5	1691	1168	0.08%	0.011%
23	4.974	1205	1208	1209	rBV3	1491	722	0.05%	0.006%
24	5.068	1221	1237	1265	rBV2	569353	1463154	100.00%	13.161%
25	5.425	1344	1348	1351	rBV6	1731	1222	0.08%	0.011%
26	5.521	1377	1378	1383	rVB5	1053	680	0.05%	0.006%
27	5.640	1399	1415	1438	rBV	438310	877561	59.98%	7.894%
28	6.093	1542	1556	1578	rBV	333982	673636	46.04%	6.060%
29	6.502	1681	1683	1689	rVB7	2651	1757	0.12%	0.016%
30	6.634	1722	1724	1727	rBV4	1150	878	0.06%	0.008%
31	6.897	1802	1806	1811	rBV7	1764	1911	0.13%	0.017%
32	6.923	1811	1814	1818	rVV4	1466	701	0.05%	0.006%
33	7.007	1826	1840	1857	rBV	191957	344776	23.56%	3.101%
34	7.267	1916	1921	1925	rBV7	1662	1287	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016664.D
 Acq On : 08 Jun 2020 17:01
 Operator : SY/MD
 Sample : L2861-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.338	1931	1943	1961	rBV	696053	1178264	80.53%	10.599%
36	7.486	1987	1989	1992	rBV2	1335	702	0.05%	0.006%
37	7.640	2028	2037	2052	rBV	130433	222357	15.20%	2.000%
38	7.740	2065	2068	2072	rBV4	1191	1217	0.08%	0.011%
39	7.897	2115	2117	2120	rBV3	1236	658	0.04%	0.006%
40	8.106	2172	2182	2200	rBV	381281	692196	47.31%	6.226%
41	8.515	2305	2309	2314	rBV6	1728	1821	0.12%	0.016%
42	8.669	2354	2357	2360	rBV5	1361	903	0.06%	0.008%
43	8.830	2403	2407	2409	rBV5	1100	999	0.07%	0.009%
44	8.875	2409	2421	2438	rVV	662412	1066260	72.87%	9.591%
45	9.148	2501	2506	2507	rBV5	1865	1401	0.10%	0.013%
46	9.206	2520	2524	2526	rBV5	1172	896	0.06%	0.008%
47	9.408	2584	2587	2589	rBV3	992	661	0.05%	0.006%
48	9.460	2601	2603	2607	rVV4	973	757	0.05%	0.007%
49	9.714	2680	2682	2685	rBV4	1689	1078	0.07%	0.010%
50	9.743	2689	2691	2694	rBV4	1165	831	0.06%	0.007%
51	9.781	2701	2703	2706	rBV3	1543	938	0.06%	0.008%
52	9.820	2712	2715	2716	rBV3	1212	714	0.05%	0.006%
53	9.830	2716	2718	2721	rVB3	1886	860	0.06%	0.008%
54	9.887	2735	2736	2740	rVB4	1566	863	0.06%	0.008%
55	9.952	2751	2756	2757	rBV4	2227	1443	0.10%	0.013%
56	10.087	2796	2798	2803	rBV6	1505	1376	0.09%	0.012%
57	10.145	2814	2816	2823	rVV5	1462	1207	0.08%	0.011%
58	10.190	2823	2830	2832	rBV8	1497	1372	0.09%	0.012%
59	10.238	2833	2845	2860	rVV	427499	676808	46.26%	6.088%
60	10.482	2917	2921	2924	rVB5	1576	1432	0.10%	0.013%
61	10.563	2942	2946	2947	rBV4	1054	848	0.06%	0.008%
62	10.640	2966	2970	2973	rBV6	1670	1472	0.10%	0.013%
63	10.759	3004	3007	3009	rBV4	1667	1240	0.08%	0.011%
64	10.788	3015	3016	3021	rVB3	1737	878	0.06%	0.008%
65	10.875	3037	3043	3047	rVV8	1725	2139	0.15%	0.019%
66	10.974	3073	3074	3078	rBV4	1216	910	0.06%	0.008%
67	11.006	3082	3084	3086	rBV3	1230	653	0.04%	0.006%
68	11.039	3092	3094	3100	rBV5	1800	1489	0.10%	0.013%
69	11.180	3136	3138	3141	rVB4	1843	946	0.06%	0.009%
70	11.202	3141	3145	3148	rBV6	2074	1726	0.12%	0.016%
71	11.273	3155	3167	3185	rBV	652300	1009570	69.00%	9.081%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016664.D
 Acq On : 08 Jun 2020 17:01
 Operator : SY/MD
 Sample : L2861-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.457	3220	3224	3225	rBV3	1397	826	0.06%	0.007%
73	11.534	3246	3248	3251	rVB2	1421	741	0.05%	0.007%
74	11.646	3266	3283	3298	rBV	738028	1160638	79.32%	10.440%
75	11.849	3344	3346	3351	rVB6	2077	1648	0.11%	0.015%
76	11.878	3351	3355	3356	rBV3	1373	812	0.06%	0.007%
77	12.251	3468	3471	3474	rBV4	1210	982	0.07%	0.009%
78	12.292	3482	3484	3487	rVB3	1994	1013	0.07%	0.009%
79	12.383	3508	3512	3513	rBV4	909	675	0.05%	0.006%
80	12.492	3541	3546	3549	rBV6	1752	1598	0.11%	0.014%
81	12.633	3583	3590	3593	rBV7	1876	2131	0.15%	0.019%
82	12.653	3593	3596	3599	rBV4	1306	1259	0.09%	0.011%
83	12.839	3652	3654	3657	rBV4	1515	935	0.06%	0.008%
84	12.923	3678	3680	3683	rBV3	1328	789	0.05%	0.007%
85	13.009	3705	3707	3711	rBV4	1651	1011	0.07%	0.009%
86	13.154	3749	3752	3755	rBV4	1736	1305	0.09%	0.012%
87	13.270	3786	3788	3792	rBV5	1482	974	0.07%	0.009%
88	13.402	3827	3829	3832	rVB4	1494	855	0.06%	0.008%
89	13.611	3891	3894	3899	rVB7	1536	1310	0.09%	0.012%
90	13.636	3899	3902	3906	rBV5	1863	1261	0.09%	0.011%
91	13.675	3912	3914	3917	rVB3	1378	723	0.05%	0.007%
92	13.919	3988	3990	3996	rVB6	1624	1103	0.08%	0.010%
93	13.948	3996	3999	4001	rBV4	1185	868	0.06%	0.008%
94	14.595	4197	4200	4202	rBV4	1968	1078	0.07%	0.010%
95	14.704	4229	4234	4236	rBV5	2078	1714	0.12%	0.015%
96	14.746	4245	4247	4251	rVB5	1186	689	0.05%	0.006%
97	14.977	4317	4319	4322	rBV3	2414	1290	0.09%	0.012%
98	15.254	4403	4405	4407	rBV4	1562	643	0.04%	0.006%
99	15.366	4437	4440	4444	rBV5	2175	2191	0.15%	0.020%
100	15.849	4587	4590	4593	rBV5	2922	2480	0.17%	0.022%


Sum of corrected areas: 11116982

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016664.D
Acq On : 08 Jun 2020 17:01
Operator : SY/MD
Sample : L2861-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

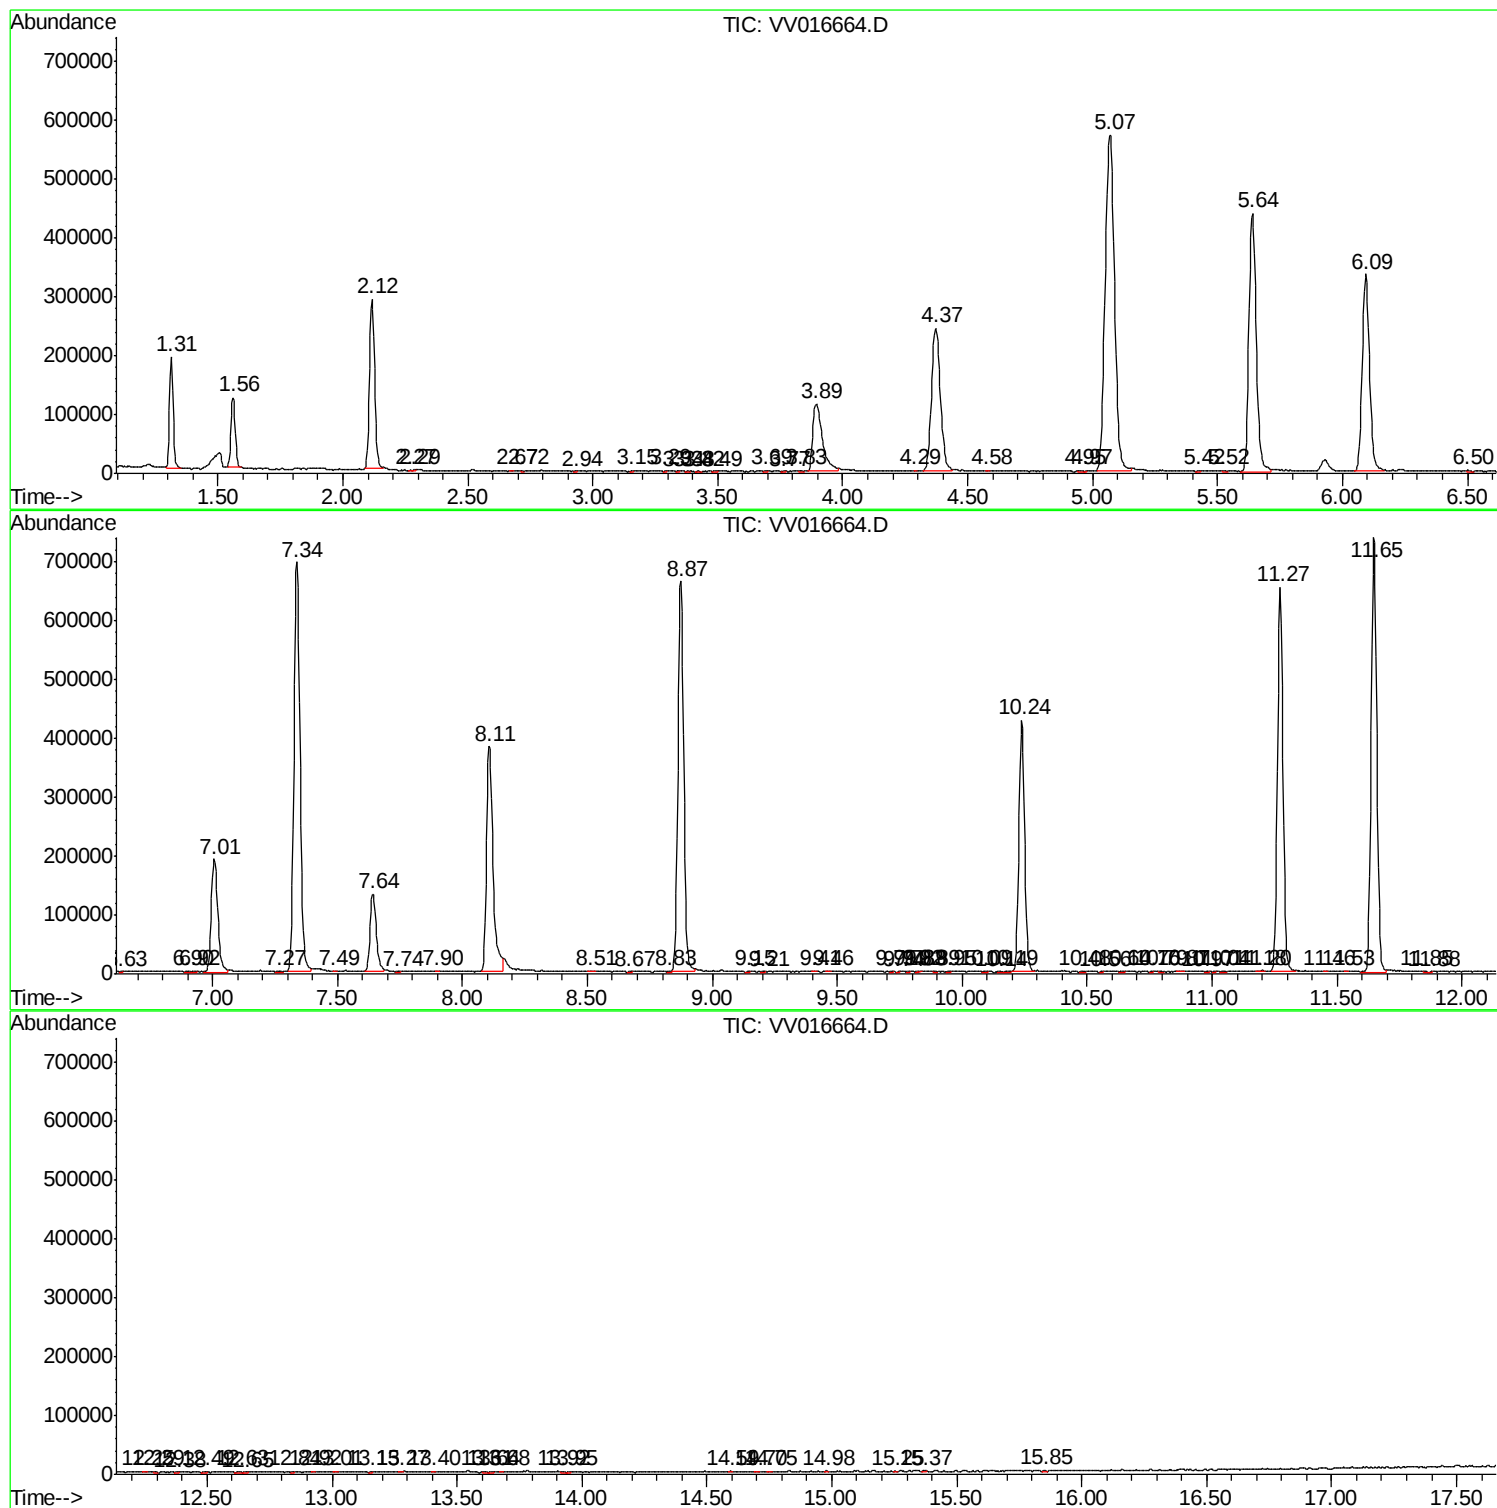

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016664.D
Acq On : 08 Jun 2020 17:01
Operator : SY/MD
Sample : L2861-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E71

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016664.D
Acq On : 08 Jun 2020 17:01
Operator : SY/MD
Sample : L2861-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E71

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc