

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016665.D
 Acq On : 08 Jun 2020 17:25
 Operator : SY/MD
 Sample : L2861-07DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E39DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	79	rVB	208428	203345	6.49%	1.215%
2	1.560	139	146	160	rVB	125399	156012	4.98%	0.932%
3	2.116	309	319	334	rBV	299479	443876	14.17%	2.652%
4	2.383	400	402	404	rBV3	986	490	0.02%	0.003%
5	2.589	460	466	475	rVB2	11119	16770	0.54%	0.100%
6	2.769	518	522	528	rBV8	2537	3343	0.11%	0.020%
7	2.852	543	548	551	rBV7	1578	1385	0.04%	0.008%
8	2.942	571	576	578	rBV5	2516	2153	0.07%	0.013%
9	3.023	597	601	605	rBV6	1619	1364	0.04%	0.008%
10	3.225	661	664	666	rBV4	976	636	0.02%	0.004%
11	3.280	678	681	682	rBV3	1351	845	0.03%	0.005%
12	3.367	706	708	711	rBV4	1023	614	0.02%	0.004%
13	3.428	723	727	728	rBV4	1403	933	0.03%	0.006%
14	3.553	764	766	768	rVB3	1319	506	0.02%	0.003%
15	3.573	770	772	773	rBV2	1361	469	0.01%	0.003%
16	3.659	796	799	803	rBV5	1435	1397	0.04%	0.008%
17	3.704	810	813	815	rBV4	885	605	0.02%	0.004%
18	3.894	861	872	900	rBV	125281	334024	10.66%	1.995%
19	4.132	945	946	948	rBV2	1114	561	0.02%	0.003%
20	4.258	983	985	988	rVB4	2047	1082	0.03%	0.006%
21	4.274	988	990	992	rBV3	1525	1024	0.03%	0.006%
22	4.373	1003	1021	1043	rBV	249780	615957	19.66%	3.680%
23	4.807	1154	1156	1158	rBV3	1512	716	0.02%	0.004%
24	4.881	1176	1179	1183	rBV3	843	733	0.02%	0.004%
25	4.901	1183	1185	1190	rVB6	1774	1334	0.04%	0.008%
26	4.930	1190	1194	1198	rBV8	1807	1556	0.05%	0.009%
27	4.987	1211	1212	1217	rBV4	891	605	0.02%	0.004%
28	5.071	1221	1238	1245	rBV2	615070	1507723	48.12%	9.007%
29	5.534	1380	1382	1384	rBV2	1015	529	0.02%	0.003%
30	5.592	1398	1400	1401	rBV2	1243	624	0.02%	0.004%
31	5.640	1402	1415	1447	rVV	439162	886730	28.30%	5.297%
32	6.093	1538	1556	1584	rBV	342673	710575	22.68%	4.245%
33	6.524	1685	1690	1695	rBV7	1876	2116	0.07%	0.013%
34	6.563	1697	1702	1705	rBV6	2021	2323	0.07%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016665.D
 Acq On : 08 Jun 2020 17:25
 Operator : SY/MD
 Sample : L2861-07DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E39DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.743	1755	1758	1760	rBV4	906	617	0.02%	0.004%
36	6.801	1773	1776	1777	rBV3	1037	638	0.02%	0.004%
37	6.830	1783	1785	1792	rVB8	1812	1527	0.05%	0.009%
38	6.862	1794	1795	1797	rVB3	1634	445	0.01%	0.003%
39	6.891	1801	1804	1807	rBV4	1256	1056	0.03%	0.006%
40	6.939	1816	1819	1821	rBV4	1605	786	0.03%	0.005%
41	6.955	1821	1824	1828	rVV4	1677	1233	0.04%	0.007%
42	7.007	1829	1840	1862	rBV2	201182	362587	11.57%	2.166%
43	7.338	1930	1943	1954	rBV	720345	1241530	39.62%	7.417%
44	7.409	1954	1965	1991	rVB	1849984	3133517	100.00%	18.720%
45	7.640	2028	2037	2053	rBV2	139808	238205	7.60%	1.423%
46	7.798	2083	2086	2091	rBV7	1851	1613	0.05%	0.010%
47	7.910	2120	2121	2124	rBV3	1455	617	0.02%	0.004%
48	7.984	2141	2144	2148	rBV5	1826	1458	0.05%	0.009%
49	8.039	2159	2161	2167	rVB6	1792	1604	0.05%	0.010%
50	8.064	2167	2169	2171	rBV3	832	485	0.02%	0.003%
51	8.106	2171	2182	2210	rBV	417177	753715	24.05%	4.503%
52	8.367	2261	2263	2266	rBV3	2119	1142	0.04%	0.007%
53	8.572	2323	2327	2329	rBV5	977	766	0.02%	0.005%
54	8.656	2349	2353	2359	rVB8	1963	2106	0.07%	0.013%
55	8.682	2359	2361	2362	rBV2	1824	624	0.02%	0.004%
56	8.714	2367	2371	2372	rBV3	892	531	0.02%	0.003%
57	8.740	2376	2379	2380	rBV3	1232	556	0.02%	0.003%
58	8.875	2407	2421	2444	rVV	663679	1088521	34.74%	6.503%
59	9.032	2459	2470	2486	rBV	633369	987837	31.52%	5.901%
60	9.158	2502	2509	2528	rVB	249357	418621	13.36%	2.501%
61	9.566	2627	2636	2652	rVB	234928	370145	11.81%	2.211%
62	9.955	2750	2757	2770	rVB	12738	19869	0.63%	0.119%
63	10.032	2778	2781	2784	rBV5	1421	961	0.03%	0.006%
64	10.055	2784	2788	2790	rBV4	1250	1148	0.04%	0.007%
65	10.170	2823	2824	2828	rBV4	1060	840	0.03%	0.005%
66	10.238	2833	2845	2859	rBV	468536	737612	23.54%	4.407%
67	10.939	3054	3063	3073	rBV	32523	52117	1.66%	0.311%
68	11.270	3155	3166	3184	rBV	703554	1071269	34.19%	6.400%
69	11.521	3241	3244	3245	rBV3	1067	537	0.02%	0.003%
70	11.553	3246	3254	3263	rVV2	15748	25439	0.81%	0.152%
71	11.646	3272	3283	3301	rBV	779702	1218311	38.88%	7.278%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016665.D
 Acq On : 08 Jun 2020 17:25
 Operator : SY/MD
 Sample : L2861-07DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E39DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.768	3313	3321	3330	rBV8	7773	14602	0.47%	0.087%
73	12.212	3457	3459	3462	rVB4	1759	813	0.03%	0.005%
74	12.305	3485	3488	3491	rBV4	1337	1052	0.03%	0.006%
75	12.572	3567	3571	3573	rBV5	902	696	0.02%	0.004%
76	12.611	3582	3583	3585	rBV2	1225	530	0.02%	0.003%
77	12.675	3600	3603	3606	rBV4	2573	1886	0.06%	0.011%
78	12.707	3610	3613	3615	rBV4	1093	660	0.02%	0.004%
79	12.804	3639	3643	3647	rBV6	2005	1454	0.05%	0.009%
80	13.022	3709	3711	3714	rBV4	806	703	0.02%	0.004%
81	13.077	3722	3728	3731	rBV7	2551	2862	0.09%	0.017%
82	13.251	3779	3782	3785	rVB5	2036	1208	0.04%	0.007%
83	13.276	3788	3790	3792	rBV3	1278	768	0.02%	0.005%
84	13.444	3837	3842	3845	rBV6	1784	1409	0.04%	0.008%
85	13.530	3859	3869	3883	rVB2	27179	43706	1.39%	0.261%
86	13.646	3896	3905	3909	rBV7	5007	7138	0.23%	0.043%
87	13.762	3938	3941	3943	rBV3	1216	750	0.02%	0.004%
88	13.862	3965	3972	3977	rBV8	2050	3042	0.10%	0.018%
89	13.910	3982	3987	3990	rBV6	1409	1400	0.04%	0.008%
90	13.990	4009	4012	4014	rBV3	1327	928	0.03%	0.006%
91	14.042	4025	4028	4030	rBV3	1538	938	0.03%	0.006%
92	14.129	4052	4055	4057	rBV3	1390	992	0.03%	0.006%
93	14.141	4057	4059	4066	rVV6	1526	1900	0.06%	0.011%
94	14.309	4108	4111	4114	rBV4	1412	1014	0.03%	0.006%
95	14.421	4144	4146	4149	rVB4	1360	694	0.02%	0.004%
96	14.620	4205	4208	4210	rBV3	1449	738	0.02%	0.004%
97	14.739	4243	4245	4248	rBV3	1422	816	0.03%	0.005%
98	14.846	4275	4278	4279	rBV2	2376	1472	0.05%	0.009%
99	14.990	4321	4323	4325	rBV3	1826	737	0.02%	0.004%
100	15.511	4483	4485	4486	rBV2	1404	519	0.02%	0.003%


Sum of corrected areas: 16738967

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016665.D
Acq On : 08 Jun 2020 17:25
Operator : SY/MD
Sample : L2861-07DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E39DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

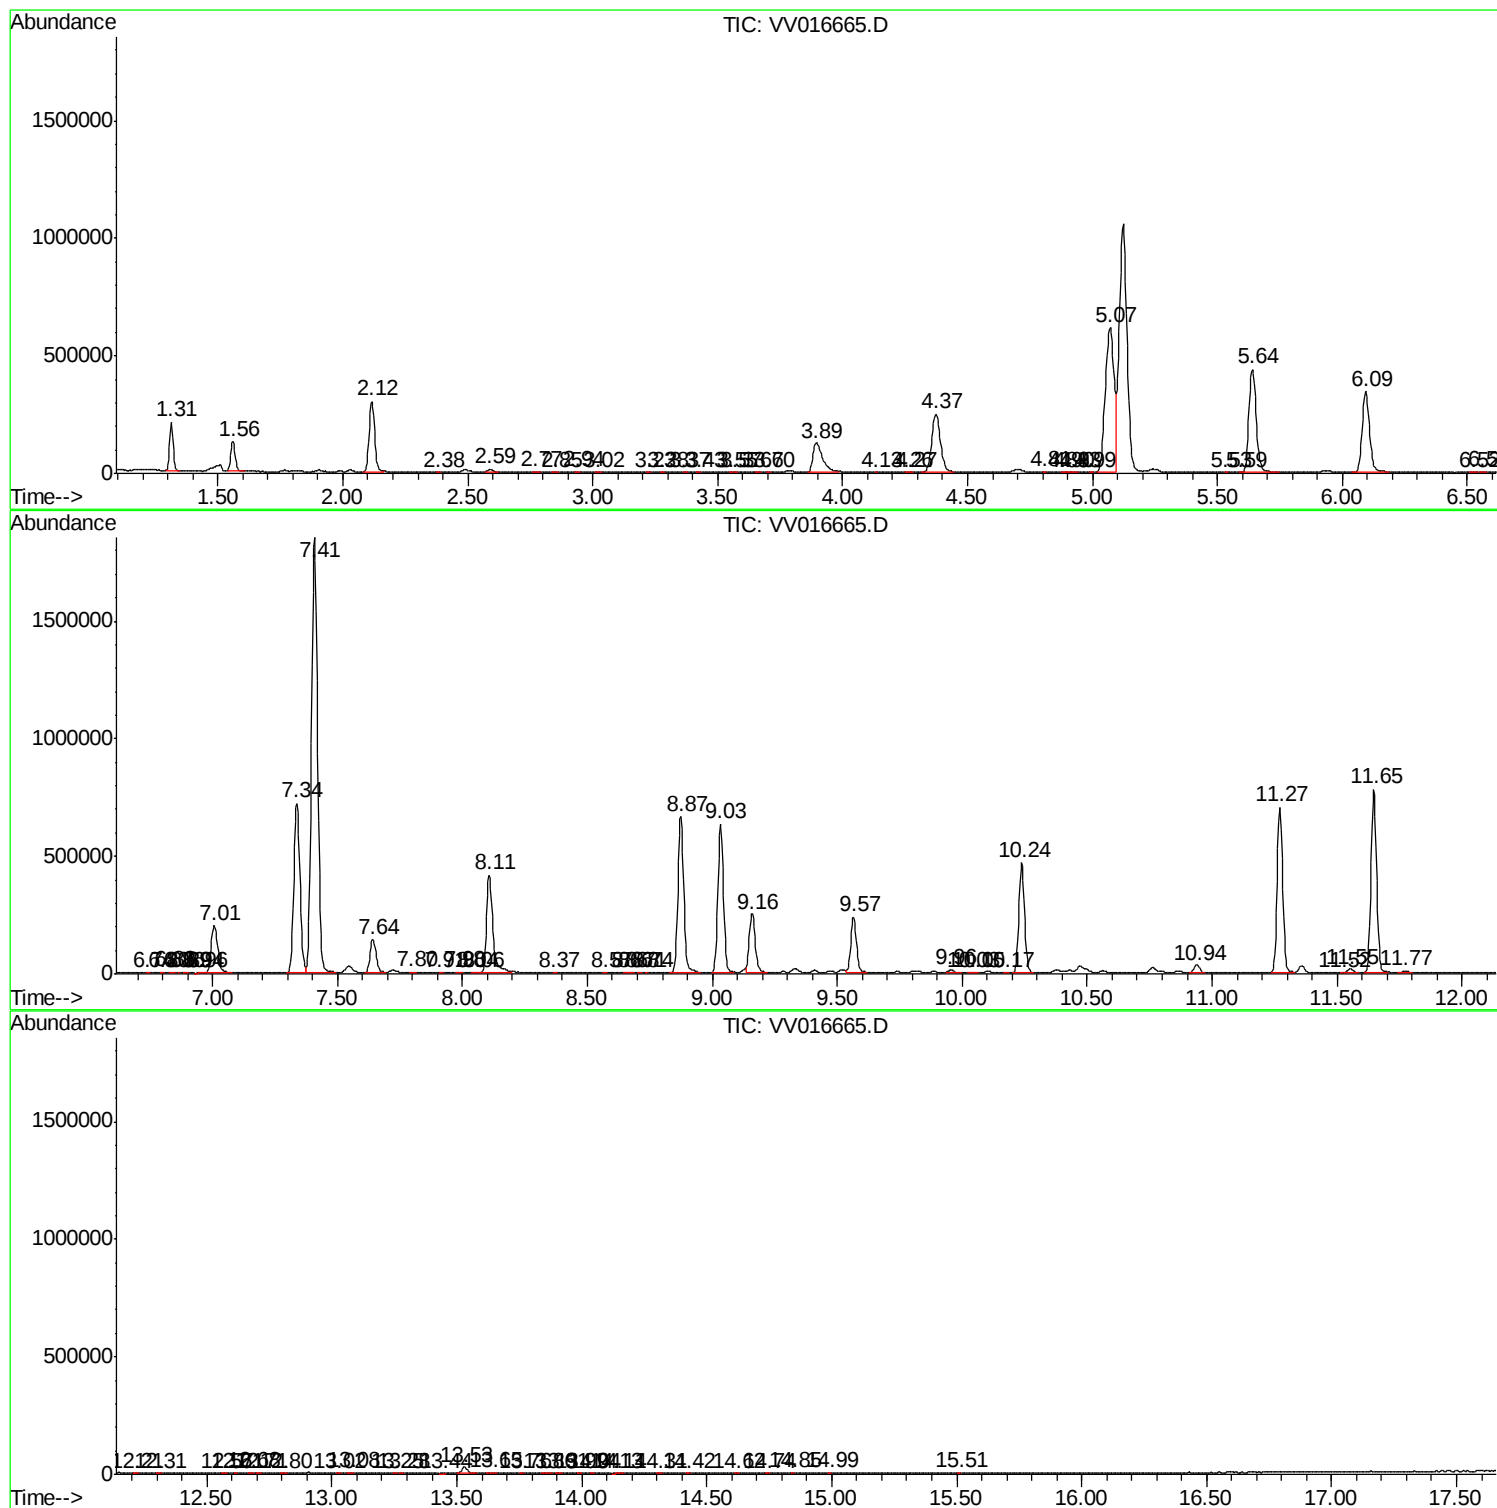

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016665.D
Acq On : 08 Jun 2020 17:25
Operator : SY/MD
Sample : L2861-07DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E39DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016665.D
Acq On : 08 Jun 2020 17:25
Operator : SY/MD
Sample : L2861-07DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E39DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc