

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016666.D
 Acq On : 08 Jun 2020 17:48
 Operator : SY/MD
 Sample : L2861-08DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E40DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	80	rVB	190809	196339	6.64%	1.218%
2	1.560	139	146	158	rVB	130299	159918	5.41%	0.992%
3	2.116	310	319	331	rBV	293145	423739	14.33%	2.629%
4	2.415	410	412	413	rBV3	788	290	0.01%	0.002%
5	2.724	505	508	510	rBV3	1494	1060	0.04%	0.007%
6	2.737	510	512	516	rBV4	1684	1474	0.05%	0.009%
7	2.872	551	554	555	rBV3	1076	492	0.02%	0.003%
8	2.917	567	568	570	rBV2	669	248	0.01%	0.002%
9	2.933	571	573	578	rVV4	1426	1269	0.04%	0.008%
10	3.100	623	625	628	rBV4	763	425	0.01%	0.003%
11	3.116	628	630	633	rVB4	1444	683	0.02%	0.004%
12	3.145	637	639	642	rVB3	1504	557	0.02%	0.003%
13	3.164	642	645	647	rBV3	1214	795	0.03%	0.005%
14	3.235	665	667	671	rBV5	1851	1349	0.05%	0.008%
15	3.280	675	681	684	rBV8	1540	1832	0.06%	0.011%
16	3.354	702	704	706	rBV3	990	505	0.02%	0.003%
17	3.412	720	722	725	rBV4	785	482	0.02%	0.003%
18	3.582	773	775	777	rBV3	1339	897	0.03%	0.006%
19	3.640	790	793	795	rBV3	1298	943	0.03%	0.006%
20	3.675	801	804	806	rBV3	1239	952	0.03%	0.006%
21	3.894	862	872	897	rBV	122192	331191	11.20%	2.055%
22	4.283	992	993	996	rVB3	2184	813	0.03%	0.005%
23	4.302	996	999	1003	rBV5	2376	2652	0.09%	0.016%
24	4.373	1008	1021	1046	rVB	240867	588276	19.90%	3.650%
25	4.553	1075	1077	1078	rBV2	628	246	0.01%	0.002%
26	5.068	1221	1237	1245	rBV2	590199	1458682	49.34%	9.050%
27	5.640	1402	1415	1437	rBV	454224	903842	30.57%	5.607%
28	6.093	1544	1556	1573	rBV	332977	666419	22.54%	4.134%
29	6.354	1634	1637	1638	rBV4	1174	589	0.02%	0.004%
30	6.450	1663	1667	1668	rBV4	1351	950	0.03%	0.006%
31	6.775	1765	1768	1769	rBV3	741	458	0.02%	0.003%
32	6.875	1797	1799	1801	rBV3	1142	562	0.02%	0.003%
33	6.891	1802	1804	1808	rVV5	2212	1170	0.04%	0.007%
34	6.913	1810	1811	1814	rBV3	1135	532	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016666.D
 Acq On : 08 Jun 2020 17:48
 Operator : SY/MD
 Sample : L2861-08DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E40DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.006	1829	1840	1862	rBV2	192330	343368	11.61%	2.130%
36	7.338	1931	1943	1954	rBV	698088	1190771	40.28%	7.387%
37	7.408	1955	1965	1987	rVB	1754639	2956322	100.00%	18.341%
38	7.640	2029	2037	2054	rVB	135802	222378	7.52%	1.380%
39	7.994	2145	2147	2148	rBV	1413	575	0.02%	0.004%
40	8.106	2172	2182	2212	rBV	403510	724976	24.52%	4.498%
41	8.476	2296	2297	2302	rBV4	872	666	0.02%	0.004%
42	8.534	2313	2315	2321	rVB7	2229	1510	0.05%	0.009%
43	8.576	2326	2328	2330	rBV3	1232	433	0.01%	0.003%
44	8.717	2370	2372	2375	rBV4	1554	1232	0.04%	0.008%
45	8.772	2387	2389	2391	rBV2	1078	516	0.02%	0.003%
46	8.875	2409	2421	2448	rBV	681866	1117826	37.81%	6.935%
47	9.032	2459	2470	2485	rBV	590469	914800	30.94%	5.675%
48	9.158	2502	2509	2526	rVB2	237481	395104	13.36%	2.451%
49	9.405	2578	2586	2595	rBV2	8899	15512	0.52%	0.096%
50	9.566	2627	2636	2659	rVB	225513	355341	12.02%	2.205%
51	10.064	2789	2791	2792	rVB2	1413	378	0.01%	0.002%
52	10.151	2817	2818	2819	rBV	935	268	0.01%	0.002%
53	10.238	2833	2845	2861	rBV	455063	720622	24.38%	4.471%
54	10.939	3055	3063	3072	rVB	29978	43186	1.46%	0.268%
55	11.174	3131	3136	3139	rBV6	3014	2759	0.09%	0.017%
56	11.270	3155	3166	3184	rBV	733112	1110296	37.56%	6.888%
57	11.646	3272	3283	3297	rBV	770838	1183001	40.02%	7.339%
58	11.971	3377	3384	3388	rBV9	2499	3396	0.11%	0.021%
59	12.042	3401	3406	3411	rBV9	2757	3432	0.12%	0.021%
60	12.087	3418	3420	3424	rVB4	1152	417	0.01%	0.003%
61	12.247	3468	3470	3472	rBV3	884	452	0.02%	0.003%
62	12.585	3573	3575	3584	rBV9	1381	1514	0.05%	0.009%
63	12.788	3636	3638	3642	rVB4	1296	721	0.02%	0.004%
64	12.826	3647	3650	3652	rBV3	1021	487	0.02%	0.003%
65	12.845	3652	3656	3658	rBV4	1397	1341	0.05%	0.008%
66	12.874	3663	3665	3668	rBV3	1691	1033	0.03%	0.006%
67	12.977	3695	3697	3700	rBV3	2036	1082	0.04%	0.007%
68	13.029	3708	3713	3715	rBV6	1751	1288	0.04%	0.008%
69	13.074	3720	3727	3728	rBV6	2965	2815	0.10%	0.017%
70	13.138	3746	3747	3752	rVB3	1475	1124	0.04%	0.007%
71	13.167	3754	3756	3758	rVV3	1116	479	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016666.D
Acq On : 08 Jun 2020 17:48
Operator : SY/MD
Sample : L2861-08DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E40DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Title : VOC Analysis

72	13.190	3761	3763	3765	rBV3	724	355	0.01%	0.002%
73	13.199	3765	3766	3768	rBV2	796	360	0.01%	0.002%
74	13.260	3782	3785	3786	rBV3	1277	662	0.02%	0.004%
75	13.366	3815	3818	3819	rBV3	2068	994	0.03%	0.006%
76	13.386	3822	3824	3826	rVV2	1706	920	0.03%	0.006%
77	13.415	3830	3833	3835	rVV3	1376	796	0.03%	0.005%
78	13.530	3861	3869	3878	rBV2	23661	35587	1.20%	0.221%
79	13.710	3923	3925	3926	rBV2	984	398	0.01%	0.002%
80	13.887	3976	3980	3985	rVB6	1888	1485	0.05%	0.009%
81	14.022	4019	4022	4024	rBV3	1355	945	0.03%	0.006%
82	14.106	4047	4048	4049	rBV	1064	279	0.01%	0.002%
83	14.161	4061	4065	4066	rBV4	1018	626	0.02%	0.004%
84	14.254	4092	4094	4096	rVB3	2138	695	0.02%	0.004%
85	14.537	4180	4182	4185	rBV4	1597	746	0.03%	0.005%
86	14.572	4191	4193	4195	rBV3	1110	492	0.02%	0.003%
87	14.919	4298	4301	4302	rBV3	1388	752	0.03%	0.005%
88	15.498	4479	4481	4484	rBV3	1676	701	0.02%	0.004%


Sum of corrected areas: 16118845

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016666.D
Acq On : 08 Jun 2020 17:48
Operator : SY/MD
Sample : L2861-08DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E40DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

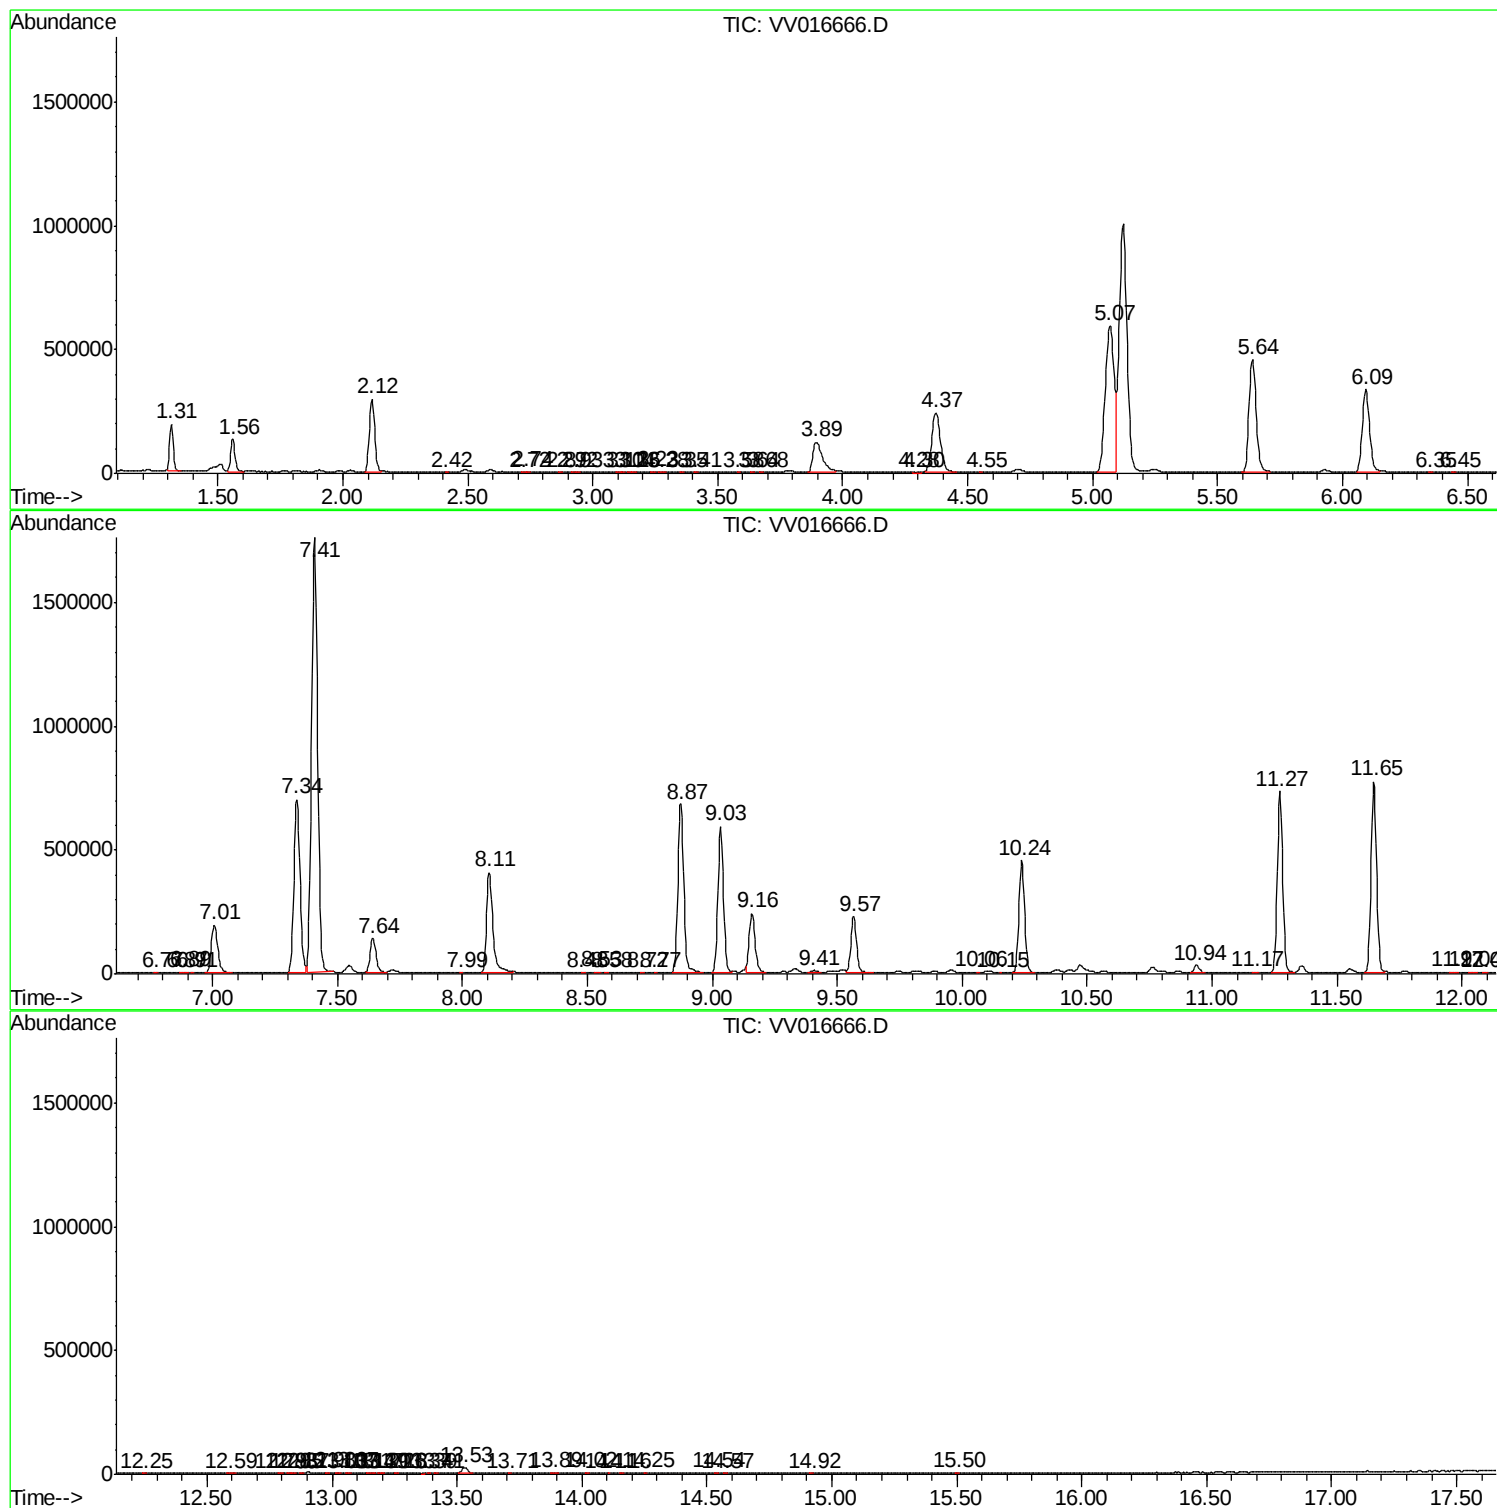

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016666.D
Acq On : 08 Jun 2020 17:48
Operator : SY/MD
Sample : L2861-08DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E40DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016666.D
Acq On : 08 Jun 2020 17:48
Operator : SY/MD
Sample : L2861-08DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E40DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
