

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016668.D
 Acq On : 08 Jun 2020 18:36
 Operator : SY/MD
 Sample : L2875-16 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	79	rVB	199388	189551	12.74%	1.688%
2	1.560	140	146	159	rVB	128675	151739	10.20%	1.351%
3	2.116	309	319	332	rBV	288417	420381	28.26%	3.743%
4	2.711	501	504	508	rBV6	849	577	0.04%	0.005%
5	2.856	547	549	551	rBV3	1305	849	0.06%	0.008%
6	2.910	563	566	570	rBV4	1643	1325	0.09%	0.012%
7	3.065	611	614	615	rBV3	1057	502	0.03%	0.004%
8	3.126	630	633	634	rBV3	1469	841	0.06%	0.007%
9	3.245	667	670	672	rBV4	1298	785	0.05%	0.007%
10	3.296	683	686	690	rBV5	1421	1243	0.08%	0.011%
11	3.415	721	723	725	rBV3	1390	791	0.05%	0.007%
12	3.444	728	732	735	rBV6	1938	1552	0.10%	0.014%
13	3.460	735	737	739	rVV3	1130	477	0.03%	0.004%
14	3.592	776	778	780	rBV4	1051	382	0.03%	0.003%
15	3.627	788	789	791	rBV2	793	267	0.02%	0.002%
16	3.663	797	800	802	rBV3	1586	1041	0.07%	0.009%
17	3.675	802	804	808	rVV5	1261	820	0.06%	0.007%
18	3.737	822	823	828	rVB3	1911	1186	0.08%	0.011%
19	3.769	828	833	834	rBV3	1626	1490	0.10%	0.013%
20	3.891	859	871	902	rBV	120071	340808	22.91%	3.035%
21	4.132	944	946	949	rBV3	2054	1006	0.07%	0.009%
22	4.373	1006	1021	1046	rVB	236188	573938	38.58%	5.111%
23	4.528	1067	1069	1071	rBV3	1228	651	0.04%	0.006%
24	4.566	1079	1081	1084	rBV3	1514	896	0.06%	0.008%
25	4.685	1117	1118	1119	rBV	1082	392	0.03%	0.003%
26	4.724	1128	1130	1134	rBV4	1416	888	0.06%	0.008%
27	4.798	1152	1153	1155	rBV2	1178	380	0.03%	0.003%
28	4.913	1187	1189	1190	rBV	1184	591	0.04%	0.005%
29	4.952	1199	1201	1204	rVB3	1411	465	0.03%	0.004%
30	5.068	1217	1237	1264	rBV2	572831	1487654	100.00%	13.247%
31	5.482	1361	1366	1370	rBV8	2119	2623	0.18%	0.023%
32	5.540	1383	1384	1385	rBV	1236	437	0.03%	0.004%
33	5.582	1395	1397	1400	rVB3	2129	1202	0.08%	0.011%
34	5.640	1400	1415	1438	rBV	443661	889347	59.78%	7.919%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016668.D
 Acq On : 08 Jun 2020 18:36
 Operator : SY/MD
 Sample : L2875-16 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.048	1539	1542	1543	rBV3	1490	824	0.06%	0.007%
36	6.093	1543	1556	1577	rVV	333509	666237	44.78%	5.932%
37	6.380	1643	1645	1648	rVB3	1134	419	0.03%	0.004%
38	6.421	1655	1658	1661	rBV5	1141	1000	0.07%	0.009%
39	6.444	1664	1665	1666	rBV	892	309	0.02%	0.003%
40	6.505	1681	1684	1686	rBV3	1329	974	0.07%	0.009%
41	6.794	1772	1774	1775	rBV2	1264	571	0.04%	0.005%
42	6.855	1791	1793	1795	rBV3	1635	954	0.06%	0.008%
43	7.007	1828	1840	1856	rBV	186659	334402	22.48%	2.978%
44	7.228	1905	1909	1913	rBV6	2107	2231	0.15%	0.020%
45	7.338	1932	1943	1959	rBV	672839	1154367	77.60%	10.279%
46	7.582	2017	2019	2021	rBV3	1420	868	0.06%	0.008%
47	7.640	2027	2037	2054	rBV	135232	228109	15.33%	2.031%
48	7.913	2121	2122	2124	rBV	1097	500	0.03%	0.004%
49	8.035	2157	2160	2163	rBV4	1229	868	0.06%	0.008%
50	8.106	2171	2182	2219	rBV	390210	730219	49.09%	6.502%
51	8.473	2294	2296	2297	rBV2	1435	545	0.04%	0.005%
52	8.560	2318	2323	2326	rBV6	2316	2264	0.15%	0.020%
53	8.646	2348	2350	2352	rBV2	928	569	0.04%	0.005%
54	8.666	2352	2356	2358	rVV5	1350	1070	0.07%	0.010%
55	8.736	2375	2378	2380	rBV4	1498	900	0.06%	0.008%
56	8.788	2393	2394	2398	rBV4	942	510	0.03%	0.005%
57	8.875	2408	2421	2442	rBV	670610	1088960	73.20%	9.697%
58	9.090	2486	2488	2490	rBV2	1118	594	0.04%	0.005%
59	9.251	2536	2538	2540	rBV4	1036	508	0.03%	0.005%
60	9.299	2552	2553	2555	rVB2	1110	256	0.02%	0.002%
61	9.421	2589	2591	2594	rBV4	1211	657	0.04%	0.006%
62	9.733	2686	2688	2691	rBV4	1634	1034	0.07%	0.009%
63	9.756	2693	2695	2703	rVB8	1913	1547	0.10%	0.014%
64	9.961	2755	2759	2762	rBV6	1625	1079	0.07%	0.010%
65	10.061	2789	2790	2792	rBV	719	323	0.02%	0.003%
66	10.103	2797	2803	2806	rVB6	1417	1594	0.11%	0.014%
67	10.129	2809	2811	2813	rBV3	1118	409	0.03%	0.004%
68	10.186	2827	2829	2830	rBV2	821	302	0.02%	0.003%
69	10.238	2833	2845	2865	rVV	445126	698496	46.95%	6.220%
70	10.524	2931	2934	2940	rVB6	1191	1080	0.07%	0.010%
71	10.640	2967	2970	2972	rBV4	1873	1437	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016668.D
 Acq On : 08 Jun 2020 18:36
 Operator : SY/MD
 Sample : L2875-16 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTT8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.740	2999	3001	3003	rBV3	1169	472	0.03%	0.004%
73	10.765	3008	3009	3012	rVB4	1673	669	0.04%	0.006%
74	11.180	3135	3138	3140	rBV3	1677	1185	0.08%	0.011%
75	11.273	3155	3167	3184	rBV	678704	1054695	70.90%	9.391%
76	11.415	3209	3211	3214	rBV3	1559	1009	0.07%	0.009%
77	11.463	3222	3226	3228	rBV5	1311	1108	0.07%	0.010%
78	11.646	3271	3283	3301	rBV	731497	1144316	76.92%	10.189%
79	11.897	3358	3361	3363	rBV4	1802	1236	0.08%	0.011%
80	11.920	3365	3368	3374	rVV7	1828	1547	0.10%	0.014%
81	12.154	3439	3441	3443	rBV3	978	521	0.04%	0.005%
82	12.190	3449	3452	3455	rBV5	1950	1600	0.11%	0.014%
83	12.222	3458	3462	3464	rBV4	1715	1256	0.08%	0.011%
84	12.289	3479	3483	3486	rBV6	1153	1014	0.07%	0.009%
85	12.421	3520	3524	3526	rBV4	2371	1479	0.10%	0.013%
86	12.614	3582	3584	3586	rBV3	737	256	0.02%	0.002%
87	12.858	3658	3660	3663	rVB4	1642	753	0.05%	0.007%
88	12.874	3663	3665	3667	rBV4	1291	771	0.05%	0.007%
89	13.154	3750	3752	3754	rBV3	1103	495	0.03%	0.004%
90	13.428	3835	3837	3840	rVB4	2269	1051	0.07%	0.009%
91	13.527	3863	3868	3869	rBV4	2515	1935	0.13%	0.017%
92	13.608	3891	3893	3896	rBV3	1479	1176	0.08%	0.010%
93	13.733	3930	3932	3934	rBV4	1346	894	0.06%	0.008%
94	13.775	3943	3945	3946	rBV2	1528	681	0.05%	0.006%
95	13.829	3959	3962	3965	rBV4	1892	1549	0.10%	0.014%
96	13.955	3998	4001	4006	rVB5	1959	1663	0.11%	0.015%
97	13.987	4009	4011	4013	rBV3	932	477	0.03%	0.004%
98	14.019	4019	4021	4027	rBV7	1442	1204	0.08%	0.011%
99	14.199	4076	4077	4078	rBV	1416	421	0.03%	0.004%
100	14.794	4260	4262	4265	rBV4	1362	868	0.06%	0.008%


Sum of corrected areas: 11230364

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016668.D
Acq On : 08 Jun 2020 18:36
Operator : SY/MD
Sample : L2875-16 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

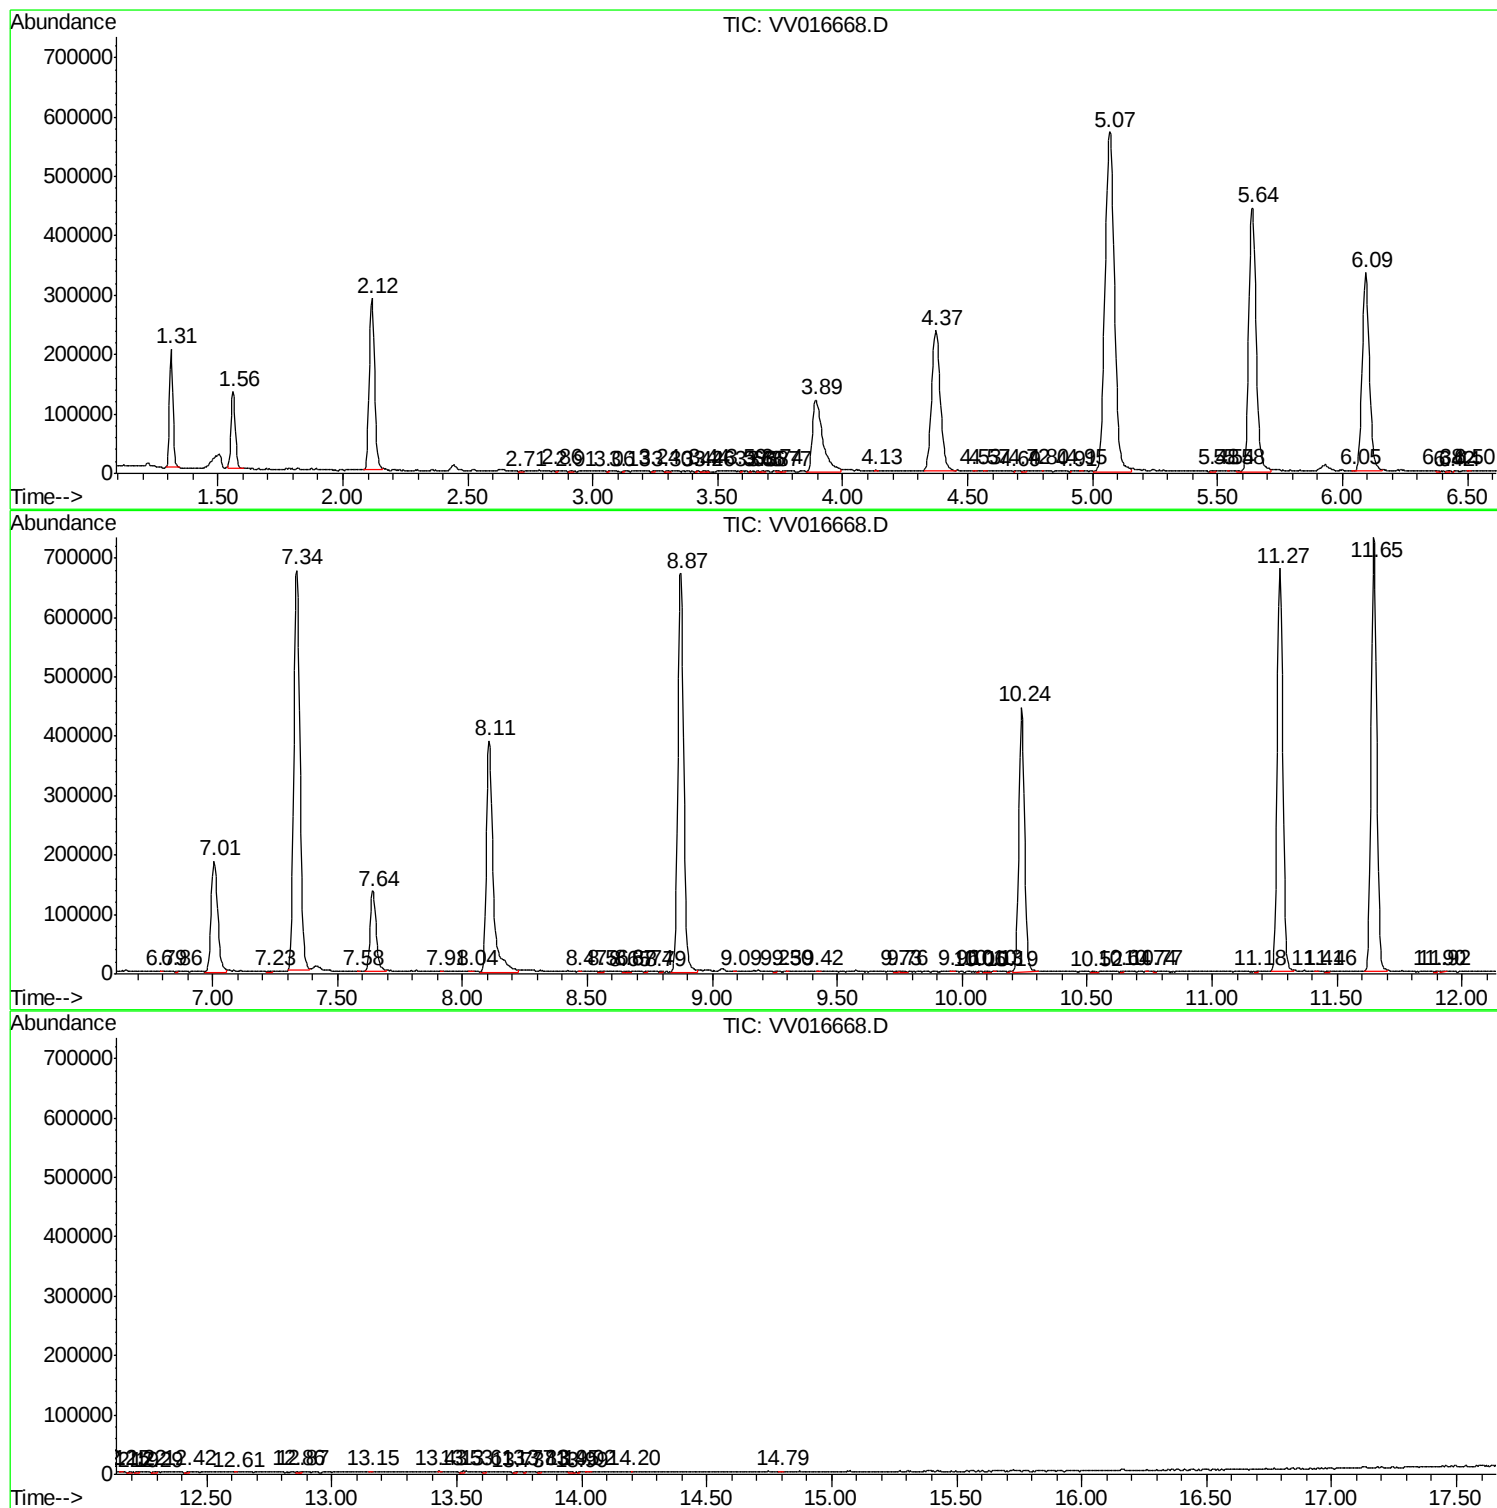

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016668.D
Acq On : 08 Jun 2020 18:36
Operator : SY/MD
Sample : L2875-16 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016668.D
Acq On : 08 Jun 2020 18:36
Operator : SY/MD
Sample : L2875-16 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTT8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc