

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016669.D
 Acq On : 08 Jun 2020 19:00
 Operator : SY/MD
 Sample : L2875-01 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	81	rVB	186512	184367	12.71%	1.688%
2	1.560	140	146	157	rVB	129027	146570	10.10%	1.342%
3	2.113	310	318	331	rVB	279379	404047	27.85%	3.700%
4	2.431	415	417	418	rBV2	1543	689	0.05%	0.006%
5	2.721	503	507	509	rBV3	1238	809	0.06%	0.007%
6	2.772	520	523	524	rBV3	1551	903	0.06%	0.008%
7	2.875	554	555	560	rBV4	1119	906	0.06%	0.008%
8	3.010	594	597	598	rBV3	1226	748	0.05%	0.007%
9	3.196	651	655	659	rBV6	1682	1602	0.11%	0.015%
10	3.364	705	707	710	rVB4	1050	557	0.04%	0.005%
11	3.380	710	712	716	rBV4	1835	1513	0.10%	0.014%
12	3.470	736	740	742	rBV3	1333	1038	0.07%	0.010%
13	3.521	752	756	759	rBV4	1102	646	0.04%	0.006%
14	3.627	785	789	791	rBV5	1232	1000	0.07%	0.009%
15	3.643	791	794	796	rVB3	1212	611	0.04%	0.006%
16	3.698	808	811	812	rBV3	1547	865	0.06%	0.008%
17	3.749	825	827	831	rBV3	1086	798	0.06%	0.007%
18	3.807	842	845	849	rBV5	954	846	0.06%	0.008%
19	3.894	861	872	900	rVV	112349	304186	20.97%	2.785%
20	4.306	997	1000	1002	rBV3	1008	700	0.05%	0.006%
21	4.373	1007	1021	1042	rVB	228954	561097	38.68%	5.138%
22	4.701	1121	1123	1125	rBV3	1273	698	0.05%	0.006%
23	4.926	1191	1193	1197	rBV4	1093	712	0.05%	0.007%
24	4.994	1211	1214	1218	rBV5	1671	1110	0.08%	0.010%
25	5.068	1220	1237	1261	rBV2	565788	1450666	100.00%	13.283%
26	5.402	1338	1341	1342	rBV3	1248	723	0.05%	0.007%
27	5.640	1398	1415	1437	rBV	439349	877372	60.48%	8.034%
28	5.929	1496	1505	1518	rBV9	9676	20313	1.40%	0.186%
29	6.026	1533	1535	1538	rBV4	1497	819	0.06%	0.007%
30	6.090	1543	1555	1578	rVV	322796	659305	45.45%	6.037%
31	6.392	1647	1649	1652	rVB4	2318	1172	0.08%	0.011%
32	6.486	1676	1678	1681	rBV4	1399	662	0.05%	0.006%
33	6.508	1681	1685	1688	rBV5	1858	1517	0.10%	0.014%
34	6.601	1709	1714	1715	rBV5	1653	1278	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016669.D
 Acq On : 08 Jun 2020 19:00
 Operator : SY/MD
 Sample : L2875-01 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.929	1813	1816	1818	rBV3	1075	622	0.04%	0.006%
36	7.007	1829	1840	1858	rBV2	182384	322949	22.26%	2.957%
37	7.174	1887	1892	1894	rBV6	2049	1586	0.11%	0.015%
38	7.338	1930	1943	1960	rBV	675476	1157509	79.79%	10.599%
39	7.640	2028	2037	2054	rBV	129515	217624	15.00%	1.993%
40	7.839	2097	2099	2100	rBV2	1111	573	0.04%	0.005%
41	8.042	2160	2162	2164	rBV3	1216	592	0.04%	0.005%
42	8.106	2172	2182	2214	rBV	382720	690776	47.62%	6.325%
43	8.473	2293	2296	2299	rBV5	1403	1179	0.08%	0.011%
44	8.524	2308	2312	2314	rVB4	1575	1118	0.08%	0.010%
45	8.589	2325	2332	2334	rBV7	978	1028	0.07%	0.009%
46	8.682	2358	2361	2364	rVB4	1461	968	0.07%	0.009%
47	8.875	2410	2421	2436	rBV	652501	1050577	72.42%	9.619%
48	9.193	2517	2520	2522	rBV4	1807	1121	0.08%	0.010%
49	9.219	2526	2528	2533	rVB5	1799	1473	0.10%	0.013%
50	9.302	2551	2554	2555	rBV3	1009	567	0.04%	0.005%
51	9.363	2568	2573	2575	rBV6	2262	1884	0.13%	0.017%
52	9.511	2615	2619	2620	rBV2	1106	714	0.05%	0.007%
53	9.752	2690	2694	2699	rBV7	1265	1177	0.08%	0.011%
54	9.775	2699	2701	2705	rBV5	1486	625	0.04%	0.006%
55	9.820	2712	2715	2718	rBV4	1694	1178	0.08%	0.011%
56	9.836	2718	2720	2724	rVB5	1633	879	0.06%	0.008%
57	9.852	2724	2725	2728	rVB3	1300	587	0.04%	0.005%
58	9.868	2728	2730	2732	rBV3	1089	735	0.05%	0.007%
59	9.939	2749	2752	2753	rBV3	2616	1311	0.09%	0.012%
60	10.003	2769	2772	2775	rBV5	1341	966	0.07%	0.009%
61	10.035	2777	2782	2783	rBV4	4481	3404	0.23%	0.031%
62	10.167	2819	2823	2825	rBV5	1374	823	0.06%	0.008%
63	10.238	2834	2845	2860	rBV	428429	661935	45.63%	6.061%
64	10.367	2882	2885	2887	rBV4	1448	881	0.06%	0.008%
65	10.383	2887	2890	2893	rVB4	1399	1076	0.07%	0.010%
66	10.569	2944	2948	2949	rBV4	1405	1225	0.08%	0.011%
67	10.698	2984	2988	2990	rBV4	1118	743	0.05%	0.007%
68	10.830	3027	3029	3032	rBV3	1715	1081	0.07%	0.010%
69	10.855	3034	3037	3038	rVV2	1421	781	0.05%	0.007%
70	10.875	3039	3043	3047	rVB5	2828	3023	0.21%	0.028%
71	10.971	3071	3073	3079	rVB7	1698	1420	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016669.D
 Acq On : 08 Jun 2020 19:00
 Operator : SY/MD
 Sample : L2875-01 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTR8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.019	3083	3088	3090	rBV5	1044	1006	0.07%	0.009%
73	11.113	3115	3117	3119	rBV4	1429	662	0.05%	0.006%
74	11.270	3155	3166	3180	rBV	660677	1008430	69.51%	9.234%
75	11.360	3193	3194	3198	rBV4	1514	998	0.07%	0.009%
76	11.486	3230	3233	3236	rBV4	1464	1008	0.07%	0.009%
77	11.518	3240	3243	3246	rVV5	1269	649	0.04%	0.006%
78	11.646	3271	3283	3302	rBV	711574	1119943	77.20%	10.255%
79	11.907	3361	3364	3366	rVB4	1703	1041	0.07%	0.010%
80	11.932	3366	3372	3373	rBV6	1115	1074	0.07%	0.010%
81	11.971	3381	3384	3385	rBV3	1132	761	0.05%	0.007%
82	12.093	3420	3422	3424	rBV3	1115	571	0.04%	0.005%
83	12.148	3435	3439	3440	rBV6	1571	792	0.05%	0.007%
84	12.283	3478	3481	3483	rBV4	1178	793	0.05%	0.007%
85	12.363	3504	3506	3511	rVB6	1819	1387	0.10%	0.013%
86	12.646	3592	3594	3599	rVB5	1466	1044	0.07%	0.010%
87	12.672	3599	3602	3603	rBV3	1261	750	0.05%	0.007%
88	12.772	3631	3633	3634	rBV	1095	570	0.04%	0.005%
89	13.151	3748	3751	3754	rBV3	1874	1278	0.09%	0.012%
90	13.183	3759	3761	3763	rBV3	1678	1045	0.07%	0.010%
91	13.299	3795	3797	3803	rVB6	1761	1488	0.10%	0.014%
92	13.328	3803	3806	3809	rBV5	1483	1104	0.08%	0.010%
93	13.363	3815	3817	3820	rBV4	1190	640	0.04%	0.006%
94	13.518	3862	3865	3866	rBV4	1255	640	0.04%	0.006%
95	14.344	4119	4122	4124	rBV3	1399	851	0.06%	0.008%
96	14.405	4138	4141	4143	rBV3	2219	1297	0.09%	0.012%
97	14.608	4202	4204	4206	rBV2	1318	795	0.05%	0.007%
98	14.717	4236	4238	4240	rBV3	1356	666	0.05%	0.006%
99	14.791	4259	4261	4265	rVB3	2245	1292	0.09%	0.012%
100	15.395	4447	4449	4452	rBV4	1990	1247	0.09%	0.011%


Sum of corrected areas: 10921377

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016669.D
Acq On : 08 Jun 2020 19:00
Operator : SY/MD
Sample : L2875-01 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

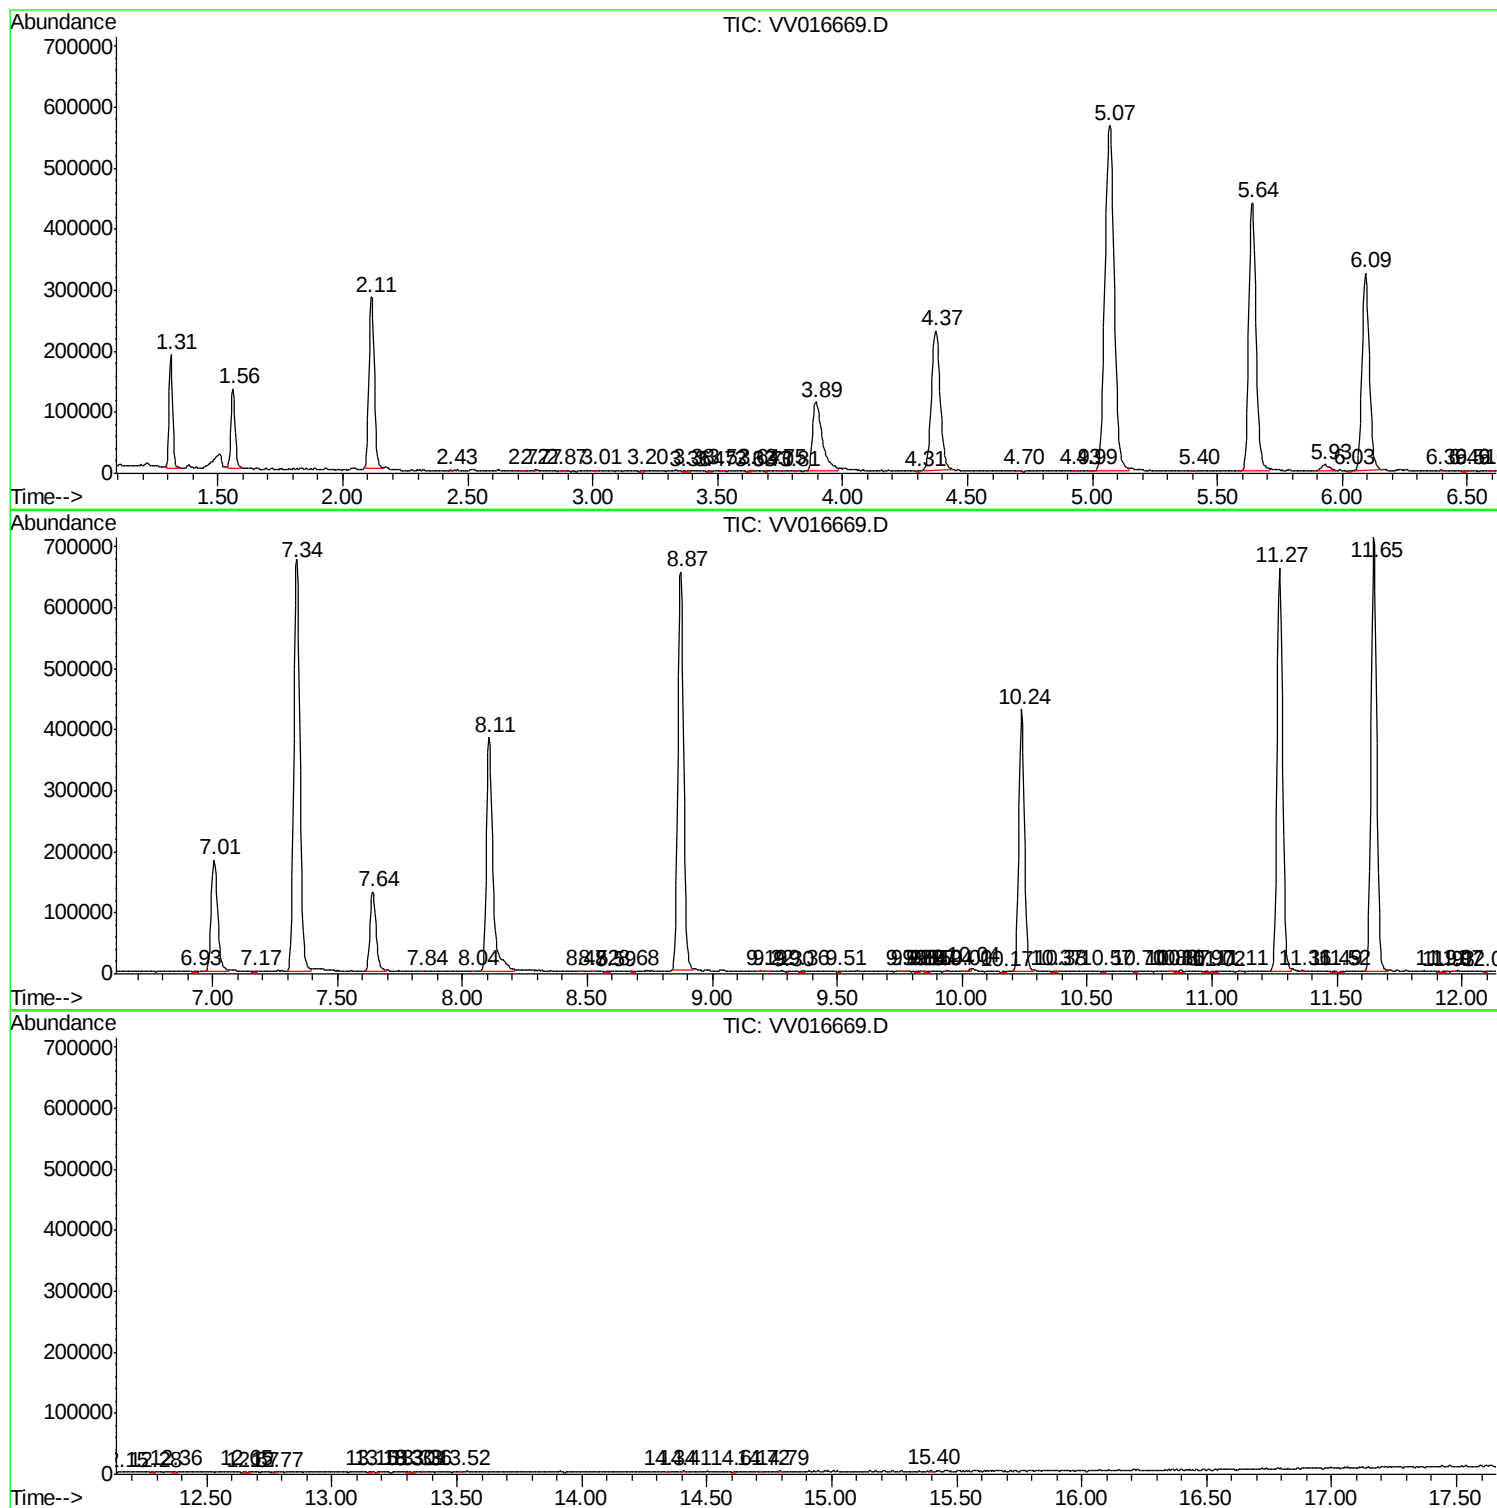

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016669.D
Acq On : 08 Jun 2020 19:00
Operator : SY/MD
Sample : L2875-01 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016669.D
Acq On : 08 Jun 2020 19:00
Operator : SY/MD
Sample : L2875-01 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTR8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc