

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016670.D
 Acq On : 08 Jun 2020 19:24
 Operator : SY/MD
 Sample : L2875-12 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	63	71	83	rVB2	574675	600898	39.40%	5.064%
2	1.563	140	147	158	rVB	132452	156266	10.25%	1.317%
3	2.116	309	319	338	rVB	298613	439567	28.82%	3.705%
4	2.425	412	415	416	rBV2	1234	661	0.04%	0.006%
5	2.621	473	476	478	rBV3	2599	1874	0.12%	0.016%
6	2.740	509	513	514	rBV4	1251	721	0.05%	0.006%
7	2.840	542	544	547	rBV4	1308	835	0.05%	0.007%
8	2.917	565	568	573	rBV7	1461	1093	0.07%	0.009%
9	3.029	601	603	606	rVB4	1511	668	0.04%	0.006%
10	3.052	606	610	611	rBV3	1208	677	0.04%	0.006%
11	3.074	615	617	621	rVB5	1550	720	0.05%	0.006%
12	3.126	631	633	634	rBV2	1455	616	0.04%	0.005%
13	3.280	679	681	685	rBV5	1343	964	0.06%	0.008%
14	3.380	708	712	713	rBV4	1102	766	0.05%	0.006%
15	3.534	757	760	762	rBV4	1557	1136	0.07%	0.010%
16	3.618	783	786	787	rBV3	1426	650	0.04%	0.005%
17	3.823	848	850	854	rVB4	1818	985	0.06%	0.008%
18	3.852	856	859	862	rBV4	1915	1238	0.08%	0.010%
19	3.897	862	873	881	rBV	125727	303975	19.93%	2.562%
20	4.373	1007	1021	1044	rVB	244558	597576	39.18%	5.036%
21	4.598	1089	1091	1094	rBV4	1309	598	0.04%	0.005%
22	4.753	1136	1139	1142	rBV4	1293	1022	0.07%	0.009%
23	4.997	1210	1215	1218	rBV7	1677	1760	0.12%	0.015%
24	5.071	1220	1238	1264	rVV2	592018	1525261	100.00%	12.855%
25	5.389	1334	1337	1340	rBV5	1901	1392	0.09%	0.012%
26	5.531	1377	1381	1383	rBV4	1901	1438	0.09%	0.012%
27	5.640	1402	1415	1434	rBV	445209	884814	58.01%	7.457%
28	5.933	1491	1506	1520	rBV6	12988	31307	2.05%	0.264%
29	6.093	1539	1556	1575	rBV	345883	699138	45.84%	5.892%
30	6.325	1621	1628	1630	rBV7	1821	1831	0.12%	0.015%
31	6.370	1639	1642	1644	rBV4	1656	948	0.06%	0.008%
32	6.421	1656	1658	1664	rVB7	2303	1324	0.09%	0.011%
33	6.466	1668	1672	1674	rBV5	1916	1436	0.09%	0.012%
34	6.531	1690	1692	1694	rBV3	1976	958	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016670.D
 Acq On : 08 Jun 2020 19:24
 Operator : SY/MD
 Sample : L2875-12 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.608	1714	1716	1721	rBV6	1368	1034	0.07%	0.009%
36	6.904	1805	1808	1812	rBV3	2218	2052	0.13%	0.017%
37	7.007	1829	1840	1860	rBV	195077	345017	22.62%	2.908%
38	7.338	1931	1943	1963	rBV	705294	1211347	79.42%	10.209%
39	7.640	2028	2037	2055	rBV	136250	230342	15.10%	1.941%
40	7.952	2128	2134	2135	rBV5	1977	1933	0.13%	0.016%
41	8.058	2164	2167	2169	rBV4	1435	942	0.06%	0.008%
42	8.106	2171	2182	2213	rBV	402223	738344	48.41%	6.223%
43	8.627	2341	2344	2346	rBV3	1661	1038	0.07%	0.009%
44	8.704	2365	2368	2370	rVB4	2042	1154	0.08%	0.010%
45	8.814	2400	2402	2406	rVB5	1542	918	0.06%	0.008%
46	8.875	2408	2421	2436	rBV	675440	1089288	71.42%	9.181%
47	9.080	2480	2485	2488	rBV6	2125	2084	0.14%	0.018%
48	9.125	2496	2499	2501	rBV3	1775	1177	0.08%	0.010%
49	9.164	2506	2511	2513	rBV5	2349	1772	0.12%	0.015%
50	9.312	2555	2557	2559	rBV2	1321	802	0.05%	0.007%
51	9.412	2584	2588	2592	rVB6	1765	1534	0.10%	0.013%
52	9.431	2592	2594	2597	rBV4	1621	1151	0.08%	0.010%
53	9.566	2634	2636	2637	rBV2	1488	777	0.05%	0.007%
54	9.695	2674	2676	2679	rBV4	1019	754	0.05%	0.006%
55	9.743	2687	2691	2694	rBV3	1525	1458	0.10%	0.012%
56	9.868	2726	2730	2731	rBV5	1183	873	0.06%	0.007%
57	10.061	2786	2790	2792	rBV5	1623	1086	0.07%	0.009%
58	10.142	2811	2815	2817	rVB4	1199	815	0.05%	0.007%
59	10.187	2826	2829	2830	rBV3	1380	590	0.04%	0.005%
60	10.238	2833	2845	2859	rVV	459858	708969	46.48%	5.975%
61	10.328	2871	2873	2875	rBV2	1160	598	0.04%	0.005%
62	10.405	2894	2897	2898	rBV3	1019	646	0.04%	0.005%
63	10.505	2924	2928	2930	rBV5	2184	1369	0.09%	0.012%
64	10.550	2940	2942	2943	rBV2	1305	607	0.04%	0.005%
65	10.572	2947	2949	2952	rBV4	1007	626	0.04%	0.005%
66	10.695	2983	2987	2989	rVB4	1171	803	0.05%	0.007%
67	10.810	3020	3023	3026	rBV4	1603	1561	0.10%	0.013%
68	10.859	3036	3038	3040	rBV3	1280	738	0.05%	0.006%
69	10.939	3061	3063	3066	rVB4	2168	1134	0.07%	0.010%
70	11.103	3111	3114	3115	rBV3	1229	690	0.05%	0.006%
71	11.270	3156	3166	3184	rVB	680554	1043716	68.43%	8.797%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016670.D
 Acq On : 08 Jun 2020 19:24
 Operator : SY/MD
 Sample : L2875-12 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.550	3251	3253	3257	rVB4	1464	891	0.06%	0.008%
73	11.646	3271	3283	3301	rBV	755276	1169723	76.69%	9.859%
74	11.813	3333	3335	3337	rBV3	1334	773	0.05%	0.007%
75	11.826	3337	3339	3344	rVB5	2173	1276	0.08%	0.011%
76	11.868	3349	3352	3354	rBV3	1247	836	0.05%	0.007%
77	11.900	3360	3362	3366	rBV2	1255	750	0.05%	0.006%
78	12.013	3392	3397	3399	rBV5	1424	1300	0.09%	0.011%
79	12.042	3403	3406	3407	rBV3	1345	721	0.05%	0.006%
80	12.212	3455	3459	3463	rBV5	2142	1784	0.12%	0.015%
81	12.360	3503	3505	3507	rBV3	1036	634	0.04%	0.005%
82	12.373	3507	3509	3510	rBV2	1409	734	0.05%	0.006%
83	12.431	3524	3527	3532	rBV6	1538	1561	0.10%	0.013%
84	12.547	3560	3563	3565	rVV4	1474	888	0.06%	0.007%
85	12.575	3570	3572	3577	rVV4	1420	936	0.06%	0.008%
86	12.659	3592	3598	3601	rBV7	2053	2370	0.16%	0.020%
87	12.768	3628	3632	3633	rBV5	1142	758	0.05%	0.006%
88	12.884	3659	3668	3670	rBV8	2042	2693	0.18%	0.023%
89	13.022	3709	3711	3713	rVB3	1475	692	0.05%	0.006%
90	13.064	3722	3724	3727	rBV3	1253	776	0.05%	0.007%
91	13.286	3790	3793	3795	rBV3	1483	940	0.06%	0.008%
92	13.376	3819	3821	3824	rBV3	1423	1161	0.08%	0.010%
93	13.646	3903	3905	3908	rBV3	1359	880	0.06%	0.007%
94	13.846	3963	3967	3969	rBV5	1493	1105	0.07%	0.009%
95	13.903	3982	3985	3988	rBV4	1553	1230	0.08%	0.010%
96	14.016	4018	4020	4022	rBV2	2601	1212	0.08%	0.010%
97	14.463	4157	4159	4161	rBV3	1022	588	0.04%	0.005%
98	14.543	4182	4184	4189	rBV4	1354	862	0.06%	0.007%
99	15.029	4333	4335	4337	rBV3	1493	594	0.04%	0.005%
100	15.450	4463	4466	4468	rBV4	1730	1387	0.09%	0.012%


Sum of corrected areas: 11864907

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016670.D
Acq On : 08 Jun 2020 19:24
Operator : SY/MD
Sample : L2875-12 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

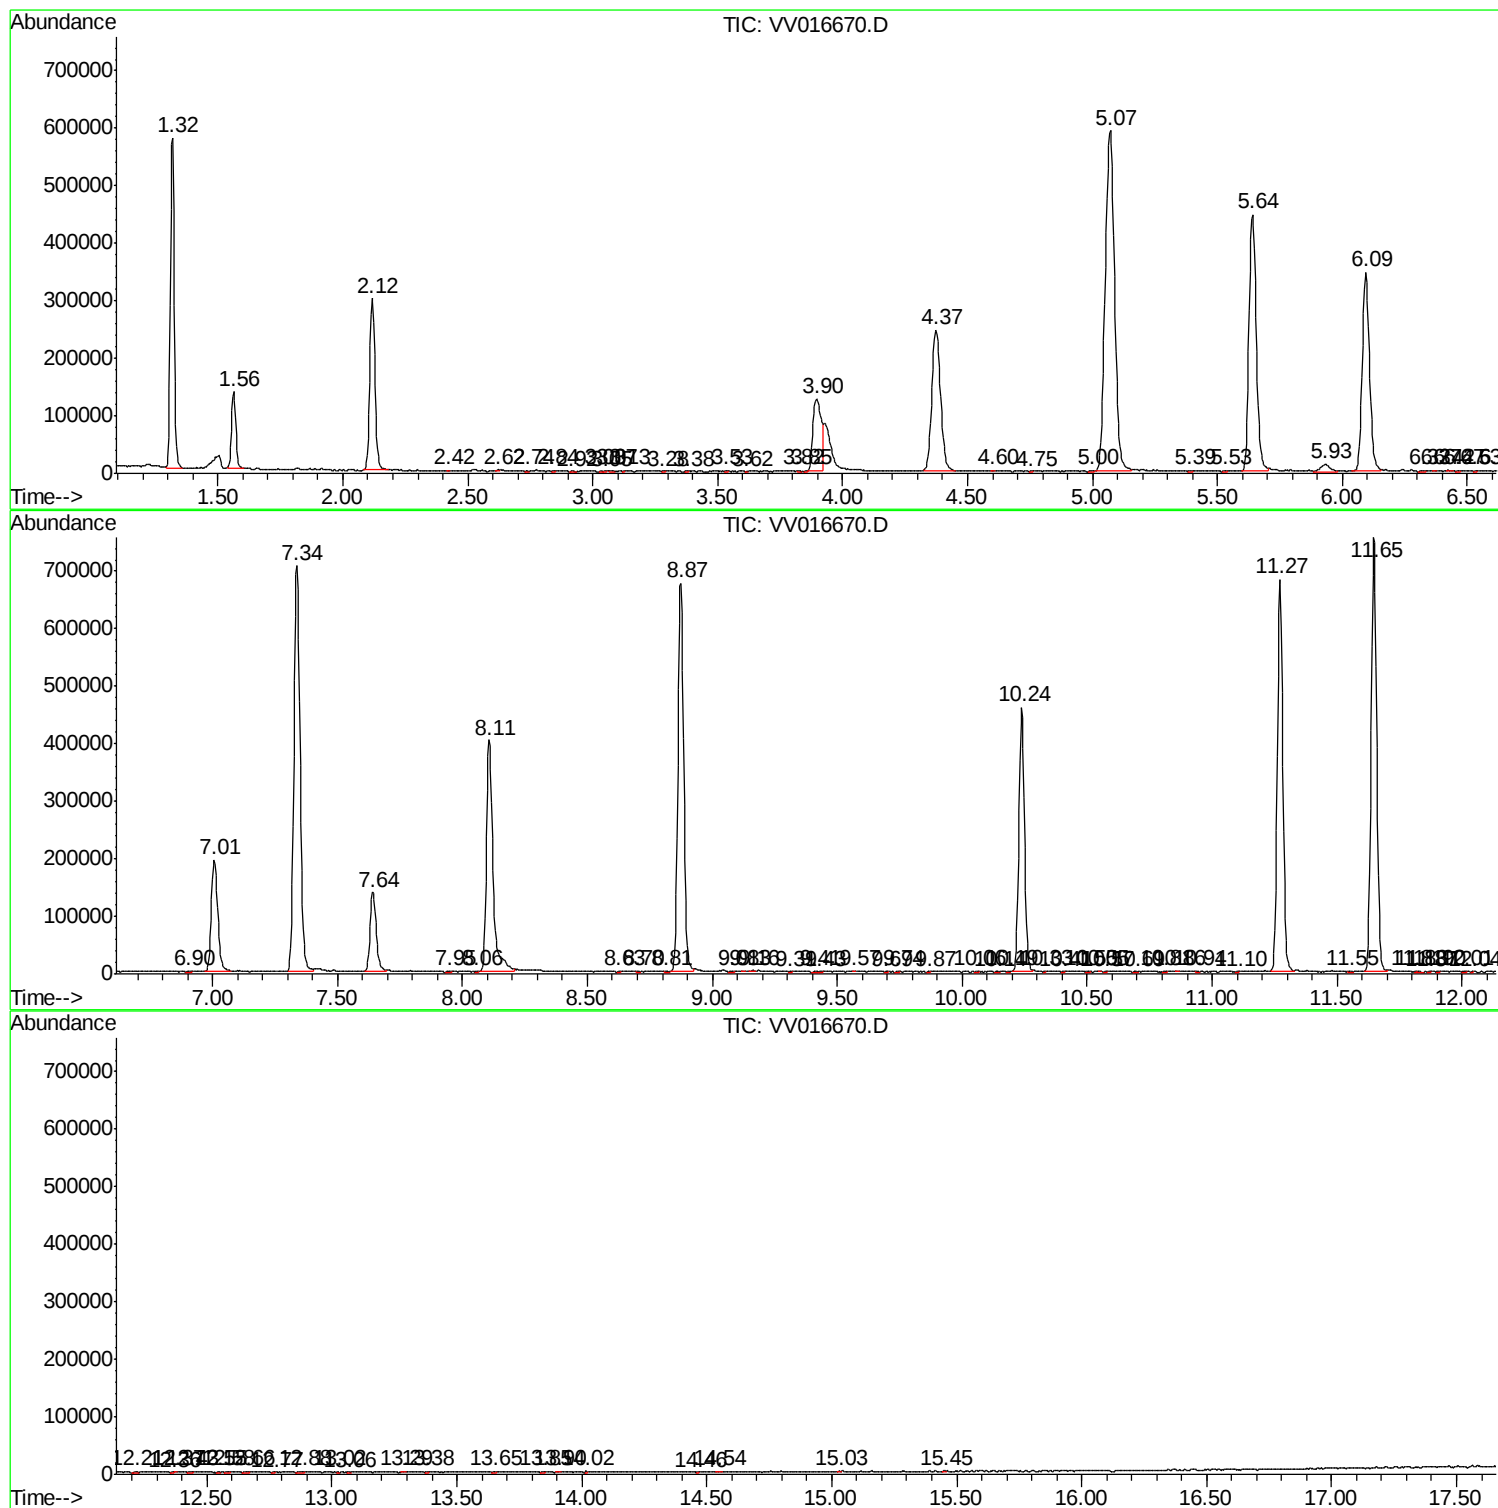

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016670.D
Acq On : 08 Jun 2020 19:24
Operator : SY/MD
Sample : L2875-12 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016670.D
Acq On : 08 Jun 2020 19:24
Operator : SY/MD
Sample : L2875-12 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc