

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016672.D
 Acq On : 08 Jun 2020 20:35
 Operator : SY/MD
 Sample : VV0608WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	81	rVB	209257	215447	13.36%	1.833%
2	1.563	140	147	160	rVB	138619	166935	10.35%	1.420%
3	2.116	310	319	333	rBV	311198	458664	28.43%	3.902%
4	2.769	518	522	523	rBV4	2990	1828	0.11%	0.016%
5	2.897	561	562	565	rBV3	1227	827	0.05%	0.007%
6	2.981	583	588	593	rBV8	1367	1513	0.09%	0.013%
7	3.042	605	607	608	rBV2	1367	675	0.04%	0.006%
8	3.097	621	624	626	rVB3	1560	827	0.05%	0.007%
9	3.145	634	639	641	rBV4	1188	1259	0.08%	0.011%
10	3.261	673	675	678	rVB4	2074	1216	0.08%	0.010%
11	3.283	678	682	684	rBV4	1941	1539	0.10%	0.013%
12	3.322	691	694	695	rBV3	1789	912	0.06%	0.008%
13	3.331	695	697	701	rVV4	1901	1081	0.07%	0.009%
14	3.351	701	703	706	rVB4	1512	973	0.06%	0.008%
15	3.373	706	710	714	rBV6	1588	1488	0.09%	0.013%
16	3.463	732	738	740	rBV6	1286	1642	0.10%	0.014%
17	3.572	770	772	775	rBV3	970	648	0.04%	0.006%
18	3.704	811	813	815	rBV3	1512	749	0.05%	0.006%
19	3.781	833	837	840	rBV6	1711	1747	0.11%	0.015%
20	3.820	847	849	853	rBV6	1555	937	0.06%	0.008%
21	3.894	860	872	907	rBV	126503	353721	21.93%	3.009%
22	4.373	1005	1021	1043	rBV	252447	624414	38.71%	5.312%
23	4.810	1151	1157	1159	rBV6	1592	1707	0.11%	0.015%
24	4.830	1161	1163	1168	rVB5	1615	1148	0.07%	0.010%
25	4.974	1206	1208	1212	rVB5	1998	1148	0.07%	0.010%
26	5.068	1219	1237	1267	rBV2	623674	1613142	100.00%	13.722%
27	5.415	1339	1345	1346	rBV6	2123	2026	0.13%	0.017%
28	5.511	1373	1375	1377	rVB3	1743	782	0.05%	0.007%
29	5.640	1402	1415	1440	rBV	431768	861406	53.40%	7.328%
30	5.929	1496	1505	1516	rBV7	14327	28234	1.75%	0.240%
31	6.093	1543	1556	1576	rBV	359778	720035	44.64%	6.125%
32	6.537	1686	1694	1696	rBV8	2186	2494	0.15%	0.021%
33	6.884	1800	1802	1807	rVB6	1288	762	0.05%	0.006%
34	7.006	1828	1840	1860	rBV	200735	364635	22.60%	3.102%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016672.D
 Acq On : 08 Jun 2020 20:35
 Operator : SY/MD
 Sample : VV0608WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.170	1888	1891	1893	rBV3	1728	1029	0.06%	0.009%
36	7.338	1931	1943	1959	rBV	726206	1258204	78.00%	10.703%
37	7.640	2026	2037	2053	rBV	142791	247464	15.34%	2.105%
38	7.765	2074	2076	2081	rVB5	1703	1302	0.08%	0.011%
39	7.794	2081	2085	2086	rBV3	1647	1333	0.08%	0.011%
40	7.920	2122	2124	2129	rBV5	858	685	0.04%	0.006%
41	7.997	2146	2148	2151	rBV3	2048	1448	0.09%	0.012%
42	8.106	2172	2182	2218	rBV	411961	771095	47.80%	6.559%
43	8.733	2374	2377	2379	rBV4	1504	1157	0.07%	0.010%
44	8.875	2407	2421	2443	rBV	639293	1049377	65.05%	8.927%
45	9.006	2460	2462	2466	rBV5	1219	730	0.05%	0.006%
46	9.093	2487	2489	2494	rVB6	2346	1856	0.12%	0.016%
47	9.129	2498	2500	2503	rBV3	1163	686	0.04%	0.006%
48	9.440	2594	2597	2600	rBV5	2420	1697	0.11%	0.014%
49	9.633	2653	2657	2659	rBV4	1243	730	0.05%	0.006%
50	9.662	2663	2666	2667	rBV3	1437	776	0.05%	0.007%
51	9.765	2694	2698	2702	rBV6	2294	2125	0.13%	0.018%
52	9.958	2753	2758	2759	rBV4	2689	2214	0.14%	0.019%
53	10.029	2777	2780	2783	rBV4	2047	1206	0.07%	0.010%
54	10.048	2783	2786	2790	rVB5	1604	1170	0.07%	0.010%
55	10.122	2803	2809	2810	rBV5	1084	942	0.06%	0.008%
56	10.180	2824	2827	2831	rBV4	1576	1131	0.07%	0.010%
57	10.238	2834	2845	2858	rBV	471030	724833	44.93%	6.166%
58	10.341	2874	2877	2879	rBV2	1422	1160	0.07%	0.010%
59	10.501	2924	2927	2932	rBV6	1220	809	0.05%	0.007%
60	10.649	2969	2973	2975	rBV4	1391	1065	0.07%	0.009%
61	10.707	2987	2991	2993	rBV4	1334	745	0.05%	0.006%
62	10.775	3011	3012	3020	rVB8	1945	1755	0.11%	0.015%
63	10.842	3030	3033	3035	rVB3	1086	664	0.04%	0.006%
64	10.932	3058	3061	3062	rBV3	2947	1524	0.09%	0.013%
65	11.061	3099	3101	3105	rBV4	892	846	0.05%	0.007%
66	11.270	3155	3166	3183	rBV	646854	983501	60.97%	8.366%
67	11.427	3213	3215	3219	rBV4	1171	1113	0.07%	0.009%
68	11.463	3223	3226	3228	rBV3	1808	980	0.06%	0.008%
69	11.595	3263	3267	3270	rVB4	1429	1051	0.07%	0.009%
70	11.646	3270	3283	3303	rBV	761312	1196566	74.18%	10.179%
71	12.112	3426	3428	3438	rBV9	1010	1358	0.08%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016672.D
 Acq On : 08 Jun 2020 20:35
 Operator : SY/MD
 Sample : VV0608WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.167	3442	3445	3448	rBV5	1113	979	0.06%	0.008%
73	12.289	3480	3483	3485	rBV3	1326	650	0.04%	0.006%
74	12.315	3488	3491	3493	rVV3	1809	1057	0.07%	0.009%
75	12.328	3493	3495	3499	rVB4	1460	1076	0.07%	0.009%
76	12.379	3507	3511	3514	rBV4	1841	1453	0.09%	0.012%
77	12.395	3514	3516	3520	rVB4	1270	946	0.06%	0.008%
78	12.559	3564	3567	3571	rBV5	1349	1253	0.08%	0.011%
79	12.678	3592	3604	3612	rBV5	5601	11170	0.69%	0.095%
80	12.723	3616	3618	3622	rVV4	1406	1039	0.06%	0.009%
81	12.910	3670	3676	3679	rBV6	1958	2079	0.13%	0.018%
82	12.955	3688	3690	3695	rVB4	1466	801	0.05%	0.007%
83	13.077	3725	3728	3731	rVB4	2359	1244	0.08%	0.011%
84	13.103	3731	3736	3738	rBV5	1699	1652	0.10%	0.014%
85	13.206	3765	3768	3769	rBV3	1626	832	0.05%	0.007%
86	13.440	3838	3841	3844	rBV3	1525	849	0.05%	0.007%
87	13.456	3844	3846	3848	rBV3	1440	641	0.04%	0.005%
88	13.498	3855	3859	3862	rBV4	1526	1251	0.08%	0.011%
89	13.527	3864	3868	3870	rBV4	3308	3063	0.19%	0.026%
90	13.839	3962	3965	3969	rBV4	2065	1432	0.09%	0.012%
91	13.861	3969	3972	3975	rBV6	1782	1804	0.11%	0.015%
92	13.990	4009	4012	4016	rBV5	1254	953	0.06%	0.008%
93	14.106	4044	4048	4050	rBV4	1836	1386	0.09%	0.012%
94	14.157	4060	4064	4067	rBV6	1429	1409	0.09%	0.012%
95	14.196	4074	4076	4081	rBV4	900	710	0.04%	0.006%
96	14.318	4112	4114	4116	rBV3	1486	703	0.04%	0.006%
97	14.366	4126	4129	4131	rBV4	1885	1075	0.07%	0.009%
98	14.633	4209	4212	4214	rBV4	1750	1207	0.07%	0.010%
99	15.160	4374	4376	4380	rVB4	2386	1121	0.07%	0.010%
100	16.922	4921	4924	4929	rBV	13335	8897	0.55%	0.076%


Sum of corrected areas: 11755620

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016672.D
Acq On : 08 Jun 2020 20:35
Operator : SY/MD
Sample : VV0608WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

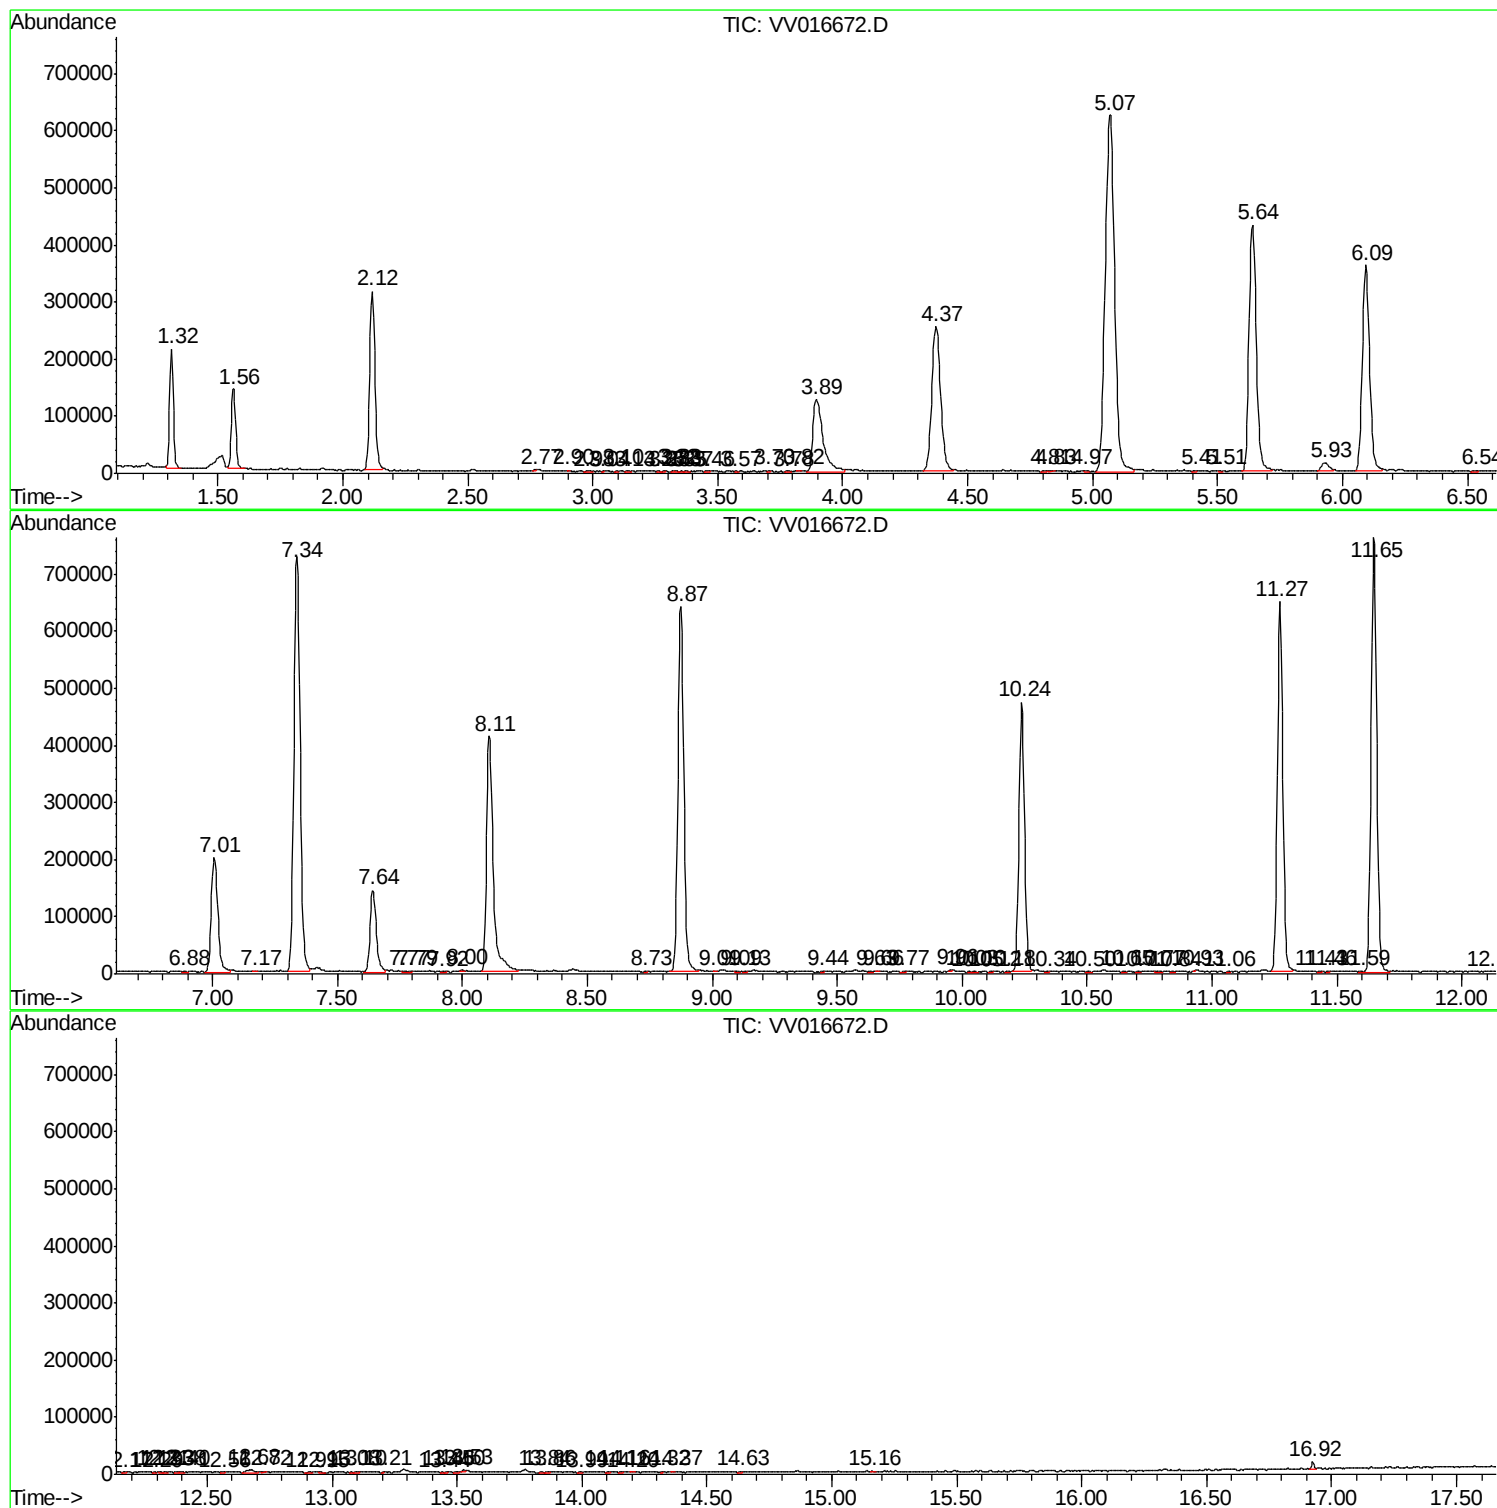

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016672.D
Acq On : 08 Jun 2020 20:35
Operator : SY/MD
Sample : VV0608WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060820\
Data File : VV016672.D
Acq On : 08 Jun 2020 20:35
Operator : SY/MD
Sample : VV0608WBL02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc