

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016673.D
 Acq On : 08 Jun 2020 20:59
 Operator : SY/MD
 Sample : L2861-19DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E67DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	81	rVB	184384	187656	13.64%	1.676%
2	1.560	140	146	156	rVB	126437	151226	10.99%	1.351%
3	2.116	309	319	334	rBV	281664	421686	30.65%	3.767%
4	2.396	404	406	412	rVB6	1181	1026	0.07%	0.009%
5	2.457	421	425	426	rBV4	2005	1575	0.11%	0.014%
6	2.711	499	504	505	rBV4	1344	810	0.06%	0.007%
7	2.830	538	541	546	rVB6	2296	1622	0.12%	0.014%
8	2.855	546	549	550	rBV2	1232	798	0.06%	0.007%
9	3.109	626	628	632	rVB4	903	537	0.04%	0.005%
10	3.132	632	635	640	rVB7	1385	1279	0.09%	0.011%
11	3.154	640	642	645	rBV3	1169	830	0.06%	0.007%
12	3.199	654	656	659	rBV3	1015	473	0.03%	0.004%
13	3.212	659	660	663	rBV2	917	565	0.04%	0.005%
14	3.244	664	670	672	rBV6	1309	1194	0.09%	0.011%
15	3.280	679	681	684	rVB3	1699	856	0.06%	0.008%
16	3.315	690	692	695	rVB3	1804	858	0.06%	0.008%
17	3.347	700	702	704	rVB3	1567	568	0.04%	0.005%
18	3.383	709	713	717	rBV7	1709	1487	0.11%	0.013%
19	3.441	728	731	733	rBV3	1832	1133	0.08%	0.010%
20	3.579	770	774	776	rBV4	1039	773	0.06%	0.007%
21	3.592	776	778	781	rVV3	737	499	0.04%	0.004%
22	3.640	791	793	799	rVB6	1251	1062	0.08%	0.009%
23	3.669	799	802	803	rBV2	1543	737	0.05%	0.007%
24	3.701	806	812	814	rBV6	1038	822	0.06%	0.007%
25	3.711	814	815	819	rVB3	1150	648	0.05%	0.006%
26	3.736	819	823	824	rBV3	1564	737	0.05%	0.007%
27	3.769	828	833	834	rBV4	1925	1216	0.09%	0.011%
28	3.894	862	872	903	rBV	118363	329875	23.98%	2.946%
29	4.142	947	949	954	rBV5	1097	573	0.04%	0.005%
30	4.283	989	993	995	rBV5	1319	818	0.06%	0.007%
31	4.373	1007	1021	1042	rVB	238313	571674	41.55%	5.106%
32	4.585	1082	1087	1091	rBV7	1214	1224	0.09%	0.011%
33	4.601	1091	1092	1096	rVB2	1175	694	0.05%	0.006%
34	4.624	1096	1099	1103	rBV5	1869	1529	0.11%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016673.D
 Acq On : 08 Jun 2020 20:59
 Operator : SY/MD
 Sample : L2861-19DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E67DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	4.820	1156	1160	1162	rBV5	1251	751	0.05%	0.007%
36	4.849	1168	1169	1172	rBV3	1114	519	0.04%	0.005%
37	4.929	1191	1194	1196	rVB4	1850	801	0.06%	0.007%
38	4.958	1201	1203	1205	rBV3	1346	540	0.04%	0.005%
39	5.071	1220	1238	1244	rBV2	581736	1375789	100.00%	12.289%
40	5.469	1359	1362	1365	rBV5	1740	846	0.06%	0.008%
41	5.511	1374	1375	1381	rBV5	1232	886	0.06%	0.008%
42	5.640	1402	1415	1436	rBV	373803	736578	53.54%	6.579%
43	5.865	1483	1485	1487	rVB4	1588	653	0.05%	0.006%
44	5.887	1487	1492	1495	rBV6	2300	1860	0.14%	0.017%
45	6.093	1539	1556	1583	rBV	330944	686568	49.90%	6.132%
46	6.383	1644	1646	1647	rBV2	1814	737	0.05%	0.007%
47	6.486	1675	1678	1680	rVB4	938	574	0.04%	0.005%
48	6.502	1680	1683	1684	rBV3	1070	553	0.04%	0.005%
49	6.585	1706	1709	1710	rBV3	1532	859	0.06%	0.008%
50	6.614	1716	1718	1722	rBV5	1185	698	0.05%	0.006%
51	6.791	1770	1773	1774	rBV3	1131	676	0.05%	0.006%
52	6.823	1781	1783	1784	rBV2	1388	554	0.04%	0.005%
53	6.868	1794	1797	1801	rBV6	1028	748	0.05%	0.007%
54	6.923	1805	1814	1815	rBV7	5218	5103	0.37%	0.046%
55	7.006	1829	1840	1860	rBV	188788	337024	24.50%	3.010%
56	7.338	1931	1943	1956	rBV	682161	1161774	84.44%	10.377%
57	7.412	1957	1966	1984	rVB	167289	298489	21.70%	2.666%
58	7.643	2027	2038	2054	rBV	137306	226362	16.45%	2.022%
59	7.865	2105	2107	2108	rBV2	1416	581	0.04%	0.005%
60	7.900	2114	2118	2123	rBV7	1577	1425	0.10%	0.013%
61	8.106	2172	2182	2215	rBV	405077	736816	53.56%	6.581%
62	8.321	2247	2249	2251	rBV4	1474	812	0.06%	0.007%
63	8.559	2317	2323	2327	rBV9	1577	2075	0.15%	0.019%
64	8.604	2333	2337	2340	rBV6	1746	1364	0.10%	0.012%
65	8.640	2346	2348	2351	rVB4	1609	771	0.06%	0.007%
66	8.662	2351	2355	2356	rBV3	1647	1181	0.09%	0.011%
67	8.685	2361	2362	2365	rBV3	1061	515	0.04%	0.005%
68	8.874	2411	2421	2432	rBV	550729	873097	63.46%	7.799%
69	9.035	2461	2471	2486	rBV	99462	170873	12.42%	1.526%
70	9.283	2539	2548	2556	rBV	9689	19917	1.45%	0.178%
71	9.405	2579	2586	2596	rVB4	24655	38407	2.79%	0.343%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016673.D
 Acq On : 08 Jun 2020 20:59
 Operator : SY/MD
 Sample : L2861-19DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E67DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	9.566	2628	2636	2646	rBV2	47215	73462	5.34%	0.656%
73	10.238	2835	2845	2859	rBV	445136	693869	50.43%	6.198%
74	11.270	3156	3166	3184	rVB	580709	882308	64.13%	7.881%
75	11.646	3273	3283	3300	rVB	737088	1144228	83.17%	10.220%
76	12.080	3416	3418	3420	rBV4	1162	637	0.05%	0.006%
77	12.881	3665	3667	3669	rBV3	1489	779	0.06%	0.007%
78	12.971	3693	3695	3697	rBV3	1281	842	0.06%	0.008%
79	13.119	3740	3741	3744	rBV3	1392	612	0.04%	0.005%
80	13.212	3768	3770	3774	rVB5	1288	813	0.06%	0.007%
81	13.234	3774	3777	3779	rBV3	2579	1696	0.12%	0.015%
82	13.466	3846	3849	3850	rBV3	2439	1225	0.09%	0.011%
83	13.948	3997	3999	4002	rVB3	1324	679	0.05%	0.006%
84	13.964	4002	4004	4005	rBV2	1189	587	0.04%	0.005%
85	14.000	4012	4015	4017	rBV4	1200	691	0.05%	0.006%
86	14.119	4049	4052	4054	rBV4	1645	794	0.06%	0.007%
87	14.154	4060	4063	4065	rVB4	1738	968	0.07%	0.009%
88	14.247	4088	4092	4098	rVB9	1948	1655	0.12%	0.015%
89	14.279	4100	4102	4104	rBV3	1551	821	0.06%	0.007%
90	14.292	4104	4106	4108	rBV2	1171	482	0.04%	0.004%
91	14.405	4139	4141	4143	rBV3	1676	1043	0.08%	0.009%
92	14.736	4242	4244	4247	rBV3	903	504	0.04%	0.005%
93	14.807	4262	4266	4270	rVB8	1704	1539	0.11%	0.014%
94	14.842	4270	4277	4279	rBV7	1917	1965	0.14%	0.018%
95	14.935	4303	4306	4307	rBV2	1578	761	0.06%	0.007%
96	15.025	4332	4334	4336	rVB3	1484	526	0.04%	0.005%
97	15.038	4336	4338	4342	rVB4	1634	745	0.05%	0.007%
98	15.061	4342	4345	4346	rBV3	1339	802	0.06%	0.007%
99	15.357	4432	4437	4439	rBV6	2765	2262	0.16%	0.020%
100	15.382	4442	4445	4447	rBV4	1909	1470	0.11%	0.013%


Sum of corrected areas: 11195601

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016673.D
Acq On : 08 Jun 2020 20:59
Operator : SY/MD
Sample : L2861-19DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E67DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

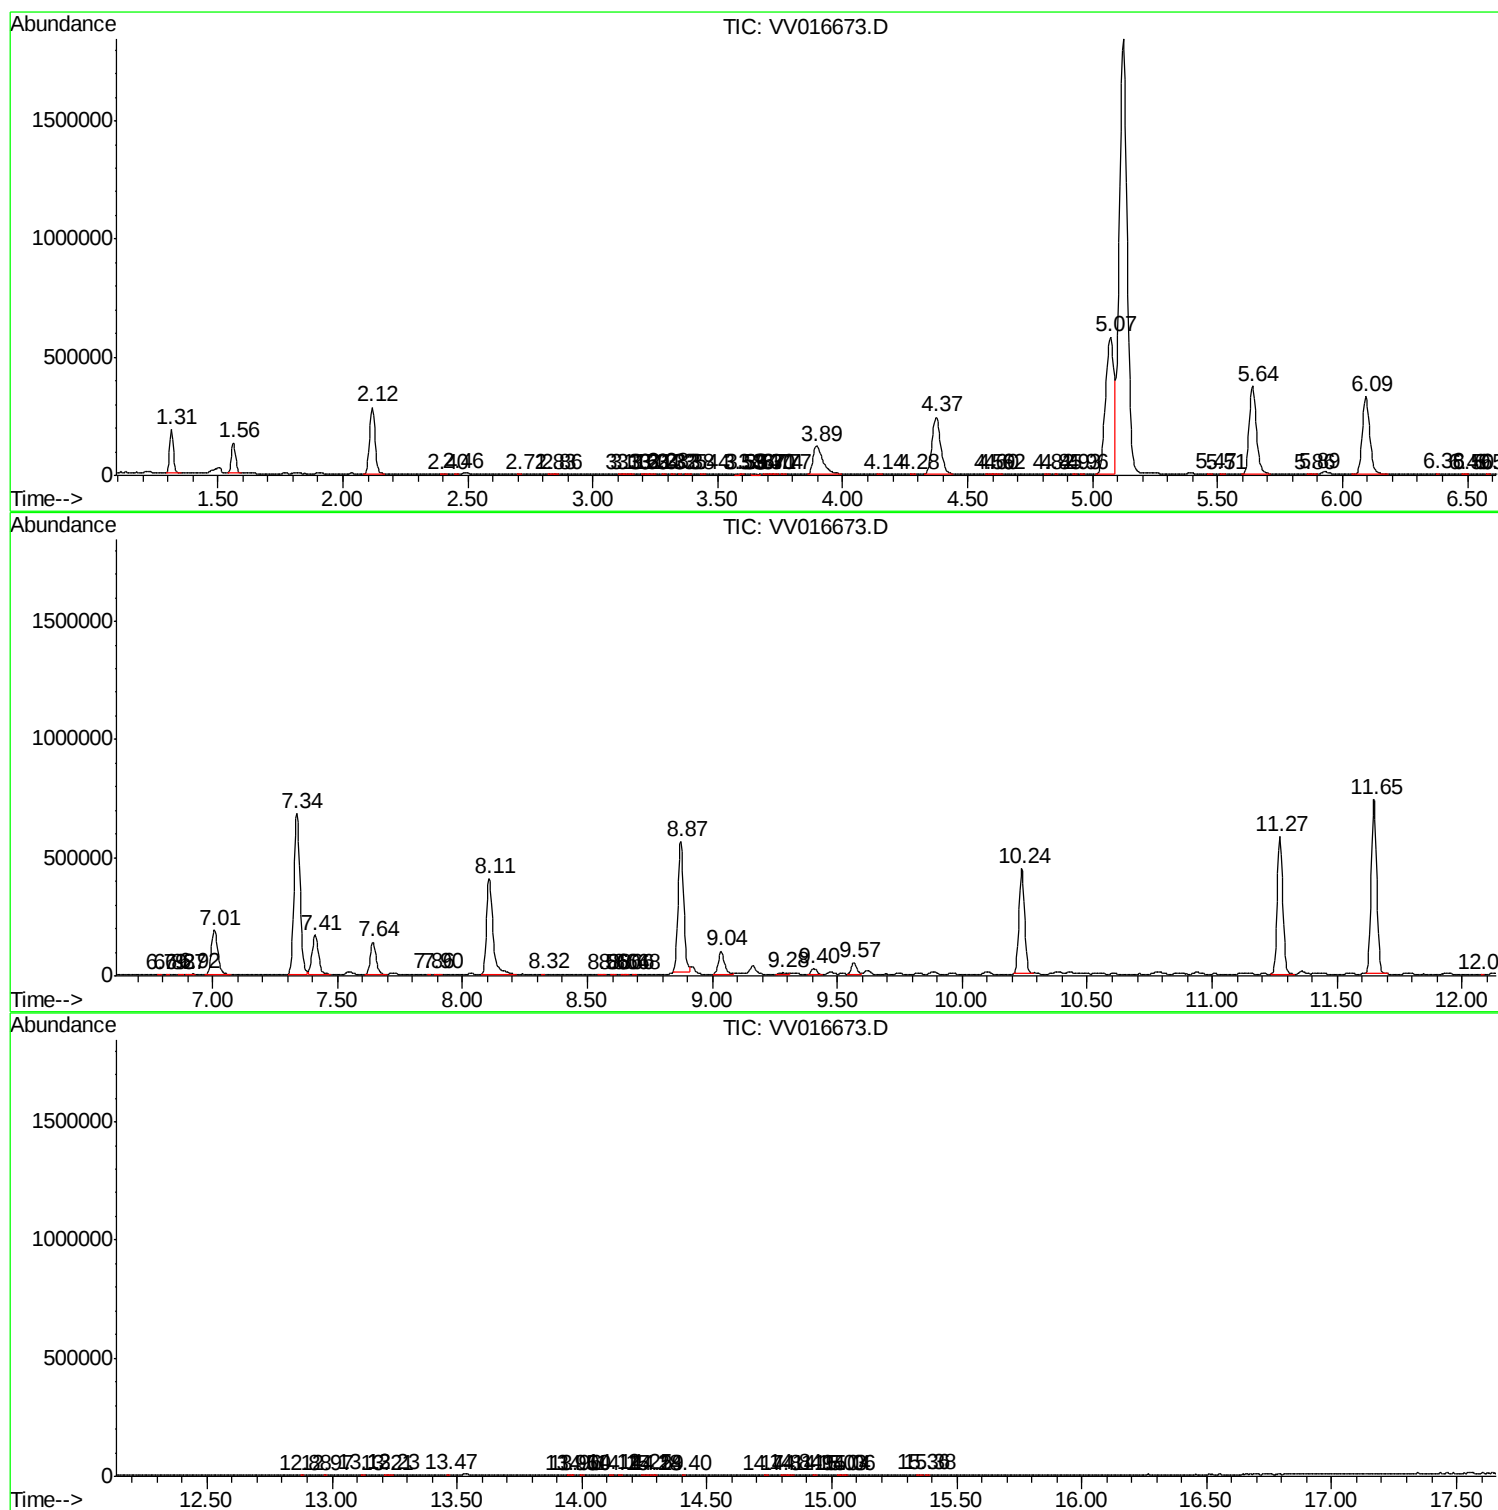

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016673.D
Acq On : 08 Jun 2020 20:59
Operator : SY/MD
Sample : L2861-19DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E67DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016673.D
Acq On : 08 Jun 2020 20:59
Operator : SY/MD
Sample : L2861-19DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E67DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc