

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016674.D
 Acq On : 08 Jun 2020 21:22
 Operator : SY/MD
 Sample : L2861-15DL2 250X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E48DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	80	rVB	188166	195008	13.98%	1.825%
2	1.557	139	145	159	rVB	121162	146864	10.53%	1.374%
3	2.116	309	319	335	rBV	274231	403834	28.96%	3.779%
4	2.399	405	407	409	rBV2	873	433	0.03%	0.004%
5	2.705	498	502	506	rBV6	1781	1437	0.10%	0.013%
6	2.730	508	510	513	rVB4	1729	960	0.07%	0.009%
7	2.824	535	539	541	rBV5	1420	961	0.07%	0.009%
8	2.955	576	580	581	rBV4	1049	780	0.06%	0.007%
9	3.061	611	613	619	rBV7	1181	800	0.06%	0.007%
10	3.103	624	626	631	rVB7	1929	1354	0.10%	0.013%
11	3.142	635	638	644	rBV8	1545	1388	0.10%	0.013%
12	3.277	677	680	681	rBV2	1104	484	0.03%	0.005%
13	3.335	694	698	701	rBV4	1523	1241	0.09%	0.012%
14	3.447	728	733	738	rBV7	2044	2671	0.19%	0.025%
15	3.496	744	748	751	rVB5	1662	992	0.07%	0.009%
16	3.531	757	759	761	rVV2	1318	461	0.03%	0.004%
17	3.595	777	779	782	rBV4	756	450	0.03%	0.004%
18	3.647	791	795	798	rBV5	1366	1126	0.08%	0.011%
19	3.666	798	801	805	rVV6	976	810	0.06%	0.008%
20	3.717	815	817	819	rBV3	1115	745	0.05%	0.007%
21	3.743	823	825	827	rVB3	1649	647	0.05%	0.006%
22	3.894	861	872	902	rBV	117474	328306	23.54%	3.072%
23	4.087	930	932	935	rBV4	1336	728	0.05%	0.007%
24	4.287	992	994	1001	rBV8	1509	1712	0.12%	0.016%
25	4.373	1006	1021	1043	rVV	228842	560301	40.18%	5.243%
26	4.505	1060	1062	1063	rBV3	1309	566	0.04%	0.005%
27	4.669	1111	1113	1115	rBV4	1092	501	0.04%	0.005%
28	4.769	1142	1144	1149	rVB6	1173	877	0.06%	0.008%
29	4.798	1151	1153	1155	rBV3	1845	714	0.05%	0.007%
30	4.852	1166	1170	1172	rBV5	1833	1229	0.09%	0.012%
31	4.994	1212	1214	1219	rBV4	1261	1074	0.08%	0.010%
32	5.071	1220	1238	1246	rBV2	554635	1394455	100.00%	13.048%
33	5.505	1369	1373	1375	rBV4	2186	1720	0.12%	0.016%
34	5.566	1389	1392	1393	rBV3	1338	770	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016674.D
 Acq On : 08 Jun 2020 21:22
 Operator : SY/MD
 Sample : L2861-15DL2 250X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E48DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.640	1403	1415	1437	rBV	384713	767009	55.00%	7.177%
36	6.094	1540	1556	1583	rBV	319407	660159	47.34%	6.177%
37	6.447	1662	1666	1668	rBV5	2118	1710	0.12%	0.016%
38	6.505	1681	1684	1685	rBV3	1385	842	0.06%	0.008%
39	6.920	1811	1813	1815	rBV3	908	479	0.03%	0.004%
40	6.962	1824	1826	1828	rBV3	1413	960	0.07%	0.009%
41	7.007	1829	1840	1862	rVV	183784	323143	23.17%	3.024%
42	7.142	1879	1882	1885	rBV4	1360	1054	0.08%	0.010%
43	7.338	1928	1943	1960	rBV	651483	1128684	80.94%	10.561%
44	7.640	2027	2037	2054	rBV2	129512	217278	15.58%	2.033%
45	7.920	2120	2124	2126	rBV4	1583	1127	0.08%	0.011%
46	8.058	2165	2167	2169	rBV2	1328	784	0.06%	0.007%
47	8.106	2172	2182	2215	rBV	386403	720930	51.70%	6.746%
48	8.566	2323	2325	2327	rBV3	1129	438	0.03%	0.004%
49	8.714	2369	2371	2373	rBV3	1207	809	0.06%	0.008%
50	8.740	2378	2379	2383	rVB4	1458	713	0.05%	0.007%
51	8.788	2392	2394	2399	rVB4	2172	1643	0.12%	0.015%
52	8.875	2409	2421	2446	rBV	573002	960284	68.86%	8.986%
53	9.036	2464	2471	2482	rVB	31129	46437	3.33%	0.435%
54	9.232	2529	2532	2534	rBV3	1689	1030	0.07%	0.010%
55	9.283	2539	2548	2557	rBV3	4270	8714	0.62%	0.082%
56	9.370	2573	2575	2576	rBV2	1119	430	0.03%	0.004%
57	9.396	2578	2583	2584	rBV5	2236	1899	0.14%	0.018%
58	9.569	2629	2637	2651	rVB4	15437	26033	1.87%	0.244%
59	9.646	2659	2661	2662	rBV2	1223	678	0.05%	0.006%
60	9.701	2674	2678	2681	rBV4	1502	1316	0.09%	0.012%
61	9.945	2750	2754	2755	rBV3	1620	1125	0.08%	0.011%
62	10.055	2786	2788	2791	rBV4	1752	1005	0.07%	0.009%
63	10.171	2822	2824	2827	rVB3	1292	706	0.05%	0.007%
64	10.238	2834	2845	2862	rBV	442754	676765	48.53%	6.333%
65	10.701	2987	2989	2993	rBV5	1600	1086	0.08%	0.010%
66	11.032	3090	3092	3094	rBV3	1394	623	0.04%	0.006%
67	11.068	3100	3103	3105	rBV3	1163	811	0.06%	0.008%
68	11.090	3108	3110	3114	rVV3	1546	1017	0.07%	0.010%
69	11.270	3154	3166	3181	rBV	598164	925388	66.36%	8.659%
70	11.547	3250	3252	3262	rVB10	2571	3851	0.28%	0.036%
71	11.646	3272	3283	3301	rBV	717826	1106362	79.34%	10.353%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016674.D
 Acq On : 08 Jun 2020 21:22
 Operator : SY/MD
 Sample : L2861-15DL2 250X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E48DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.116	3423	3429	3431	rBV6	1899	1731	0.12%	0.016%
73	12.215	3458	3460	3464	rBV3	1215	648	0.05%	0.006%
74	12.235	3464	3466	3469	rBV3	1574	1188	0.09%	0.011%
75	12.309	3483	3489	3491	rBV7	1684	1623	0.12%	0.015%
76	12.396	3514	3516	3517	rBV2	1177	437	0.03%	0.004%
77	12.431	3525	3527	3530	rBV3	1353	961	0.07%	0.009%
78	12.498	3546	3548	3553	rVB5	1543	1337	0.10%	0.013%
79	12.534	3553	3559	3561	rBV5	1244	1336	0.10%	0.013%
80	12.585	3573	3575	3576	rBV2	1096	435	0.03%	0.004%
81	12.727	3614	3619	3621	rBV4	1456	1359	0.10%	0.013%
82	12.759	3627	3629	3631	rBV3	1125	510	0.04%	0.005%
83	12.891	3667	3670	3671	rBV3	1297	810	0.06%	0.008%
84	13.006	3702	3706	3708	rBV4	1073	684	0.05%	0.006%
85	13.045	3716	3718	3721	rBV3	1728	1021	0.07%	0.010%
86	13.084	3726	3730	3734	rVB6	1814	1713	0.12%	0.016%
87	13.254	3780	3783	3785	rBV3	1668	1183	0.08%	0.011%
88	13.350	3810	3813	3815	rBV3	1276	808	0.06%	0.008%
89	13.531	3864	3869	3877	rBV4	5072	6977	0.50%	0.065%
90	13.727	3928	3930	3932	rBV2	1569	571	0.04%	0.005%
91	13.826	3959	3961	3962	rBV2	1192	452	0.03%	0.004%
92	13.952	3998	4000	4004	rVB5	1843	1105	0.08%	0.010%
93	13.987	4008	4011	4016	rBV6	1292	1333	0.10%	0.012%
94	14.019	4018	4021	4024	rBV4	1788	1505	0.11%	0.014%
95	14.170	4065	4068	4070	rBV4	1276	940	0.07%	0.009%
96	14.424	4143	4147	4148	rBV4	1152	774	0.06%	0.007%
97	14.540	4181	4183	4185	rBV3	1138	646	0.05%	0.006%
98	14.733	4240	4243	4247	rBV5	2213	1459	0.10%	0.014%
99	15.016	4328	4331	4334	rBV4	1762	1257	0.09%	0.012%
100	15.177	4376	4381	4384	rBV6	2066	2353	0.17%	0.022%


Sum of corrected areas: 10686877

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016674.D
Acq On : 08 Jun 2020 21:22
Operator : SY/MD
Sample : L2861-15DL2 250X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E48DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

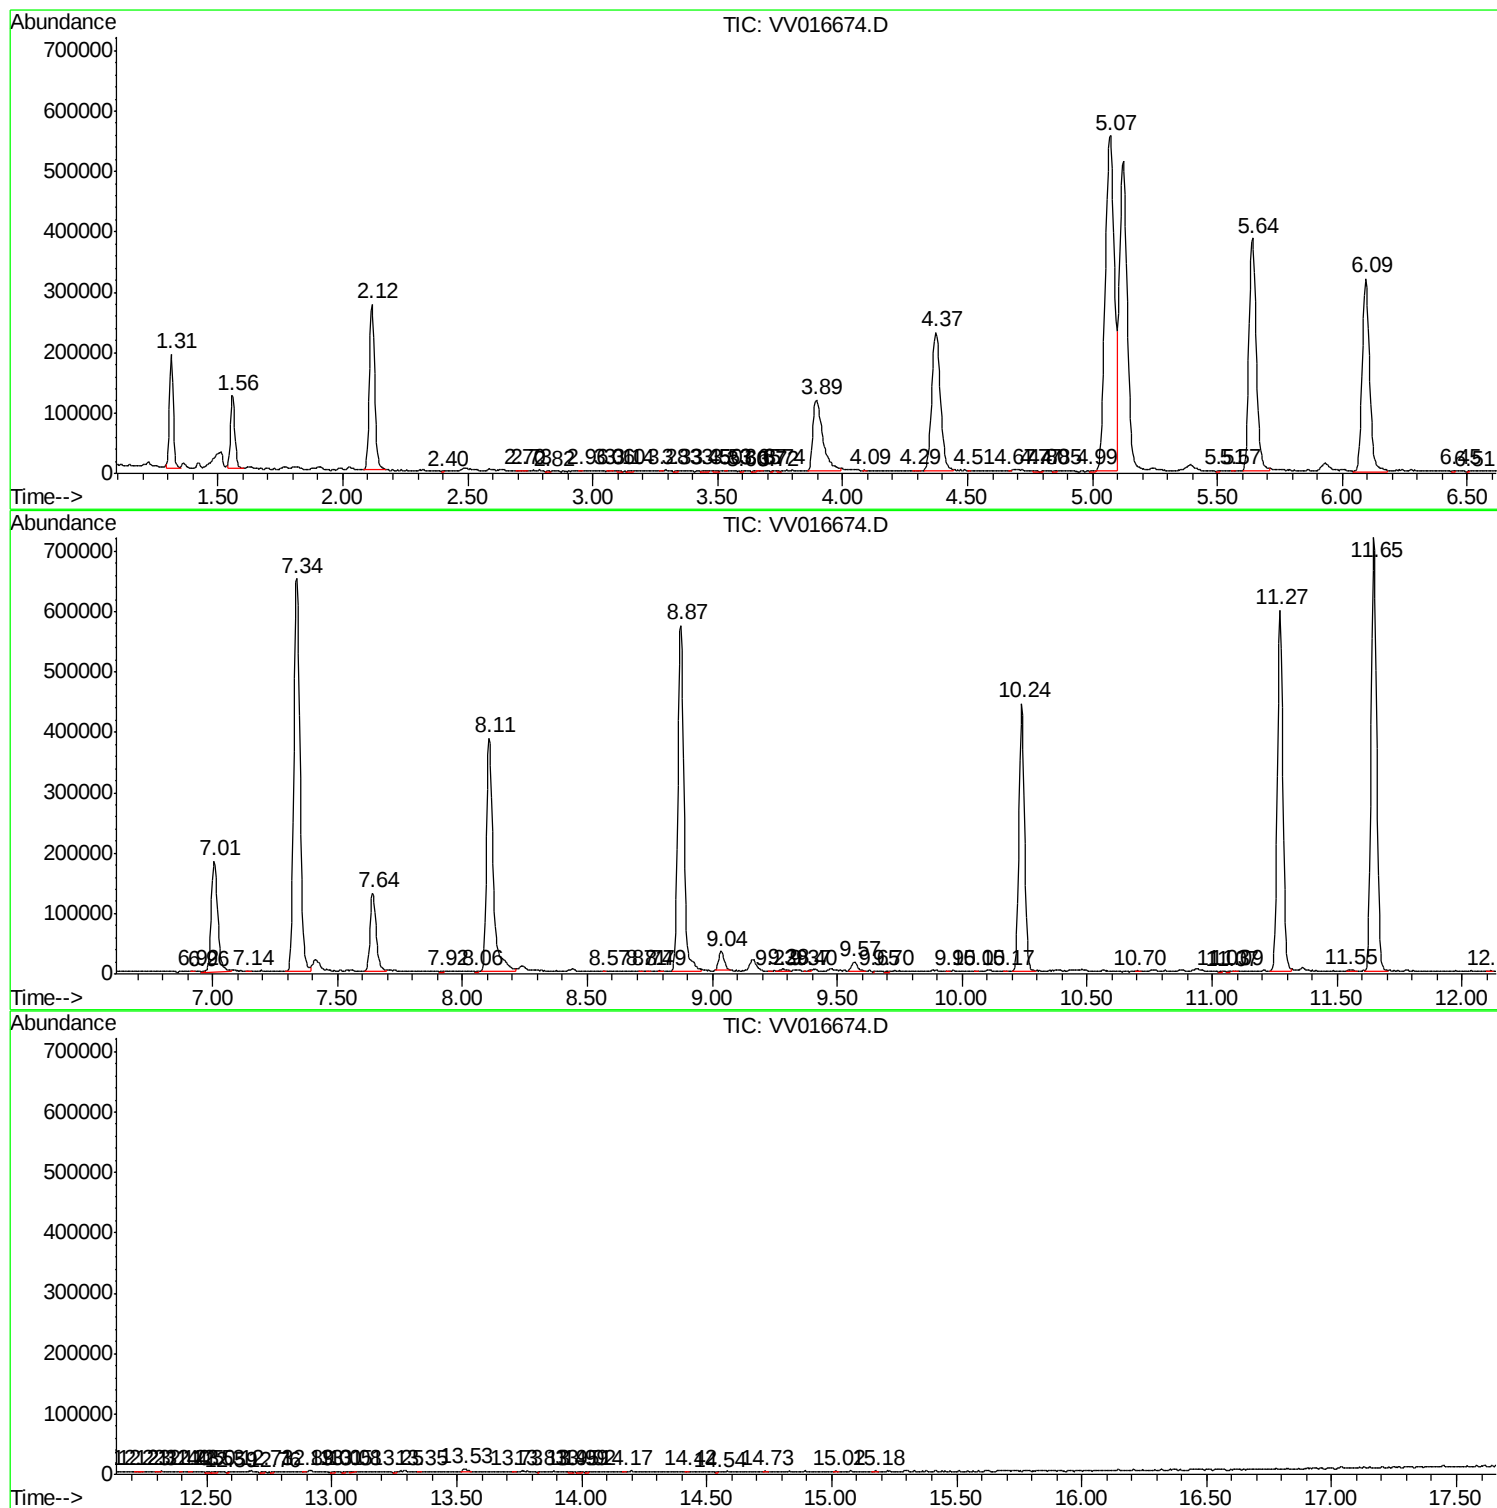

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016674.D
Acq On : 08 Jun 2020 21:22
Operator : SY/MD
Sample : L2861-15DL2 250X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E48DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016674.D
Acq On : 08 Jun 2020 21:22
Operator : SY/MD
Sample : L2861-15DL2 250X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E48DL2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc