

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016676.D
 Acq On : 08 Jun 2020 22:10
 Operator : SY/MD
 Sample : L2875-03DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB2	310004	335263	23.85%	2.954%
2	1.563	141	147	159	rVB	127606	151691	10.79%	1.336%
3	2.116	310	319	333	rBV	264541	390111	27.75%	3.437%
4	2.267	364	366	370	rBV5	1893	1461	0.10%	0.013%
5	2.473	427	430	432	rBV4	1166	534	0.04%	0.005%
6	2.749	511	516	517	rBV4	2316	1551	0.11%	0.014%
7	2.913	565	567	570	rVB5	1265	646	0.05%	0.006%
8	2.936	572	574	576	rVV3	1148	483	0.03%	0.004%
9	3.032	601	604	606	rBV3	1900	1230	0.09%	0.011%
10	3.081	617	619	623	rBV5	1136	575	0.04%	0.005%
11	3.116	627	630	632	rVB4	1581	915	0.07%	0.008%
12	3.241	667	669	674	rVB6	1747	1061	0.08%	0.009%
13	3.360	704	706	708	rVB3	1176	539	0.04%	0.005%
14	3.383	710	713	714	rBV2	1064	620	0.04%	0.005%
15	3.415	719	723	727	rBV6	1736	1801	0.13%	0.016%
16	3.511	748	753	754	rBV3	2261	1427	0.10%	0.013%
17	3.585	772	776	778	rBV4	1228	1191	0.08%	0.010%
18	3.618	784	786	789	rVB3	706	466	0.03%	0.004%
19	3.656	793	798	800	rBV6	1267	1271	0.09%	0.011%
20	3.692	808	809	811	rVB2	1777	580	0.04%	0.005%
21	3.933	862	884	912	rVV2	355237	1135344	80.76%	10.003%
22	4.248	980	982	985	rBV3	2031	1386	0.10%	0.012%
23	4.373	1007	1021	1047	rVB	227085	552377	39.29%	4.867%
24	4.801	1151	1154	1156	rBV4	1342	882	0.06%	0.008%
25	4.929	1192	1194	1197	rBV4	806	475	0.03%	0.004%
26	5.071	1221	1238	1261	rBV2	549713	1405898	100.00%	12.387%
27	5.572	1390	1394	1397	rBV6	1966	1535	0.11%	0.014%
28	5.640	1403	1415	1439	rBV	404521	797542	56.73%	7.027%
29	5.875	1487	1488	1492	rBV3	1047	471	0.03%	0.004%
30	6.093	1544	1556	1577	rBV	318655	629972	44.81%	5.550%
31	6.338	1627	1632	1635	rBV4	1758	1567	0.11%	0.014%
32	6.425	1653	1659	1660	rBV5	1638	1471	0.10%	0.013%
33	6.473	1672	1674	1679	rBV5	1151	1037	0.07%	0.009%
34	6.495	1679	1681	1683	rBV2	848	468	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016676.D
 Acq On : 08 Jun 2020 22:10
 Operator : SY/MD
 Sample : L2875-03DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.592	1709	1711	1715	rBV5	1356	1054	0.07%	0.009%
36	7.007	1828	1840	1863	rBV	177195	322008	22.90%	2.837%
37	7.238	1908	1912	1914	rBV5	1534	1351	0.10%	0.012%
38	7.338	1928	1943	1959	rBV	636058	1095213	77.90%	9.649%
39	7.640	2028	2037	2052	rBV	125226	209156	14.88%	1.843%
40	7.843	2098	2100	2103	rVB2	1211	625	0.04%	0.006%
41	7.968	2137	2139	2140	rBV2	1353	535	0.04%	0.005%
42	7.997	2146	2148	2150	rBV2	1547	978	0.07%	0.009%
43	8.106	2171	2182	2215	rBV	369347	697943	49.64%	6.149%
44	8.370	2261	2264	2266	rBV4	1130	825	0.06%	0.007%
45	8.560	2321	2323	2329	rBV7	1411	1146	0.08%	0.010%
46	8.826	2404	2406	2408	rBV3	1324	694	0.05%	0.006%
47	8.875	2408	2421	2445	rVV	595986	975092	69.36%	8.591%
48	9.084	2483	2486	2491	rBV6	1612	1675	0.12%	0.015%
49	9.122	2494	2498	2499	rVV3	976	570	0.04%	0.005%
50	9.296	2550	2552	2554	rBV3	1190	558	0.04%	0.005%
51	9.418	2588	2590	2592	rBV3	1143	596	0.04%	0.005%
52	9.514	2618	2620	2621	rBV2	1393	540	0.04%	0.005%
53	9.595	2642	2645	2647	rBV3	1371	907	0.06%	0.008%
54	9.691	2673	2675	2679	rBV5	1258	1085	0.08%	0.010%
55	9.801	2705	2709	2713	rBV5	1432	1415	0.10%	0.012%
56	9.884	2731	2735	2739	rVB6	1614	1275	0.09%	0.011%
57	9.904	2739	2741	2744	rBV2	1689	1000	0.07%	0.009%
58	9.984	2764	2766	2768	rBV3	1158	485	0.03%	0.004%
59	10.116	2803	2807	2810	rVB5	1549	1227	0.09%	0.011%
60	10.238	2833	2845	2862	rBV	409723	644336	45.83%	5.677%
61	10.871	3039	3042	3045	rBV5	1279	830	0.06%	0.007%
62	10.971	3070	3073	3078	rVB4	2000	1312	0.09%	0.012%
63	11.026	3088	3090	3092	rBV3	971	590	0.04%	0.005%
64	11.100	3109	3113	3114	rBV5	1713	1208	0.09%	0.011%
65	11.199	3141	3144	3145	rBV2	1269	731	0.05%	0.006%
66	11.270	3155	3166	3185	rBV	580342	895768	63.72%	7.892%
67	11.543	3247	3251	3252	rBV3	1292	841	0.06%	0.007%
68	11.646	3272	3283	3300	rBV	658207	1031284	73.35%	9.086%
69	11.797	3328	3330	3331	rBV2	1390	589	0.04%	0.005%
70	11.903	3361	3363	3366	rBV3	1048	501	0.04%	0.004%
71	11.916	3366	3367	3370	rBV4	1245	584	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016676.D
 Acq On : 08 Jun 2020 22:10
 Operator : SY/MD
 Sample : L2875-03DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.993	3389	3391	3394	rBV4	1447	945	0.07%	0.008%
73	12.022	3395	3400	3404	rVV6	1566	1838	0.13%	0.016%
74	12.058	3407	3411	3414	rBV5	1444	1122	0.08%	0.010%
75	12.103	3423	3425	3428	rBV3	1439	910	0.06%	0.008%
76	12.219	3459	3461	3466	rVB4	2050	1187	0.08%	0.010%
77	12.244	3466	3469	3471	rBV3	1291	802	0.06%	0.007%
78	12.312	3488	3490	3493	rVB3	1337	652	0.05%	0.006%
79	12.338	3493	3498	3500	rBV5	1935	1771	0.13%	0.016%
80	12.373	3508	3509	3513	rVB4	1406	722	0.05%	0.006%
81	12.492	3543	3546	3551	rBV6	1363	1385	0.10%	0.012%
82	12.669	3600	3601	3604	rBV3	1209	502	0.04%	0.004%
83	12.797	3639	3641	3645	rVB4	1998	1192	0.08%	0.011%
84	12.820	3645	3648	3649	rBV2	1453	622	0.04%	0.005%
85	12.871	3660	3664	3665	rBV3	1311	872	0.06%	0.008%
86	12.993	3701	3702	3704	rBV2	1347	535	0.04%	0.005%
87	13.074	3725	3727	3731	rBV5	1344	975	0.07%	0.009%
88	13.341	3808	3810	3814	rVV4	1177	676	0.05%	0.006%
89	13.363	3814	3817	3819	rVB4	1262	556	0.04%	0.005%
90	13.434	3835	3839	3840	rBV4	944	594	0.04%	0.005%
91	13.473	3847	3851	3855	rBV6	1385	1397	0.10%	0.012%
92	13.566	3877	3880	3881	rBV3	1772	1005	0.07%	0.009%
93	13.717	3923	3927	3928	rBV3	1280	908	0.06%	0.008%
94	13.878	3975	3977	3980	rBV4	1352	890	0.06%	0.008%
95	14.386	4128	4135	4138	rBV8	2096	2482	0.18%	0.022%
96	14.437	4148	4151	4152	rBV2	1009	616	0.04%	0.005%
97	14.604	4201	4203	4206	rBV4	1194	736	0.05%	0.006%
98	15.061	4341	4345	4346	rBV3	1505	978	0.07%	0.009%
99	15.717	4546	4549	4551	rBV3	2564	1681	0.12%	0.015%
100	15.775	4564	4567	4569	rVB3	2439	1291	0.09%	0.011%


Sum of corrected areas: 11350210

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016676.D
Acq On : 08 Jun 2020 22:10
Operator : SY/MD
Sample : L2875-03DL 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

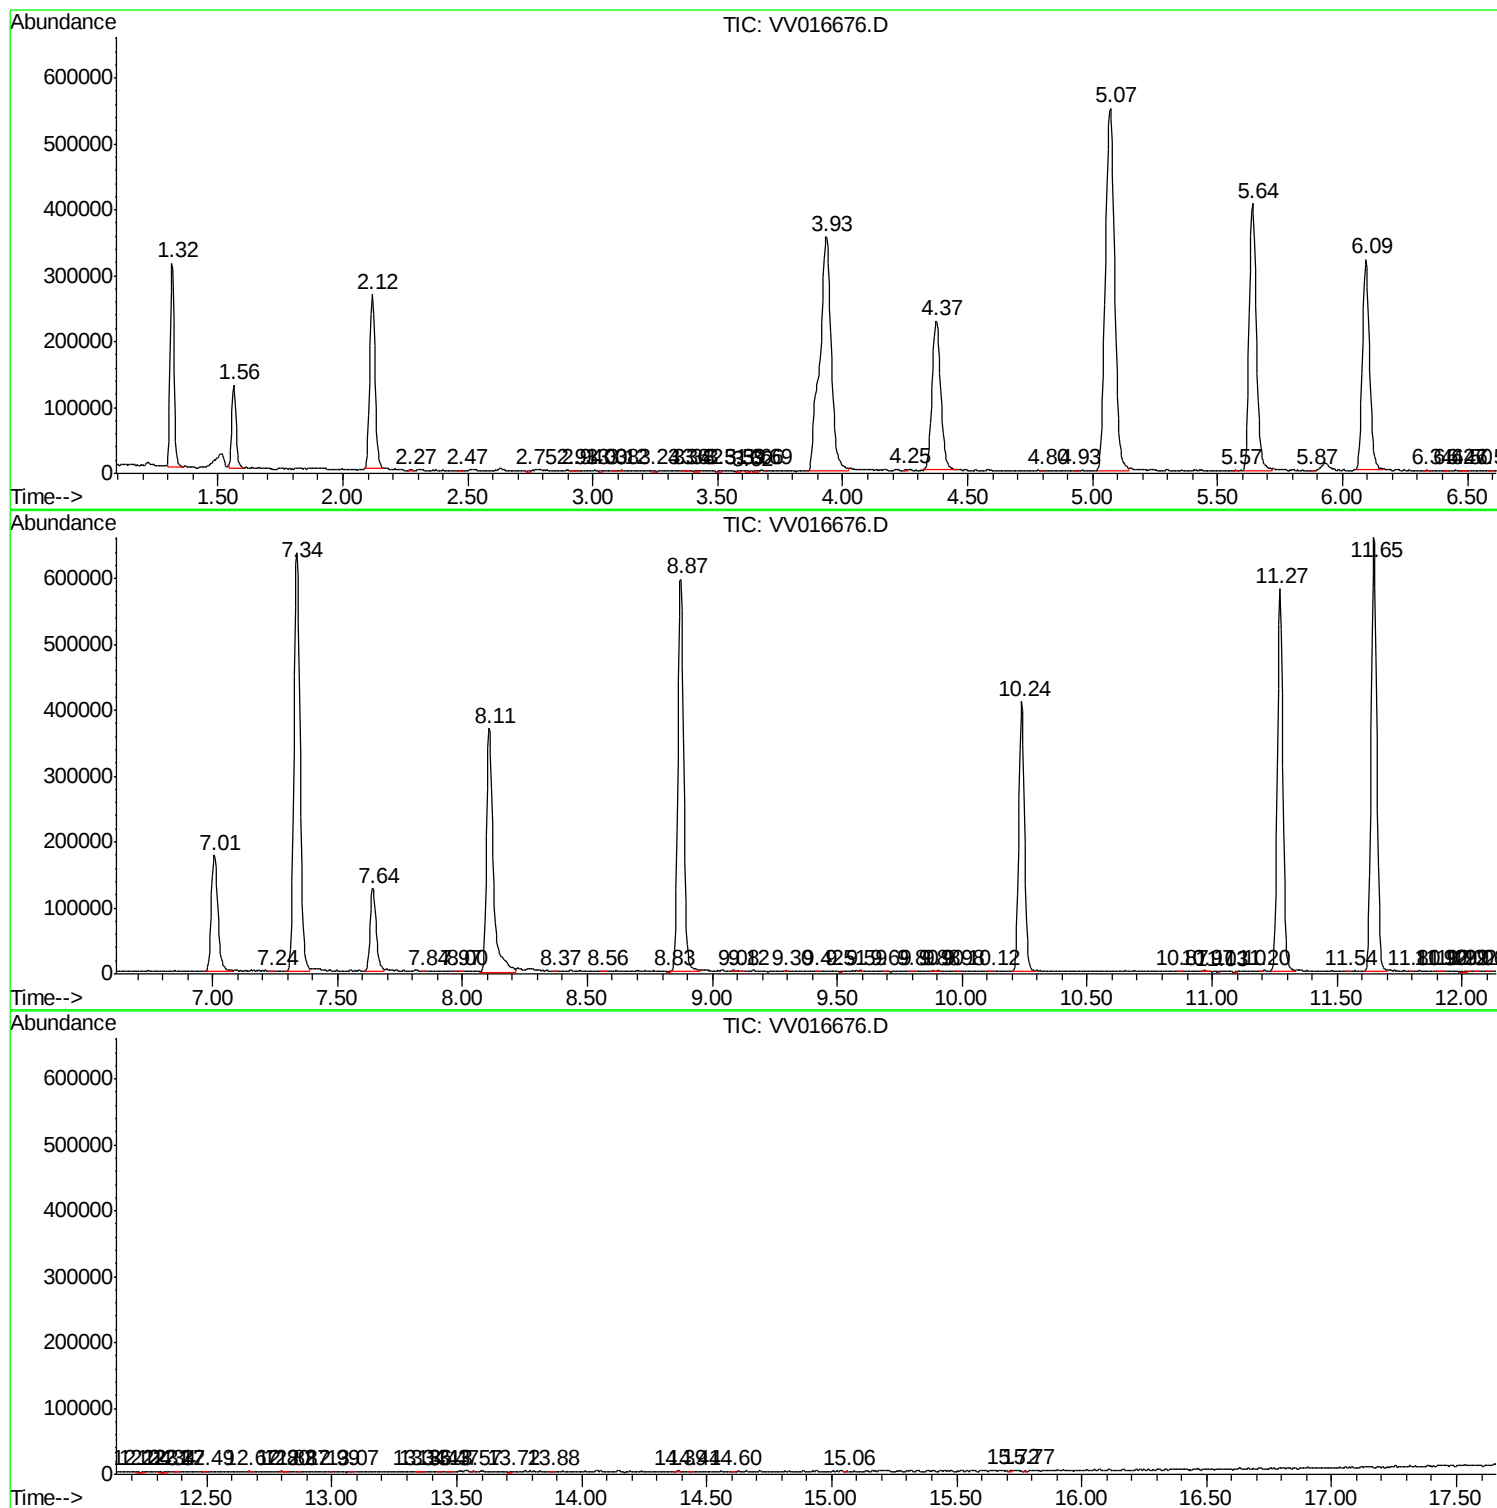

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016676.D
Acq On : 08 Jun 2020 22:10
Operator : SY/MD
Sample : L2875-03DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016676.D
Acq On : 08 Jun 2020 22:10
Operator : SY/MD
Sample : L2875-03DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS1DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc