

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016677.D
 Acq On : 08 Jun 2020 22:34
 Operator : SY/MD
 Sample : L2875-05DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB2	318106	334211	23.64%	3.007%
2	1.560	139	146	157	rVB	117916	141036	9.98%	1.269%
3	2.116	310	319	337	rVB	268039	395645	27.99%	3.560%
4	2.370	396	398	402	rVB5	1803	1047	0.07%	0.009%
5	2.392	402	405	407	rBV3	1638	1078	0.08%	0.010%
6	2.444	420	421	425	rBV4	1529	929	0.07%	0.008%
7	2.508	438	441	442	rBV3	1595	916	0.06%	0.008%
8	2.727	506	509	513	rBV6	1556	1223	0.09%	0.011%
9	2.765	517	521	524	rBV6	1768	1560	0.11%	0.014%
10	3.032	601	604	607	rBV4	1553	991	0.07%	0.009%
11	3.126	630	633	635	rBV3	1476	863	0.06%	0.008%
12	3.174	646	648	653	rVB5	2133	1329	0.09%	0.012%
13	3.293	682	685	686	rBV3	2090	1132	0.08%	0.010%
14	3.540	759	762	767	rVV5	1677	1246	0.09%	0.011%
15	3.566	767	770	774	rVV5	1114	872	0.06%	0.008%
16	3.736	819	823	825	rBV4	1496	1099	0.08%	0.010%
17	3.759	828	830	838	rVB9	1757	1917	0.14%	0.017%
18	3.933	861	884	903	rBV2	210566	769278	54.42%	6.922%
19	4.309	997	1001	1002	rBV3	1598	906	0.06%	0.008%
20	4.373	1002	1021	1044	rVV	228411	562981	39.83%	5.065%
21	4.560	1075	1079	1083	rBV7	1669	1469	0.10%	0.013%
22	4.717	1124	1128	1133	rBV8	2128	2332	0.16%	0.021%
23	4.794	1149	1152	1158	rVB8	1704	1587	0.11%	0.014%
24	4.855	1165	1171	1176	rVB10	1799	2074	0.15%	0.019%
25	4.878	1176	1178	1182	rBV4	1752	1384	0.10%	0.012%
26	5.071	1219	1238	1268	rVV2	545976	1413629	100.00%	12.719%
27	5.441	1349	1353	1355	rBV3	1651	1345	0.10%	0.012%
28	5.640	1400	1415	1436	rBV	394291	794645	56.21%	7.150%
29	5.907	1494	1498	1499	rBV4	3825	2182	0.15%	0.020%
30	6.032	1535	1537	1541	rVV4	1640	1294	0.09%	0.012%
31	6.093	1541	1556	1579	rVV	318886	640795	45.33%	5.766%
32	6.318	1621	1626	1627	rBV4	1227	975	0.07%	0.009%
33	6.383	1642	1646	1649	rBV4	1335	1125	0.08%	0.010%
34	6.630	1716	1723	1724	rBV6	1275	1501	0.11%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016677.D
 Acq On : 08 Jun 2020 22:34
 Operator : SY/MD
 Sample : L2875-05DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETT57DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.006	1829	1840	1861	rVV	176276	314674	22.26%	2.831%
36	7.132	1877	1879	1882	rVB4	1743	866	0.06%	0.008%
37	7.244	1910	1914	1916	rBV4	1459	979	0.07%	0.009%
38	7.338	1930	1943	1962	rBV	643114	1112649	78.71%	10.011%
39	7.640	2027	2037	2056	rVV	126535	214251	15.16%	1.928%
40	7.971	2137	2140	2144	rBV4	1709	1709	0.12%	0.015%
41	8.109	2172	2183	2210	rBV	362407	686680	48.58%	6.178%
42	8.553	2317	2321	2325	rBV6	1316	1040	0.07%	0.009%
43	8.829	2403	2407	2408	rBV2	1049	814	0.06%	0.007%
44	8.874	2409	2421	2441	rVV	589513	956277	67.65%	8.604%
45	9.161	2505	2510	2511	rBV4	1973	1320	0.09%	0.012%
46	9.293	2547	2551	2554	rBV5	2154	1365	0.10%	0.012%
47	9.379	2575	2578	2581	rVB4	1822	1014	0.07%	0.009%
48	9.572	2634	2638	2641	rBV6	2173	2038	0.14%	0.018%
49	9.688	2671	2674	2676	rBV4	1517	1048	0.07%	0.009%
50	9.704	2676	2679	2685	rVB7	1954	1954	0.14%	0.018%
51	9.733	2685	2688	2691	rBV3	1401	1035	0.07%	0.009%
52	9.797	2704	2708	2710	rBV4	1673	1381	0.10%	0.012%
53	9.820	2713	2715	2718	rVV4	1759	1050	0.07%	0.009%
54	10.000	2767	2771	2777	rBV6	1632	1486	0.11%	0.013%
55	10.032	2779	2781	2784	rBV4	1234	843	0.06%	0.008%
56	10.048	2784	2786	2791	rVV5	1815	1175	0.08%	0.011%
57	10.119	2806	2808	2812	rVV3	1977	1352	0.10%	0.012%
58	10.151	2815	2818	2826	rVV8	1525	1431	0.10%	0.013%
59	10.238	2832	2845	2859	rBV	424504	660500	46.72%	5.943%
60	10.395	2890	2894	2895	rBV4	1335	1000	0.07%	0.009%
61	10.591	2952	2955	2958	rBV6	1244	813	0.06%	0.007%
62	10.624	2958	2965	2969	rVV9	1482	2043	0.14%	0.018%
63	10.672	2975	2980	2984	rVB8	1471	1584	0.11%	0.014%
64	10.710	2987	2992	2999	rVB8	1570	2022	0.14%	0.018%
65	10.743	2999	3002	3004	rBV2	1704	822	0.06%	0.007%
66	10.858	3035	3038	3040	rBV3	1260	995	0.07%	0.009%
67	11.032	3089	3092	3094	rBV4	1185	845	0.06%	0.008%
68	11.061	3098	3101	3104	rVB5	1465	1011	0.07%	0.009%
69	11.167	3132	3134	3137	rVB4	1406	823	0.06%	0.007%
70	11.270	3155	3166	3186	rBV	600805	921801	65.21%	8.294%
71	11.344	3186	3189	3193	rVB5	2135	1213	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016677.D
 Acq On : 08 Jun 2020 22:34
 Operator : SY/MD
 Sample : L2875-05DL 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.572	3257	3260	3262	rBV3	1978	1192	0.08%	0.011%
73	11.585	3262	3264	3267	rVV4	1319	948	0.07%	0.009%
74	11.646	3270	3283	3299	rBV	688449	1086978	76.89%	9.780%
75	11.759	3315	3318	3322	rBV4	1474	1456	0.10%	0.013%
76	11.858	3345	3349	3353	rBV8	1832	1607	0.11%	0.014%
77	11.890	3356	3359	3363	rBV6	1651	1445	0.10%	0.013%
78	12.183	3447	3450	3452	rBV4	1462	796	0.06%	0.007%
79	12.292	3480	3484	3488	rVB7	1906	1974	0.14%	0.018%
80	12.411	3516	3521	3523	rBV5	1542	1353	0.10%	0.012%
81	12.517	3552	3554	3559	rVB5	1365	1031	0.07%	0.009%
82	12.556	3564	3566	3572	rBV6	1110	1305	0.09%	0.012%
83	12.595	3575	3578	3580	rBV3	1309	795	0.06%	0.007%
84	12.710	3612	3614	3618	rBV4	1282	1008	0.07%	0.009%
85	12.816	3645	3647	3650	rVB4	1703	979	0.07%	0.009%
86	12.836	3650	3653	3657	rBV5	1954	1725	0.12%	0.016%
87	13.070	3721	3726	3730	rVB7	1741	1613	0.11%	0.015%
88	13.099	3730	3735	3740	rBV8	1813	2539	0.18%	0.023%
89	13.206	3763	3768	3770	rBV5	1642	1474	0.10%	0.013%
90	13.665	3909	3911	3915	rBV4	1164	843	0.06%	0.008%
91	13.852	3967	3969	3972	rBV3	1623	949	0.07%	0.009%
92	13.935	3989	3995	3999	rVB7	1622	1555	0.11%	0.014%
93	14.074	4035	4038	4040	rBV4	2022	1255	0.09%	0.011%
94	14.334	4116	4119	4120	rBV4	2162	1381	0.10%	0.012%
95	14.421	4139	4146	4148	rBV6	2171	2308	0.16%	0.021%
96	14.485	4162	4166	4167	rBV4	1506	1208	0.09%	0.011%
97	14.530	4177	4180	4182	rBV4	1145	841	0.06%	0.008%
98	14.585	4194	4197	4198	rBV2	1323	834	0.06%	0.008%
99	14.646	4214	4216	4221	rVB5	1535	1131	0.08%	0.010%
100	14.964	4313	4315	4318	rBV3	1611	1208	0.09%	0.011%


Sum of corrected areas: 11114230

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016677.D
Acq On : 08 Jun 2020 22:34
Operator : SY/MD
Sample : L2875-05DL 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

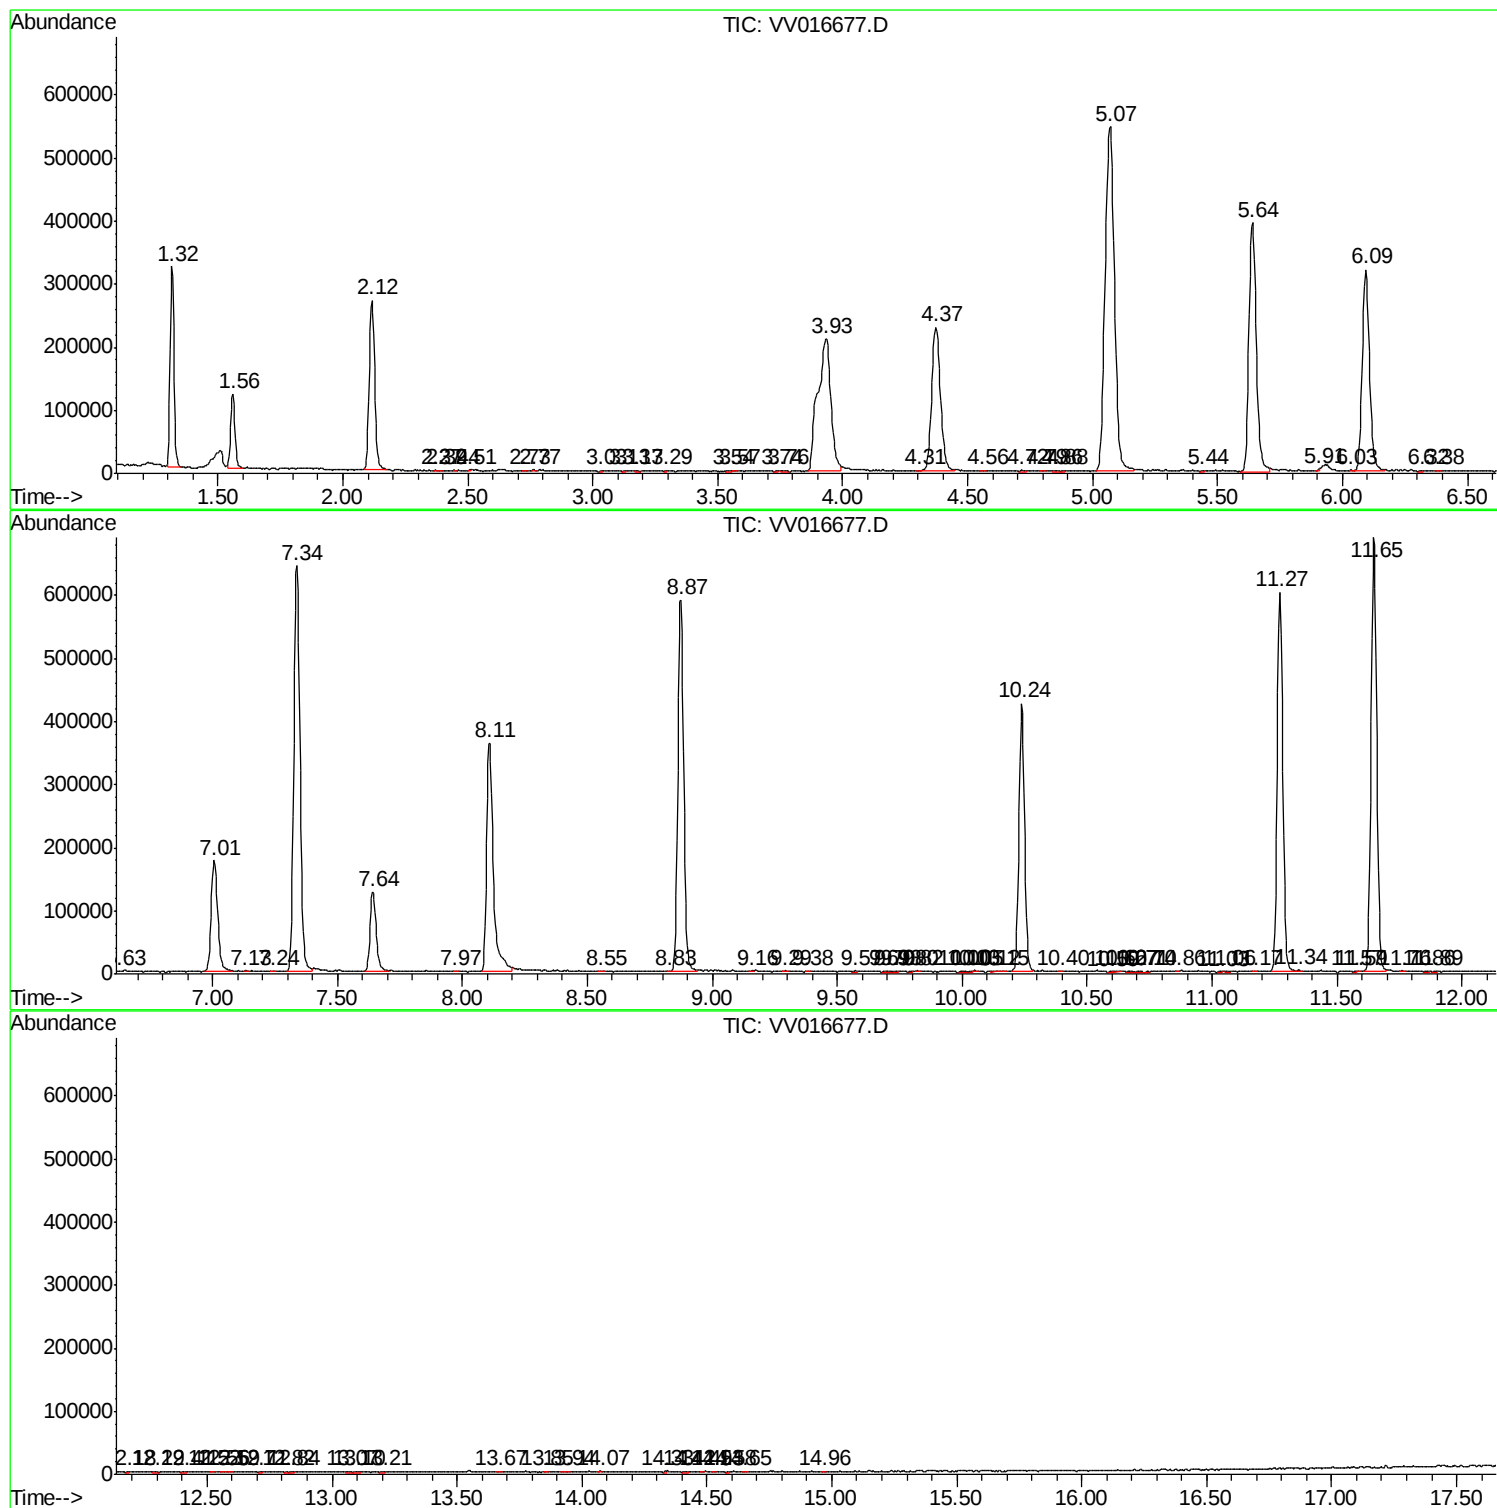

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016677.D
Acq On : 08 Jun 2020 22:34
Operator : SY/MD
Sample : L2875-05DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060820\
Data File : VV016677.D
Acq On : 08 Jun 2020 22:34
Operator : SY/MD
Sample : L2875-05DL 50X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTS7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc