

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016679.D
 Acq On : 08 Jun 2020 23:21
 Operator : SY/MD
 Sample : L2895-14DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB2	202341	224379	15.48%	1.972%
2	2.113	308	318	334	rVB	274426	407312	28.11%	3.579%
3	2.264	362	365	367	rBV4	1585	1196	0.08%	0.011%
4	2.518	431	444	450	rBV4	5048	9473	0.65%	0.083%
5	2.772	517	523	524	rBV5	3627	3374	0.23%	0.030%
6	2.897	557	562	563	rBV4	1270	1038	0.07%	0.009%
7	3.039	604	606	610	rVV4	1776	941	0.06%	0.008%
8	3.177	646	649	652	rBV5	1206	1091	0.08%	0.010%
9	3.196	652	655	657	rVV4	1650	1136	0.08%	0.010%
10	3.258	672	674	676	rBV3	1714	947	0.07%	0.008%
11	3.331	695	697	700	rVV2	1116	640	0.04%	0.006%
12	3.441	729	731	734	rBV4	960	643	0.04%	0.006%
13	3.486	742	745	748	rBV4	1793	1312	0.09%	0.012%
14	3.576	770	773	775	rBV3	1448	966	0.07%	0.008%
15	3.614	779	785	790	rVB6	1257	1371	0.09%	0.012%
16	3.762	829	831	834	rBV3	1890	1408	0.10%	0.012%
17	3.933	863	884	914	rBV3	297998	947746	65.40%	8.328%
18	4.232	973	977	979	rBV4	1615	1333	0.09%	0.012%
19	4.373	1007	1021	1043	rVB	232367	561707	38.76%	4.936%
20	4.511	1060	1064	1066	rBV5	1625	1184	0.08%	0.010%
21	4.592	1087	1089	1094	rBV5	1701	1692	0.12%	0.015%
22	4.820	1159	1160	1163	rVB3	1938	869	0.06%	0.008%
23	4.843	1163	1167	1171	rBV6	1538	1504	0.10%	0.013%
24	4.868	1171	1175	1178	rBV4	1700	1716	0.12%	0.015%
25	4.913	1187	1189	1193	rVB4	1665	1105	0.08%	0.010%
26	4.933	1193	1195	1197	rBV3	1937	1170	0.08%	0.010%
27	5.003	1213	1217	1218	rBV3	1184	698	0.05%	0.006%
28	5.068	1218	1237	1265	rBV2	567583	1449138	100.00%	12.734%
29	5.637	1400	1414	1438	rBV	397560	793748	54.77%	6.975%
30	5.827	1469	1473	1477	rBV6	1867	1735	0.12%	0.015%
31	5.936	1491	1507	1525	rBV5	86276	188739	13.02%	1.659%
32	6.093	1544	1556	1574	rBV	318879	633860	43.74%	5.570%
33	6.399	1649	1651	1657	rVB6	1793	1382	0.10%	0.012%
34	6.444	1663	1665	1667	rBV3	1217	652	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016679.D
 Acq On : 08 Jun 2020 23:21
 Operator : SY/MD
 Sample : L2895-14DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.489	1676	1679	1681	rBV3	1782	1204	0.08%	0.011%
36	6.595	1710	1712	1714	rBV3	960	603	0.04%	0.005%
37	6.637	1723	1725	1727	rBV3	1403	624	0.04%	0.005%
38	6.904	1804	1808	1810	rBV5	1052	890	0.06%	0.008%
39	6.949	1817	1822	1824	rBV5	1132	923	0.06%	0.008%
40	7.007	1827	1840	1861	rBV	182316	327183	22.58%	2.875%
41	7.338	1931	1943	1960	rBV	652846	1127567	77.81%	9.908%
42	7.582	2015	2019	2020	rBV4	961	702	0.05%	0.006%
43	7.598	2022	2024	2025	rVV2	1702	642	0.04%	0.006%
44	7.640	2028	2037	2057	rVB	129680	221177	15.26%	1.944%
45	7.875	2107	2110	2113	rBV5	1477	827	0.06%	0.007%
46	7.897	2115	2117	2121	rVB5	1184	698	0.05%	0.006%
47	8.113	2171	2184	2216	rBV	340302	725129	50.04%	6.372%
48	8.396	2270	2272	2274	rBV3	1305	749	0.05%	0.007%
49	8.511	2306	2308	2310	rBV3	1215	697	0.05%	0.006%
50	8.733	2373	2377	2379	rBV5	1493	926	0.06%	0.008%
51	8.875	2409	2421	2436	rBV	585253	940307	64.89%	8.263%
52	9.116	2494	2496	2500	rVB5	1552	799	0.06%	0.007%
53	9.148	2503	2506	2508	rBV3	1595	784	0.05%	0.007%
54	9.187	2515	2518	2520	rBV3	1427	987	0.07%	0.009%
55	9.344	2565	2567	2570	rBV4	1174	591	0.04%	0.005%
56	9.392	2580	2582	2585	rBV4	1294	666	0.05%	0.006%
57	9.463	2602	2604	2607	rBV3	1314	759	0.05%	0.007%
58	9.569	2633	2637	2638	rBV4	1132	860	0.06%	0.008%
59	9.662	2663	2666	2668	rBV5	1867	982	0.07%	0.009%
60	9.723	2682	2685	2688	rBV4	1500	951	0.07%	0.008%
61	9.769	2697	2699	2703	rBV5	1739	1274	0.09%	0.011%
62	9.855	2724	2726	2729	rVB4	1311	709	0.05%	0.006%
63	9.920	2744	2746	2751	rVB6	1298	853	0.06%	0.007%
64	9.977	2761	2764	2765	rBV3	1137	595	0.04%	0.005%
65	10.064	2789	2791	2794	rBV4	1574	936	0.06%	0.008%
66	10.087	2794	2798	2800	rVV4	1445	960	0.07%	0.008%
67	10.100	2800	2802	2805	rVV2	1152	640	0.04%	0.006%
68	10.116	2805	2807	2814	rVB6	2330	1815	0.13%	0.016%
69	10.148	2814	2817	2821	rVB6	1668	1238	0.09%	0.011%
70	10.177	2821	2826	2829	rBV4	1471	1558	0.11%	0.014%
71	10.238	2833	2845	2867	rBV	420591	678982	46.85%	5.966%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016679.D
 Acq On : 08 Jun 2020 23:21
 Operator : SY/MD
 Sample : L2895-14DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.756	3004	3006	3009	rBV4	957	609	0.04%	0.005%
73	10.801	3017	3020	3024	rBV4	1410	1094	0.08%	0.010%
74	10.997	3078	3081	3083	rBV4	1847	990	0.07%	0.009%
75	11.096	3110	3112	3117	rVV7	1634	1469	0.10%	0.013%
76	11.273	3155	3167	3183	rBV	606531	938524	64.76%	8.247%
77	11.395	3203	3205	3208	rBV4	1577	960	0.07%	0.008%
78	11.460	3224	3225	3229	rVB4	1912	879	0.06%	0.008%
79	11.649	3273	3284	3301	rVB	717220	1118024	77.15%	9.824%
80	11.907	3361	3364	3368	rBV6	1445	1248	0.09%	0.011%
81	12.055	3408	3410	3411	rBV2	1156	601	0.04%	0.005%
82	12.309	3488	3489	3493	rBV4	1054	706	0.05%	0.006%
83	12.460	3533	3536	3541	rBV7	1639	1442	0.10%	0.013%
84	12.482	3541	3543	3546	rVV4	2077	1322	0.09%	0.012%
85	12.720	3615	3617	3620	rBV4	1190	709	0.05%	0.006%
86	12.804	3640	3643	3646	rBV3	1453	1070	0.07%	0.009%
87	13.010	3703	3707	3709	rBV5	1791	1387	0.10%	0.012%
88	13.270	3785	3788	3792	rVB5	1302	869	0.06%	0.008%
89	13.299	3792	3797	3802	rBV9	2476	2488	0.17%	0.022%
90	13.328	3802	3806	3809	rVV5	951	738	0.05%	0.006%
91	13.530	3866	3869	3870	rBV3	1281	755	0.05%	0.007%
92	14.029	4023	4024	4026	rBV2	1333	595	0.04%	0.005%
93	14.061	4032	4034	4037	rBV3	1905	1071	0.07%	0.009%
94	14.161	4061	4065	4067	rVB4	1659	1013	0.07%	0.009%
95	14.309	4108	4111	4113	rBV4	1175	817	0.06%	0.007%
96	14.370	4126	4130	4131	rBV3	1265	856	0.06%	0.008%
97	14.421	4143	4146	4151	rVB7	1533	1220	0.08%	0.011%
98	14.627	4208	4210	4215	rBV5	1456	1270	0.09%	0.011%
99	14.727	4239	4241	4244	rBV3	1227	762	0.05%	0.007%
100	15.598	4510	4512	4516	rBV4	2202	1610	0.11%	0.014%


Sum of corrected areas: 11380090

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016679.D
Acq On : 08 Jun 2020 23:21
Operator : SY/MD
Sample : L2895-14DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
EW01DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

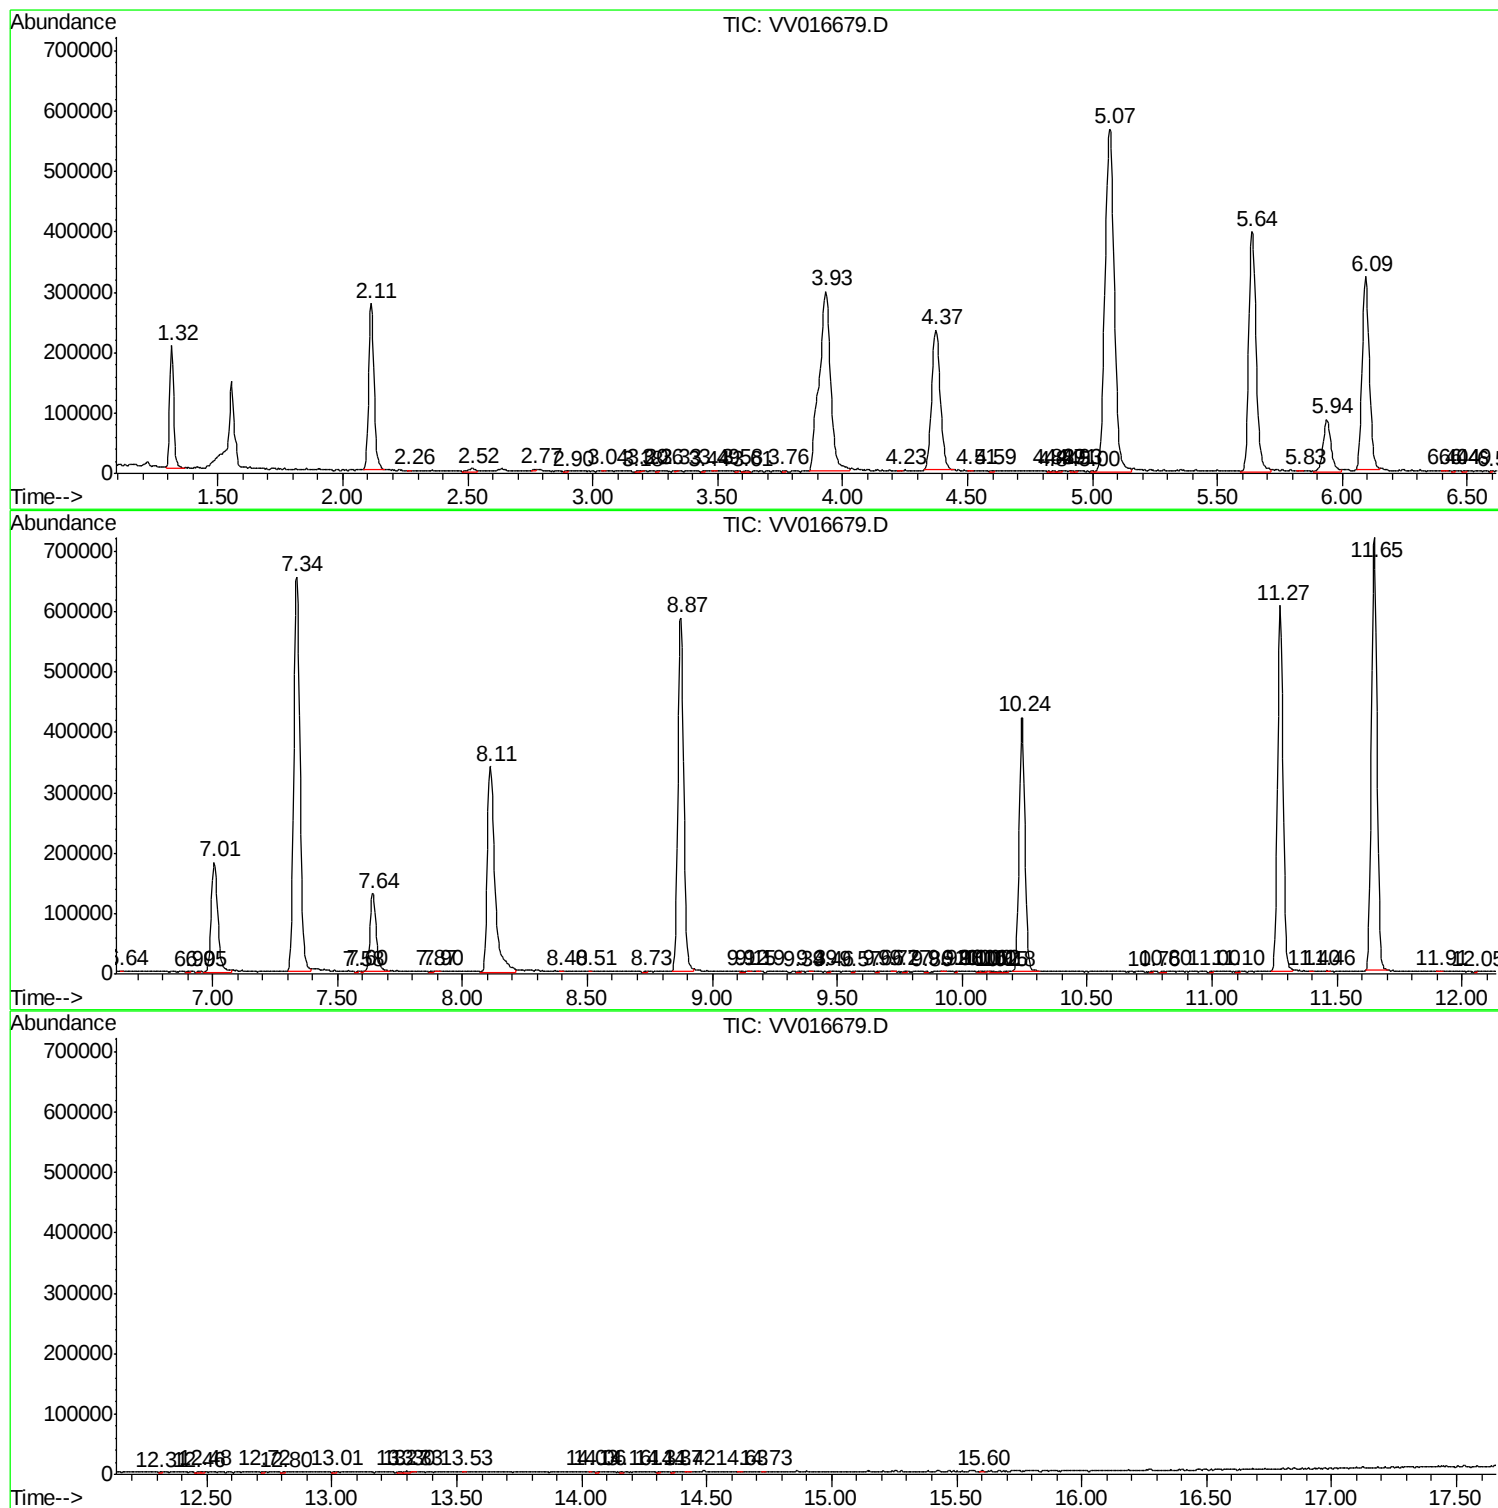

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016679.D
Acq On : 08 Jun 2020 23:21
Operator : SY/MD
Sample : L2895-14DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016679.D
Acq On : 08 Jun 2020 23:21
Operator : SY/MD
Sample : L2895-14DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L1DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc