

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016680.D
 Acq On : 08 Jun 2020 23:45
 Operator : SY/MD
 Sample : L2895-17DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	85	rVB2	201669	220950	16.65%	2.048%
2	2.113	309	318	333	rVB	252868	377777	28.46%	3.501%
3	2.306	377	378	381	rBV3	1341	803	0.06%	0.007%
4	2.431	416	417	420	rBV3	1202	701	0.05%	0.006%
5	2.592	465	467	469	rBV3	1420	841	0.06%	0.008%
6	2.756	516	518	519	rBV2	1421	521	0.04%	0.005%
7	2.823	537	539	544	rBV5	1460	1205	0.09%	0.011%
8	2.933	571	573	576	rBV4	1176	693	0.05%	0.006%
9	3.010	594	597	598	rBV3	1112	650	0.05%	0.006%
10	3.039	604	606	609	rBV3	1119	577	0.04%	0.005%
11	3.129	632	634	637	rBV3	1267	733	0.06%	0.007%
12	3.460	735	737	738	rBV2	949	521	0.04%	0.005%
13	3.479	741	743	746	rBV3	1248	810	0.06%	0.008%
14	3.512	751	753	756	rVB3	1678	955	0.07%	0.009%
15	3.524	756	757	761	rBV3	1185	839	0.06%	0.008%
16	3.634	787	791	796	rBV8	1242	1235	0.09%	0.011%
17	3.766	827	832	835	rBV7	1387	1531	0.12%	0.014%
18	3.814	846	847	850	rVB3	1735	532	0.04%	0.005%
19	3.833	850	853	856	rBV5	1906	1623	0.12%	0.015%
20	3.930	863	883	907	rBV2	359904	1086082	81.82%	10.066%
21	4.370	1005	1020	1046	rBV	214175	523876	39.47%	4.856%
22	4.653	1106	1108	1110	rBV3	1167	531	0.04%	0.005%
23	4.788	1148	1150	1153	rBV4	909	434	0.03%	0.004%
24	4.942	1197	1198	1205	rVB5	1618	1494	0.11%	0.014%
25	4.971	1205	1207	1208	rBV2	1127	518	0.04%	0.005%
26	5.068	1221	1237	1261	rBV2	520694	1327397	100.00%	12.303%
27	5.637	1401	1414	1437	rBV	387668	775750	58.44%	7.190%
28	5.888	1490	1492	1493	rBV2	1424	627	0.05%	0.006%
29	6.090	1543	1555	1577	rBV	298664	602428	45.38%	5.584%
30	6.299	1617	1620	1623	rVB4	1035	577	0.04%	0.005%
31	6.331	1628	1630	1632	rBV2	1094	587	0.04%	0.005%
32	6.450	1666	1667	1668	rBV	1528	513	0.04%	0.005%
33	6.569	1700	1704	1707	rVB3	1436	1008	0.08%	0.009%
34	6.601	1709	1714	1715	rBV4	1449	1080	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016680.D
 Acq On : 08 Jun 2020 23:45
 Operator : SY/MD
 Sample : L2895-17DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.634	1722	1724	1727	rBV4	1713	1120	0.08%	0.010%
36	6.650	1727	1729	1730	rBV2	1551	701	0.05%	0.006%
37	6.820	1779	1782	1785	rBV5	1803	1086	0.08%	0.010%
38	6.852	1789	1792	1794	rBV3	1817	912	0.07%	0.008%
39	7.007	1828	1840	1862	rBV2	166971	304851	22.97%	2.825%
40	7.180	1888	1894	1897	rBV7	2488	2593	0.20%	0.024%
41	7.296	1927	1930	1931	rBV3	2309	1303	0.10%	0.012%
42	7.338	1931	1943	1962	rVV	605649	1046842	78.86%	9.703%
43	7.640	2028	2037	2058	rBV2	117823	197434	14.87%	1.830%
44	7.772	2076	2078	2080	rBV3	1534	858	0.06%	0.008%
45	7.846	2099	2101	2106	rBV6	1292	849	0.06%	0.008%
46	8.019	2153	2155	2158	rBV4	1741	874	0.07%	0.008%
47	8.109	2173	2183	2218	rBV	324971	680169	51.24%	6.304%
48	8.524	2308	2312	2315	rBV6	1912	1796	0.14%	0.017%
49	8.679	2358	2360	2367	rVB5	2392	2078	0.16%	0.019%
50	8.711	2367	2370	2373	rBV5	1115	879	0.07%	0.008%
51	8.727	2373	2375	2378	rBV4	1619	1028	0.08%	0.010%
52	8.807	2398	2400	2403	rBV4	748	432	0.03%	0.004%
53	8.871	2409	2420	2436	rBV	569328	929406	70.02%	8.614%
54	9.219	2526	2528	2532	rVB4	1598	902	0.07%	0.008%
55	9.376	2573	2577	2581	rBV7	1135	1286	0.10%	0.012%
56	9.460	2601	2603	2606	rBV3	993	771	0.06%	0.007%
57	9.650	2660	2662	2664	rBV2	1030	428	0.03%	0.004%
58	9.736	2686	2689	2690	rBV2	1323	746	0.06%	0.007%
59	9.849	2719	2724	2727	rBV5	1258	1287	0.10%	0.012%
60	9.923	2745	2747	2749	rBV3	1088	641	0.05%	0.006%
61	10.023	2774	2778	2781	rBV6	1587	1215	0.09%	0.011%
62	10.074	2791	2794	2797	rBV4	1018	669	0.05%	0.006%
63	10.087	2797	2798	2804	rVB4	1134	748	0.06%	0.007%
64	10.238	2833	2845	2858	rBV	396447	635503	47.88%	5.890%
65	10.514	2926	2931	2934	rBV7	1496	1463	0.11%	0.014%
66	10.630	2964	2967	2969	rBV3	1194	762	0.06%	0.007%
67	10.746	3000	3003	3006	rBV5	1437	1176	0.09%	0.011%
68	10.785	3012	3015	3017	rBV4	1392	942	0.07%	0.009%
69	10.904	3050	3052	3054	rBV3	1420	705	0.05%	0.007%
70	11.010	3083	3085	3088	rBV4	1235	777	0.06%	0.007%
71	11.273	3155	3167	3187	rBV	602662	932394	70.24%	8.642%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016680.D
 Acq On : 08 Jun 2020 23:45
 Operator : SY/MD
 Sample : L2895-17DL 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.421	3211	3213	3215	rBV3	1230	706	0.05%	0.007%
73	11.649	3271	3284	3297	rBV	687713	1066132	80.32%	9.881%
74	11.894	3357	3360	3363	rBV2	1395	1108	0.08%	0.010%
75	12.077	3415	3417	3420	rBV3	1251	776	0.06%	0.007%
76	12.093	3420	3422	3426	rVB5	1312	731	0.06%	0.007%
77	12.283	3477	3481	3483	rBV5	1234	910	0.07%	0.008%
78	12.450	3531	3533	3538	rBV4	2334	1933	0.15%	0.018%
79	12.521	3553	3555	3560	rBV4	857	661	0.05%	0.006%
80	12.669	3599	3601	3604	rBV4	1082	644	0.05%	0.006%
81	12.727	3614	3619	3620	rBV5	1588	1319	0.10%	0.012%
82	12.778	3634	3635	3637	rBV	1283	567	0.04%	0.005%
83	12.826	3648	3650	3652	rBV3	1561	629	0.05%	0.006%
84	12.878	3662	3666	3669	rBV4	1597	1157	0.09%	0.011%
85	12.926	3678	3681	3682	rBV3	1300	631	0.05%	0.006%
86	13.042	3716	3717	3720	rVB3	937	446	0.03%	0.004%
87	13.119	3738	3741	3744	rVB5	2127	1352	0.10%	0.013%
88	13.135	3744	3746	3751	rVB5	2367	1797	0.14%	0.017%
89	13.157	3751	3753	3757	rBV4	2299	1741	0.13%	0.016%
90	13.225	3772	3774	3778	rBV4	1423	1110	0.08%	0.010%
91	13.383	3821	3823	3824	rBV2	1042	569	0.04%	0.005%
92	13.534	3869	3870	3877	rBV5	1479	1413	0.11%	0.013%
93	13.685	3912	3917	3922	rBV7	2426	3196	0.24%	0.030%
94	13.736	3931	3933	3936	rVB4	1415	530	0.04%	0.005%
95	13.961	3998	4003	4006	rVB6	1576	1635	0.12%	0.015%
96	14.212	4078	4081	4084	rBV4	1638	1042	0.08%	0.010%
97	14.415	4141	4144	4147	rBV4	1279	841	0.06%	0.008%
98	14.527	4177	4179	4182	rBV4	1103	553	0.04%	0.005%
99	14.630	4209	4211	4213	rBV3	1096	499	0.04%	0.005%
100	14.701	4230	4233	4234	rBV2	1101	650	0.05%	0.006%


Sum of corrected areas: 10789303

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016680.D
Acq On : 08 Jun 2020 23:45
Operator : SY/MD
Sample : L2895-17DL 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

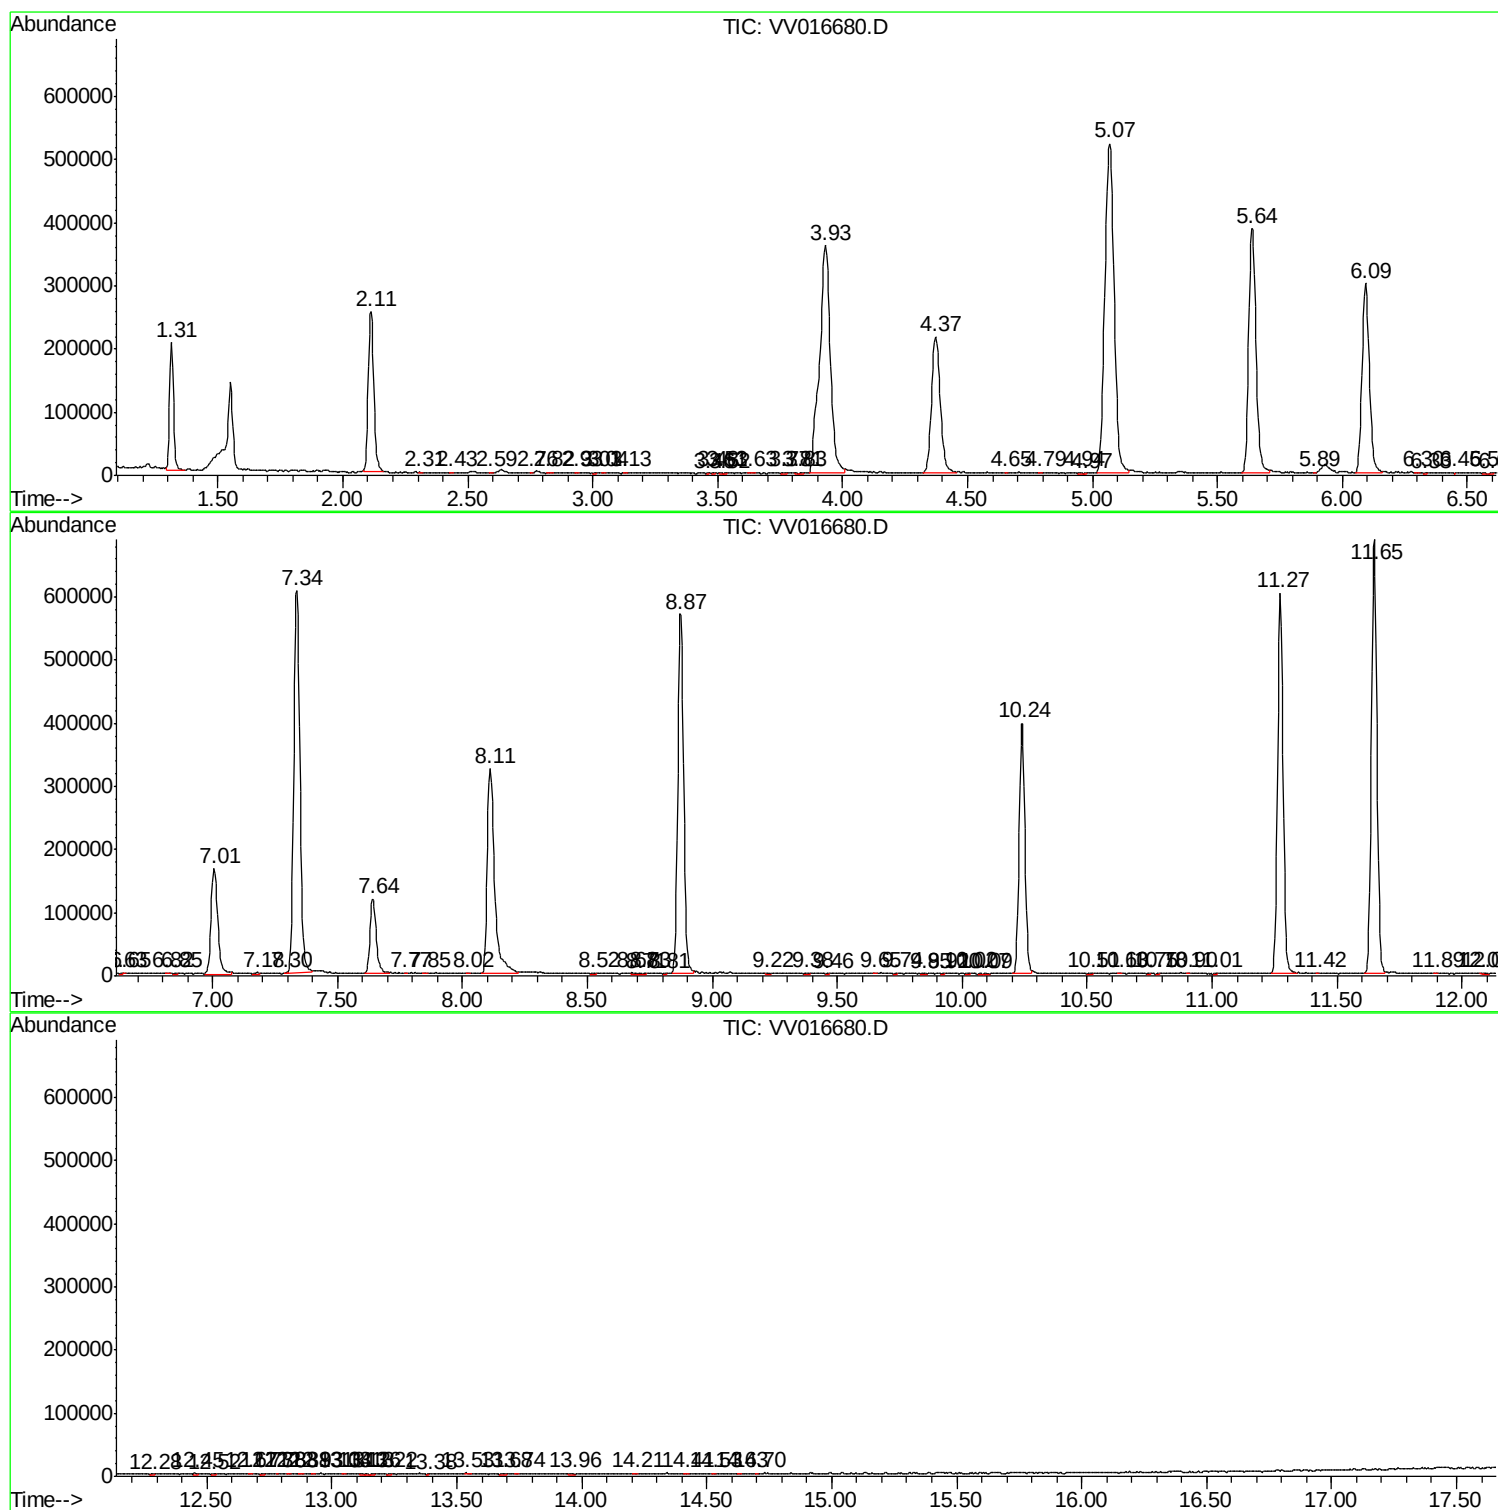

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016680.D
Acq On : 08 Jun 2020 23:45
Operator : SY/MD
Sample : L2895-17DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016680.D
Acq On : 08 Jun 2020 23:45
Operator : SY/MD
Sample : L2895-17DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L5DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
