

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016682.D
 Acq On : 09 Jun 2020 00:32
 Operator : SY/MD
 Sample : L2875-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	79	rVB2	243080	255041	18.35%	2.200%
2	1.560	140	146	159	rVB	120592	140248	10.09%	1.210%
3	2.116	310	319	336	rVB	264381	394151	28.36%	3.400%
4	2.598	466	469	474	rVB8	1560	1333	0.10%	0.011%
5	2.624	474	477	478	rBV2	1734	726	0.05%	0.006%
6	2.778	516	525	532	rBV9	5590	9718	0.70%	0.084%
7	2.878	553	556	558	rBV4	975	658	0.05%	0.006%
8	3.399	712	718	724	rVB10	1755	1822	0.13%	0.016%
9	3.428	724	727	729	rBV3	1135	722	0.05%	0.006%
10	3.527	756	758	761	rBV4	972	651	0.05%	0.006%
11	3.672	800	803	806	rVB4	1210	829	0.06%	0.007%
12	3.685	806	807	811	rVB4	1556	972	0.07%	0.008%
13	3.711	811	815	819	rBV5	1397	1476	0.11%	0.013%
14	3.749	823	827	829	rBV4	1339	993	0.07%	0.009%
15	3.775	829	835	836	rBV4	2142	1647	0.12%	0.014%
16	3.933	862	884	912	rVV2	466867	1389924	100.00%	11.991%
17	4.167	955	957	959	rBV3	1404	751	0.05%	0.006%
18	4.183	959	962	964	rBV4	1678	994	0.07%	0.009%
19	4.373	1008	1021	1044	rVB	222371	532415	38.31%	4.593%
20	4.498	1055	1060	1063	rBV6	1626	1536	0.11%	0.013%
21	4.608	1092	1094	1098	rVB4	1940	1146	0.08%	0.010%
22	4.695	1120	1121	1127	rBV5	1231	1094	0.08%	0.009%
23	4.762	1138	1142	1144	rBV5	1999	1369	0.10%	0.012%
24	4.826	1159	1162	1163	rBV3	1177	762	0.05%	0.007%
25	4.884	1179	1180	1183	rBV3	1423	955	0.07%	0.008%
26	4.926	1191	1193	1197	rBV5	1308	1123	0.08%	0.010%
27	5.071	1219	1238	1263	rBV2	527997	1368868	98.49%	11.809%
28	5.640	1402	1415	1440	rBV	391950	783775	56.39%	6.762%
29	5.936	1496	1507	1525	rVB2	119095	238731	17.18%	2.060%
30	6.093	1544	1556	1575	rBV	303242	608264	43.76%	5.247%
31	6.453	1665	1668	1670	rBV3	2453	1310	0.09%	0.011%
32	6.514	1685	1687	1691	rBV4	1513	1139	0.08%	0.010%
33	6.550	1696	1698	1700	rBV3	1158	662	0.05%	0.006%
34	6.595	1709	1712	1716	rVB4	1575	1031	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016682.D
 Acq On : 09 Jun 2020 00:32
 Operator : SY/MD
 Sample : L2875-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.617	1716	1719	1721	rBV4	1228	959	0.07%	0.008%
36	7.006	1827	1840	1855	rBV	171691	300523	21.62%	2.593%
37	7.338	1930	1943	1963	rBV	627899	1071154	77.07%	9.241%
38	7.643	2028	2038	2056	rBV	119764	201362	14.49%	1.737%
39	7.852	2101	2103	2105	rBV2	1566	819	0.06%	0.007%
40	7.865	2105	2107	2113	rVB6	2102	1562	0.11%	0.013%
41	7.997	2146	2148	2151	rBV4	1594	904	0.07%	0.008%
42	8.106	2172	2182	2215	rBV	361559	684609	49.26%	5.906%
43	8.379	2265	2267	2270	rBV3	1600	883	0.06%	0.008%
44	8.662	2351	2355	2357	rBV4	1074	1010	0.07%	0.009%
45	8.733	2373	2377	2382	rBV7	2208	1993	0.14%	0.017%
46	8.813	2400	2402	2405	rBV4	971	754	0.05%	0.007%
47	8.829	2405	2407	2408	rVV2	1592	742	0.05%	0.006%
48	8.874	2408	2421	2444	rVV	587090	954882	68.70%	8.238%
49	9.141	2501	2504	2507	rBV5	1823	1195	0.09%	0.010%
50	9.341	2562	2566	2567	rBV3	1419	1030	0.07%	0.009%
51	9.408	2584	2587	2590	rBV5	1482	1248	0.09%	0.011%
52	9.501	2613	2616	2620	rBV6	1698	1691	0.12%	0.015%
53	9.579	2634	2640	2645	rBV8	2155	2602	0.19%	0.022%
54	9.620	2650	2653	2658	rVB6	1497	1394	0.10%	0.012%
55	9.640	2658	2659	2662	rBV3	1536	832	0.06%	0.007%
56	9.717	2681	2683	2686	rBV2	1151	653	0.05%	0.006%
57	9.807	2708	2711	2719	rBV8	1572	1914	0.14%	0.017%
58	10.013	2772	2775	2780	rVB7	1779	1504	0.11%	0.013%
59	10.138	2810	2814	2816	rBV4	1266	766	0.06%	0.007%
60	10.196	2830	2832	2834	rBV3	1488	833	0.06%	0.007%
61	10.238	2834	2845	2861	rVV	412249	639235	45.99%	5.515%
62	10.572	2945	2949	2951	rBV5	1948	1714	0.12%	0.015%
63	10.685	2980	2984	2986	rBV5	1307	911	0.07%	0.008%
64	10.807	3018	3022	3025	rVB5	1545	1396	0.10%	0.012%
65	10.826	3025	3028	3031	rBV4	1077	739	0.05%	0.006%
66	10.878	3040	3044	3047	rBV5	1744	1723	0.12%	0.015%
67	10.897	3047	3050	3052	rBV2	986	683	0.05%	0.006%
68	11.061	3099	3101	3104	rBV4	1025	663	0.05%	0.006%
69	11.270	3155	3166	3185	rBV	590835	900749	64.81%	7.771%
70	11.646	3273	3283	3300	rVB	655863	1028023	73.96%	8.869%
71	11.784	3324	3326	3330	rVB4	1933	1116	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016682.D
 Acq On : 09 Jun 2020 00:32
 Operator : SY/MD
 Sample : L2875-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.935	3371	3373	3378	rBV5	1731	1243	0.09%	0.011%
73	11.958	3378	3380	3385	rVV5	1314	948	0.07%	0.008%
74	12.164	3439	3444	3446	rBV4	1666	1603	0.12%	0.014%
75	12.267	3472	3476	3477	rBV3	1297	1053	0.08%	0.009%
76	12.302	3485	3487	3490	rBV4	1209	877	0.06%	0.008%
77	12.652	3591	3596	3597	rBV4	1886	1552	0.11%	0.013%
78	12.707	3609	3613	3616	rBV6	1484	829	0.06%	0.007%
79	12.736	3620	3622	3628	rVB6	1415	1037	0.07%	0.009%
80	12.762	3628	3630	3633	rVB3	2213	1085	0.08%	0.009%
81	12.784	3633	3637	3639	rBV4	1388	977	0.07%	0.008%
82	12.861	3658	3661	3663	rBV3	1199	747	0.05%	0.006%
83	12.951	3684	3689	3691	rBV3	1167	935	0.07%	0.008%
84	12.974	3694	3696	3699	rBV3	1033	730	0.05%	0.006%
85	13.006	3701	3706	3707	rBV4	1763	1383	0.10%	0.012%
86	13.064	3722	3724	3726	rBV3	1194	641	0.05%	0.006%
87	13.154	3746	3752	3754	rBV5	1865	1858	0.13%	0.016%
88	13.173	3754	3758	3762	rVV7	1269	1279	0.09%	0.011%
89	13.196	3762	3765	3767	rVV4	1883	947	0.07%	0.008%
90	13.234	3774	3777	3780	rBV4	1167	959	0.07%	0.008%
91	13.279	3786	3791	3792	rBV5	1344	1092	0.08%	0.009%
92	13.521	3862	3866	3868	rBV6	1536	1183	0.09%	0.010%
93	13.614	3893	3895	3899	rVB3	1775	902	0.06%	0.008%
94	13.739	3931	3934	3937	rBV4	1330	1006	0.07%	0.009%
95	13.755	3937	3939	3942	rVV2	1069	707	0.05%	0.006%
96	13.775	3942	3945	3948	rVB4	1910	1273	0.09%	0.011%
97	13.980	4006	4009	4011	rVB4	1325	670	0.05%	0.006%
98	14.029	4021	4024	4025	rBV3	1580	756	0.05%	0.007%
99	14.366	4125	4129	4131	rBV5	1338	916	0.07%	0.008%
100	14.598	4198	4201	4203	rBV3	1181	752	0.05%	0.006%


Sum of corrected areas: 11591546

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016682.D
Acq On : 09 Jun 2020 00:32
Operator : SY/MD
Sample : L2875-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

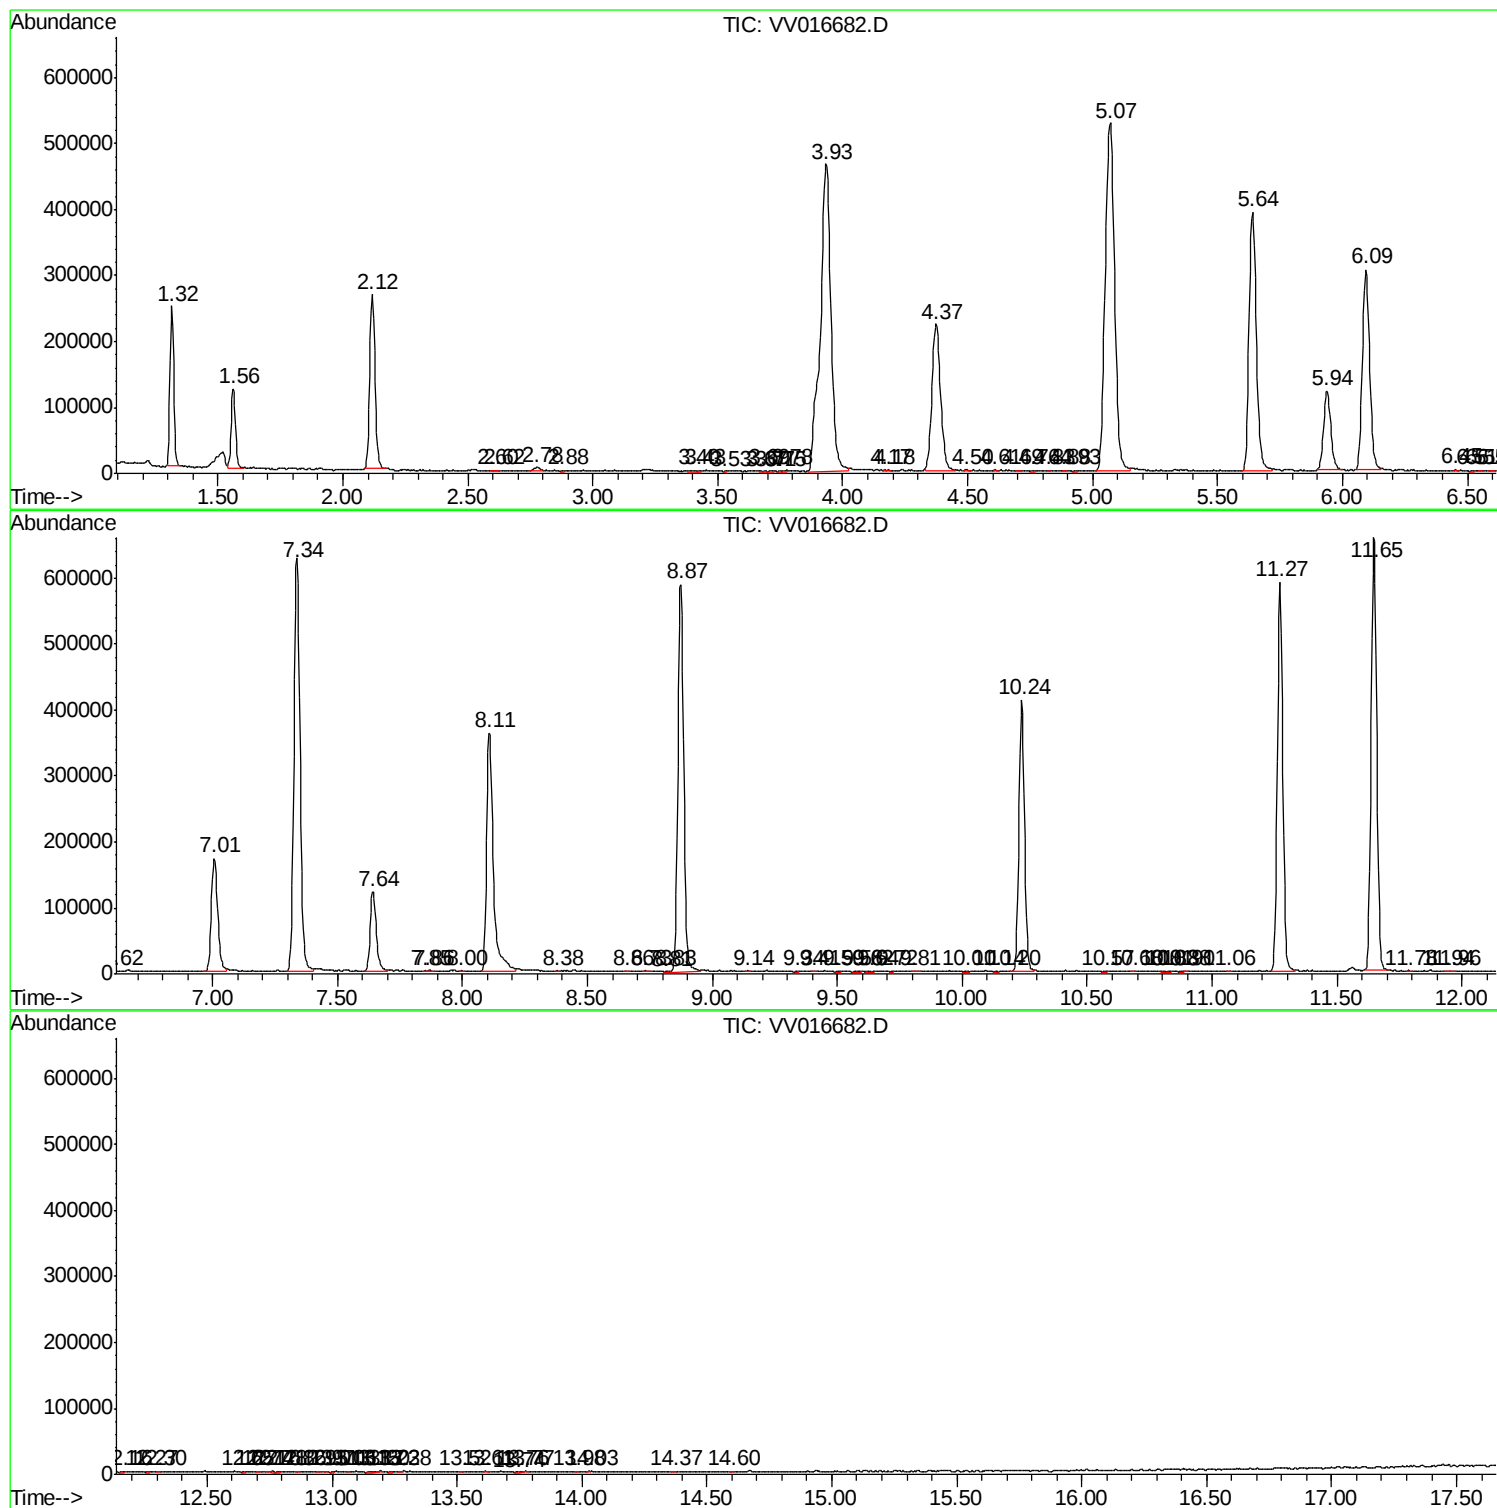

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016682.D
Acq On : 09 Jun 2020 00:32
Operator : SY/MD
Sample : L2875-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016682.D
Acq On : 09 Jun 2020 00:32
Operator : SY/MD
Sample : L2875-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc