

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016683.D
 Acq On : 09 Jun 2020 00:56
 Operator : SY/MD
 Sample : L2875-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	82	rVB	170662	177290	12.86%	1.671%
2	1.563	142	147	159	rVB	116022	134891	9.78%	1.271%
3	2.116	310	319	334	rBV	262494	384077	27.85%	3.619%
4	2.463	425	427	429	rBV3	1412	793	0.06%	0.007%
5	2.721	505	507	509	rBV3	1390	527	0.04%	0.005%
6	2.968	582	584	587	rBV3	1052	574	0.04%	0.005%
7	3.004	591	595	598	rBV5	1812	1584	0.11%	0.015%
8	3.087	619	621	623	rBV2	1262	528	0.04%	0.005%
9	3.171	645	647	652	rBV5	846	556	0.04%	0.005%
10	3.209	656	659	662	rBV4	1412	1234	0.09%	0.012%
11	3.393	711	716	720	rBV7	1085	1055	0.08%	0.010%
12	3.428	725	727	731	rBV4	1063	679	0.05%	0.006%
13	3.460	734	737	738	rBV3	1186	521	0.04%	0.005%
14	3.518	753	755	758	rVB3	973	539	0.04%	0.005%
15	3.541	759	762	766	rVV4	1211	795	0.06%	0.007%
16	3.576	770	773	775	rBV3	2110	1451	0.11%	0.014%
17	3.631	785	790	793	rBV6	1704	1226	0.09%	0.012%
18	3.669	799	802	805	rVV4	1865	1341	0.10%	0.013%
19	3.740	821	824	825	rBV3	2158	1333	0.10%	0.013%
20	3.766	829	832	834	rBV3	1259	644	0.05%	0.006%
21	3.811	843	846	849	rVB5	889	719	0.05%	0.007%
22	3.836	852	854	855	rBV2	1275	628	0.05%	0.006%
23	3.897	861	873	907	rBV	107170	307050	22.27%	2.893%
24	4.277	989	991	993	rBV3	975	518	0.04%	0.005%
25	4.325	1003	1006	1007	rBV3	2330	1375	0.10%	0.013%
26	4.373	1007	1021	1047	rVB	224100	544803	39.51%	5.134%
27	4.582	1084	1086	1087	rBV2	1372	560	0.04%	0.005%
28	4.714	1125	1127	1130	rBV4	1414	791	0.06%	0.007%
29	4.920	1186	1191	1194	rBV7	1588	1490	0.11%	0.014%
30	5.071	1219	1238	1260	rBV2	540531	1378938	100.00%	12.994%
31	5.502	1369	1372	1375	rBV3	1456	1139	0.08%	0.011%
32	5.540	1382	1384	1388	rBV5	958	566	0.04%	0.005%
33	5.640	1401	1415	1441	rBV	417979	839658	60.89%	7.912%
34	5.778	1455	1458	1461	rBV4	2083	1928	0.14%	0.018%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016683.D
 Acq On : 09 Jun 2020 00:56
 Operator : SY/MD
 Sample : L2875-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	5.936	1497	1507	1533	rVB2	158944	321399	23.31%	3.029%
36	6.093	1543	1556	1583	rBV	312160	628364	45.57%	5.921%
37	6.502	1681	1683	1686	rBV4	1320	596	0.04%	0.006%
38	6.788	1769	1772	1774	rBV3	962	623	0.05%	0.006%
39	6.946	1817	1821	1822	rBV4	1231	842	0.06%	0.008%
40	7.007	1830	1840	1854	rBV	168702	295616	21.44%	2.786%
41	7.338	1930	1943	1961	rBV	632783	1080896	78.39%	10.185%
42	7.640	2028	2037	2054	rVB2	122088	201331	14.60%	1.897%
43	8.016	2150	2154	2156	rBV4	1247	780	0.06%	0.007%
44	8.032	2156	2159	2162	rBV3	2072	1481	0.11%	0.014%
45	8.109	2173	2183	2200	rBV	346193	632054	45.84%	5.956%
46	8.582	2328	2330	2333	rBV4	1322	935	0.07%	0.009%
47	8.679	2358	2360	2361	rBV2	1119	518	0.04%	0.005%
48	8.875	2407	2421	2439	rBV	627268	1013993	73.53%	9.555%
49	9.286	2547	2549	2552	rBV4	1767	874	0.06%	0.008%
50	9.312	2552	2557	2560	rVV7	1549	1127	0.08%	0.011%
51	9.405	2583	2586	2590	rBV6	1290	1051	0.08%	0.010%
52	9.492	2610	2613	2617	rBV5	1171	1105	0.08%	0.010%
53	9.543	2626	2629	2632	rBV3	1170	729	0.05%	0.007%
54	9.688	2671	2674	2677	rBV3	1225	971	0.07%	0.009%
55	9.711	2677	2681	2685	rVV7	1799	1659	0.12%	0.016%
56	9.788	2701	2705	2708	rBV6	1314	1066	0.08%	0.010%
57	9.990	2766	2768	2772	rVB4	1650	764	0.06%	0.007%
58	10.016	2772	2776	2779	rBV5	1739	1468	0.11%	0.014%
59	10.087	2796	2798	2800	rBV2	1368	731	0.05%	0.007%
60	10.238	2832	2845	2863	rBV	408679	642467	46.59%	6.054%
61	10.402	2893	2896	2899	rBV4	2904	2154	0.16%	0.020%
62	10.460	2911	2914	2919	rBV7	1395	1481	0.11%	0.014%
63	10.624	2961	2965	2969	rVB6	1324	1120	0.08%	0.011%
64	10.650	2969	2973	2974	rBV4	1349	1060	0.08%	0.010%
65	10.659	2974	2976	2980	rVB5	2269	1390	0.10%	0.013%
66	10.685	2980	2984	2987	rVB5	882	663	0.05%	0.006%
67	10.704	2987	2990	2993	rBV4	952	906	0.07%	0.009%
68	10.839	3030	3032	3035	rBV4	1058	811	0.06%	0.008%
69	11.051	3096	3098	3099	rBV2	1117	609	0.04%	0.006%
70	11.090	3106	3110	3114	rBV6	1295	1384	0.10%	0.013%
71	11.109	3114	3116	3119	rBV4	822	581	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016683.D
 Acq On : 09 Jun 2020 00:56
 Operator : SY/MD
 Sample : L2875-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.170	3133	3135	3139	rVB3	1330	909	0.07%	0.009%
73	11.270	3155	3166	3184	rBV	604456	935424	67.84%	8.815%
74	11.486	3228	3233	3236	rBV6	2294	2086	0.15%	0.020%
75	11.514	3239	3242	3243	rBV3	1019	643	0.05%	0.006%
76	11.646	3272	3283	3301	rVB	645403	1010675	73.29%	9.524%
77	12.186	3449	3451	3454	rBV4	1151	644	0.05%	0.006%
78	12.251	3469	3471	3473	rBV3	1344	623	0.05%	0.006%
79	12.273	3476	3478	3480	rVB3	1726	785	0.06%	0.007%
80	12.312	3488	3490	3499	rBV8	1942	1984	0.14%	0.019%
81	12.476	3537	3541	3544	rBV4	923	840	0.06%	0.008%
82	12.585	3573	3575	3577	rBV3	1333	547	0.04%	0.005%
83	12.669	3597	3601	3602	rBV4	1252	728	0.05%	0.007%
84	12.820	3645	3648	3650	rVB4	1739	1046	0.08%	0.010%
85	12.987	3698	3700	3704	rBV5	1084	639	0.05%	0.006%
86	13.048	3716	3719	3722	rBV5	1598	1189	0.09%	0.011%
87	13.289	3790	3794	3798	rVB7	1901	1820	0.13%	0.017%
88	13.312	3798	3801	3805	rBV5	1651	1600	0.12%	0.015%
89	13.405	3827	3830	3833	rBV3	1457	995	0.07%	0.009%
90	13.440	3838	3841	3843	rBV3	1992	1224	0.09%	0.012%
91	13.672	3910	3913	3919	rBV6	1180	1512	0.11%	0.014%
92	13.765	3940	3942	3945	rBV4	1312	907	0.07%	0.009%
93	13.868	3972	3974	3978	rBV4	850	525	0.04%	0.005%
94	13.920	3987	3990	3991	rBV2	1579	690	0.05%	0.007%
95	14.174	4065	4069	4070	rBV4	1121	739	0.05%	0.007%
96	14.460	4154	4158	4161	rBV4	1849	1425	0.10%	0.013%
97	14.524	4176	4178	4183	rVB4	1360	850	0.06%	0.008%
98	14.849	4274	4279	4281	rBV5	2284	1759	0.13%	0.017%
99	15.482	4473	4476	4479	rBV4	1803	1375	0.10%	0.013%
100	15.659	4529	4531	4533	rBV3	1462	640	0.05%	0.006%


Sum of corrected areas: 10612223

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016683.D
Acq On : 09 Jun 2020 00:56
Operator : SY/MD
Sample : L2875-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

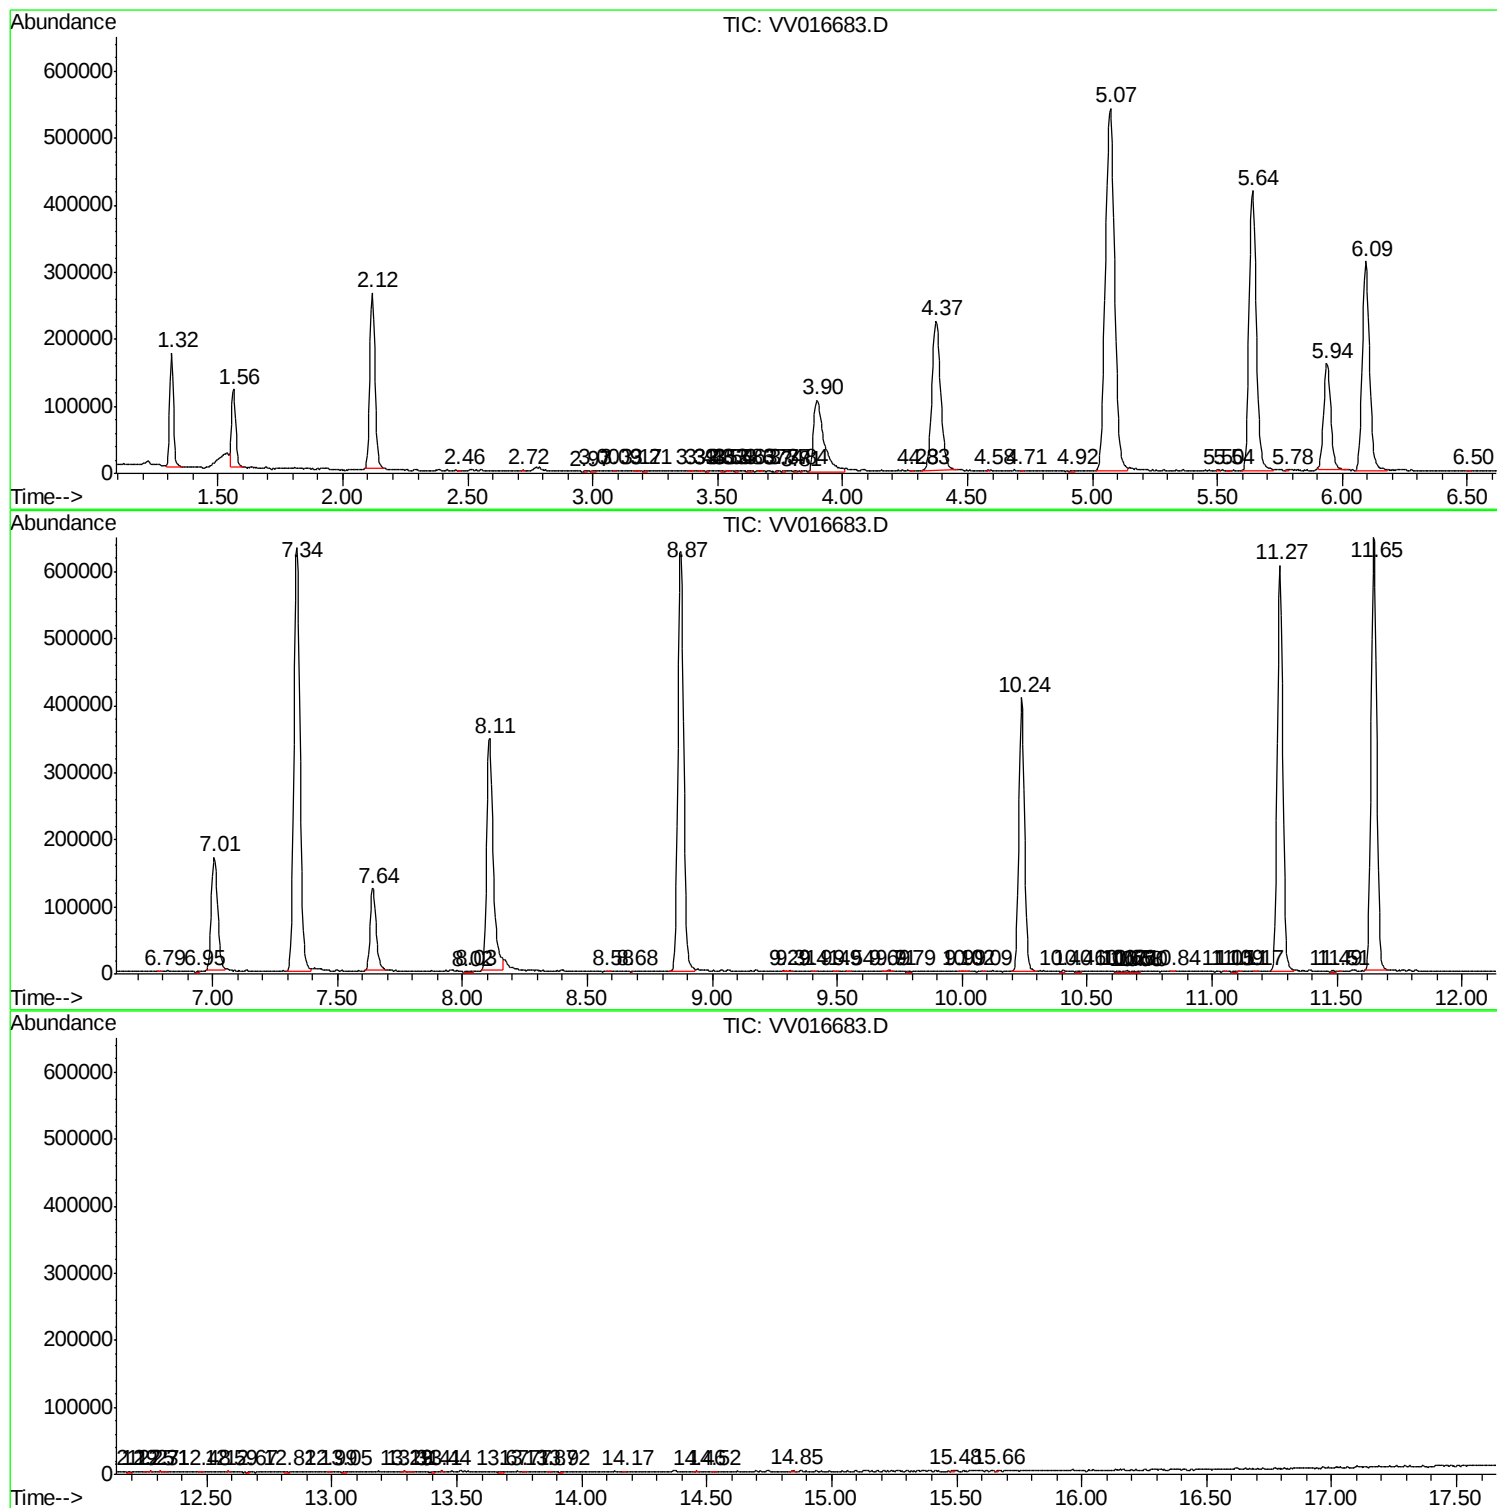

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016683.D
Acq On : 09 Jun 2020 00:56
Operator : SY/MD
Sample : L2875-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016683.D
Acq On : 09 Jun 2020 00:56
Operator : SY/MD
Sample : L2875-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc