

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016684.D
 Acq On : 09 Jun 2020 01:20
 Operator : SY/MD
 Sample : L2875-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB2	211441	222812	16.16%	2.149%
2	1.563	141	147	163	rVB	117479	137365	9.96%	1.325%
3	2.116	311	319	335	rVB	256724	380672	27.61%	3.671%
4	2.441	418	420	424	rBV5	1596	1113	0.08%	0.011%
5	2.817	536	537	542	rVB4	1467	857	0.06%	0.008%
6	3.087	616	621	622	rBV3	1141	778	0.06%	0.008%
7	3.103	624	626	630	rVB3	1256	775	0.06%	0.007%
8	3.280	678	681	684	rBV4	1115	1005	0.07%	0.010%
9	3.434	726	729	732	rBV5	1801	1021	0.07%	0.010%
10	3.524	753	757	760	rBV4	1122	914	0.07%	0.009%
11	3.621	784	787	790	rBV4	1472	1253	0.09%	0.012%
12	3.659	795	799	801	rBV3	1181	873	0.06%	0.008%
13	3.711	813	815	817	rBV2	1500	809	0.06%	0.008%
14	3.794	838	841	853	rVB2	2231	3407	0.25%	0.033%
15	3.894	862	872	905	rBV	106600	325312	23.60%	3.137%
16	4.232	974	977	981	rBV4	1507	1352	0.10%	0.013%
17	4.373	1007	1021	1045	rBV	221968	534509	38.77%	5.155%
18	4.540	1070	1073	1075	rBV3	1433	1058	0.08%	0.010%
19	4.749	1136	1138	1141	rBV4	2098	1179	0.09%	0.011%
20	4.772	1141	1145	1151	rVB8	1986	2299	0.17%	0.022%
21	4.801	1151	1154	1155	rBV4	1300	778	0.06%	0.008%
22	4.923	1188	1192	1194	rBV4	1662	1417	0.10%	0.014%
23	5.003	1212	1217	1220	rVB7	1138	888	0.06%	0.009%
24	5.071	1220	1238	1264	rBV2	536745	1378502	100.00%	13.294%
25	5.270	1298	1300	1302	rBV3	1553	805	0.06%	0.008%
26	5.296	1305	1308	1314	rVB6	2685	2455	0.18%	0.024%
27	5.328	1314	1318	1319	rBV3	1545	1182	0.09%	0.011%
28	5.544	1381	1385	1387	rBV4	1876	1204	0.09%	0.012%
29	5.640	1402	1415	1433	rBV	417903	833903	60.49%	8.042%
30	5.888	1490	1492	1494	rBV2	1640	1002	0.07%	0.010%
31	6.093	1544	1556	1573	rBV	306597	611314	44.35%	5.895%
32	6.338	1629	1632	1634	rBV4	1583	919	0.07%	0.009%
33	6.505	1680	1684	1689	rBV7	1219	1452	0.11%	0.014%
34	6.598	1709	1713	1716	rBV6	1607	1555	0.11%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016684.D
 Acq On : 09 Jun 2020 01:20
 Operator : SY/MD
 Sample : L2875-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.804	1774	1777	1782	rVB7	1716	1551	0.11%	0.015%
36	6.855	1788	1793	1795	rBV4	1470	1391	0.10%	0.013%
37	6.872	1795	1798	1801	rVV5	1278	891	0.06%	0.009%
38	7.007	1830	1840	1854	rBV	168939	296608	21.52%	2.860%
39	7.219	1904	1906	1911	rBV4	1613	1185	0.09%	0.011%
40	7.338	1931	1943	1962	rBV	618518	1074461	77.94%	10.362%
41	7.643	2025	2038	2052	rBV	119888	206948	15.01%	1.996%
42	8.000	2145	2149	2151	rVB2	2275	1273	0.09%	0.012%
43	8.016	2151	2154	2157	rBV4	1814	1068	0.08%	0.010%
44	8.106	2172	2182	2215	rBV	350331	667000	48.39%	6.432%
45	8.412	2274	2277	2281	rBV6	1598	1401	0.10%	0.014%
46	8.463	2291	2293	2300	rVB6	1746	1732	0.13%	0.017%
47	8.765	2383	2387	2392	rVB8	1597	1686	0.12%	0.016%
48	8.794	2392	2396	2399	rBV5	1161	1106	0.08%	0.011%
49	8.875	2409	2421	2442	rVV	632077	1013758	73.54%	9.776%
50	9.158	2506	2509	2513	rBV5	2047	1467	0.11%	0.014%
51	9.216	2525	2527	2531	rBV4	1100	838	0.06%	0.008%
52	9.293	2549	2551	2554	rVB5	1379	750	0.05%	0.007%
53	9.367	2569	2574	2578	rVV8	1700	1733	0.13%	0.017%
54	9.418	2588	2590	2595	rBV5	1632	1048	0.08%	0.010%
55	9.547	2626	2630	2634	rBV6	1707	1886	0.14%	0.018%
56	9.749	2690	2693	2694	rBV3	1318	728	0.05%	0.007%
57	9.810	2710	2712	2716	rBV5	1246	848	0.06%	0.008%
58	9.859	2723	2727	2730	rVB5	1353	1076	0.08%	0.010%
59	9.926	2744	2748	2752	rBV7	1300	1389	0.10%	0.013%
60	10.039	2779	2783	2787	rBV6	1163	937	0.07%	0.009%
61	10.238	2832	2845	2860	rBV	402652	631521	45.81%	6.090%
62	10.396	2890	2894	2895	rBV3	1725	1024	0.07%	0.010%
63	10.498	2921	2926	2929	rBV7	2577	2224	0.16%	0.021%
64	10.563	2944	2946	2950	rVB4	1263	930	0.07%	0.009%
65	10.592	2950	2955	2960	rBV8	1674	1765	0.13%	0.017%
66	10.643	2967	2971	2972	rBV3	1445	958	0.07%	0.009%
67	10.672	2977	2980	2985	rBV6	1341	1209	0.09%	0.012%
68	10.775	3010	3012	3015	rVB5	2031	1004	0.07%	0.010%
69	10.965	3069	3071	3075	rVB5	1999	1067	0.08%	0.010%
70	11.100	3109	3113	3114	rBV5	1208	909	0.07%	0.009%
71	11.119	3117	3119	3123	rVB5	1128	729	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016684.D
 Acq On : 09 Jun 2020 01:20
 Operator : SY/MD
 Sample : L2875-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTY3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.145	3123	3127	3129	rBV4	1594	1390	0.10%	0.013%
73	11.170	3132	3135	3139	rBV5	1249	922	0.07%	0.009%
74	11.270	3154	3166	3184	rBV	607735	944120	68.49%	9.105%
75	11.518	3240	3243	3246	rVB5	1507	882	0.06%	0.009%
76	11.547	3246	3252	3254	rBV6	2515	2544	0.18%	0.025%
77	11.646	3272	3283	3298	rBV	654414	1008940	73.19%	9.730%
78	12.045	3405	3407	3411	rBV5	1631	1042	0.08%	0.010%
79	12.132	3432	3434	3437	rBV3	1843	1225	0.09%	0.012%
80	12.309	3487	3489	3494	rBV4	2320	2219	0.16%	0.021%
81	12.344	3496	3500	3502	rBV4	1053	896	0.06%	0.009%
82	12.627	3585	3588	3591	rBV4	1658	1156	0.08%	0.011%
83	12.649	3591	3595	3598	rBV4	1404	1181	0.09%	0.011%
84	12.849	3654	3657	3661	rBV4	1370	1147	0.08%	0.011%
85	13.254	3780	3783	3785	rBV4	1618	1094	0.08%	0.011%
86	13.283	3789	3792	3797	rBV5	1424	1397	0.10%	0.013%
87	13.386	3820	3824	3825	rBV4	1578	935	0.07%	0.009%
88	13.408	3825	3831	3834	rVB5	1377	1533	0.11%	0.015%
89	13.685	3912	3917	3921	rVB6	1221	1198	0.09%	0.012%
90	13.756	3937	3939	3945	rVB6	1415	968	0.07%	0.009%
91	13.910	3985	3987	3993	rVB6	1909	1481	0.11%	0.014%
92	13.936	3993	3995	3997	rBV3	1285	750	0.05%	0.007%
93	13.997	4012	4014	4017	rVB3	1669	826	0.06%	0.008%
94	14.016	4017	4020	4022	rBV4	1450	777	0.06%	0.007%
95	14.080	4038	4040	4044	rBV4	1438	1117	0.08%	0.011%
96	14.199	4075	4077	4079	rBV3	1469	795	0.06%	0.008%
97	14.337	4118	4120	4126	rBV6	1288	1102	0.08%	0.011%
98	14.556	4186	4188	4190	rBV3	1353	865	0.06%	0.008%
99	15.463	4467	4470	4471	rBV3	2390	1323	0.10%	0.013%
100	15.736	4553	4555	4558	rBV4	1629	936	0.07%	0.009%


Sum of corrected areas: 10369599

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016684.D
Acq On : 09 Jun 2020 01:20
Operator : SY/MD
Sample : L2875-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

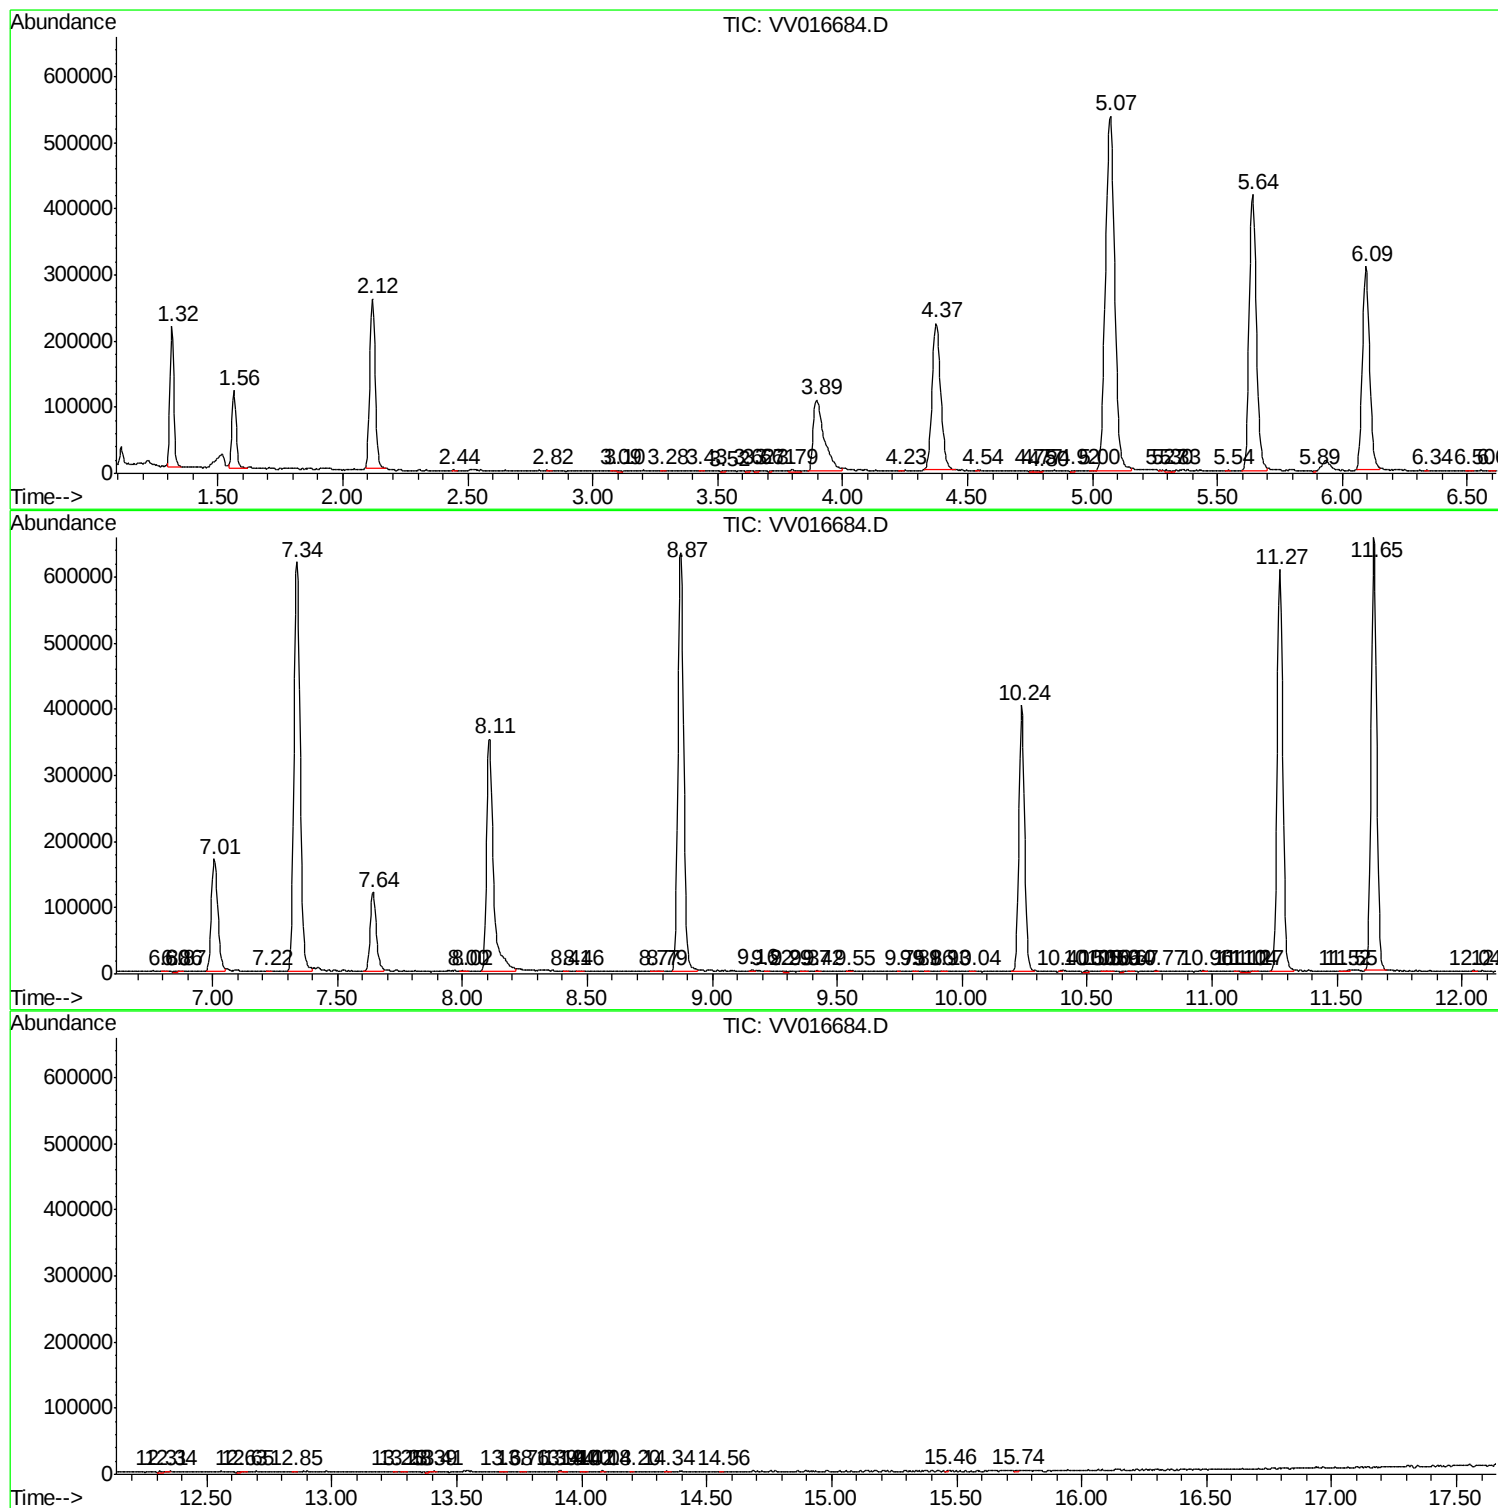

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016684.D
Acq On : 09 Jun 2020 01:20
Operator : SY/MD
Sample : L2875-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016684.D
Acq On : 09 Jun 2020 01:20
Operator : SY/MD
Sample : L2875-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTY3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc