

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016685.D
 Acq On : 09 Jun 2020 01:44
 Operator : SY/MD
 Sample : L2895-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETW41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	79	rVB	168502	175328	12.34%	1.655%
2	1.563	141	147	157	rVB	117033	138401	9.74%	1.306%
3	2.119	310	320	336	rBV	266651	396861	27.93%	3.745%
4	2.438	416	419	421	rBV4	1537	979	0.07%	0.009%
5	2.573	458	461	464	rBV4	1854	1091	0.08%	0.010%
6	2.772	519	523	526	rBV6	1957	1491	0.10%	0.014%
7	2.894	555	561	565	rBV10	1234	1818	0.13%	0.017%
8	3.042	598	607	610	rBV10	1172	1108	0.08%	0.010%
9	3.065	611	614	616	rBV4	1589	1040	0.07%	0.010%
10	3.193	652	654	661	rVB7	2211	2066	0.15%	0.019%
11	3.293	681	685	688	rBV5	1716	1452	0.10%	0.014%
12	3.315	690	692	695	rVV3	1687	972	0.07%	0.009%
13	3.338	695	699	702	rVB5	2285	1711	0.12%	0.016%
14	3.412	719	722	723	rBV3	1499	780	0.05%	0.007%
15	3.544	759	763	765	rBV4	1194	987	0.07%	0.009%
16	3.685	803	807	808	rBV2	1095	807	0.06%	0.008%
17	3.743	823	825	831	rVB5	1033	809	0.06%	0.008%
18	3.820	846	849	854	rVB7	1391	1437	0.10%	0.014%
19	3.846	854	857	861	rBV5	1609	1384	0.10%	0.013%
20	3.897	861	873	895	rBV	109749	293933	20.68%	2.774%
21	4.200	964	967	968	rBV3	1290	813	0.06%	0.008%
22	4.219	971	973	977	rBV4	1678	1033	0.07%	0.010%
23	4.373	1004	1021	1044	rBV	237738	602175	42.37%	5.683%
24	4.601	1088	1092	1094	rBV4	1498	1233	0.09%	0.012%
25	4.856	1169	1171	1175	rVB5	2112	1302	0.09%	0.012%
26	4.894	1179	1183	1185	rVB3	1550	1094	0.08%	0.010%
27	5.071	1220	1238	1259	rBV2	559690	1421160	100.00%	13.411%
28	5.492	1365	1369	1374	rVV8	1639	1957	0.14%	0.018%
29	5.556	1383	1389	1392	rBV6	1864	2285	0.16%	0.022%
30	5.640	1403	1415	1433	rBV	412177	812286	57.16%	7.665%
31	5.926	1491	1504	1518	rBV9	12544	30248	2.13%	0.285%
32	6.093	1539	1556	1582	rBV	323439	660523	46.48%	6.233%
33	6.328	1627	1629	1631	rVB3	1925	809	0.06%	0.008%
34	6.357	1631	1638	1642	rBV10	2099	2879	0.20%	0.027%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016685.D
 Acq On : 09 Jun 2020 01:44
 Operator : SY/MD
 Sample : L2895-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETW41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.450	1662	1667	1668	rBV4	1348	1073	0.08%	0.010%
36	6.486	1674	1678	1679	rBV3	1471	1015	0.07%	0.010%
37	6.540	1689	1695	1697	rBV7	2293	2419	0.17%	0.023%
38	6.653	1724	1730	1733	rBV7	1867	1718	0.12%	0.016%
39	6.717	1748	1750	1754	rBV5	1322	1138	0.08%	0.011%
40	7.007	1827	1840	1858	rVV	175629	314105	22.10%	2.964%
41	7.193	1894	1898	1901	rVB6	1361	1007	0.07%	0.010%
42	7.338	1929	1943	1961	rBV	653549	1121368	78.91%	10.582%
43	7.643	2028	2038	2053	rBV	123982	210063	14.78%	1.982%
44	7.814	2089	2091	2097	rVB5	1961	1534	0.11%	0.014%
45	7.843	2097	2100	2104	rBV5	1923	1243	0.09%	0.012%
46	7.913	2117	2122	2123	rBV4	1502	916	0.06%	0.009%
47	8.109	2172	2183	2218	rBV	361332	693126	48.77%	6.541%
48	8.531	2311	2314	2317	rBV4	1832	1309	0.09%	0.012%
49	8.691	2361	2364	2370	rVB6	1601	1495	0.11%	0.014%
50	8.724	2370	2374	2377	rBV6	929	886	0.06%	0.008%
51	8.833	2403	2408	2409	rBV4	1289	1128	0.08%	0.011%
52	8.875	2410	2421	2438	rVV	616309	990475	69.69%	9.347%
53	9.215	2525	2527	2532	rVB5	1463	1233	0.09%	0.012%
54	9.328	2557	2562	2564	rBV5	1574	1252	0.09%	0.012%
55	9.453	2598	2601	2603	rBV4	1128	745	0.05%	0.007%
56	9.576	2637	2639	2644	rVB4	1785	1163	0.08%	0.011%
57	9.868	2727	2730	2732	rBV3	1328	842	0.06%	0.008%
58	9.900	2736	2740	2744	rBV7	1629	1712	0.12%	0.016%
59	9.971	2759	2762	2763	rBV3	1376	905	0.06%	0.009%
60	10.074	2792	2794	2798	rVB4	1284	770	0.05%	0.007%
61	10.238	2832	2845	2858	rBV	423866	660759	46.49%	6.236%
62	10.444	2905	2909	2912	rBV4	1325	1084	0.08%	0.010%
63	10.469	2914	2917	2920	rVB	7707	4412	0.31%	0.042%
64	10.492	2920	2924	2926	rBV3	1807	1427	0.10%	0.013%
65	10.868	3039	3041	3044	rBV3	1647	1030	0.07%	0.010%
66	10.939	3058	3063	3065	rBV6	1340	1365	0.10%	0.013%
67	11.016	3084	3087	3091	rBV5	1038	876	0.06%	0.008%
68	11.174	3131	3136	3139	rVB7	1228	1013	0.07%	0.010%
69	11.199	3140	3144	3147	rBV5	1924	1481	0.10%	0.014%
70	11.270	3154	3166	3185	rBV	613476	919211	64.68%	8.675%
71	11.466	3225	3227	3232	rVB5	1745	1289	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016685.D
 Acq On : 09 Jun 2020 01:44
 Operator : SY/MD
 Sample : L2895-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETW41

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.502	3233	3238	3240	rVV5	1387	1064	0.07%	0.010%
73	11.646	3272	3283	3301	rBV	676240	1051787	74.01%	9.926%
74	11.794	3326	3329	3330	rBV3	1521	870	0.06%	0.008%
75	11.897	3356	3361	3364	rBV7	1368	1420	0.10%	0.013%
76	12.257	3470	3473	3477	rVB5	1318	1117	0.08%	0.011%
77	12.283	3477	3481	3484	rBV5	1461	1262	0.09%	0.012%
78	12.595	3576	3578	3582	rBV4	1035	939	0.07%	0.009%
79	12.723	3614	3618	3622	rBV6	1290	1115	0.08%	0.011%
80	12.823	3646	3649	3654	rVB6	1470	1145	0.08%	0.011%
81	12.858	3656	3660	3662	rBV5	1261	1059	0.07%	0.010%
82	12.897	3670	3672	3674	rBV3	1323	831	0.06%	0.008%
83	13.251	3778	3782	3784	rBV4	1259	926	0.07%	0.009%
84	13.411	3829	3832	3834	rBV4	1425	796	0.06%	0.008%
85	13.482	3850	3854	3857	rBV4	1156	1082	0.08%	0.010%
86	13.537	3866	3871	3876	rBV8	2045	2576	0.18%	0.024%
87	13.575	3882	3883	3889	rVB5	1434	964	0.07%	0.009%
88	13.617	3893	3896	3899	rBV4	1263	970	0.07%	0.009%
89	13.701	3920	3922	3924	rVB3	1878	768	0.05%	0.007%
90	13.807	3953	3955	3960	rVB4	1234	832	0.06%	0.008%
91	13.858	3966	3971	3975	rBV8	1164	1369	0.10%	0.013%
92	13.952	3997	4000	4003	rVB3	1439	1011	0.07%	0.010%
93	13.993	4007	4013	4016	rBV8	2136	1537	0.11%	0.015%
94	14.032	4023	4025	4027	rBV3	1322	813	0.06%	0.008%
95	14.071	4035	4037	4042	rVB6	1594	1051	0.07%	0.010%
96	14.222	4081	4084	4086	rBV3	1723	988	0.07%	0.009%
97	14.424	4145	4147	4152	rVB4	949	758	0.05%	0.007%
98	14.672	4219	4224	4228	rVB7	1773	1527	0.11%	0.014%
99	15.054	4338	4343	4346	rBV5	1648	1642	0.12%	0.015%
100	15.456	4465	4468	4471	rBV4	2576	1604	0.11%	0.015%


Sum of corrected areas: 10596662

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016685.D
Acq On : 09 Jun 2020 01:44
Operator : SY/MD
Sample : L2895-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETW41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

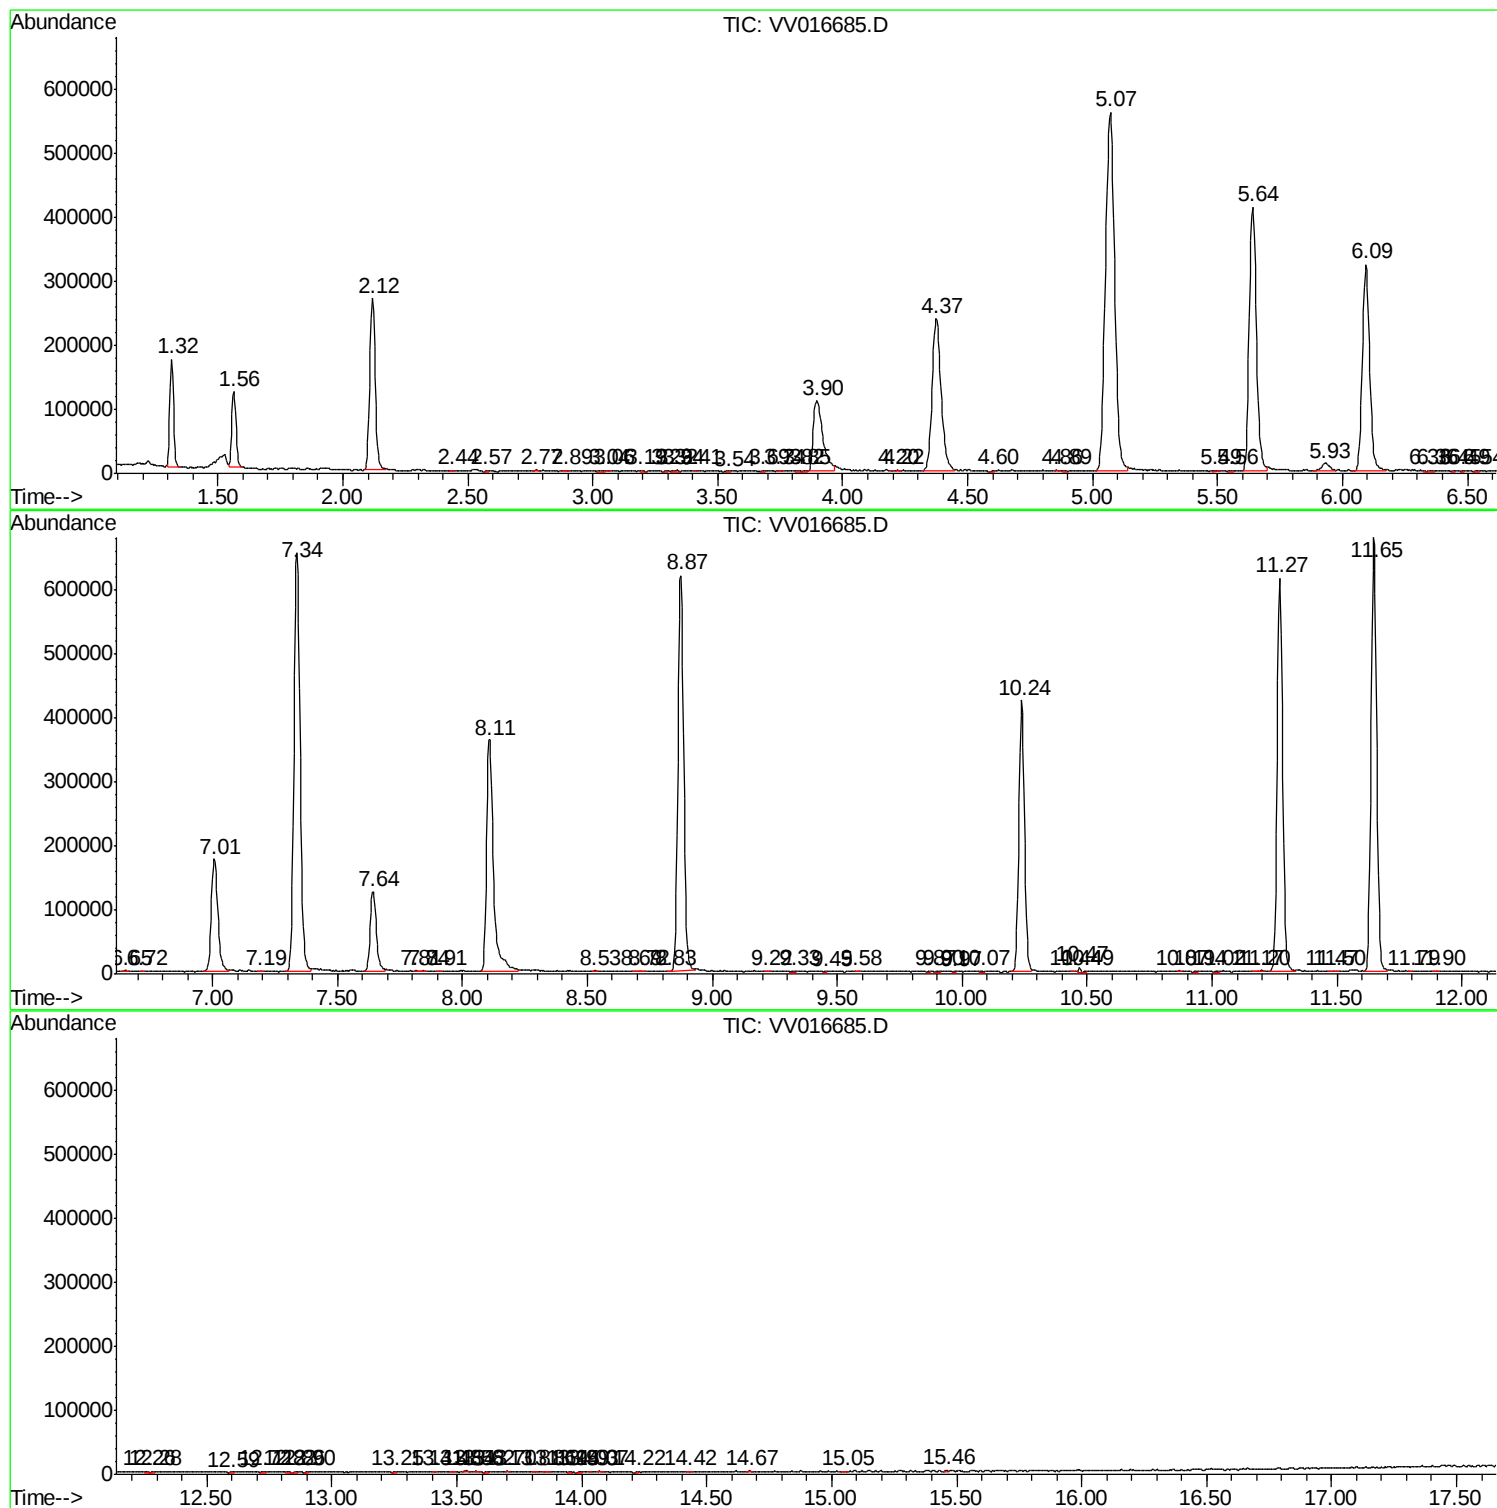

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016685.D
Acq On : 09 Jun 2020 01:44
Operator : SY/MD
Sample : L2895-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETW41

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016685.D
Acq On : 09 Jun 2020 01:44
Operator : SY/MD
Sample : L2895-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETW41

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc