

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016686.D
 Acq On : 09 Jun 2020 02:07
 Operator : SY/MD
 Sample : L2895-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0G8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	183800	195145	13.46%	1.846%
2	1.563	143	147	159	rVB	121020	133398	9.20%	1.262%
3	2.119	310	320	334	rBV	270301	402033	27.73%	3.802%
4	2.463	425	427	429	rVB3	1427	693	0.05%	0.007%
5	2.634	473	480	483	rBV9	2001	2734	0.19%	0.026%
6	2.656	485	487	491	rVB3	2275	1280	0.09%	0.012%
7	2.682	491	495	497	rBV4	1213	915	0.06%	0.009%
8	2.775	517	524	526	rBV6	2996	2694	0.19%	0.025%
9	3.042	604	607	609	rVV4	1303	919	0.06%	0.009%
10	3.129	630	634	637	rBV3	942	862	0.06%	0.008%
11	3.145	637	639	642	rVV4	1454	737	0.05%	0.007%
12	3.187	650	652	654	rBV3	1532	818	0.06%	0.008%
13	3.212	654	660	662	rVV6	1859	1332	0.09%	0.013%
14	3.290	680	684	687	rBV5	2010	1665	0.11%	0.016%
15	3.335	693	698	700	rBV5	1139	896	0.06%	0.008%
16	3.386	711	714	720	rVB7	1788	1959	0.14%	0.019%
17	3.434	725	729	731	rVV4	1430	968	0.07%	0.009%
18	3.521	752	756	759	rBV6	2181	1717	0.12%	0.016%
19	3.733	820	822	826	rBV4	1338	958	0.07%	0.009%
20	3.814	846	847	851	rBV3	1091	744	0.05%	0.007%
21	3.901	862	874	877	rBV	122182	213441	14.72%	2.019%
22	4.142	947	949	951	rBV3	1647	821	0.06%	0.008%
23	4.373	1008	1021	1041	rVB	233025	559639	38.60%	5.293%
24	4.679	1112	1116	1122	rBV9	1871	2408	0.17%	0.023%
25	4.846	1166	1168	1172	rVV4	2171	1324	0.09%	0.013%
26	5.010	1215	1219	1220	rBV3	1163	710	0.05%	0.007%
27	5.071	1220	1238	1263	rVV2	562260	1449870	100.00%	13.712%
28	5.640	1402	1415	1439	rBV	424294	841880	58.07%	7.962%
29	6.093	1542	1556	1574	rBV	325381	655875	45.24%	6.203%
30	6.489	1675	1679	1686	rVB9	2361	2710	0.19%	0.026%
31	6.527	1689	1691	1695	rBV4	1446	1097	0.08%	0.010%
32	6.582	1704	1708	1710	rBV4	1229	1013	0.07%	0.010%
33	6.605	1710	1715	1719	rVV6	1620	1532	0.11%	0.014%
34	6.643	1723	1727	1728	rBV4	2221	1757	0.12%	0.017%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016686.D
 Acq On : 09 Jun 2020 02:07
 Operator : SY/MD
 Sample : L2895-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0G8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.691	1740	1742	1745	rBV4	1815	995	0.07%	0.009%
36	6.798	1770	1775	1777	rBV4	1638	1093	0.08%	0.010%
37	7.007	1829	1840	1859	rBV	180518	319775	22.06%	3.024%
38	7.251	1913	1916	1919	rBV4	1441	882	0.06%	0.008%
39	7.338	1930	1943	1965	rBV	665477	1144069	78.91%	10.820%
40	7.640	2027	2037	2055	rBV	126399	220025	15.18%	2.081%
41	7.849	2098	2102	2103	rBV4	1153	869	0.06%	0.008%
42	7.997	2146	2148	2152	rVB4	1283	789	0.05%	0.007%
43	8.019	2152	2155	2160	rBV7	1636	1179	0.08%	0.011%
44	8.109	2172	2183	2212	rBV	371666	695974	48.00%	6.582%
45	8.486	2298	2300	2305	rVB4	1228	857	0.06%	0.008%
46	8.595	2332	2334	2337	rVB4	1863	722	0.05%	0.007%
47	8.653	2350	2352	2358	rVB6	2363	2019	0.14%	0.019%
48	8.685	2358	2362	2363	rBV2	1639	1059	0.07%	0.010%
49	8.698	2363	2366	2371	rBV7	1497	1492	0.10%	0.014%
50	8.756	2382	2384	2387	rBV4	1552	1043	0.07%	0.010%
51	8.875	2409	2421	2438	rBV	629608	1014793	69.99%	9.598%
52	9.161	2506	2510	2512	rBV5	1629	1652	0.11%	0.016%
53	9.190	2517	2519	2522	rVV4	1739	976	0.07%	0.009%
54	9.437	2593	2596	2597	rBV3	1265	679	0.05%	0.006%
55	9.627	2652	2655	2659	rBV5	1408	1103	0.08%	0.010%
56	9.656	2662	2664	2670	rVB6	2306	1753	0.12%	0.017%
57	9.685	2670	2673	2676	rBV4	1370	854	0.06%	0.008%
58	9.772	2698	2700	2705	rBV5	1259	1022	0.07%	0.010%
59	10.238	2834	2845	2862	rVV	417083	656268	45.26%	6.207%
60	10.331	2871	2874	2878	rBV4	1658	1178	0.08%	0.011%
61	10.350	2878	2880	2883	rBV4	1379	788	0.05%	0.007%
62	10.444	2904	2909	2910	rBV4	1422	990	0.07%	0.009%
63	10.498	2925	2926	2932	rVB4	1215	766	0.05%	0.007%
64	10.579	2948	2951	2953	rVB4	1950	1150	0.08%	0.011%
65	10.598	2956	2957	2962	rVV5	958	712	0.05%	0.007%
66	10.659	2968	2976	2979	rBV8	1886	2322	0.16%	0.022%
67	10.977	3070	3075	3078	rBV6	2072	1850	0.13%	0.017%
68	11.000	3080	3082	3085	rVV3	1525	837	0.06%	0.008%
69	11.016	3085	3087	3092	rVV5	1378	863	0.06%	0.008%
70	11.039	3092	3094	3097	rVB3	1644	990	0.07%	0.009%
71	11.231	3149	3154	3155	rBV4	1382	1243	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016686.D
 Acq On : 09 Jun 2020 02:07
 Operator : SY/MD
 Sample : L2895-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0G8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.270	3155	3166	3191	rVB	593837	930956	64.21%	8.805%
73	11.447	3218	3221	3225	rBV5	1264	840	0.06%	0.008%
74	11.482	3229	3232	3236	rVB4	1182	878	0.06%	0.008%
75	11.646	3272	3283	3299	rBV	669860	1039124	71.67%	9.828%
76	11.820	3332	3337	3341	rBV7	1869	2098	0.14%	0.020%
77	11.858	3347	3349	3354	rVB5	2462	1247	0.09%	0.012%
78	11.910	3362	3365	3367	rBV3	1696	1150	0.08%	0.011%
79	12.129	3429	3433	3436	rBV5	1390	1255	0.09%	0.012%
80	12.476	3537	3541	3542	rBV4	1270	946	0.07%	0.009%
81	12.543	3559	3562	3567	rBV7	1169	1234	0.09%	0.012%
82	12.813	3643	3646	3650	rVB4	2006	1515	0.10%	0.014%
83	12.836	3650	3653	3654	rBV3	1295	757	0.05%	0.007%
84	12.942	3680	3686	3691	rVB10	1787	2301	0.16%	0.022%
85	13.055	3719	3721	3726	rBV5	1242	899	0.06%	0.009%
86	13.399	3825	3828	3829	rBV3	1240	682	0.05%	0.006%
87	13.617	3892	3896	3899	rBV6	1576	1068	0.07%	0.010%
88	13.694	3916	3920	3921	rBV2	1261	875	0.06%	0.008%
89	13.707	3921	3924	3926	rBV4	1900	1141	0.08%	0.011%
90	13.878	3972	3977	3978	rBV4	1557	837	0.06%	0.008%
91	13.900	3982	3984	3987	rVV4	1849	814	0.06%	0.008%
92	13.974	4003	4007	4010	rBV5	1322	1134	0.08%	0.011%
93	14.087	4039	4042	4046	rBV4	1592	1376	0.09%	0.013%
94	14.177	4067	4070	4072	rBV4	1893	878	0.06%	0.008%
95	14.305	4107	4110	4115	rBV6	1114	1032	0.07%	0.010%
96	14.440	4149	4152	4154	rBV3	1453	1032	0.07%	0.010%
97	14.698	4230	4232	4237	rBV6	1361	1070	0.07%	0.010%
98	14.826	4270	4272	4275	rBV3	1810	907	0.06%	0.009%
99	15.106	4356	4359	4360	rBV2	2366	1074	0.07%	0.010%
100	16.019	4641	4643	4649	rBV6	1948	2138	0.15%	0.020%


Sum of corrected areas: 10573433

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016686.D
Acq On : 09 Jun 2020 02:07
Operator : SY/MD
Sample : L2895-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0G8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

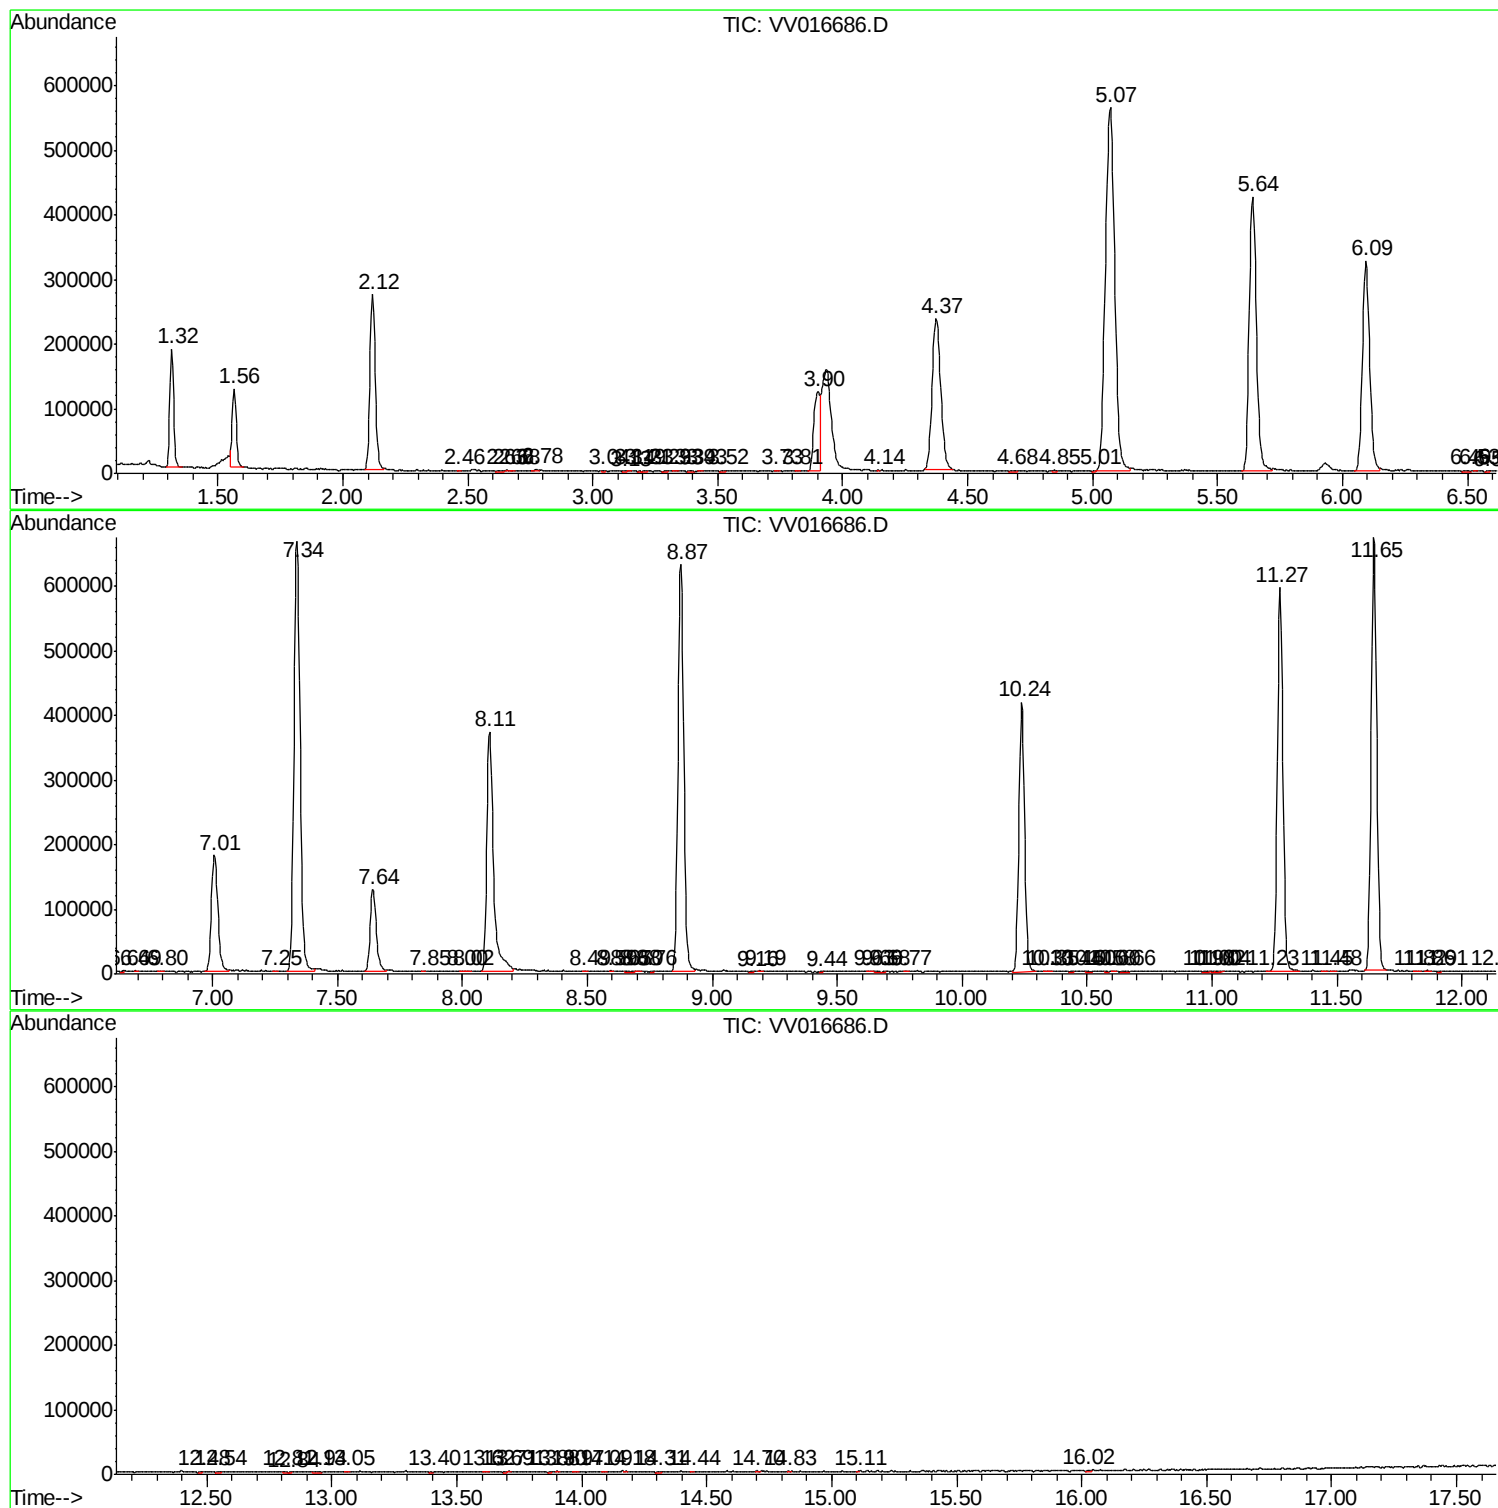

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016686.D
Acq On : 09 Jun 2020 02:07
Operator : SY/MD
Sample : L2895-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0G8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016686.D
Acq On : 09 Jun 2020 02:07
Operator : SY/MD
Sample : L2895-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0G8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc