

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016688.D
 Acq On : 09 Jun 2020 02:55
 Operator : SY/MD
 Sample : L2895-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	82	rVB2	296772	325378	17.22%	2.483%
2	1.566	143	148	165	rVB	121405	141976	7.51%	1.083%
3	2.119	311	320	339	rVB	270259	408376	21.61%	3.116%
4	2.637	477	481	482	rBV4	1956	1331	0.07%	0.010%
5	2.971	582	585	586	rBV3	948	666	0.04%	0.005%
6	2.981	586	588	592	rVB5	1848	1125	0.06%	0.009%
7	3.000	592	594	596	rBV3	1453	664	0.04%	0.005%
8	3.148	632	640	641	rBV6	2431	2552	0.14%	0.019%
9	3.206	651	658	660	rBV6	4638	5475	0.29%	0.042%
10	3.309	686	690	693	rVB5	1155	675	0.04%	0.005%
11	3.335	695	698	701	rBV5	1066	785	0.04%	0.006%
12	3.444	728	732	735	rBV3	1596	1443	0.08%	0.011%
13	3.505	749	751	752	rBV2	1376	755	0.04%	0.006%
14	3.524	755	757	760	rVB4	1028	692	0.04%	0.005%
15	3.566	768	770	775	rBV4	1340	1235	0.07%	0.009%
16	3.820	846	849	851	rBV3	1170	795	0.04%	0.006%
17	3.936	862	885	913	rBV2	673536	1889612	100.00%	14.419%
18	4.373	1008	1021	1040	rVV2	230268	553847	29.31%	4.226%
19	4.572	1081	1083	1088	rBV5	1107	777	0.04%	0.006%
20	4.756	1136	1140	1142	rBV5	2103	1533	0.08%	0.012%
21	4.888	1177	1181	1186	rVB8	1598	1357	0.07%	0.010%
22	4.965	1201	1205	1208	rVB5	1301	994	0.05%	0.008%
23	5.071	1220	1238	1264	rBV2	554459	1434320	75.91%	10.945%
24	5.373	1331	1332	1334	rBV2	1565	751	0.04%	0.006%
25	5.498	1368	1371	1372	rBV2	1249	644	0.03%	0.005%
26	5.640	1402	1415	1444	rBV	423365	834164	44.14%	6.365%
27	5.939	1494	1508	1524	rBV5	63277	140342	7.43%	1.071%
28	6.093	1544	1556	1576	rVB	321421	641411	33.94%	4.894%
29	6.296	1617	1619	1621	rBV3	2144	1097	0.06%	0.008%
30	6.344	1631	1634	1638	rBV4	1551	1233	0.07%	0.009%
31	6.463	1668	1671	1672	rBV3	1151	703	0.04%	0.005%
32	6.582	1705	1708	1711	rVB3	1521	806	0.04%	0.006%
33	6.675	1735	1737	1740	rVB3	2156	1027	0.05%	0.008%
34	6.727	1750	1753	1756	rBV4	1675	1084	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016688.D
 Acq On : 09 Jun 2020 02:55
 Operator : SY/MD
 Sample : L2895-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.807	1776	1778	1780	rBV2	1455	787	0.04%	0.006%
36	6.839	1786	1788	1791	rVB3	1445	684	0.04%	0.005%
37	7.006	1830	1840	1858	rBV	179173	308589	16.33%	2.355%
38	7.254	1915	1917	1919	rBV3	1694	812	0.04%	0.006%
39	7.286	1925	1927	1930	rBV4	1329	820	0.04%	0.006%
40	7.338	1930	1943	1959	rBV	648552	1119400	59.24%	8.542%
41	7.640	2028	2037	2053	rBV	122963	209666	11.10%	1.600%
42	7.997	2136	2148	2166	rVV	415448	691712	36.61%	5.278%
43	8.109	2173	2183	2217	rBV	365267	677969	35.88%	5.173%
44	8.740	2375	2379	2383	rBV6	1646	1653	0.09%	0.013%
45	8.810	2399	2401	2404	rBV3	1286	973	0.05%	0.007%
46	8.875	2409	2421	2441	rBV	622532	1011980	53.55%	7.722%
47	9.112	2492	2495	2499	rVB5	1901	1494	0.08%	0.011%
48	9.215	2524	2527	2530	rBV4	1829	1210	0.06%	0.009%
49	9.299	2550	2553	2555	rBV5	1022	664	0.04%	0.005%
50	9.331	2561	2563	2565	rBV3	1243	650	0.03%	0.005%
51	9.437	2593	2596	2603	rBV7	1856	1910	0.10%	0.015%
52	9.534	2623	2626	2628	rBV3	1199	836	0.04%	0.006%
53	9.675	2666	2670	2671	rVV4	1294	670	0.04%	0.005%
54	9.784	2701	2704	2706	rBV4	1450	866	0.05%	0.007%
55	9.833	2716	2719	2721	rBV3	1454	937	0.05%	0.007%
56	9.948	2752	2755	2757	rVB3	1775	922	0.05%	0.007%
57	9.965	2757	2760	2761	rBV3	1138	779	0.04%	0.006%
58	10.151	2814	2818	2824	rBV8	2049	1849	0.10%	0.014%
59	10.238	2834	2845	2858	rBV	421562	652396	34.53%	4.978%
60	10.466	2914	2916	2922	rBV6	1060	1137	0.06%	0.009%
61	10.511	2927	2930	2934	rBV4	1503	1433	0.08%	0.011%
62	10.534	2934	2937	2938	rBV3	1800	976	0.05%	0.007%
63	10.608	2957	2960	2963	rBV4	1860	1160	0.06%	0.009%
64	10.810	3021	3023	3026	rBV4	1165	770	0.04%	0.006%
65	10.842	3031	3033	3036	rBV4	1368	1046	0.06%	0.008%
66	10.887	3043	3047	3053	rVB8	2425	1979	0.10%	0.015%
67	10.919	3053	3057	3058	rBV3	1274	833	0.04%	0.006%
68	11.013	3084	3086	3088	rBV3	1244	655	0.03%	0.005%
69	11.148	3123	3128	3130	rBV5	1403	1220	0.06%	0.009%
70	11.270	3153	3166	3184	rBV	601565	935806	49.52%	7.141%
71	11.646	3272	3283	3299	rVB	660598	1032414	54.64%	7.878%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016688.D
 Acq On : 09 Jun 2020 02:55
 Operator : SY/MD
 Sample : L2895-20
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0M2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.800	3327	3331	3333	rBV3	1513	1188	0.06%	0.009%
73	11.871	3349	3353	3355	rBV4	1671	1327	0.07%	0.010%
74	11.910	3362	3365	3369	rBV5	1184	959	0.05%	0.007%
75	11.971	3382	3384	3392	rVB9	2073	1916	0.10%	0.015%
76	12.003	3392	3394	3399	rBV5	1123	851	0.05%	0.006%
77	12.119	3428	3430	3438	rVB7	1302	1322	0.07%	0.010%
78	12.177	3445	3448	3453	rBV5	1912	1974	0.10%	0.015%
79	12.260	3471	3474	3476	rBV2	1240	729	0.04%	0.006%
80	12.591	3574	3577	3582	rBV6	1484	1265	0.07%	0.010%
81	12.685	3603	3606	3608	rBV4	1228	952	0.05%	0.007%
82	12.765	3626	3631	3634	rBV6	2442	1763	0.09%	0.013%
83	12.788	3636	3638	3641	rVV4	1193	727	0.04%	0.006%
84	12.810	3643	3645	3650	rVB5	2502	1668	0.09%	0.013%
85	12.836	3650	3653	3656	rBV3	1914	1304	0.07%	0.010%
86	13.215	3766	3771	3776	rVB9	1631	1989	0.11%	0.015%
87	13.244	3776	3780	3781	rBV3	1328	759	0.04%	0.006%
88	13.283	3789	3792	3794	rBV3	2339	1382	0.07%	0.011%
89	13.386	3820	3824	3828	rBV6	1433	1280	0.07%	0.010%
90	13.411	3830	3832	3834	rBV3	1484	721	0.04%	0.006%
91	13.456	3841	3846	3850	rVB6	2101	2204	0.12%	0.017%
92	13.572	3880	3882	3885	rVB4	1343	760	0.04%	0.006%
93	13.595	3885	3889	3890	rBV4	1301	815	0.04%	0.006%
94	13.649	3903	3906	3908	rBV4	1522	857	0.05%	0.007%
95	13.694	3917	3920	3923	rBV5	1765	1178	0.06%	0.009%
96	14.353	4123	4125	4128	rBV4	1351	802	0.04%	0.006%
97	14.472	4159	4162	4163	rBV2	1368	729	0.04%	0.006%
98	14.910	4295	4298	4302	rBV4	1616	1017	0.05%	0.008%
99	15.042	4337	4339	4341	rBV3	1121	701	0.04%	0.005%
100	15.517	4483	4487	4490	rBV6	2598	2311	0.12%	0.018%


Sum of corrected areas: 13104732

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016688.D
Acq On : 09 Jun 2020 02:55
Operator : SY/MD
Sample : L2895-20
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0M2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

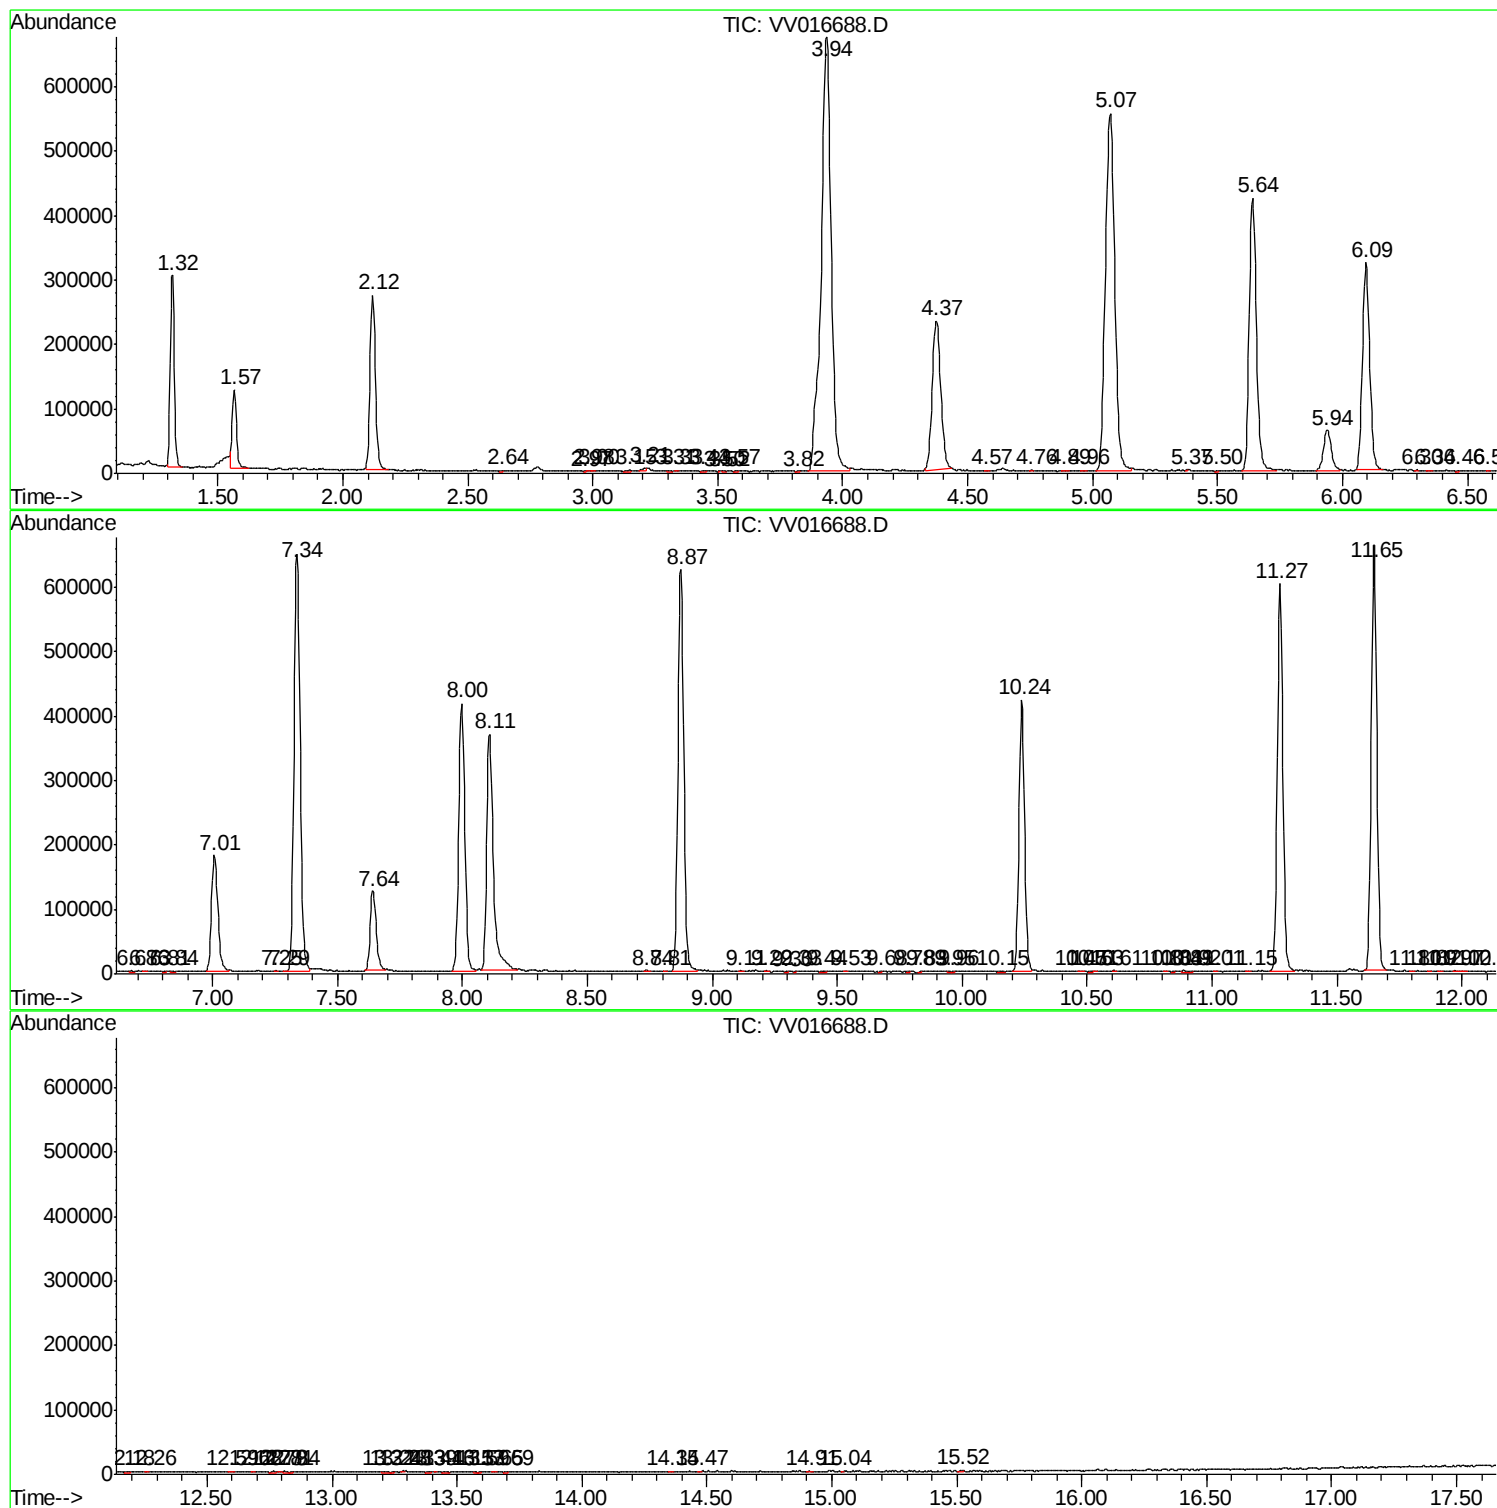

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016688.D
Acq On : 09 Jun 2020 02:55
Operator : SY/MD
Sample : L2895-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0M2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016688.D
Acq On : 09 Jun 2020 02:55
Operator : SY/MD
Sample : L2895-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0M2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc