

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016689.D
 Acq On : 09 Jun 2020 03:18
 Operator : SY/MD
 Sample : L2895-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0LO

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	79	rVB	158437	162869	12.17%	1.615%
2	1.560	139	146	161	rVB	109516	133196	9.96%	1.321%
3	1.975	272	275	277	rBV3	2299	1531	0.11%	0.015%
4	2.116	309	319	333	rBV	248898	368705	27.56%	3.656%
5	2.405	403	409	413	rBV6	2198	2525	0.19%	0.025%
6	2.627	474	478	479	rBV4	1313	847	0.06%	0.008%
7	2.714	502	505	507	rVB4	1636	823	0.06%	0.008%
8	2.746	512	515	516	rBV3	1425	703	0.05%	0.007%
9	2.862	549	551	554	rBV3	1253	772	0.06%	0.008%
10	2.881	555	557	560	rVB4	1558	766	0.06%	0.008%
11	2.917	561	568	570	rBV9	1784	1312	0.10%	0.013%
12	3.045	603	608	609	rBV5	1725	1390	0.10%	0.014%
13	3.113	626	629	633	rBV6	1833	1423	0.11%	0.014%
14	3.209	656	659	666	rBV9	1605	1525	0.11%	0.015%
15	3.335	694	698	701	rVB6	1456	1178	0.09%	0.012%
16	3.585	774	776	780	rVB4	1393	957	0.07%	0.009%
17	3.611	780	784	788	rBV7	1889	1989	0.15%	0.020%
18	3.695	806	810	812	rBV4	1285	829	0.06%	0.008%
19	3.859	859	861	862	rBV2	1554	702	0.05%	0.007%
20	3.894	862	872	902	rVV	108822	301412	22.53%	2.989%
21	4.116	938	941	942	rBV4	1277	784	0.06%	0.008%
22	4.373	1007	1021	1049	rVB	216683	528385	39.49%	5.239%
23	4.846	1164	1168	1169	rBV3	2505	1664	0.12%	0.016%
24	5.071	1220	1238	1262	rBV2	514578	1337866	100.00%	13.266%
25	5.318	1313	1315	1318	rBV4	1825	1201	0.09%	0.012%
26	5.463	1357	1360	1364	rVB5	1729	874	0.07%	0.009%
27	5.640	1402	1415	1441	rBV	388987	778775	58.21%	7.722%
28	5.933	1497	1506	1518	rVB8	9719	20439	1.53%	0.203%
29	6.093	1543	1556	1573	rBV2	297340	602184	45.01%	5.971%
30	6.441	1660	1664	1667	rVB5	1401	975	0.07%	0.010%
31	6.486	1675	1678	1684	rBV8	2016	2062	0.15%	0.020%
32	6.531	1686	1692	1694	rVB6	1196	954	0.07%	0.009%
33	6.621	1715	1720	1723	rBV7	1758	1912	0.14%	0.019%
34	6.897	1803	1806	1809	rBV4	923	752	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016689.D
 Acq On : 09 Jun 2020 03:18
 Operator : SY/MD
 Sample : L2895-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0LO

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.933	1813	1817	1820	rBV5	1202	1060	0.08%	0.011%
36	7.007	1829	1840	1858	rBV2	164509	294736	22.03%	2.923%
37	7.338	1931	1943	1959	rVV	595646	1027379	76.79%	10.187%
38	7.640	2028	2037	2055	rBV	117026	201424	15.06%	1.997%
39	8.109	2173	2183	2211	rBV	367505	678268	50.70%	6.726%
40	8.447	2284	2288	2291	rVB6	1935	1265	0.09%	0.013%
41	8.547	2313	2319	2320	rBV5	952	948	0.07%	0.009%
42	8.675	2355	2359	2361	rBV5	1100	873	0.07%	0.009%
43	8.691	2361	2364	2371	rVB9	1557	1321	0.10%	0.013%
44	8.801	2396	2398	2401	rVB3	1506	724	0.05%	0.007%
45	8.875	2408	2421	2440	rBV	587667	950821	71.07%	9.428%
46	9.325	2559	2561	2565	rVB5	1361	898	0.07%	0.009%
47	9.347	2565	2568	2571	rBV3	1075	821	0.06%	0.008%
48	9.431	2591	2594	2598	rVB4	1874	1437	0.11%	0.014%
49	9.569	2632	2637	2639	rBV5	3137	2916	0.22%	0.029%
50	9.694	2673	2676	2679	rBV4	1529	938	0.07%	0.009%
51	9.791	2704	2706	2711	rVB6	1213	743	0.06%	0.007%
52	9.820	2712	2715	2717	rBV4	1166	762	0.06%	0.008%
53	9.907	2740	2742	2745	rBV3	1048	768	0.06%	0.008%
54	10.029	2778	2780	2783	rBV4	1376	953	0.07%	0.009%
55	10.058	2788	2789	2795	rBV5	861	961	0.07%	0.010%
56	10.087	2795	2798	2802	rVB6	1946	1555	0.12%	0.015%
57	10.116	2802	2807	2810	rBV6	1955	1909	0.14%	0.019%
58	10.238	2830	2845	2860	rBV	415375	651821	48.72%	6.463%
59	10.334	2873	2875	2878	rBV4	1317	792	0.06%	0.008%
60	10.453	2908	2912	2913	rBV4	1245	1004	0.08%	0.010%
61	10.765	3007	3009	3011	rVB3	2083	811	0.06%	0.008%
62	10.862	3035	3039	3043	rBV6	1504	1367	0.10%	0.014%
63	10.926	3057	3059	3061	rBV3	1807	854	0.06%	0.008%
64	11.058	3095	3100	3101	rBV4	1075	860	0.06%	0.009%
65	11.212	3146	3148	3152	rVB3	2998	1941	0.15%	0.019%
66	11.270	3152	3166	3182	rBV	590931	913288	68.26%	9.056%
67	11.466	3224	3227	3228	rBV3	1762	987	0.07%	0.010%
68	11.559	3246	3256	3264	rBV10	4917	11494	0.86%	0.114%
69	11.646	3272	3283	3300	rBV	650535	1026462	76.72%	10.178%
70	11.813	3332	3335	3337	rBV3	2004	1185	0.09%	0.012%
71	11.849	3344	3346	3351	rBV5	1301	1022	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016689.D
 Acq On : 09 Jun 2020 03:18
 Operator : SY/MD
 Sample : L2895-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0LO

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.884	3354	3357	3360	rBV4	1537	934	0.07%	0.009%
73	12.048	3406	3408	3411	rBV4	1442	891	0.07%	0.009%
74	12.064	3411	3413	3416	rVV3	1516	737	0.06%	0.007%
75	12.090	3416	3421	3424	rVV6	1854	1660	0.12%	0.016%
76	12.174	3445	3447	3450	rBV4	1094	702	0.05%	0.007%
77	12.331	3490	3496	3499	rBV6	1713	1633	0.12%	0.016%
78	12.466	3536	3538	3540	rBV3	1653	747	0.06%	0.007%
79	12.675	3601	3603	3606	rBV2	1337	793	0.06%	0.008%
80	12.730	3616	3620	3623	rBV5	1927	1811	0.14%	0.018%
81	12.784	3633	3637	3640	rBV5	1052	905	0.07%	0.009%
82	12.862	3658	3661	3662	rBV2	1477	949	0.07%	0.009%
83	12.932	3681	3683	3686	rBV4	991	719	0.05%	0.007%
84	13.074	3726	3727	3732	rBV4	995	846	0.06%	0.008%
85	13.299	3795	3797	3802	rBV5	1517	1409	0.11%	0.014%
86	13.405	3827	3830	3832	rVB4	1352	797	0.06%	0.008%
87	13.463	3843	3848	3851	rBV6	1999	1921	0.14%	0.019%
88	13.485	3853	3855	3858	rBV4	1034	718	0.05%	0.007%
89	13.537	3866	3871	3873	rBV4	1760	1438	0.11%	0.014%
90	13.633	3897	3901	3908	rBV9	1238	1674	0.13%	0.017%
91	13.681	3912	3916	3920	rVB6	2325	2181	0.16%	0.022%
92	13.704	3920	3923	3925	rBV4	2225	1227	0.09%	0.012%
93	14.199	4072	4077	4080	rBV6	2797	2405	0.18%	0.024%
94	14.225	4080	4085	4086	rBV5	1178	849	0.06%	0.008%
95	14.280	4100	4102	4106	rBV4	1087	719	0.05%	0.007%
96	14.399	4136	4139	4143	rVB5	1162	908	0.07%	0.009%
97	14.575	4192	4194	4197	rBV3	1155	744	0.06%	0.007%
98	14.987	4319	4322	4328	rVB6	1508	1475	0.11%	0.015%
99	15.016	4328	4331	4333	rBV2	1080	739	0.06%	0.007%
100	15.505	4481	4483	4485	rBV3	1545	711	0.05%	0.007%


Sum of corrected areas: 10084891

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016689.D
Acq On : 09 Jun 2020 03:18
Operator : SY/MD
Sample : L2895-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0LO

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

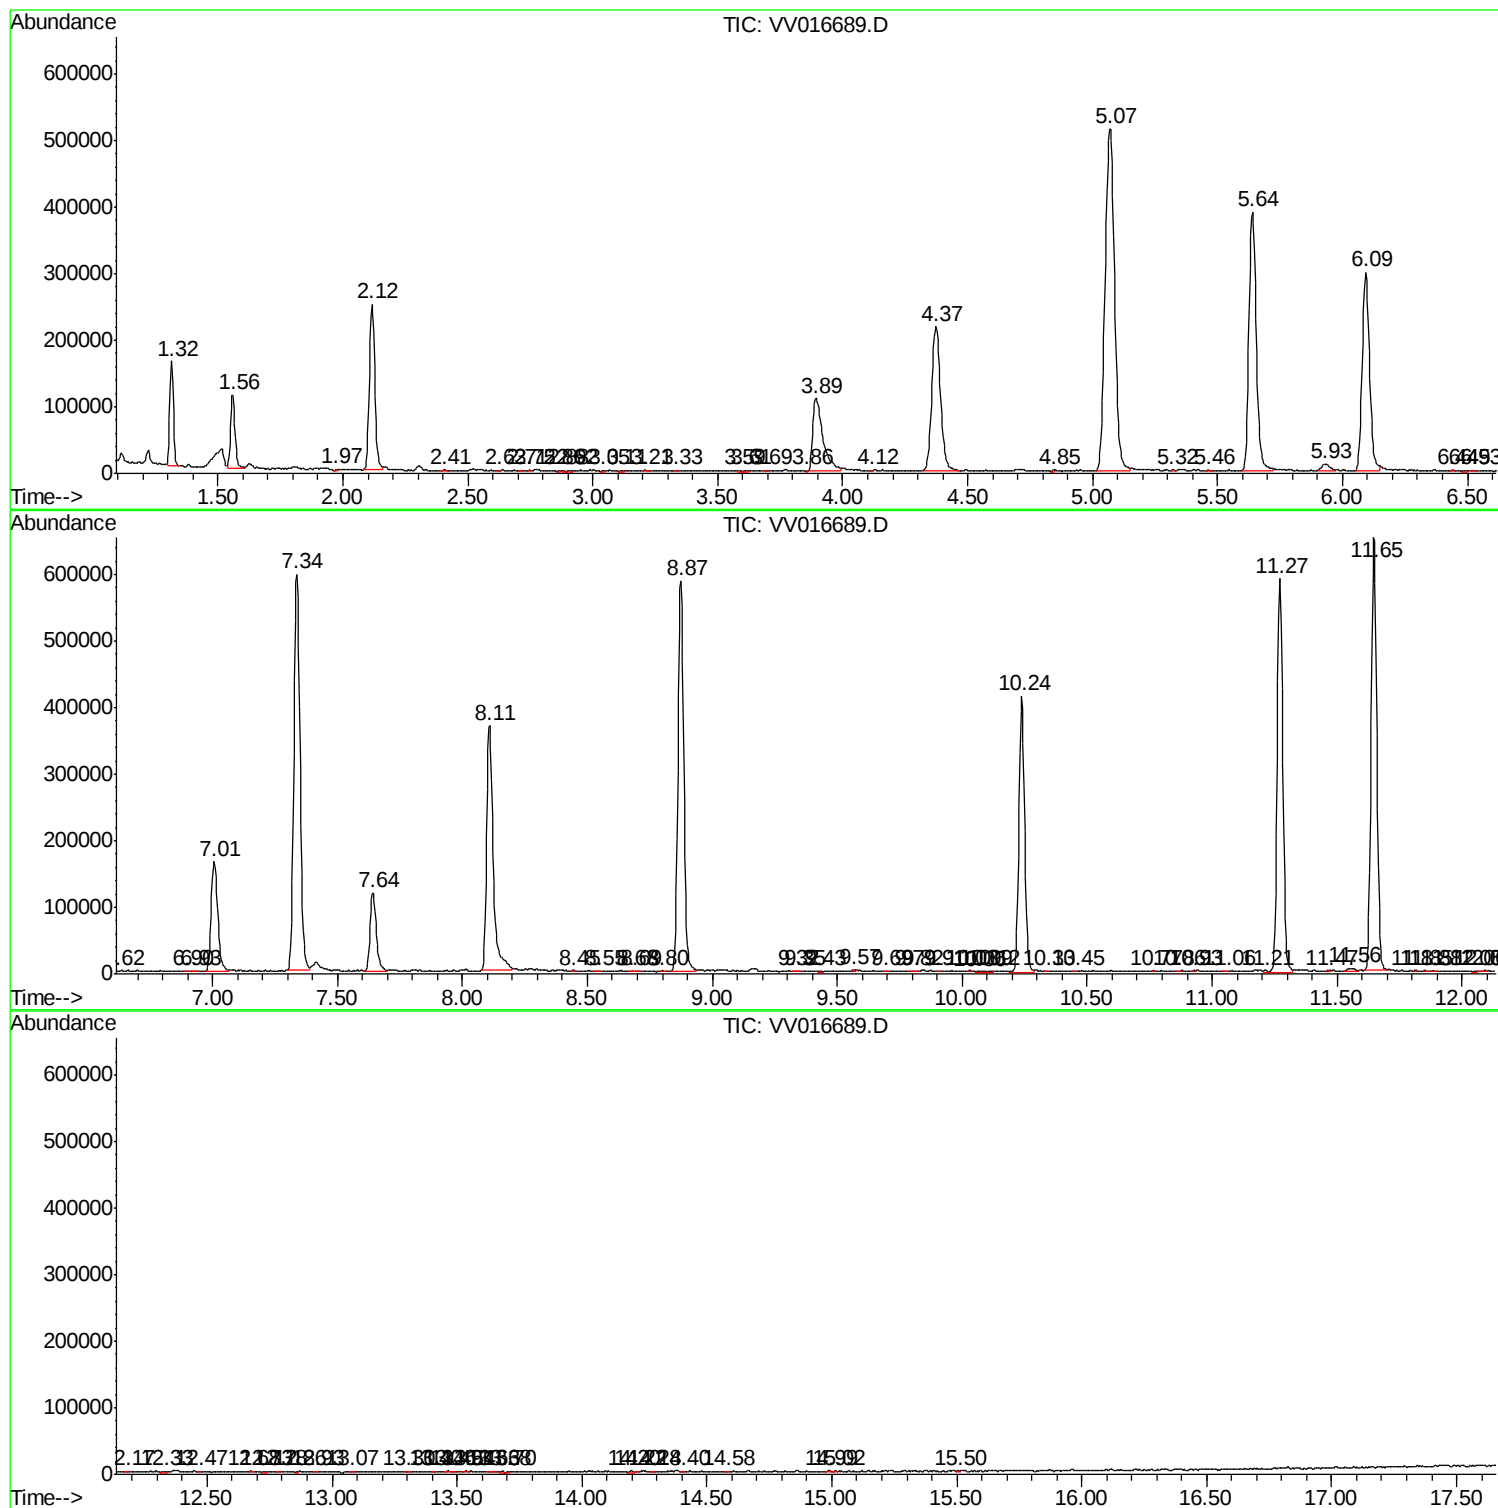

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016689.D
Acq On : 09 Jun 2020 03:18
Operator : SY/MD
Sample : L2895-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0LO

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016689.D
Acq On : 09 Jun 2020 03:18
Operator : SY/MD
Sample : L2895-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0LO

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc