

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016690.D
 Acq On : 09 Jun 2020 03:42
 Operator : SY/MD
 Sample : L2901-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	179300	182400	12.91%	1.749%
2	1.563	140	147	159	rVB	112386	133481	9.45%	1.280%
3	2.116	310	319	335	rBV	263076	386869	27.38%	3.710%
4	2.733	508	511	514	rVB2	1677	1041	0.07%	0.010%
5	2.769	517	522	524	rBV3	2257	1986	0.14%	0.019%
6	2.804	531	533	538	rVB4	2062	1577	0.11%	0.015%
7	2.833	538	542	543	rBV2	1089	708	0.05%	0.007%
8	3.052	608	610	613	rBV4	1999	1289	0.09%	0.012%
9	3.119	627	631	634	rBV5	1227	1097	0.08%	0.011%
10	3.209	647	659	675	rVV2	32352	71270	5.04%	0.683%
11	3.405	717	720	721	rBV3	1554	926	0.07%	0.009%
12	3.438	726	730	733	rBV6	2246	2297	0.16%	0.022%
13	3.547	762	764	767	rBV4	1031	729	0.05%	0.007%
14	3.592	775	778	779	rBV3	1798	933	0.07%	0.009%
15	3.698	809	811	814	rVB4	1392	653	0.05%	0.006%
16	3.788	837	839	842	rBV2	1471	593	0.04%	0.006%
17	3.894	860	872	906	rBV2	107985	391731	27.73%	3.756%
18	4.235	974	978	979	rBV4	1494	1047	0.07%	0.010%
19	4.312	1000	1002	1004	rBV3	1303	762	0.05%	0.007%
20	4.373	1004	1021	1042	rVV	226617	557398	39.46%	5.345%
21	4.611	1093	1095	1099	rBV5	1311	721	0.05%	0.007%
22	4.994	1211	1214	1216	rBV3	1222	771	0.05%	0.007%
23	5.071	1220	1238	1269	rVV2	536863	1412727	100.00%	13.546%
24	5.640	1402	1415	1438	rVV	393202	790226	55.94%	7.577%
25	6.093	1542	1556	1581	rBV	310841	633387	44.83%	6.073%
26	6.463	1667	1671	1674	rVB5	1502	917	0.06%	0.009%
27	6.489	1676	1679	1685	rVB8	1763	1667	0.12%	0.016%
28	6.521	1685	1689	1694	rBV7	1386	1443	0.10%	0.014%
29	6.553	1695	1699	1700	rBV4	1310	801	0.06%	0.008%
30	6.582	1706	1708	1712	rBV4	962	912	0.06%	0.009%
31	6.788	1770	1772	1776	rVB5	1356	757	0.05%	0.007%
32	6.810	1776	1779	1781	rVB4	1499	620	0.04%	0.006%
33	7.007	1829	1840	1861	rBV	168617	302388	21.40%	2.900%
34	7.280	1922	1925	1929	rVB5	1280	921	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016690.D
 Acq On : 09 Jun 2020 03:42
 Operator : SY/MD
 Sample : L2901-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.338	1931	1943	1963	rVV	635996	1086467	76.91%	10.418%
36	7.640	2028	2037	2053	rBV	117323	200548	14.20%	1.923%
37	7.749	2067	2071	2073	rBV4	2000	1453	0.10%	0.014%
38	7.936	2125	2129	2130	rBV3	1302	864	0.06%	0.008%
39	7.997	2144	2148	2149	rBV4	1703	1175	0.08%	0.011%
40	8.071	2168	2171	2172	rVV3	1278	692	0.05%	0.007%
41	8.106	2172	2182	2219	rVV	348911	672025	47.57%	6.444%
42	8.498	2302	2304	2307	rVB4	1938	856	0.06%	0.008%
43	8.518	2307	2310	2312	rBV3	1966	1337	0.09%	0.013%
44	8.582	2327	2330	2331	rBV3	1446	698	0.05%	0.007%
45	8.659	2350	2354	2357	rBV5	1712	1641	0.12%	0.016%
46	8.875	2410	2421	2443	rBV	590685	945126	66.90%	9.063%
47	9.000	2459	2460	2463	rBV2	1130	592	0.04%	0.006%
48	9.216	2524	2527	2531	rVB4	1978	1741	0.12%	0.017%
49	9.318	2555	2559	2562	rVB4	1936	1294	0.09%	0.012%
50	9.351	2566	2569	2570	rBV3	1263	725	0.05%	0.007%
51	9.402	2582	2585	2587	rBV2	1328	936	0.07%	0.009%
52	9.531	2624	2625	2631	rBV6	961	674	0.05%	0.006%
53	9.627	2651	2655	2657	rBV4	1414	1250	0.09%	0.012%
54	9.794	2704	2707	2713	rVB5	1503	1107	0.08%	0.011%
55	9.823	2713	2716	2720	rBV5	1507	1183	0.08%	0.011%
56	9.936	2748	2751	2754	rBV5	967	738	0.05%	0.007%
57	9.955	2754	2757	2760	rBV4	1401	1026	0.07%	0.010%
58	10.026	2776	2779	2780	rBV3	1565	658	0.05%	0.006%
59	10.238	2834	2845	2861	rBV	401239	636729	45.07%	6.105%
60	10.341	2875	2877	2879	rBV3	1376	653	0.05%	0.006%
61	10.441	2906	2908	2911	rBV3	1161	795	0.06%	0.008%
62	10.627	2964	2966	2970	rVB3	1937	918	0.06%	0.009%
63	10.730	2996	2998	3001	rBV3	1100	854	0.06%	0.008%
64	11.032	3087	3092	3097	rBV9	1375	1875	0.13%	0.018%
65	11.058	3097	3100	3102	rVB4	1803	954	0.07%	0.009%
66	11.148	3125	3128	3129	rBV3	1092	715	0.05%	0.007%
67	11.183	3137	3139	3141	rBV3	1908	1107	0.08%	0.011%
68	11.270	3154	3166	3185	rBV	568306	891630	63.11%	8.550%
69	11.379	3197	3200	3204	rBV6	1422	1359	0.10%	0.013%
70	11.563	3250	3257	3265	rBV9	3781	6110	0.43%	0.059%
71	11.646	3272	3283	3300	rBV	671322	1039427	73.58%	9.967%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016690.D
 Acq On : 09 Jun 2020 03:42
 Operator : SY/MD
 Sample : L2901-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.965	3379	3382	3384	rBV3	1289	877	0.06%	0.008%
73	12.003	3391	3394	3395	rBV3	1694	1004	0.07%	0.010%
74	12.119	3426	3430	3433	rBV6	693	619	0.04%	0.006%
75	12.164	3442	3444	3446	rBV3	1355	605	0.04%	0.006%
76	12.196	3452	3454	3456	rBV3	1312	719	0.05%	0.007%
77	12.225	3459	3463	3464	rBV4	1828	1395	0.10%	0.013%
78	12.309	3486	3489	3493	rBV4	1212	1102	0.08%	0.011%
79	12.537	3556	3560	3565	rBV6	1606	1854	0.13%	0.018%
80	12.698	3608	3610	3615	rBV4	1165	1044	0.07%	0.010%
81	12.733	3619	3621	3623	rBV3	1411	844	0.06%	0.008%
82	12.752	3625	3627	3630	rVV3	1489	685	0.05%	0.007%
83	12.791	3634	3639	3640	rBV4	1201	1227	0.09%	0.012%
84	12.939	3682	3685	3688	rBV3	1650	1176	0.08%	0.011%
85	13.064	3721	3724	3730	rVB7	820	908	0.06%	0.009%
86	13.093	3730	3733	3736	rBV4	1550	1324	0.09%	0.013%
87	13.231	3774	3776	3778	rBV3	1134	611	0.04%	0.006%
88	13.260	3781	3785	3787	rBV3	1644	1297	0.09%	0.012%
89	13.354	3811	3814	3818	rBV5	1641	1509	0.11%	0.014%
90	13.649	3902	3906	3909	rBV5	1424	1077	0.08%	0.010%
91	13.897	3980	3983	3987	rVV6	1723	1520	0.11%	0.015%
92	14.096	4042	4045	4049	rVB4	2645	2016	0.14%	0.019%
93	14.125	4049	4054	4058	rBV8	1594	1915	0.14%	0.018%
94	14.154	4061	4063	4065	rBV3	1563	679	0.05%	0.007%
95	14.289	4102	4105	4108	rBV3	2291	1513	0.11%	0.015%
96	14.386	4132	4135	4136	rBV3	1546	709	0.05%	0.007%
97	15.090	4352	4354	4356	rBV3	1449	874	0.06%	0.008%
98	15.148	4367	4372	4375	rBV7	2147	2050	0.15%	0.020%
99	15.247	4399	4403	4405	rBV3	2000	1495	0.11%	0.014%
100	16.013	4639	4641	4644	rBV3	2384	1308	0.09%	0.013%


Sum of corrected areas: 10428933

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016690.D
Acq On : 09 Jun 2020 03:42
Operator : SY/MD
Sample : L2901-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

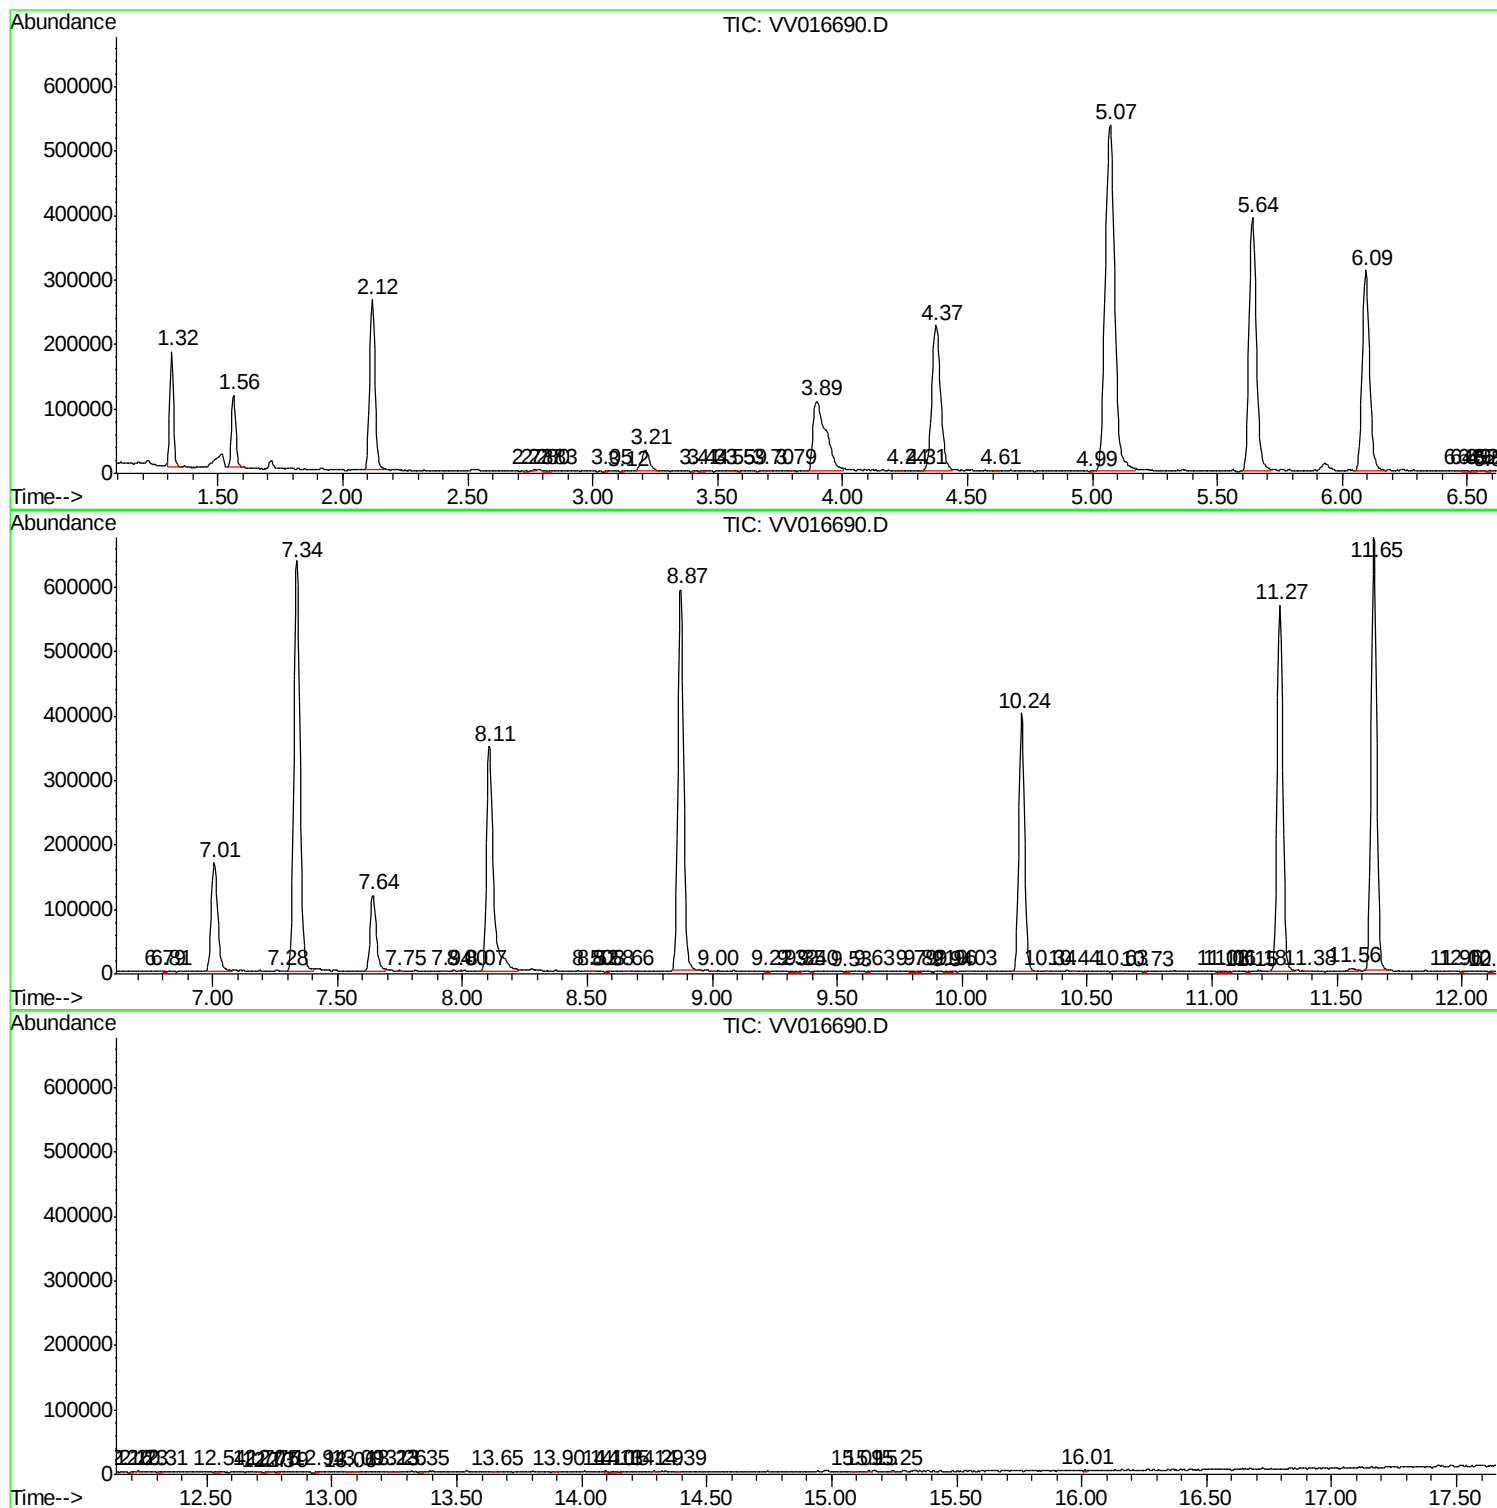

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016690.D
Acq On : 09 Jun 2020 03:42
Operator : SY/MD
Sample : L2901-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016690.D
Acq On : 09 Jun 2020 03:42
Operator : SY/MD
Sample : L2901-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc