

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016691.D
 Acq On : 09 Jun 2020 04:06
 Operator : SY/MD
 Sample : L2901-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	175961	172991	12.84%	1.716%
2	1.560	140	146	159	rVB	115599	138899	10.31%	1.378%
3	2.116	310	319	333	rVB	256292	368784	27.37%	3.658%
4	2.431	411	417	420	rBV8	1296	1573	0.12%	0.016%
5	2.566	457	459	462	rBV4	1113	695	0.05%	0.007%
6	2.695	496	499	502	rBV4	1631	1064	0.08%	0.011%
7	2.901	561	563	566	rBV3	1024	688	0.05%	0.007%
8	3.058	608	612	615	rBV5	1258	1143	0.08%	0.011%
9	3.187	649	652	653	rBV3	2177	1307	0.10%	0.013%
10	3.296	681	686	687	rBV5	1723	1560	0.12%	0.015%
11	3.373	709	710	717	rVB7	1638	992	0.07%	0.010%
12	3.402	717	719	721	rVB3	1591	686	0.05%	0.007%
13	3.563	765	769	771	rBV4	1557	964	0.07%	0.010%
14	3.621	786	787	793	rVB5	2172	1301	0.10%	0.013%
15	3.717	814	817	821	rBV5	1502	1335	0.10%	0.013%
16	3.746	824	826	831	rVV6	989	662	0.05%	0.007%
17	3.807	842	845	848	rVV4	1390	1161	0.09%	0.012%
18	3.894	862	872	904	rBV2	105347	334826	24.85%	3.322%
19	4.373	1006	1021	1050	rVB	219288	531752	39.46%	5.275%
20	4.627	1097	1100	1101	rBV3	1257	807	0.06%	0.008%
21	4.685	1115	1118	1121	rVB4	1506	841	0.06%	0.008%
22	4.772	1143	1145	1148	rBV3	1409	967	0.07%	0.010%
23	4.810	1153	1157	1159	rBV5	1797	1496	0.11%	0.015%
24	4.862	1170	1173	1177	rVB6	1464	1186	0.09%	0.012%
25	4.949	1199	1200	1204	rVB3	1378	731	0.05%	0.007%
26	4.971	1204	1207	1209	rBV2	1862	1035	0.08%	0.010%
27	5.071	1220	1238	1266	rBV2	523313	1347496	100.00%	13.368%
28	5.556	1386	1389	1392	rBV4	1144	711	0.05%	0.007%
29	5.640	1403	1415	1445	rBV	384089	765189	56.79%	7.591%
30	5.852	1478	1481	1486	rVB6	2110	1986	0.15%	0.020%
31	5.933	1494	1506	1519	rBV9	10156	23857	1.77%	0.237%
32	6.093	1544	1556	1582	rVB	301915	607664	45.10%	6.028%
33	6.444	1662	1665	1667	rBV3	1134	729	0.05%	0.007%
34	6.727	1747	1753	1755	rBV7	1043	1190	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016691.D
 Acq On : 09 Jun 2020 04:06
 Operator : SY/MD
 Sample : L2901-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.762	1759	1764	1767	rBV6	1444	1493	0.11%	0.015%
36	6.871	1796	1798	1803	rVB5	1590	1161	0.09%	0.012%
37	7.006	1829	1840	1862	rBV2	161320	289335	21.47%	2.870%
38	7.190	1893	1897	1899	rBV4	1616	1243	0.09%	0.012%
39	7.264	1919	1920	1925	rBV3	1125	666	0.05%	0.007%
40	7.338	1931	1943	1963	rVV	605547	1043667	77.45%	10.353%
41	7.640	2027	2037	2055	rBV	115253	197430	14.65%	1.959%
42	7.794	2081	2085	2089	rBV7	2200	1520	0.11%	0.015%
43	7.849	2098	2102	2106	rBV7	1440	1434	0.11%	0.014%
44	7.936	2127	2129	2131	rBV3	1531	659	0.05%	0.007%
45	8.106	2173	2182	2215	rBV	329997	643254	47.74%	6.381%
46	8.521	2307	2311	2313	rBV5	1207	871	0.06%	0.009%
47	8.556	2319	2322	2326	rBV5	1580	1750	0.13%	0.017%
48	8.875	2407	2421	2441	rBV	578570	942919	69.98%	9.354%
49	9.158	2507	2509	2511	rBV3	1357	868	0.06%	0.009%
50	9.428	2588	2593	2597	rBV7	1391	1405	0.10%	0.014%
51	9.518	2618	2621	2623	rVB4	1364	703	0.05%	0.007%
52	9.807	2709	2711	2715	rVB4	1567	1234	0.09%	0.012%
53	9.836	2715	2720	2722	rBV5	1285	1114	0.08%	0.011%
54	9.907	2739	2742	2744	rBV3	1346	668	0.05%	0.007%
55	9.955	2755	2757	2762	rVB5	1368	750	0.06%	0.007%
56	9.981	2762	2765	2766	rBV2	1315	752	0.06%	0.007%
57	10.013	2772	2775	2778	rVB3	1648	1004	0.07%	0.010%
58	10.039	2778	2783	2785	rBV5	1278	985	0.07%	0.010%
59	10.174	2823	2825	2828	rBV3	1911	1203	0.09%	0.012%
60	10.238	2834	2845	2862	rBV	396986	625614	46.43%	6.206%
61	10.537	2935	2938	2939	rBV3	1780	901	0.07%	0.009%
62	10.630	2965	2967	2973	rBV7	1816	1172	0.09%	0.012%
63	10.653	2973	2974	2978	rVB2	1623	1067	0.08%	0.011%
64	10.778	3011	3013	3016	rBV4	1237	893	0.07%	0.009%
65	10.997	3078	3081	3084	rBV5	2063	1411	0.10%	0.014%
66	11.029	3089	3091	3093	rBV3	1336	678	0.05%	0.007%
67	11.119	3116	3119	3121	rBV3	1407	851	0.06%	0.008%
68	11.132	3121	3123	3125	rBV3	1085	716	0.05%	0.007%
69	11.270	3151	3166	3183	rBV	595875	915107	67.91%	9.078%
70	11.482	3228	3232	3234	rVV4	1168	849	0.06%	0.008%
71	11.556	3245	3255	3256	rBV8	3371	4507	0.33%	0.045%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016691.D
 Acq On : 09 Jun 2020 04:06
 Operator : SY/MD
 Sample : L2901-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTQ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3271	3283	3301	rBV	664515	1041195	77.27%	10.329%
73	12.045	3403	3407	3409	rBV4	1322	1111	0.08%	0.011%
74	12.264	3474	3475	3479	rBV4	869	660	0.05%	0.007%
75	12.376	3506	3510	3514	rBV5	1717	1365	0.10%	0.014%
76	12.460	3534	3536	3539	rVB2	1471	785	0.06%	0.008%
77	12.498	3544	3548	3549	rBV4	1147	714	0.05%	0.007%
78	12.797	3636	3641	3647	rBV7	1236	1532	0.11%	0.015%
79	12.823	3647	3649	3654	rBV5	1463	1308	0.10%	0.013%
80	12.865	3659	3662	3664	rBV4	1347	830	0.06%	0.008%
81	13.071	3723	3726	3727	rBV3	1288	813	0.06%	0.008%
82	13.106	3735	3737	3740	rBV3	1330	811	0.06%	0.008%
83	13.180	3758	3760	3764	rVB3	1485	737	0.05%	0.007%
84	13.305	3797	3799	3801	rVB3	1333	718	0.05%	0.007%
85	13.325	3802	3805	3809	rVB5	1521	827	0.06%	0.008%
86	13.347	3809	3812	3816	rVB4	1741	1431	0.11%	0.014%
87	13.370	3816	3819	3824	rBV7	1773	1923	0.14%	0.019%
88	13.534	3869	3870	3874	rVB4	1493	951	0.07%	0.009%
89	13.681	3909	3916	3917	rBV5	1086	1281	0.10%	0.013%
90	13.932	3992	3994	3997	rBV4	973	670	0.05%	0.007%
91	13.968	4003	4005	4011	rBV6	1088	1188	0.09%	0.012%
92	14.090	4040	4043	4051	rVB9	1941	2003	0.15%	0.020%
93	14.196	4074	4076	4078	rBV3	1221	656	0.05%	0.007%
94	14.257	4092	4095	4098	rBV3	1366	939	0.07%	0.009%
95	14.337	4118	4120	4124	rBV5	1298	704	0.05%	0.007%
96	14.389	4133	4136	4139	rBV4	1379	700	0.05%	0.007%
97	14.588	4193	4198	4203	rBV9	1680	1577	0.12%	0.016%
98	14.710	4234	4236	4238	rBV3	1329	847	0.06%	0.008%
99	15.212	4390	4392	4395	rVV4	1700	983	0.07%	0.010%
100	15.244	4400	4402	4406	rBV5	1144	953	0.07%	0.009%


Sum of corrected areas: 10080334

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016691.D
Acq On : 09 Jun 2020 04:06
Operator : SY/MD
Sample : L2901-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

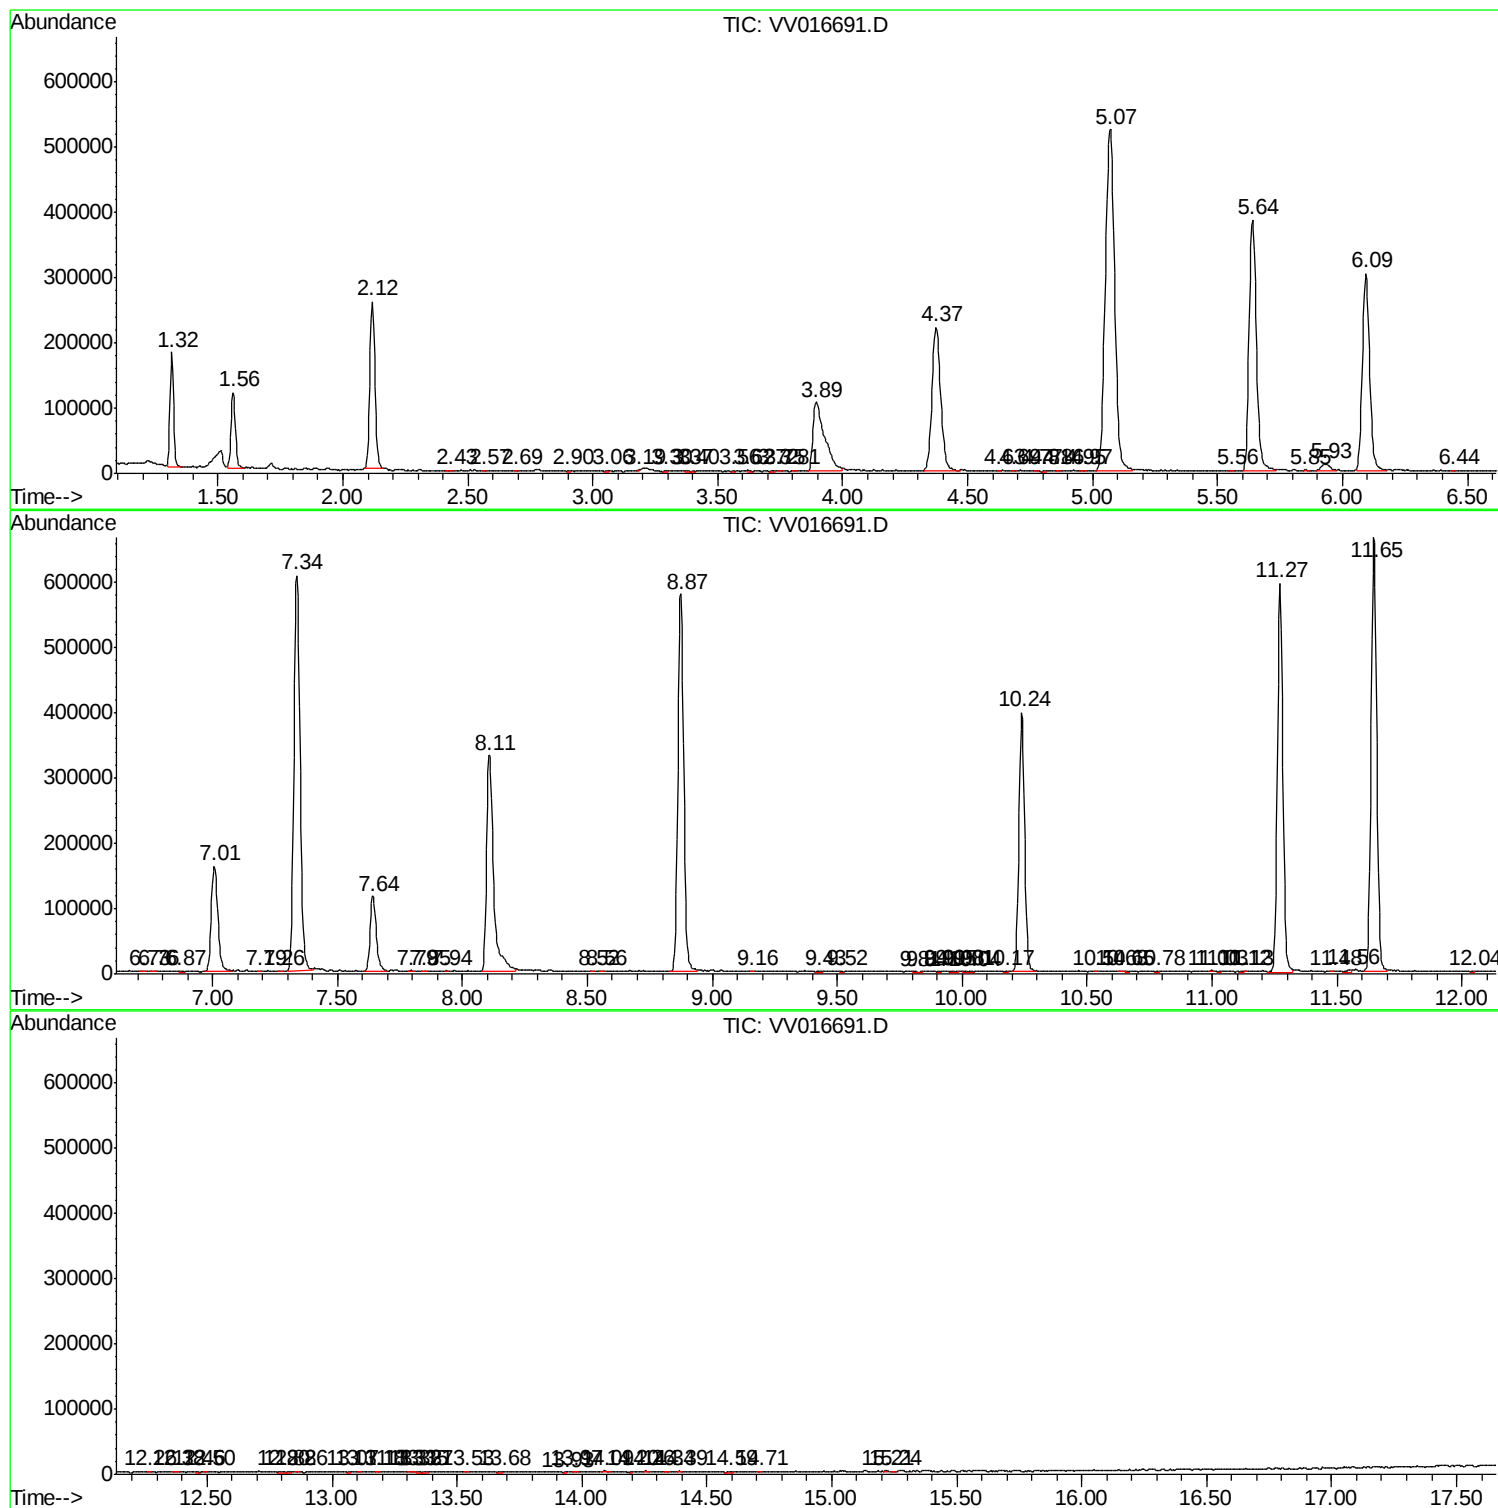

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016691.D
Acq On : 09 Jun 2020 04:06
Operator : SY/MD
Sample : L2901-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016691.D
Acq On : 09 Jun 2020 04:06
Operator : SY/MD
Sample : L2901-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTQ3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc