

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016694.D
 Acq On : 09 Jun 2020 05:17
 Operator : SY/MD
 Sample : L2901-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB2	187409	194426	14.45%	1.930%
2	1.563	141	147	159	rVB	110629	130198	9.68%	1.293%
3	2.116	310	319	334	rVB	252977	374661	27.85%	3.720%
4	2.489	431	435	437	rBV4	1901	1557	0.12%	0.015%
5	2.553	453	455	457	rVB3	1635	777	0.06%	0.008%
6	2.576	457	462	465	rBV7	1577	1376	0.10%	0.014%
7	2.611	471	473	476	rBV4	1823	1272	0.09%	0.013%
8	2.923	568	570	574	rBV4	1152	808	0.06%	0.008%
9	2.975	585	586	590	rVB4	1775	633	0.05%	0.006%
10	2.997	590	593	596	rVB3	1866	923	0.07%	0.009%
11	3.052	608	610	614	rBV3	985	660	0.05%	0.007%
12	3.319	690	693	697	rBV6	1421	954	0.07%	0.009%
13	3.364	704	707	708	rBV3	1200	662	0.05%	0.007%
14	3.415	721	723	728	rVB6	1796	1346	0.10%	0.013%
15	3.463	734	738	739	rBV3	1323	678	0.05%	0.007%
16	3.897	862	873	876	rBV2	112224	194111	14.43%	1.927%
17	4.238	976	979	983	rBV5	1370	1089	0.08%	0.011%
18	4.309	999	1001	1004	rBV4	1400	846	0.06%	0.008%
19	4.373	1007	1021	1041	rVV	218496	534371	39.72%	5.305%
20	4.778	1144	1147	1148	rBV2	1172	766	0.06%	0.008%
21	4.810	1154	1157	1160	rBV4	1057	869	0.06%	0.009%
22	4.946	1197	1199	1203	rBV5	1176	751	0.06%	0.007%
23	4.997	1211	1215	1219	rBV5	1434	1188	0.09%	0.012%
24	5.071	1219	1238	1260	rBV2	520918	1345461	100.00%	13.358%
25	5.319	1312	1315	1317	rBV3	1799	1224	0.09%	0.012%
26	5.454	1354	1357	1359	rBV3	1738	1089	0.08%	0.011%
27	5.566	1387	1392	1397	rBV9	2606	2500	0.19%	0.025%
28	5.640	1402	1415	1447	rVV	401353	805513	59.87%	7.997%
29	5.929	1496	1505	1515	rBV9	11919	23418	1.74%	0.232%
30	6.093	1543	1556	1580	rVB	305231	609438	45.30%	6.051%
31	6.380	1641	1645	1650	rBV7	1426	1639	0.12%	0.016%
32	6.518	1686	1688	1690	rBV3	1300	827	0.06%	0.008%
33	6.560	1699	1701	1707	rBV6	1513	1368	0.10%	0.014%
34	6.804	1773	1777	1778	rBV3	1315	1108	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016694.D
 Acq On : 09 Jun 2020 05:17
 Operator : SY/MD
 Sample : L2901-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.939	1815	1819	1822	rBV5	1450	1138	0.08%	0.011%
36	7.007	1829	1840	1860	rBV	162673	288322	21.43%	2.863%
37	7.338	1930	1943	1960	rBV	619110	1061049	78.86%	10.534%
38	7.643	2029	2038	2050	rBV	114940	187086	13.90%	1.857%
39	7.878	2108	2111	2113	rBV5	1533	759	0.06%	0.008%
40	7.936	2127	2129	2132	rBV3	1669	1227	0.09%	0.012%
41	8.058	2165	2167	2170	rBV3	1494	845	0.06%	0.008%
42	8.106	2173	2182	2209	rVV	353034	652309	48.48%	6.476%
43	8.621	2338	2342	2344	rBV4	1277	940	0.07%	0.009%
44	8.711	2368	2370	2374	rBV2	1157	690	0.05%	0.007%
45	8.759	2381	2385	2388	rBV5	1335	1101	0.08%	0.011%
46	8.781	2391	2392	2396	rVB4	1594	960	0.07%	0.010%
47	8.875	2409	2421	2437	rBV	598498	972650	72.29%	9.657%
48	9.161	2508	2510	2513	rBV4	1417	766	0.06%	0.008%
49	9.524	2619	2623	2625	rBV5	1358	882	0.07%	0.009%
50	9.563	2630	2635	2636	rBV4	1308	1089	0.08%	0.011%
51	9.653	2660	2663	2664	rBV3	1263	735	0.05%	0.007%
52	9.759	2694	2696	2699	rBV5	1131	860	0.06%	0.009%
53	9.775	2699	2701	2706	rVB4	2112	1164	0.09%	0.012%
54	9.807	2709	2711	2713	rBV2	1230	657	0.05%	0.007%
55	9.881	2733	2734	2739	rVB5	1519	876	0.07%	0.009%
56	9.910	2739	2743	2746	rBV5	1483	1129	0.08%	0.011%
57	9.994	2764	2769	2771	rVB5	1791	1391	0.10%	0.014%
58	10.051	2785	2787	2791	rVB4	2004	1096	0.08%	0.011%
59	10.077	2791	2795	2797	rBV4	1870	1526	0.11%	0.015%
60	10.125	2808	2810	2815	rVB3	1221	665	0.05%	0.007%
61	10.170	2820	2824	2827	rBV5	1484	958	0.07%	0.010%
62	10.238	2829	2845	2862	rBV	400615	634693	47.17%	6.301%
63	10.621	2962	2964	2968	rBV4	1179	715	0.05%	0.007%
64	10.736	2998	3000	3004	rBV5	1076	793	0.06%	0.008%
65	11.071	3100	3104	3108	rBV5	913	846	0.06%	0.008%
66	11.096	3110	3112	3115	rVV4	1870	1063	0.08%	0.011%
67	11.209	3145	3147	3150	rBV4	1721	1014	0.08%	0.010%
68	11.270	3155	3166	3183	rBV	604820	938191	69.73%	9.314%
69	11.386	3200	3202	3206	rVB5	2177	1568	0.12%	0.016%
70	11.646	3272	3283	3298	rBV	667905	1042330	77.47%	10.348%
71	11.887	3355	3358	3364	rVB7	2014	1948	0.14%	0.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060820\
 Data File : VV016694.D
 Acq On : 09 Jun 2020 05:17
 Operator : SY/MD
 Sample : L2901-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETTS6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.923	3364	3369	3371	rBV4	1973	1515	0.11%	0.015%
73	11.971	3382	3384	3387	rVB2	1416	656	0.05%	0.007%
74	12.029	3398	3402	3403	rBV4	999	725	0.05%	0.007%
75	12.148	3435	3439	3442	rBV5	2044	1739	0.13%	0.017%
76	12.267	3474	3476	3481	rBV5	1283	1154	0.09%	0.011%
77	12.421	3522	3524	3527	rVV2	881	643	0.05%	0.006%
78	12.460	3533	3536	3539	rBV5	1396	987	0.07%	0.010%
79	12.627	3586	3588	3592	rVB5	1045	706	0.05%	0.007%
80	12.662	3595	3599	3602	rBV5	1009	764	0.06%	0.008%
81	12.730	3617	3620	3623	rBV5	1561	1148	0.09%	0.011%
82	12.887	3665	3669	3671	rBV5	1480	1141	0.08%	0.011%
83	13.074	3725	3727	3729	rBV3	1085	668	0.05%	0.007%
84	13.106	3734	3737	3739	rBV4	1274	737	0.05%	0.007%
85	13.231	3774	3776	3779	rBV5	1287	702	0.05%	0.007%
86	13.328	3803	3806	3808	rBV4	875	616	0.05%	0.006%
87	13.473	3845	3851	3853	rBV6	1505	1309	0.10%	0.013%
88	13.823	3956	3960	3961	rBV3	1497	824	0.06%	0.008%
89	13.874	3972	3976	3978	rBV4	1099	772	0.06%	0.008%
90	13.926	3989	3992	3993	rBV3	1062	647	0.05%	0.006%
91	14.183	4068	4072	4075	rBV7	2275	1713	0.13%	0.017%
92	14.222	4079	4084	4087	rBV7	1218	1317	0.10%	0.013%
93	14.260	4092	4096	4097	rBV3	996	650	0.05%	0.006%
94	14.312	4109	4112	4115	rBV4	1198	896	0.07%	0.009%
95	14.759	4248	4251	4253	rBV3	1942	1275	0.09%	0.013%
96	14.794	4258	4262	4264	rBV4	2034	1659	0.12%	0.016%
97	14.823	4269	4271	4273	rBV3	1106	626	0.05%	0.006%
98	15.103	4356	4358	4360	rBV2	1530	682	0.05%	0.007%
99	15.251	4402	4404	4407	rVB4	1472	833	0.06%	0.008%
100	15.508	4482	4484	4486	rBV3	1648	733	0.05%	0.007%


Sum of corrected areas: 10072375

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060820\
Data File : VV016694.D
Acq On : 09 Jun 2020 05:17
Operator : SY/MD
Sample : L2901-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

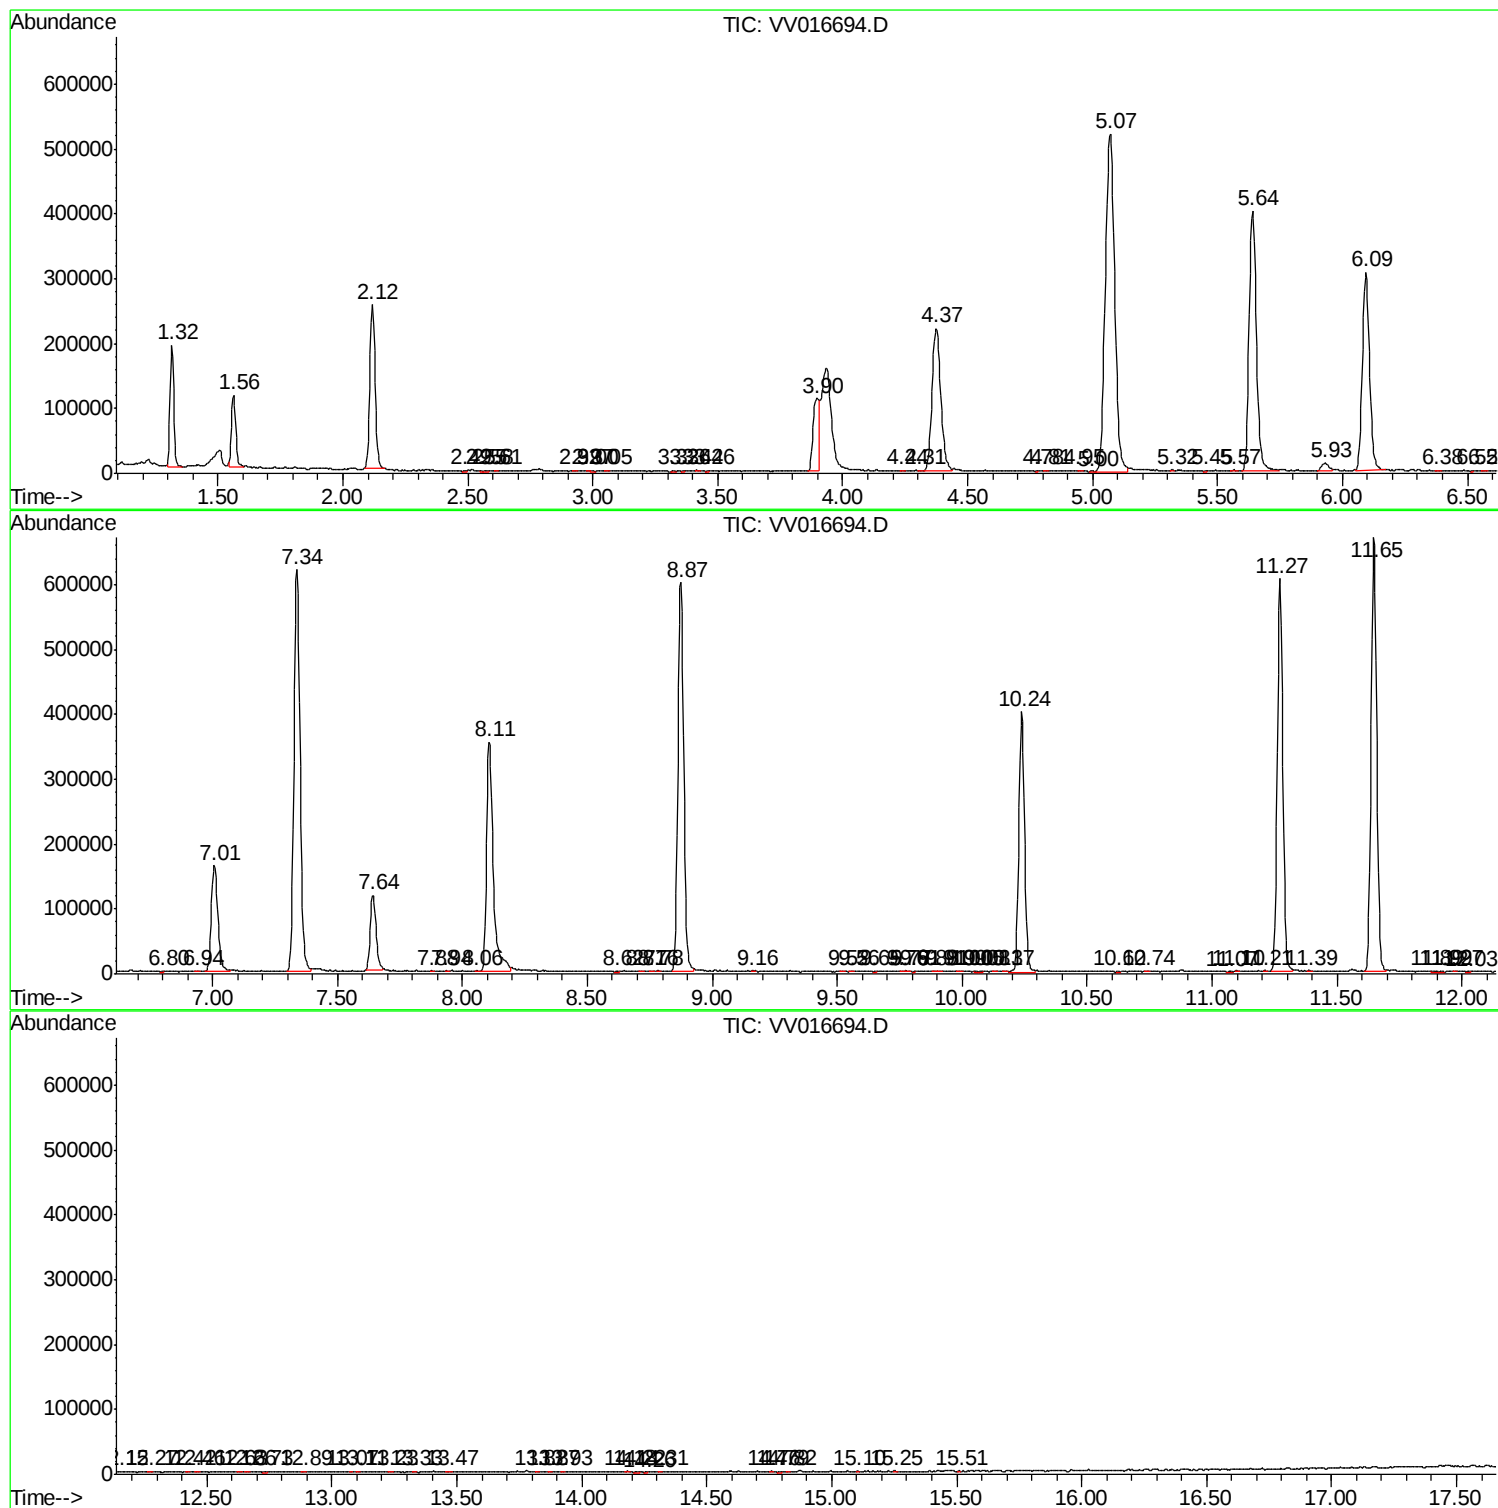

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016694.D
Acq On : 09 Jun 2020 05:17
Operator : SY/MD
Sample : L2901-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060820\
Data File : VV016694.D
Acq On : 09 Jun 2020 05:17
Operator : SY/MD
Sample : L2901-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTS6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc