


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV060820\
 Data File : VV016646.D
 Acq On : 08 Jun 2020 08:28
 Operator : SY/MD
 Sample : BFB83
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB83

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Tue Jun 09 03:29:34 2020

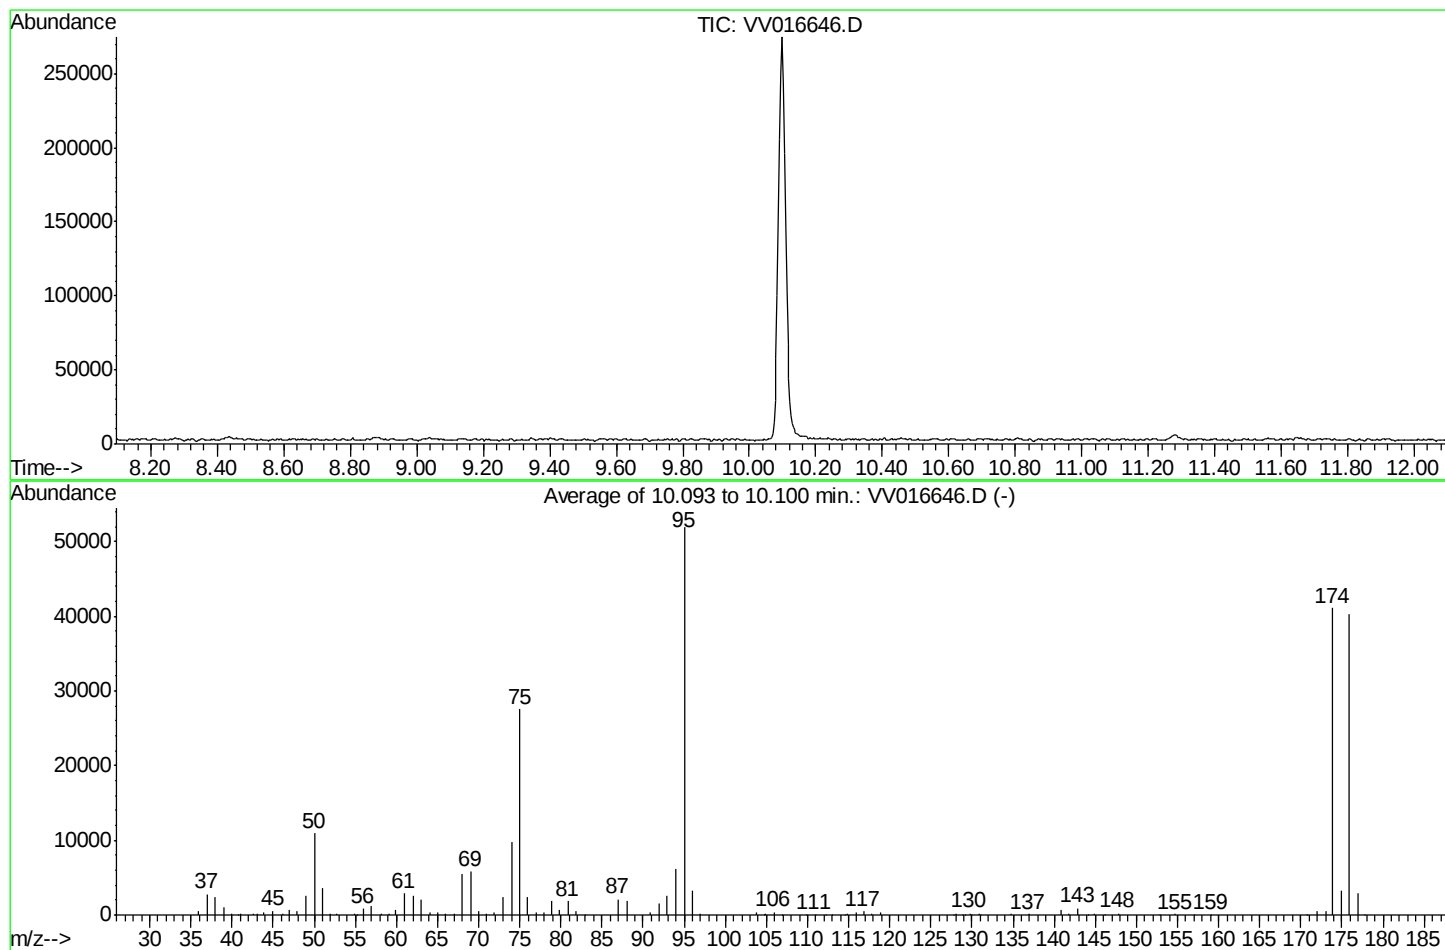

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	10973	PASS
75	95	30	80	53.1	27605	PASS
95	95	100	100	100.0	51938	PASS
96	95	5	9	6.3	3277	PASS
173	174	0.00	2	1.1	443	PASS
174	95	50	120	79.1	41088	PASS
175	174	5	9	8.1	3315	PASS
176	174	95	101	98.2	40365	PASS
177	176	5	9	7.1	2882	PASS

m/z	Abundance
36.00	588.0
37.00	2643.0
38.00	2385.0
39.00	1312.0
39.90	524.0
40.80	106.0
42.60	133.0
43.10	170.0
44.00	754.0
45.00	614.0
46.20	175.0
47.00	676.0
47.90	440.0
49.00	2375.0
50.00	10379.0
51.00	3628.0
51.90	176.0
52.70	113.0
54.00	111.0
54.90	176.0
55.90	802.0
57.00	1318.0
58.10	156.0
59.00	109.0
59.90	689.0
60.90	2796.0
62.00	2625.0
63.00	1955.0
64.10	381.0
64.90	461.0
66.10	102.0
67.10	199.0
68.00	5232.0
69.00	5459.0
70.00	473.0
71.10	103.0
71.90	377.0
73.00	2266.0
74.00	9459.0
75.00	26392.0
76.00	2417.0
76.90	355.0
77.90	263.0
78.90	1635.0
79.80	565.0
80.90	1800.0
81.80	535.0
83.00	107.0
87.00	1840.0
88.00	1845.0
90.80	264.0
92.00	1472.0
93.00	2364.0
94.00	5966.0
95.00	48904.0
96.00	3411.0
97.00	137.0
103.90	352.0
105.00	157.0
106.00	316.0
106.80	148.0
109.80	163.0
110.90	143.0
112.20	110.0
112.90	127.0
114.90	124.0
115.90	289.0
116.80	401.0
117.80	176.0
118.80	332.0
127.70	169.0
129.10	124.0
129.70	143.0
130.00	163.0
130.80	158.0
134.80	119.0
136.90	171.0
140.90	680.0
142.90	891.0
144.10	103.0
145.00	112.0
147.80	169.0
154.70	114.0
159.10	110.0
172.00	494.0
173.90	37480.0
174.90	3012.0
175.90	36904.0
176.90	2749.0
177.70	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
36.00	558.0
37.00	2900.0
38.00	2558.0
39.00	1182.0
39.90	550.0
41.00	155.0
42.70	132.0
43.10	135.0
44.00	866.0
45.00	713.0
46.10	150.0
47.00	704.0
47.80	461.0
49.00	2786.0
50.00	11508.0
51.00	3618.0
52.00	190.0
52.70	115.0
55.20	182.0
56.00	793.0
57.00	1407.0
58.10	151.0
59.00	116.0
59.80	687.0
61.00	2962.0
62.00	2740.0
63.00	2112.0
64.10	384.0
64.90	381.0
66.00	135.0
67.10	200.0
68.00	5659.0
69.00	6048.0
70.00	497.0
71.00	122.0
71.90	414.0
73.00	2408.0
74.00	10052.0
75.00	28616.0
76.00	2564.0
76.90	357.0
77.90	302.0
78.90	1992.0
79.80	643.0
80.90	1955.0
81.90	592.0
82.90	112.0
86.90	2100.0
88.00	1950.0
90.80	376.0
92.00	1632.0
93.00	2610.0
94.00	6451.0
95.00	53720.0
96.00	3376.0
97.00	160.0
103.90	371.0
104.80	152.0
105.00	141.0
105.90	379.0
106.90	126.0
109.80	189.0
110.90	106.0
112.20	103.0
112.90	123.0
114.90	120.0
115.90	289.0
116.80	495.0
117.90	228.0
118.80	368.0
128.00	182.0
129.70	210.0
130.80	132.0
134.80	135.0
136.90	181.0
140.90	720.0
141.80	121.0
142.90	920.0
144.90	149.0
146.10	116.0
147.80	213.0
152.90	116.0
154.80	130.0
157.00	132.0
159.10	111.0
170.70	123.0
172.00	513.0
173.00	631.0
173.90	42296.0
174.90	3451.0
175.90	41744.0
176.90	2996.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
35.20	110.0
35.90	554.0
37.00	3079.0
38.00	2424.0
39.00	1092.0
39.90	551.0
41.00	227.0
42.70	145.0
43.90	791.0
45.00	671.0
46.10	114.0
47.00	721.0
47.80	436.0
49.00	2740.0
50.00	11400.0
51.00	3349.0
52.00	205.0
52.80	145.0
54.90	208.0
56.00	786.0
57.00	1445.0
58.10	146.0
59.10	103.0
59.80	636.0
61.00	2960.0
62.00	2602.0
63.00	2080.0
64.10	352.0
65.00	313.0
65.90	164.0
67.10	217.0
68.00	5744.0
69.00	5873.0
70.00	421.0
70.90	137.0
71.90	402.0
73.00	2362.0
74.00	9641.0
75.00	27808.0
76.00	2428.0
77.00	398.0
77.90	291.0
78.90	2039.0
79.90	629.0
80.80	1871.0
81.90	569.0
86.90	2294.0
88.00	1924.0
90.80	418.0
92.00	1678.0
92.90	2583.0
94.00	6231.0
95.00	53192.0
96.00	3044.0
96.90	191.0
103.80	307.0
104.70	177.0
105.90	382.0
109.80	154.0
114.60	110.0
114.80	104.0
115.90	282.0
116.80	493.0
117.90	269.0
118.90	370.0
128.00	173.0
128.80	108.0
129.80	229.0
131.00	133.0
134.70	165.0
136.90	151.0
140.80	633.0
141.80	162.0
142.90	801.0
144.80	155.0
146.10	100.0
147.80	248.0
152.90	118.0
154.80	176.0
157.00	129.0
170.70	131.0
172.00	459.0
173.00	700.0
173.90	43488.0
174.90	3484.0
175.90	42448.0
176.90	2902.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
35.00	143.0
35.60	101.0
36.30	111.0
37.00	116.0
37.50	123.0
38.10	105.0
38.60	161.0
39.20	110.0
39.90	394.0
41.70	175.0
43.90	377.0
45.20	113.0
45.80	108.0
48.70	105.0
50.20	122.0
53.10	124.0
53.80	110.0
54.50	127.0
56.80	119.0
75.80	105.0
99.50	114.0
109.80	107.0
148.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83