

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031461.D
 Acq On : 08 Jun 2023 20:54
 Operator : SY/MD
 Sample : 03106-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FC9

Quant Time: Jun 09 06:34:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 09 06:27:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	239112	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	248687	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	117987	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	79437	37.759	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	75.520%		
7) Chloroethane-d5	1.532	69	81952	48.115	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.240%		
11) 1,1-Dichloroethene-d2	2.060	65	41759	41.882	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.760%		
21) 2-Butanone-d5	3.796	46	144720	95.186	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	95.190%		
24) Chloroform-d	4.256	84	193241	48.289	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.580%		
26) 1,2-Dichloroethane-d4	4.944	65	134124	49.961	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.920%		
32) Benzene-d6	4.963	84	337344	45.946	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.900%		
36) 1,2-Dichloropropane-d6	5.992	67	124739	48.877	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.760%		
41) Toluene-d8	7.249	98	286260	42.442	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.880%		
43) trans-1,3-Dichloroprop...	7.558	79	51604	40.142	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.280%		
47) 2-Hexanone-d5	8.030	63	71437	74.319	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	74.320%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	140537	43.635	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.260%		
66) 1,2-Dichlorobenzene-d4	11.567	152	114992	52.539	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.080%		
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.063	96	1195	1.253	ug/L	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031461.D
Acq On : 08 Jun 2023 20:54
Operator : SY/MD
Sample : 03106-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FC9

Quant Time: Jun 09 06:34:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 09 06:27:10 2023
Response via : Initial Calibration

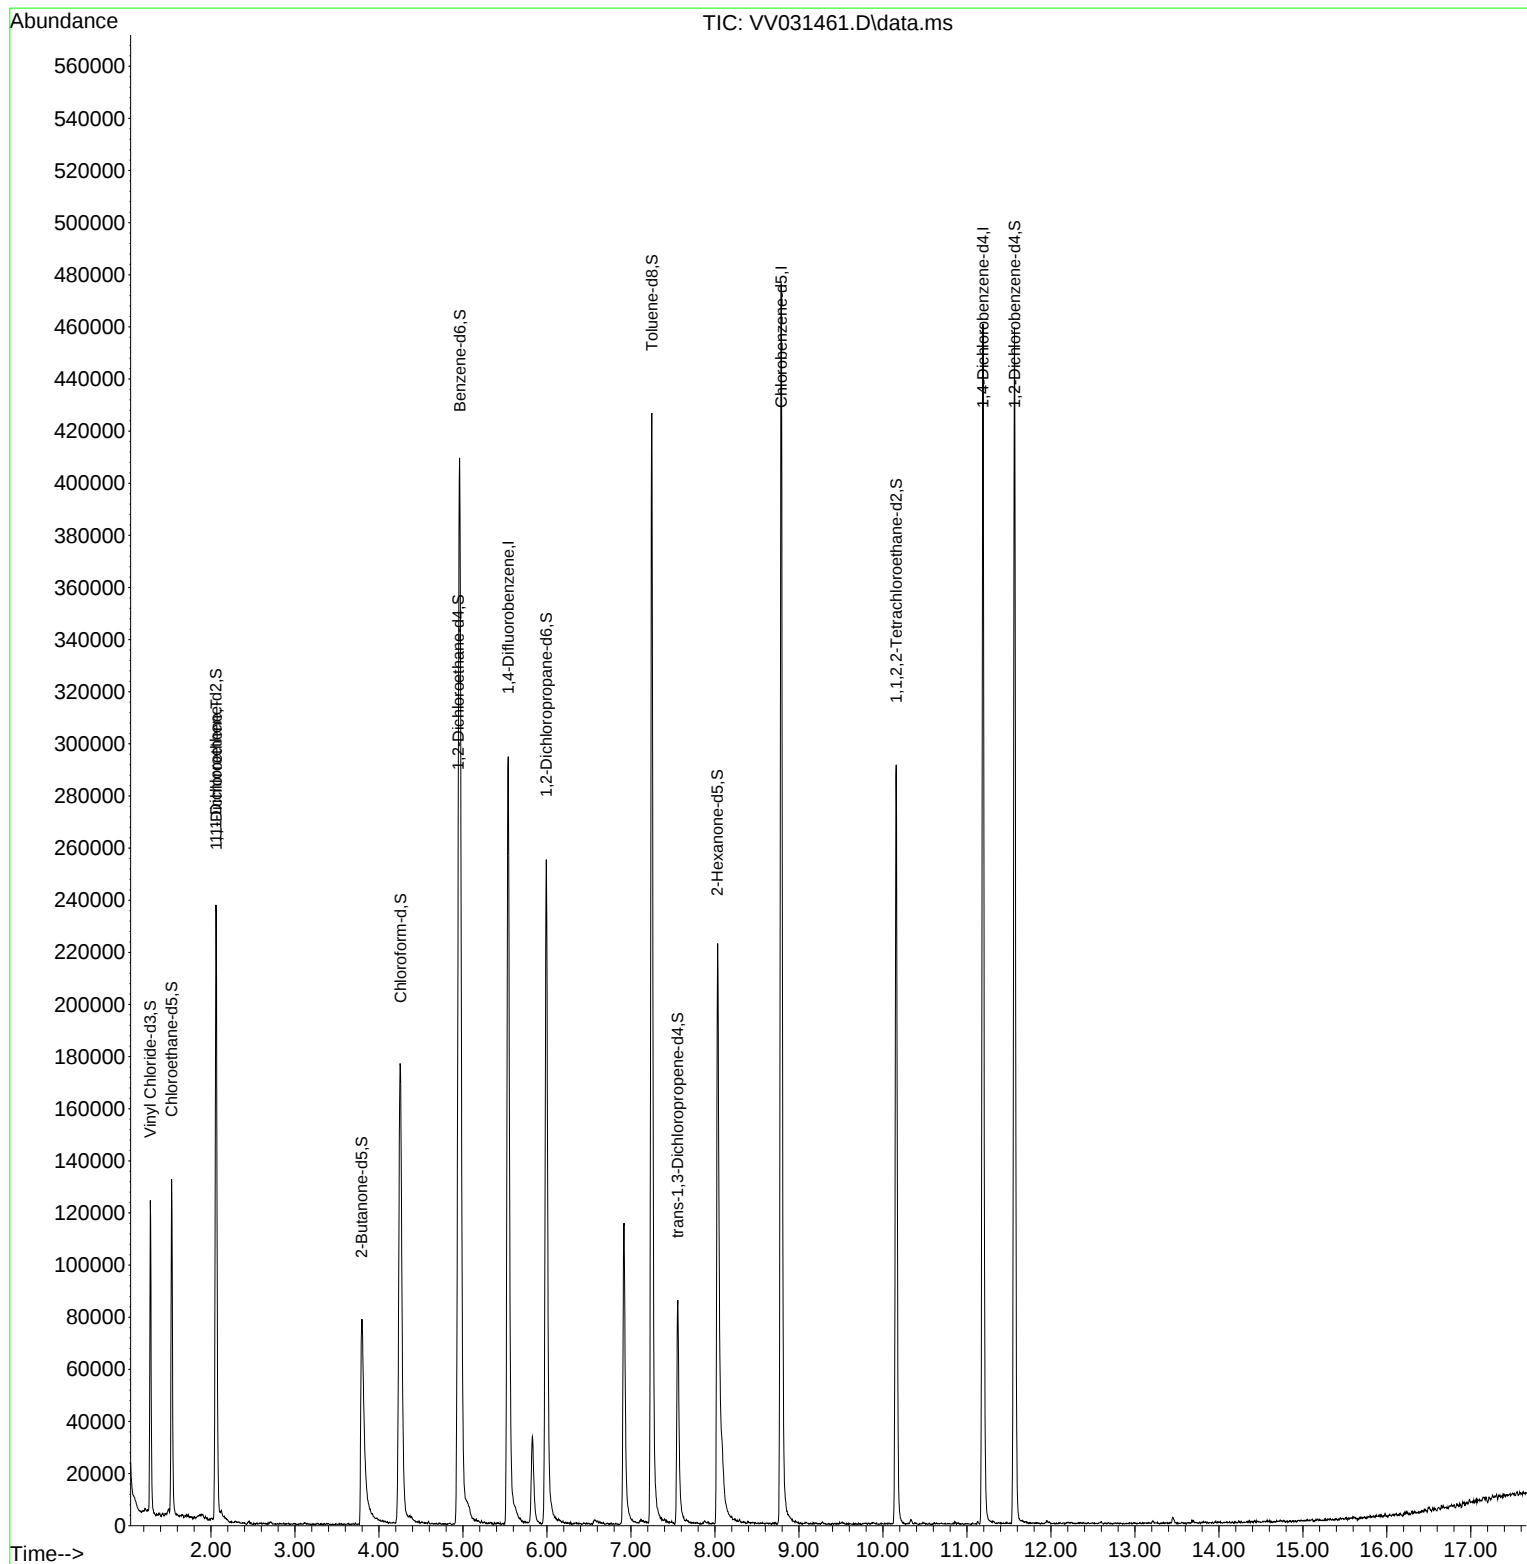

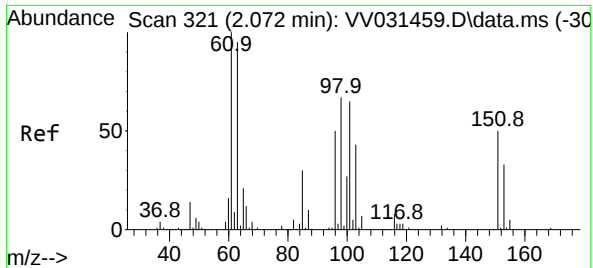

#12
 1,1-Dichloroethene
 Concen: 1.253 ug/L
 RT: 2.063 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV031461.D
 Acq: 08 Jun 2023 20:54

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FC9

Tgt Ion: 96 Resp: 1195
 Ion Ratio Lower Upper
 96 100
 61 1275.4 143.9 267.3#
 63 9783.5 158.3 293.9#

