




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031467.D
 Acq On : 08 Jun 2023 23:16
 Operator : SY/MD
 Sample : 03106-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD8

Manual IntegrationsAPPROVED

Quant Time: Jun 09 06:54:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 09 06:27:10 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 06/09/2023
 Supervised By :Mahesh Dadoda 06/09/2023

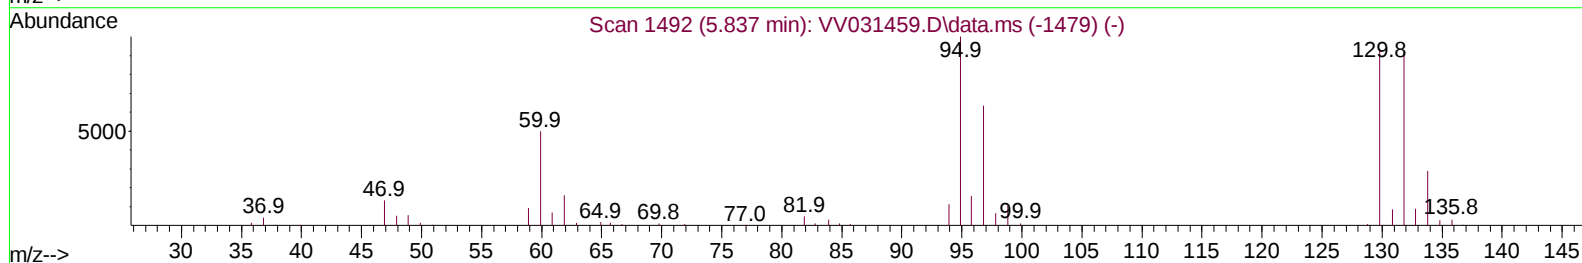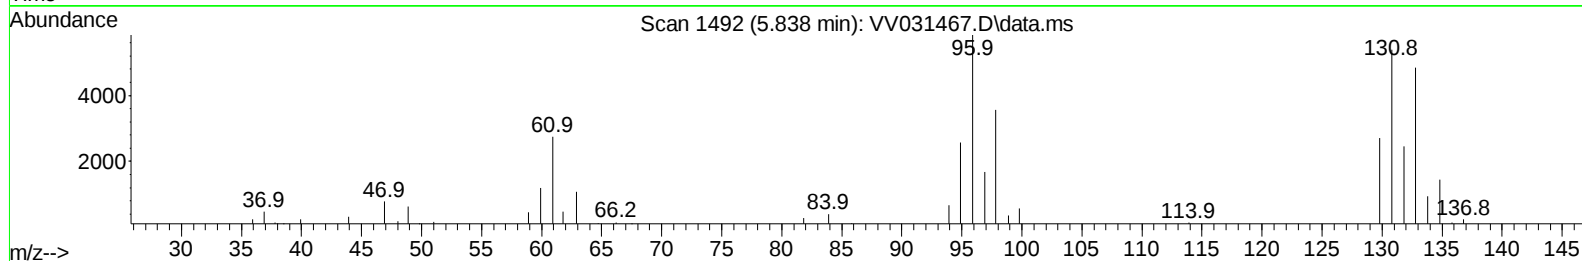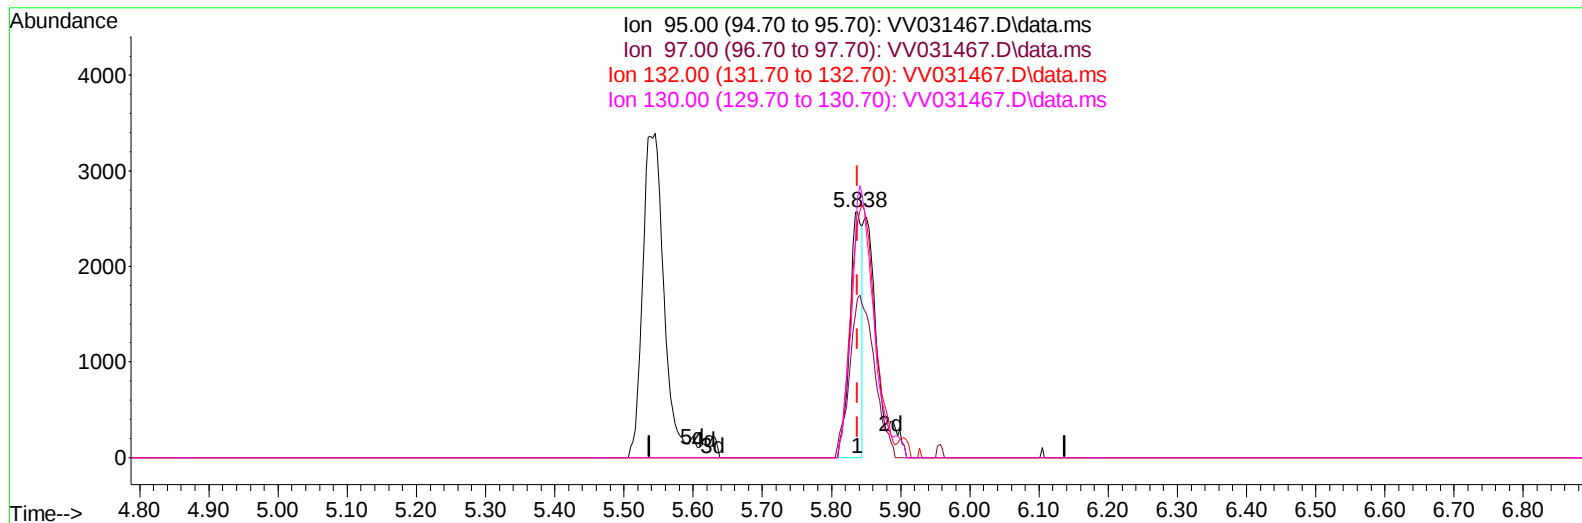

TIC: VV031467.D\data.ms

(34) Trichloroethene (T)

5.838min (+ 0.000) 1.92 ug/L

response 3149

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	63.10	64.88
132.00	91.70	95.41
130.00	95.30	105.48




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031467.D
Acq On : 08 Jun 2023 23:16
Operator : SY/MD
Sample : 03106-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD8

Manual IntegrationsAPPROVED

Quant Time: Jun 09 06:54:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 09 06:27:10 2023
Response via : Initial Calibration

Reviewed By :John Carlone 06/09/2023
Supervised By :Mahesh Dadoda 06/09/2023

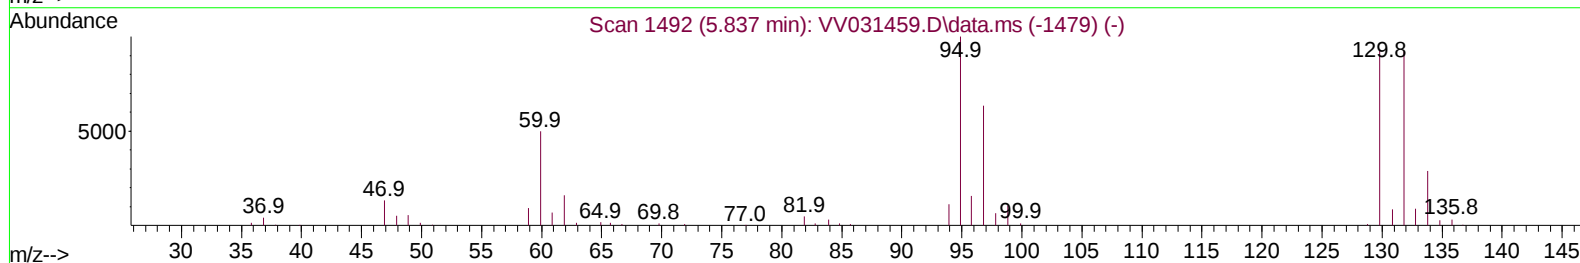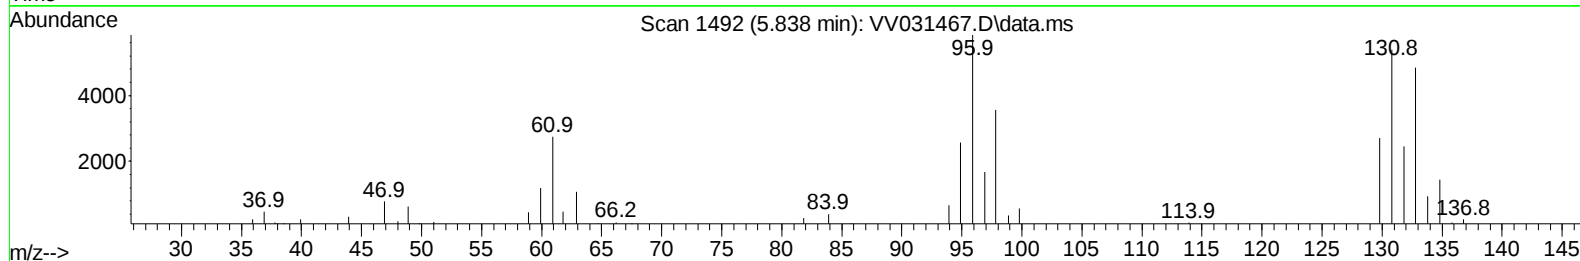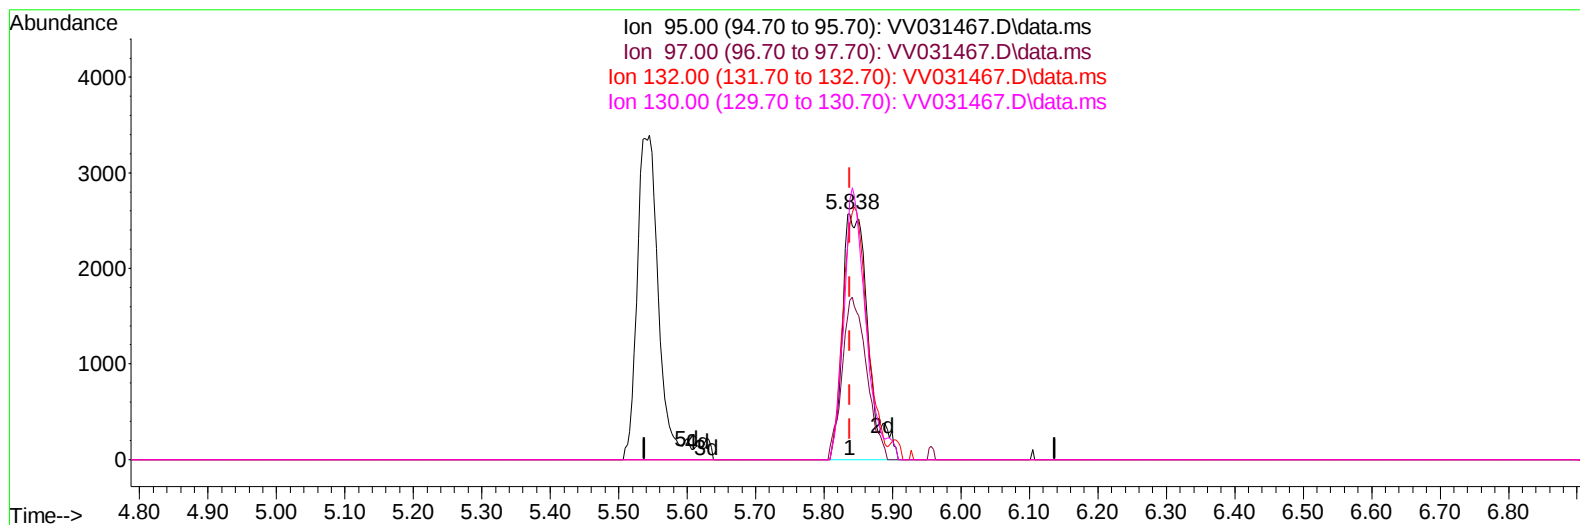

TIC: VV031467.D\data.ms

(34) Trichloroethene (T)

5.838min (+ 0.000) 4.05 ug/L m

response 6636

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	63.10	64.88
132.00	91.70	95.41
130.00	95.30	105.48

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031467.D
 Acq On : 08 Jun 2023 23:16
 Operator : SY/MD
 Sample : 03106-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD8

Manual IntegrationsAPPROVED

Quant Time: Jun 09 06:54:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 09 06:27:10 2023
 Response via : Initial Calibration

Reviewed By : John Carlone 06/09/2023
 Supervised By : Mahesh Dadoda 06/09/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	232236	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	235798	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	111260	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	77934	38.141	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	76.280%	
7) Chloroethane-d5	1.532	69	77357	46.762	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	93.520%	
11) 1,1-Dichloroethene-d2	2.063	65	41947	43.316	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	86.640%	
21) 2-Butanone-d5	3.796	46	149194	101.034	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	101.030%	
24) Chloroform-d	4.256	84	192855	49.619	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	99.240%	
26) 1,2-Dichloroethane-d4	4.950	65	134510	51.588	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	103.180%	
32) Benzene-d6	4.966	84	333857	47.956	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.920%	
36) 1,2-Dichloropropane-d6	5.995	67	123608	51.081	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	102.160%	
41) Toluene-d8	7.249	98	287105	44.894	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	89.780%	
43) trans-1,3-Dichloroprop...	7.558	79	52279	42.889	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.780%	
47) 2-Hexanone-d5	8.034	63	76593	84.039	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	84.040%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	142297	46.596	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	93.200%	
66) 1,2-Dichlorobenzene-d4	11.567	152	115224	55.828	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	111.660%	
Target Compounds						
25) Chloroform	4.288	83	7057	2.083	ug/L	Qvalue 98
34) Trichloroethene	5.838	95	6636m	4.048	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031467.D
Acq On : 08 Jun 2023 23:16
Operator : SY/MD
Sample : 03106-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD8

Manual IntegrationsAPPROVED

Quant Time: Jun 09 06:54:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 09 06:27:10 2023
Response via : Initial Calibration

Reviewed By :John Carlone 06/09/2023
Supervised By :Mahesh Dadoda 06/09/2023

