

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060823\
 Data File : VW031458.D
 Acq On : 08 Jun 2023 19:01
 Operator : SY/MD
 Sample : 03098-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEQ1

Quant Time: Jun 09 05:13:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 09 05:07:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	183569	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	192536	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	90153	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	62133	38.470	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.940%
7) Chloroethane-d5	1.532	69	64163	49.069	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.140%
11) 1,1-Dichloroethene-d2	2.063	65	33291	43.491	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.980%
21) 2-Butanone-d5	3.796	46	134009	114.810	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	114.810%
24) Chloroform-d	4.256	84	163226	53.130	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.260%
26) 1,2-Dichloroethane-d4	4.947	65	115544	56.062	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	112.120%
32) Benzene-d6	4.966	84	278118	48.926	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.860%
36) 1,2-Dichloropropane-d6	5.995	67	103912	52.591	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.180%
41) Toluene-d8	7.249	98	229806	44.009	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.020%
43) trans-1,3-Dichloroprop...	7.558	79	44622	44.833	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.660%
47) 2-Hexanone-d5	8.034	63	67331	90.476	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.480%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	130786	52.450	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	104.900%
66) 1,2-Dichlorobenzene-d4	11.567	152	90161	53.912	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.820%
Target Compounds						
13) Acetone	2.127	43	3682	3.526	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031458.D
Acq On : 08 Jun 2023 19:01
Operator : SY/MD
Sample : 03098-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEQ1

Quant Time: Jun 09 05:13:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 09 05:07:24 2023
Response via : Initial Calibration

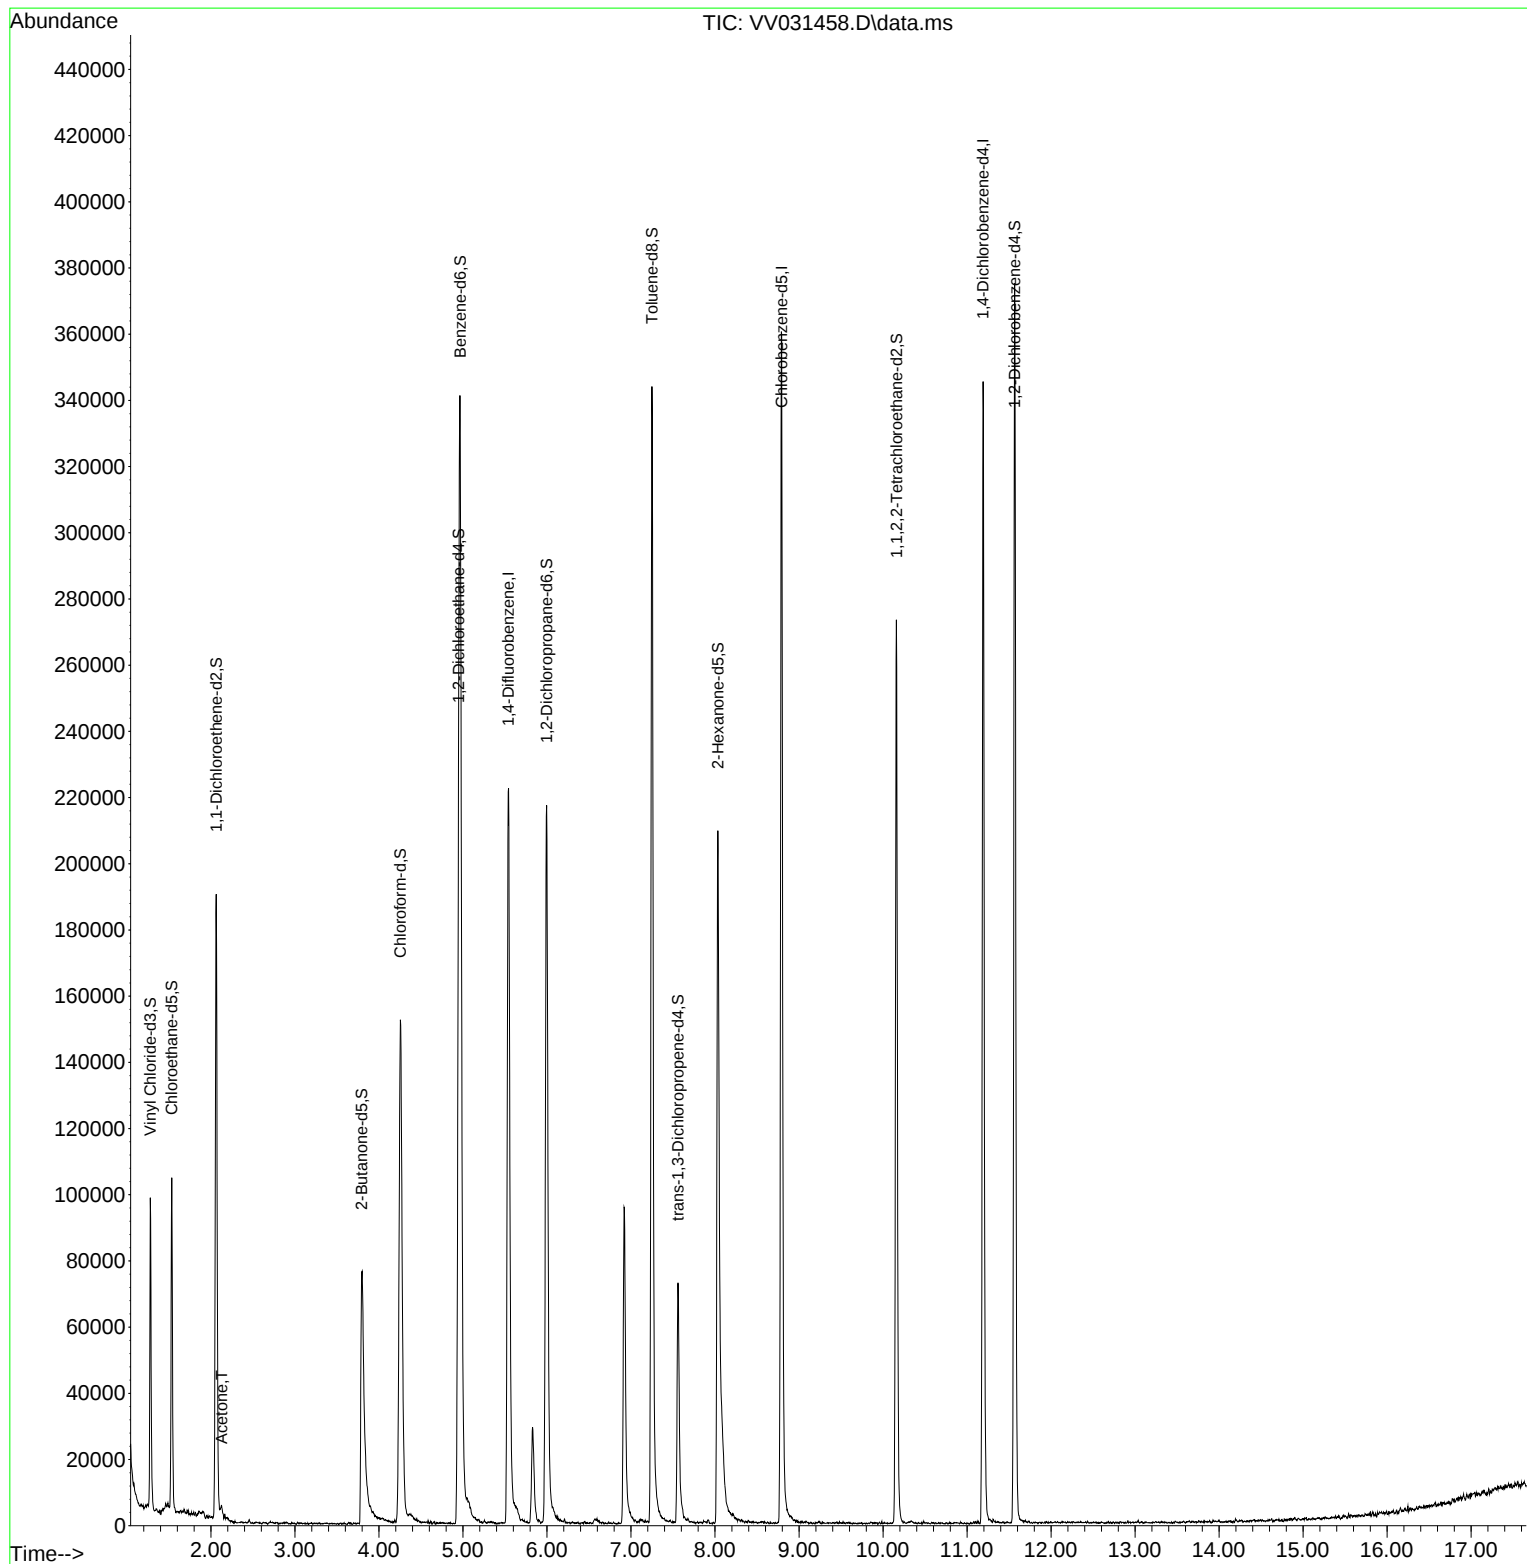

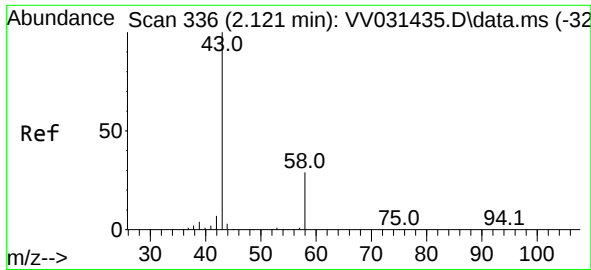

#13

Acetone

Concen: 3.526 ug/L

RT: 2.127 min Scan# 31

Delta R.T. 0.006 min

Lab File: VV031458.D


Acq: 08 Jun 2023 19:01

Instrument :

MSVOA_V

ClientSampleId :

EZEQ1

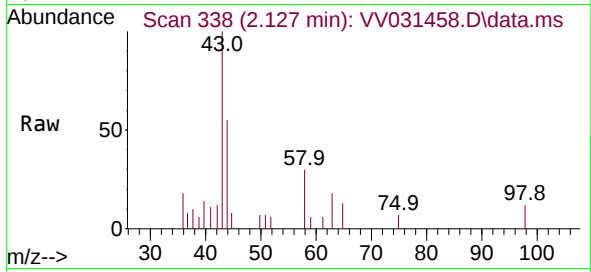

Tgt Ion: 43 Resp: 3682

Ion Ratio Lower Upper

43 100

58 23.5 0.0 61.0

