

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031437.D
 Acq On : 08 Jun 2023 10:22
 Operator : SY/MD
 Sample : 02992-05DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C02DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

Signal : TIC: VV031437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	140759	149175	13.21%	1.673%
2	1.532	146	153	165	rVB	125403	148628	13.16%	1.667%
3	2.060	307	317	331	rBV	260548	384113	34.02%	4.309%
4	2.394	418	421	425	rBV4	940	753	0.07%	0.008%
5	2.561	469	473	476	rBV4	880	679	0.06%	0.008%
6	2.709	507	519	535	rVV2	16699	35342	3.13%	0.396%
7	2.825	553	555	560	rVB3	386	252	0.02%	0.003%
8	2.873	567	570	572	rBV	247	148	0.01%	0.002%
9	2.928	586	587	591	rBV2	241	178	0.02%	0.002%
10	3.002	608	610	611	rBV	258	141	0.01%	0.002%
11	3.034	618	620	621	rBV	372	160	0.01%	0.002%
12	3.104	638	642	644	rBV	425	276	0.02%	0.003%
13	3.211	673	675	679	rVB2	377	239	0.02%	0.003%
14	3.233	679	682	684	rBV2	360	208	0.02%	0.002%
15	3.275	693	695	699	rVV2	280	153	0.01%	0.002%
16	3.349	715	718	721	rBV3	382	243	0.02%	0.003%
17	3.522	768	772	774	rBV	470	337	0.03%	0.004%
18	3.606	794	798	800	rBV	524	385	0.03%	0.004%
19	3.731	836	837	840	rBV2	291	138	0.01%	0.002%
20	3.793	846	856	892	rBV	87556	270578	23.97%	3.035%
21	4.252	984	999	1028	rBV	181233	474277	42.01%	5.321%
22	4.651	1120	1123	1124	rBV	305	152	0.01%	0.002%
23	4.703	1137	1139	1145	rVB3	464	433	0.04%	0.005%
24	4.773	1155	1161	1163	rBV3	423	465	0.04%	0.005%
25	4.805	1169	1171	1173	rBV2	436	253	0.02%	0.003%
26	4.960	1202	1219	1244	rBV2	420589	1129008	100.00%	12.665%
27	5.371	1344	1347	1350	rVB2	501	261	0.02%	0.003%
28	5.538	1387	1399	1441	rBV	302149	643534	57.00%	7.219%
29	5.738	1459	1461	1463	rBV2	658	290	0.03%	0.003%
30	5.831	1480	1490	1506	rBV5	38417	84322	7.47%	0.946%
31	5.992	1527	1540	1559	rBV	258485	535570	47.44%	6.008%
32	6.313	1638	1640	1642	rVB2	526	215	0.02%	0.002%
33	6.352	1649	1652	1656	rBV3	412	298	0.03%	0.003%
34	6.384	1659	1662	1663	rVB	526	216	0.02%	0.002%
35	6.400	1665	1667	1671	rBV2	526	272	0.02%	0.003%
36	6.519	1701	1704	1707	rBV3	212	155	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031437.D
 Acq On : 08 Jun 2023 10:22
 Operator : SY/MD
 Sample : 02992-05DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C02DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.567	1716	1719	1721	rBV	341	214	0.02%	0.002%
38	6.577	1721	1722	1725	rVV2	626	285	0.03%	0.003%
39	6.593	1725	1727	1728	rVV	371	150	0.01%	0.002%
40	6.603	1728	1730	1733	rVB	537	268	0.02%	0.003%
41	6.667	1746	1750	1755	rVB3	467	436	0.04%	0.005%
42	6.699	1756	1760	1761	rBV2	618	356	0.03%	0.004%
43	6.780	1782	1785	1787	rBV3	510	268	0.02%	0.003%
44	6.815	1793	1796	1801	rBV3	465	296	0.03%	0.003%
45	6.918	1816	1828	1847	rBV	128297	245525	21.75%	2.754%
46	7.249	1919	1931	1957	rBV	468326	829253	73.45%	9.303%
47	7.558	2017	2027	2049	rBV	97279	176853	15.66%	1.984%
48	7.789	2096	2099	2103	rBV4	632	583	0.05%	0.007%
49	7.821	2107	2109	2112	rBV	253	141	0.01%	0.002%
50	7.841	2112	2115	2118	rBV3	483	309	0.03%	0.003%
51	7.911	2122	2137	2156	rBV	232096	401890	35.60%	4.508%
52	8.034	2165	2175	2215	rBV2	245733	547352	48.48%	6.140%
53	8.506	2320	2322	2325	rBV4	950	491	0.04%	0.006%
54	8.542	2331	2333	2338	rVB3	687	335	0.03%	0.004%
55	8.577	2342	2344	2346	rBV	457	158	0.01%	0.002%
56	8.612	2353	2355	2357	rBV3	391	184	0.02%	0.002%
57	8.641	2361	2364	2366	rBV3	956	469	0.04%	0.005%
58	8.734	2390	2393	2396	rBV2	542	331	0.03%	0.004%
59	8.789	2398	2410	2444	rVV	479637	815595	72.24%	9.149%
60	9.021	2475	2482	2484	rBV4	844	824	0.07%	0.009%
61	9.197	2534	2537	2541	rBV2	464	348	0.03%	0.004%
62	9.239	2548	2550	2551	rBV2	426	213	0.02%	0.002%
63	9.265	2556	2558	2560	rVB	543	215	0.02%	0.002%
64	9.281	2560	2563	2565	rBV	615	343	0.03%	0.004%
65	9.307	2569	2571	2573	rBV2	307	150	0.01%	0.002%
66	9.455	2615	2617	2619	rBV	395	210	0.02%	0.002%
67	9.487	2625	2627	2631	rBV	611	353	0.03%	0.004%
68	9.509	2631	2634	2636	rBV2	567	363	0.03%	0.004%
69	9.632	2669	2672	2673	rBV3	508	259	0.02%	0.003%
70	9.661	2677	2681	2683	rBV3	453	311	0.03%	0.003%
71	9.725	2698	2701	2702	rBV3	381	234	0.02%	0.003%
72	9.831	2732	2734	2737	rVB3	465	191	0.02%	0.002%
73	9.931	2763	2765	2767	rVB	526	206	0.02%	0.002%
74	9.966	2773	2776	2779	rVB2	412	248	0.02%	0.003%
75	10.159	2821	2836	2859	rBV	304872	489476	43.35%	5.491%
76	10.326	2882	2888	2892	rBV3	612	638	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031437.D
 Acq On : 08 Jun 2023 10:22
 Operator : SY/MD
 Sample : 02992-05DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C02DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.384	2903	2906	2907	rBV	294	159	0.01%	0.002%
78	10.406	2911	2913	2917	rVB2	453	245	0.02%	0.003%
79	10.442	2922	2924	2928	rBV2	324	188	0.02%	0.002%
80	10.593	2969	2971	2975	rVB2	498	292	0.03%	0.003%
81	10.725	3010	3012	3015	rBV2	441	224	0.02%	0.003%
82	10.773	3025	3027	3031	rVB2	487	211	0.02%	0.002%
83	10.992	3091	3095	3102	rVB3	602	683	0.06%	0.008%
84	11.033	3106	3108	3110	rVB2	503	214	0.02%	0.002%
85	11.053	3110	3114	3117	rBV2	370	318	0.03%	0.004%
86	11.120	3128	3135	3137	rBV3	626	607	0.05%	0.007%
87	11.133	3137	3139	3142	rVV2	953	607	0.05%	0.007%
88	11.191	3146	3157	3179	rBV	470538	752543	66.66%	8.442%
89	11.410	3223	3225	3228	rBV2	755	467	0.04%	0.005%
90	11.439	3231	3234	3235	rBV2	356	196	0.02%	0.002%
91	11.567	3262	3274	3302	rBV	489564	771250	68.31%	8.652%
92	11.718	3319	3321	3323	rBV2	716	293	0.03%	0.003%
93	11.731	3323	3325	3327	rBV2	502	216	0.02%	0.002%
94	11.943	3389	3391	3394	rBV2	430	235	0.02%	0.003%
95	11.979	3400	3402	3403	rBV	392	191	0.02%	0.002%
96	12.529	3571	3573	3577	rBV	380	317	0.03%	0.004%
97	12.770	3645	3648	3651	rBV2	601	460	0.04%	0.005%
98	13.213	3781	3786	3791	rVB4	1459	1424	0.13%	0.016%
99	13.451	3854	3860	3870	rVB5	3111	4329	0.38%	0.049%
100	13.599	3904	3906	3909	rBV2	514	281	0.02%	0.003%




Sum of corrected areas: 8914121

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031437.D
Acq On : 08 Jun 2023 10:22
Operator : SY/MD
Sample : 02992-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C02DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

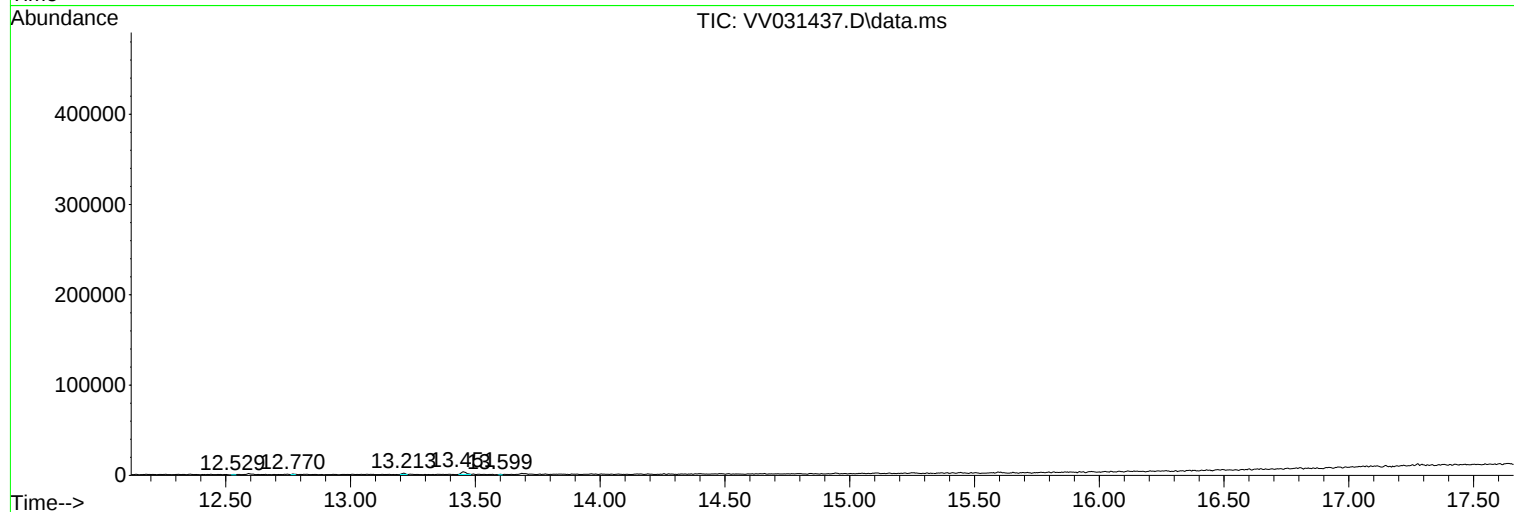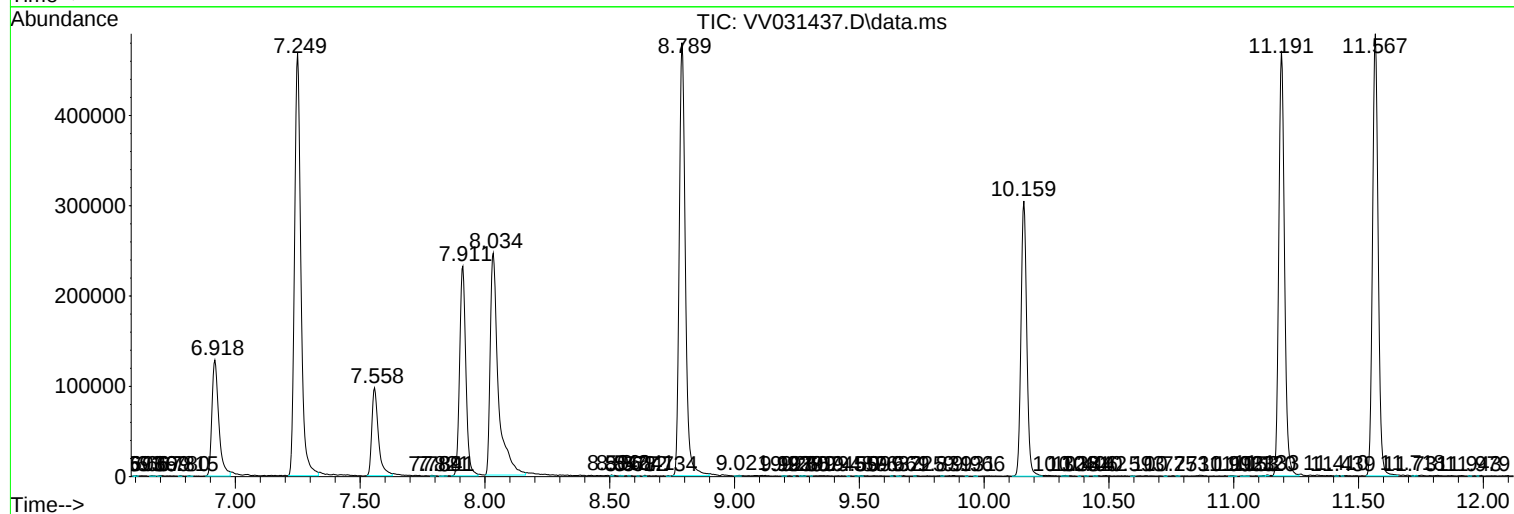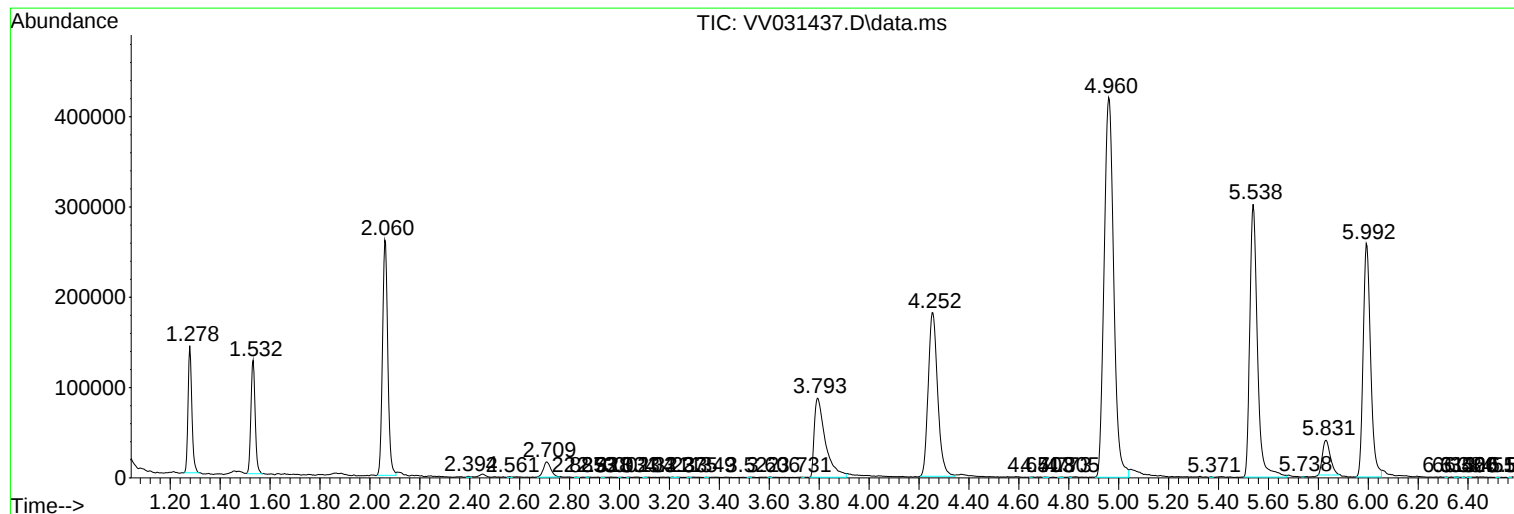

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031437.D
Acq On : 08 Jun 2023 10:22
Operator : SY/MD
Sample : 02992-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C02DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031437.D
Acq On : 08 Jun 2023 10:22
Operator : SY/MD
Sample : 02992-05DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C02DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------