

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031438.D
 Acq On : 08 Jun 2023 10:46
 Operator : SY/MD
 Sample : 02992-09DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C11DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

Signal : TIC: VV031438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	137563	149926	13.61%	1.667%
2	1.532	146	153	167	rVB	121160	142713	12.96%	1.587%
3	2.060	308	317	333	rBV	252972	369011	33.50%	4.103%
4	2.449	431	438	443	rBV5	3399	4855	0.44%	0.054%
5	2.548	465	469	470	rBV2	915	630	0.06%	0.007%
6	2.700	511	516	525	rBV7	2406	4374	0.40%	0.049%
7	2.770	536	538	545	rVB2	369	293	0.03%	0.003%
8	2.970	599	600	604	rVB2	551	279	0.03%	0.003%
9	2.992	605	607	611	rVB2	353	219	0.02%	0.002%
10	3.015	611	614	616	rBV2	479	270	0.02%	0.003%
11	3.114	642	645	648	rVB2	697	434	0.04%	0.005%
12	3.140	650	653	655	rBV2	435	297	0.03%	0.003%
13	3.163	658	660	663	rVB3	398	240	0.02%	0.003%
14	3.217	675	677	681	rVB3	389	280	0.03%	0.003%
15	3.240	681	684	687	rBV2	479	313	0.03%	0.003%
16	3.391	727	731	733	rBV2	344	258	0.02%	0.003%
17	3.442	743	747	748	rBV2	327	206	0.02%	0.002%
18	3.593	791	794	798	rBV3	438	287	0.03%	0.003%
19	3.629	803	805	812	rVB	413	396	0.04%	0.004%
20	3.709	829	830	833	rBV2	419	170	0.02%	0.002%
21	3.796	846	857	883	rBV	95399	294955	26.78%	3.280%
22	4.169	971	973	979	rBV2	452	252	0.02%	0.003%
23	4.256	984	1000	1023	rBV	176145	460195	41.78%	5.117%
24	4.674	1128	1130	1133	rBV2	376	179	0.02%	0.002%
25	4.751	1152	1154	1155	rVB	561	172	0.02%	0.002%
26	4.770	1155	1160	1163	rBV2	440	466	0.04%	0.005%
27	4.963	1202	1220	1242	rBV2	414376	1101437	100.00%	12.247%
28	5.314	1327	1329	1331	rBV	371	225	0.02%	0.003%
29	5.388	1350	1352	1355	rVB2	479	262	0.02%	0.003%
30	5.423	1360	1363	1366	rVV3	760	441	0.04%	0.005%
31	5.455	1371	1373	1378	rVB2	861	566	0.05%	0.006%
32	5.481	1378	1381	1385	rBV3	524	419	0.04%	0.005%
33	5.539	1385	1399	1419	rBV	291470	607525	55.16%	6.755%
34	5.838	1478	1492	1513	rBV6	76387	184617	16.76%	2.053%
35	5.995	1528	1541	1560	rBV	253968	529716	48.09%	5.890%
36	6.288	1628	1632	1635	rVB2	532	384	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031438.D
 Acq On : 08 Jun 2023 10:46
 Operator : SY/MD
 Sample : 02992-09DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C11DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.323	1640	1643	1644	rBV2	460	186	0.02%	0.002%
38	6.381	1659	1661	1663	rBV2	576	307	0.03%	0.003%
39	6.420	1670	1673	1676	rBV3	445	330	0.03%	0.004%
40	6.468	1686	1688	1691	rVB2	643	289	0.03%	0.003%
41	6.535	1705	1709	1712	rBV2	433	402	0.04%	0.004%
42	6.654	1744	1746	1753	rVB4	588	552	0.05%	0.006%
43	6.687	1753	1756	1762	rBV4	672	783	0.07%	0.009%
44	6.806	1787	1793	1795	rBV2	498	411	0.04%	0.005%
45	6.822	1796	1798	1801	rVV2	362	209	0.02%	0.002%
46	6.860	1807	1810	1812	rBV2	383	232	0.02%	0.003%
47	6.918	1816	1828	1850	rBV	122802	238372	21.64%	2.650%
48	7.249	1919	1931	1961	rBV	444959	805211	73.11%	8.953%
49	7.558	2018	2027	2050	rBV2	92990	167826	15.24%	1.866%
50	7.818	2106	2108	2110	rBV2	389	191	0.02%	0.002%
51	7.912	2124	2137	2157	rVV	357613	619539	56.25%	6.889%
52	8.031	2165	2174	2218	rBV2	254537	546541	49.62%	6.077%
53	8.529	2325	2329	2334	rBV5	545	559	0.05%	0.006%
54	8.593	2347	2349	2350	rBV	461	178	0.02%	0.002%
55	8.789	2399	2410	2441	rBV	464421	784724	71.25%	8.725%
56	9.021	2481	2482	2488	rVB2	740	394	0.04%	0.004%
57	9.053	2490	2492	2496	rVB3	823	405	0.04%	0.005%
58	9.137	2514	2518	2520	rVV2	377	269	0.02%	0.003%
59	9.156	2520	2524	2526	rBV3	257	172	0.02%	0.002%
60	9.278	2558	2562	2563	rBV2	474	338	0.03%	0.004%
61	9.346	2580	2583	2586	rBV2	454	299	0.03%	0.003%
62	9.375	2590	2592	2598	rVB5	674	485	0.04%	0.005%
63	9.516	2633	2636	2638	rBV2	845	544	0.05%	0.006%
64	9.680	2683	2687	2689	rBV	514	335	0.03%	0.004%
65	9.690	2689	2690	2697	rVV3	507	463	0.04%	0.005%
66	9.735	2701	2704	2709	rVB2	424	284	0.03%	0.003%
67	9.757	2709	2711	2714	rBV2	288	185	0.02%	0.002%
68	9.776	2714	2717	2720	rBV2	439	260	0.02%	0.003%
69	9.973	2776	2778	2781	rVB3	483	287	0.03%	0.003%
70	9.989	2781	2783	2786	rBV3	373	240	0.02%	0.003%
71	10.021	2789	2793	2794	rBV	374	309	0.03%	0.003%
72	10.066	2804	2807	2809	rBV2	670	503	0.05%	0.006%
73	10.159	2823	2836	2861	rBV	298275	483301	43.88%	5.374%
74	10.439	2920	2923	2925	rBV2	342	230	0.02%	0.003%
75	10.484	2933	2937	2938	rBV2	442	284	0.03%	0.003%
76	10.622	2976	2980	2981	rBV2	258	202	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031438.D
 Acq On : 08 Jun 2023 10:46
 Operator : SY/MD
 Sample : 02992-09DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C11DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.706	3004	3006	3009	rBV3	438	295	0.03%	0.003%
78	10.863	3053	3055	3056	rBV	592	213	0.02%	0.002%
79	11.191	3145	3157	3178	rBV	459823	724496	65.78%	8.056%
80	11.567	3262	3274	3290	rBV	465931	744970	67.64%	8.283%
81	11.918	3379	3383	3387	rBV2	662	495	0.04%	0.006%
82	12.088	3434	3436	3439	rBV3	569	369	0.03%	0.004%
83	12.236	3478	3482	3486	rBV2	663	550	0.05%	0.006%
84	12.259	3487	3489	3492	rVB2	442	227	0.02%	0.003%
85	12.275	3492	3494	3495	rBV	519	216	0.02%	0.002%
86	12.329	3508	3511	3514	rBV3	486	399	0.04%	0.004%
87	12.889	3681	3685	3686	rBV2	682	437	0.04%	0.005%
88	13.072	3740	3742	3745	rBV3	470	228	0.02%	0.003%
89	13.275	3802	3805	3808	rBV2	901	449	0.04%	0.005%
90	13.342	3823	3826	3828	rBV2	793	492	0.04%	0.005%
91	13.355	3828	3830	3833	rVB2	489	185	0.02%	0.002%
92	13.455	3854	3861	3862	rBV3	1315	1316	0.12%	0.015%
93	13.574	3896	3898	3899	rBV	450	173	0.02%	0.002%
94	13.603	3903	3907	3911	rVV4	604	533	0.05%	0.006%
95	13.683	3930	3932	3933	rBV2	828	375	0.03%	0.004%
96	13.802	3966	3969	3972	rVB2	681	439	0.04%	0.005%
97	14.091	4056	4059	4066	rBV5	627	778	0.07%	0.009%
98	14.120	4066	4068	4071	rVB2	839	333	0.03%	0.004%
99	14.140	4071	4074	4078	rBV5	754	726	0.07%	0.008%
100	14.310	4122	4127	4131	rBV5	937	1033	0.09%	0.011%




Sum of corrected areas: 8993620

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031438.D
Acq On : 08 Jun 2023 10:46
Operator : SY/MD
Sample : 02992-09DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C11DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

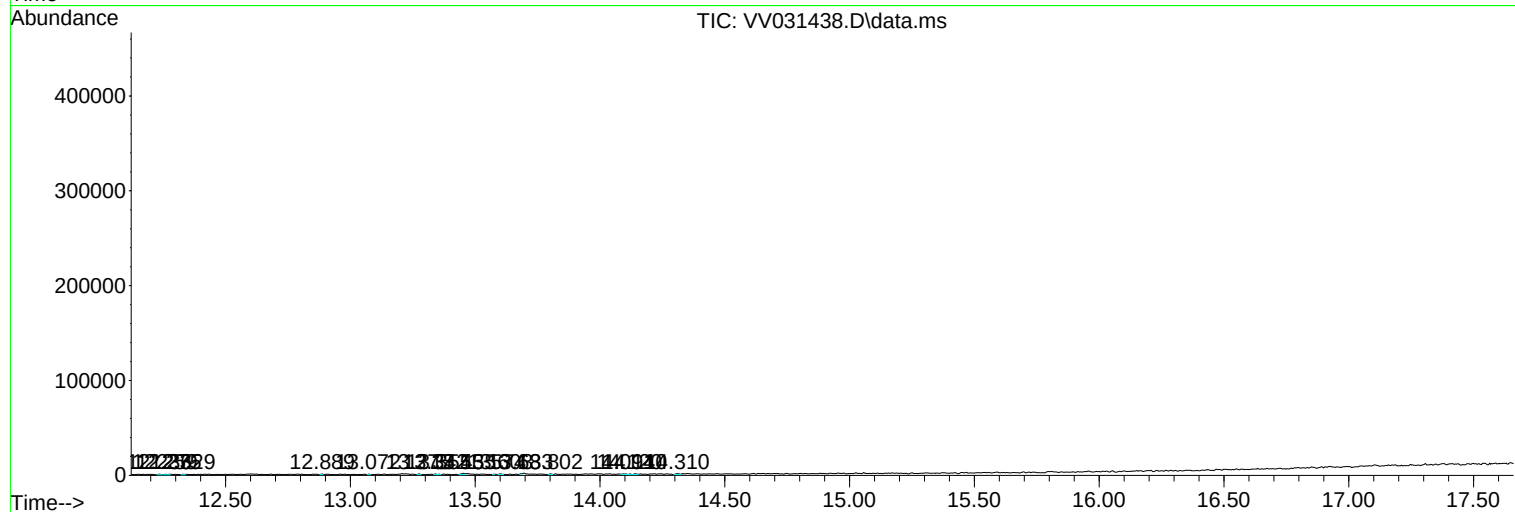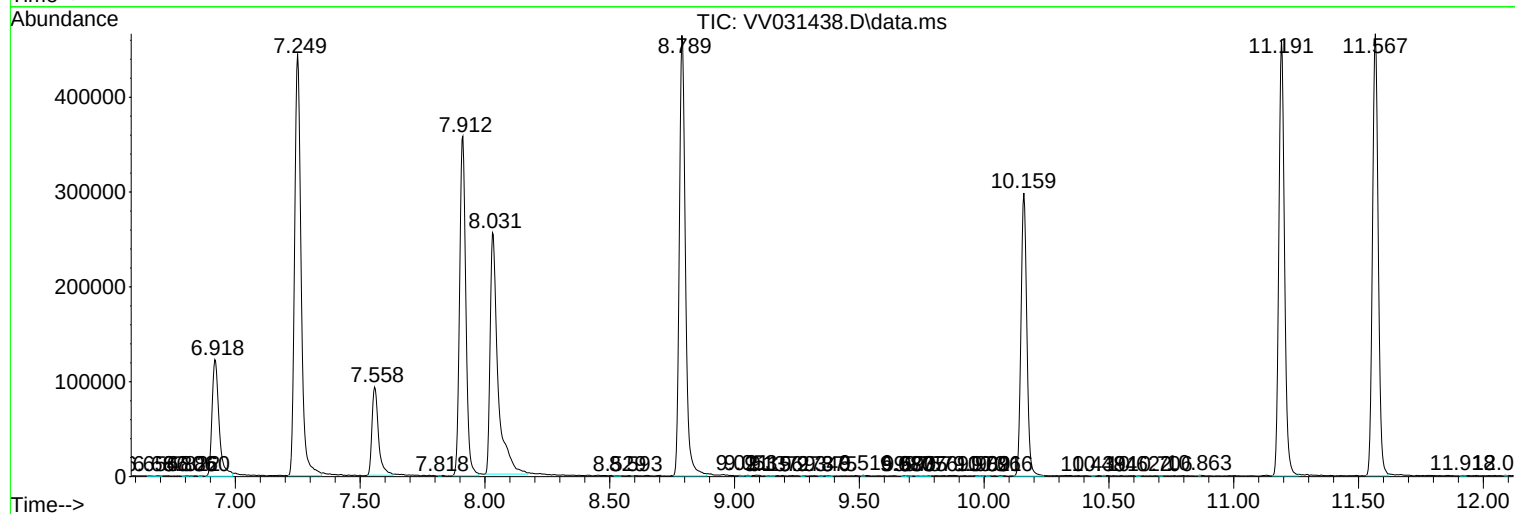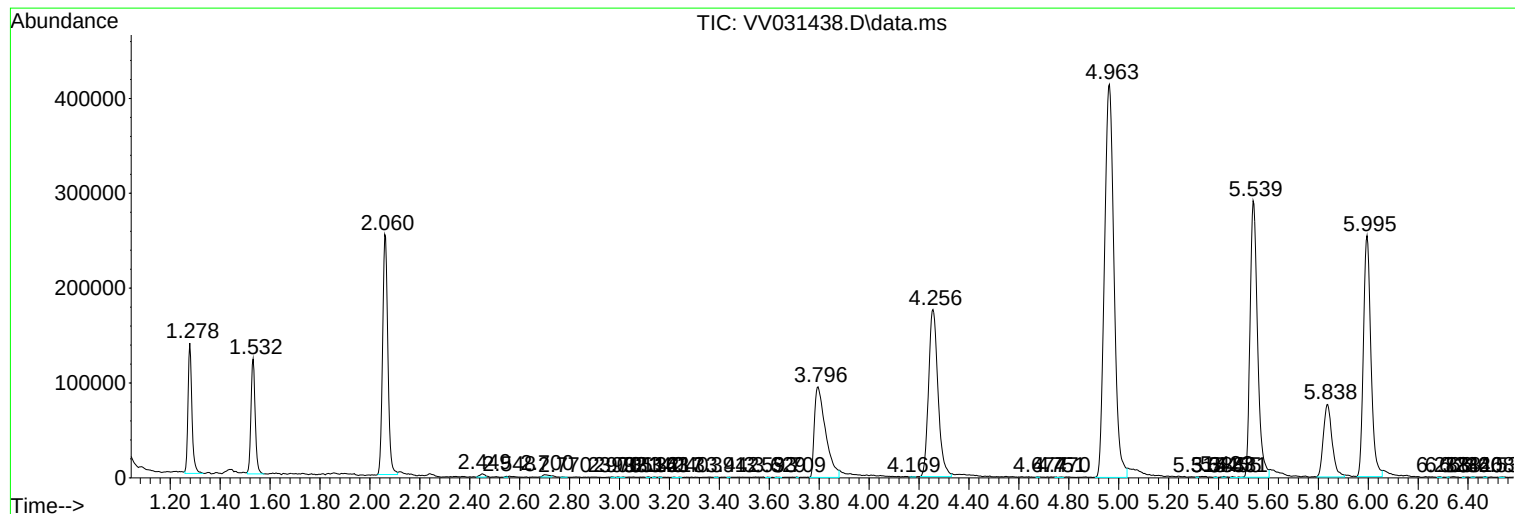

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031438.D
Acq On : 08 Jun 2023 10:46
Operator : SY/MD
Sample : 02992-09DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C11DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031438.D
Acq On : 08 Jun 2023 10:46
Operator : SY/MD
Sample : 02992-09DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C11DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc