

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031439.D
 Acq On : 08 Jun 2023 11:09
 Operator : SY/MD
 Sample : 02992-10 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

Signal : TIC: VV031439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	129604	140238	13.05%	1.546%
2	1.532	146	153	171	rVB	117541	139108	12.94%	1.534%
3	2.060	308	317	334	rBV	246822	358021	33.31%	3.947%
4	2.446	430	437	449	rVB6	2820	5309	0.49%	0.059%
5	2.658	501	503	505	rBV	305	176	0.02%	0.002%
6	2.680	508	510	512	rVV	289	135	0.01%	0.001%
7	2.709	516	519	528	rVB7	1366	1681	0.16%	0.019%
8	2.857	560	565	566	rBV2	343	241	0.02%	0.003%
9	2.892	574	576	579	rBV	253	93	0.01%	0.001%
10	2.957	592	596	597	rBV2	303	197	0.02%	0.002%
11	2.992	605	607	608	rBV2	228	76	0.01%	0.001%
12	3.011	611	613	614	rBV2	315	106	0.01%	0.001%
13	3.066	626	630	631	rBV2	375	263	0.02%	0.003%
14	3.085	634	636	638	rVV	379	168	0.02%	0.002%
15	3.108	641	643	644	rVB	434	104	0.01%	0.001%
16	3.240	681	684	685	rBV	154	85	0.01%	0.001%
17	3.282	694	697	703	rVB3	448	481	0.04%	0.005%
18	3.323	708	710	714	rVB2	300	153	0.01%	0.002%
19	3.346	714	717	718	rBV3	198	112	0.01%	0.001%
20	3.381	723	728	729	rBV3	251	194	0.02%	0.002%
21	3.417	737	739	741	rBV2	614	284	0.03%	0.003%
22	3.455	749	751	754	rVB	513	251	0.02%	0.003%
23	3.474	754	757	761	rBV2	361	247	0.02%	0.003%
24	3.491	761	762	765	rVB	315	151	0.01%	0.002%
25	3.516	765	770	771	rBV	311	244	0.02%	0.003%
26	3.526	771	773	774	rBV	224	104	0.01%	0.001%
27	3.581	788	790	792	rVB	378	122	0.01%	0.001%
28	3.606	792	798	800	rBV3	471	468	0.04%	0.005%
29	3.626	800	804	807	rVB2	689	483	0.04%	0.005%
30	3.642	807	809	810	rBV2	199	99	0.01%	0.001%
31	3.658	810	814	818	rVB2	479	354	0.03%	0.004%
32	3.680	818	821	823	rBV	271	208	0.02%	0.002%
33	3.722	832	834	835	rVB2	339	92	0.01%	0.001%
34	3.793	846	856	890	rBV	91600	293422	27.30%	3.235%
35	4.256	984	1000	1027	rBV2	173587	455522	42.38%	5.022%
36	4.626	1112	1115	1119	rVB4	494	316	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031439.D
 Acq On : 08 Jun 2023 11:09
 Operator : SY/MD
 Sample : 02992-10 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	4.815	1173	1174	1176	rBV	243	79	0.01%	0.001%
38	4.857	1185	1187	1190	rBV4	422	296	0.03%	0.003%
39	4.963	1202	1220	1242	rBV2	404833	1074875	100.00%	11.851%
40	5.359	1341	1343	1345	rVB2	744	361	0.03%	0.004%
41	5.371	1345	1347	1350	rBV2	492	284	0.03%	0.003%
42	5.433	1364	1366	1368	rBV	422	211	0.02%	0.002%
43	5.539	1388	1399	1423	rBV	288915	604977	56.28%	6.670%
44	5.838	1479	1492	1517	rBV2	209349	453597	42.20%	5.001%
45	5.995	1528	1541	1574	rBV	253623	527281	49.06%	5.814%
46	6.249	1619	1620	1623	rBV2	394	229	0.02%	0.003%
47	6.281	1629	1630	1632	rVB	254	50	0.00%	0.001%
48	6.294	1632	1634	1637	rBV3	581	326	0.03%	0.004%
49	6.362	1653	1655	1662	rVB3	993	815	0.08%	0.009%
50	6.394	1662	1665	1667	rBV2	404	210	0.02%	0.002%
51	6.407	1667	1669	1670	rBV	411	185	0.02%	0.002%
52	6.506	1696	1700	1704	rBV3	378	442	0.04%	0.005%
53	6.551	1712	1714	1715	rBV	305	122	0.01%	0.001%
54	6.577	1720	1722	1725	rBV	390	260	0.02%	0.003%
55	6.690	1755	1757	1758	rBV	412	161	0.01%	0.002%
56	6.725	1765	1768	1770	rVB	288	164	0.02%	0.002%
57	6.780	1781	1785	1788	rBV	581	413	0.04%	0.005%
58	6.847	1803	1806	1808	rBV3	414	294	0.03%	0.003%
59	6.860	1808	1810	1813	rVB2	348	162	0.02%	0.002%
60	6.918	1817	1828	1846	rBV	123553	232980	21.68%	2.569%
61	7.172	1905	1907	1913	rVB4	788	635	0.06%	0.007%
62	7.249	1919	1931	1954	rBV	437032	783711	72.91%	8.641%
63	7.558	2017	2027	2050	rBV	91557	169465	15.77%	1.868%
64	7.735	2079	2082	2084	rBV3	584	369	0.03%	0.004%
65	7.912	2124	2137	2163	rBV	320213	555088	51.64%	6.120%
66	8.034	2165	2175	2219	rVV2	255274	545901	50.79%	6.019%
67	8.368	2278	2279	2282	rBV2	578	341	0.03%	0.004%
68	8.789	2398	2410	2438	rBV	461955	777517	72.34%	8.573%
69	9.053	2490	2492	2493	rBV	648	274	0.03%	0.003%
70	9.082	2499	2501	2503	rBV3	680	307	0.03%	0.003%
71	9.198	2535	2537	2540	rBV2	380	226	0.02%	0.002%
72	9.285	2562	2564	2568	rVB3	463	292	0.03%	0.003%
73	9.423	2605	2607	2610	rBV2	378	204	0.02%	0.002%
74	9.487	2624	2627	2633	rBV3	959	1010	0.09%	0.011%
75	9.616	2666	2667	2669	rBV	429	186	0.02%	0.002%
76	9.876	2740	2748	2753	rBV5	816	1358	0.13%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031439.D
 Acq On : 08 Jun 2023 11:09
 Operator : SY/MD
 Sample : 02992-10 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.047	2799	2801	2803	rBV2	223	108	0.01%	0.001%
78	10.159	2823	2836	2860	rBV	298751	476704	44.35%	5.256%
79	10.365	2896	2900	2903	rBV4	669	587	0.05%	0.006%
80	10.420	2913	2917	2919	rBV	550	368	0.03%	0.004%
81	10.558	2957	2960	2961	rBV	388	168	0.02%	0.002%
82	10.696	2998	3003	3006	rBV	747	528	0.05%	0.006%
83	10.719	3006	3010	3011	rBV	329	193	0.02%	0.002%
84	10.850	3049	3051	3052	rBV	701	276	0.03%	0.003%
85	10.940	3077	3079	3082	rBV3	555	282	0.03%	0.003%
86	10.963	3085	3086	3088	rBV	311	165	0.02%	0.002%
87	11.014	3100	3102	3103	rBV	261	69	0.01%	0.001%
88	11.104	3124	3130	3131	rBV2	529	479	0.04%	0.005%
89	11.191	3145	3157	3182	rBV	450152	711713	66.21%	7.847%
90	11.400	3220	3222	3225	rVB3	506	261	0.02%	0.003%
91	11.436	3231	3233	3235	rBV2	539	282	0.03%	0.003%
92	11.567	3261	3274	3292	rBV	471946	740689	68.91%	8.167%
93	11.956	3393	3395	3399	rVB4	575	368	0.03%	0.004%
94	11.992	3404	3406	3409	rVV2	590	227	0.02%	0.003%
95	12.091	3436	3437	3441	rBV2	455	230	0.02%	0.003%
96	12.191	3466	3468	3472	rVB4	591	295	0.03%	0.003%
97	12.538	3574	3576	3578	rBV2	527	261	0.02%	0.003%
98	12.673	3616	3618	3621	rBV3	282	93	0.01%	0.001%
99	13.423	3848	3851	3853	rBV2	592	354	0.03%	0.004%




Sum of corrected areas: 9069666

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031439.D
Acq On : 08 Jun 2023 11:09
Operator : SY/MD
Sample : 02992-10 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

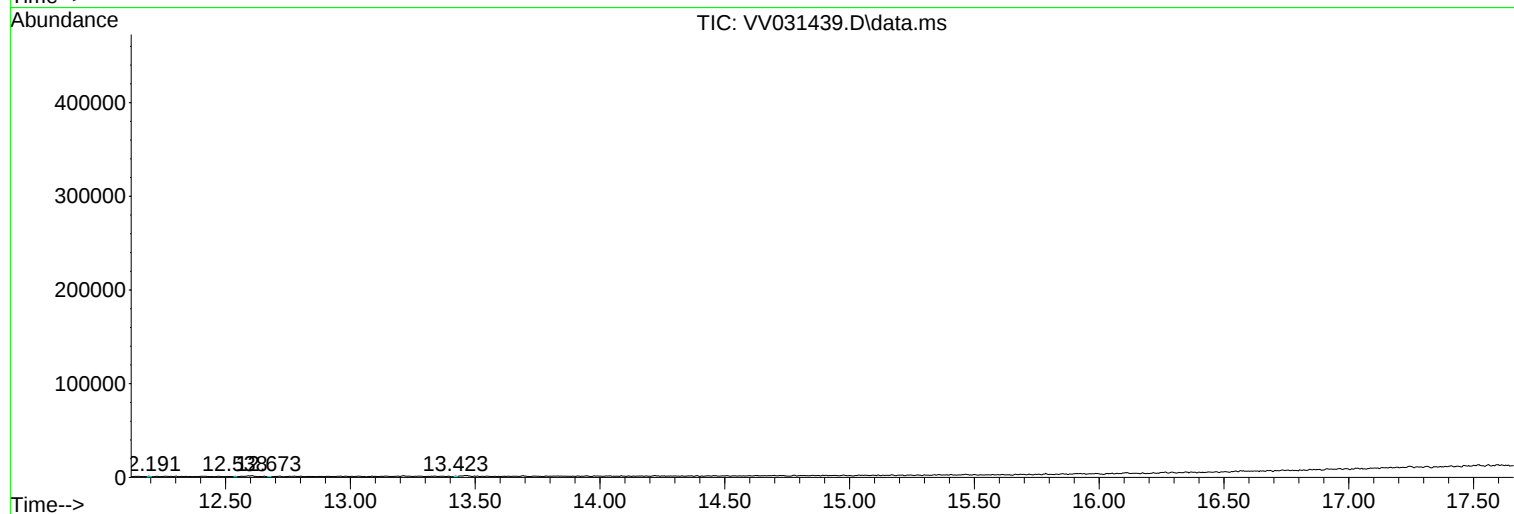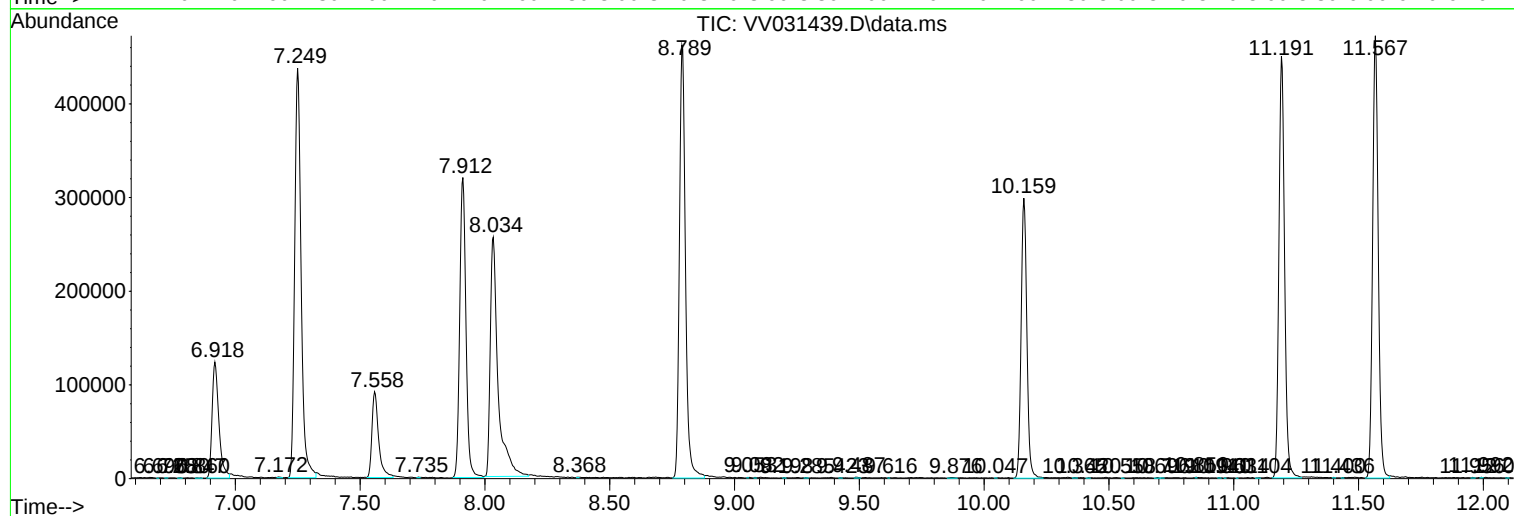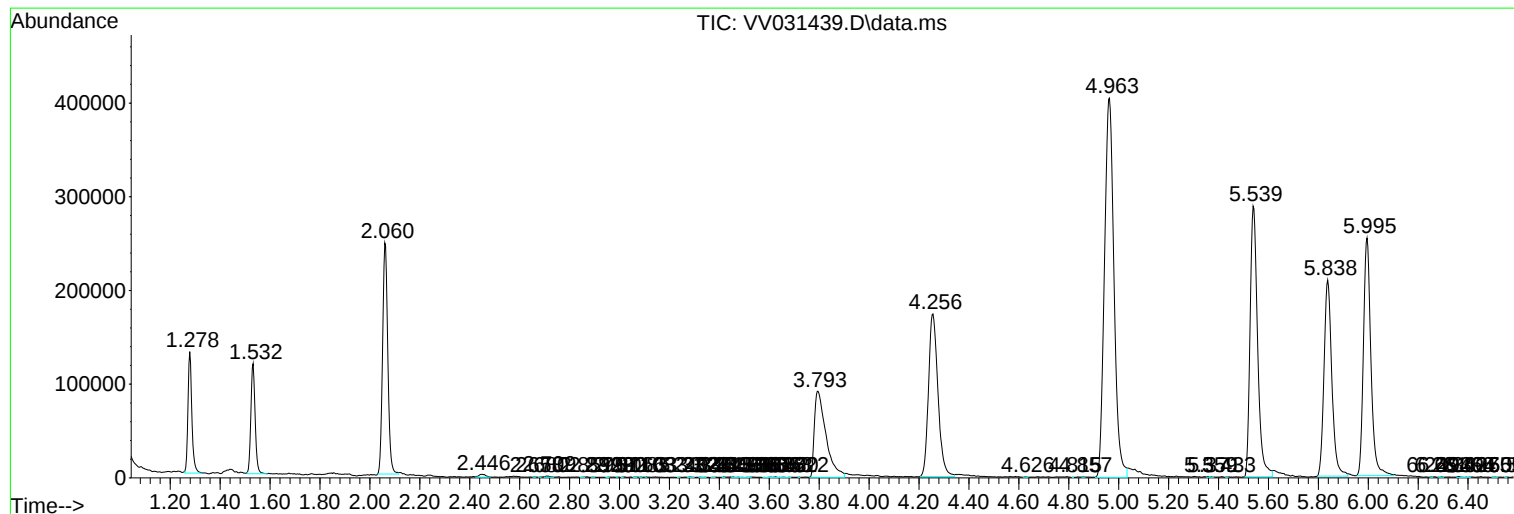

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031439.D
Acq On : 08 Jun 2023 11:09
Operator : SY/MD
Sample : 02992-10 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031439.D
Acq On : 08 Jun 2023 11:09
Operator : SY/MD
Sample : 02992-10 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------