

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031440.D
 Acq On : 08 Jun 2023 11:33
 Operator : SY/MD
 Sample : 03076-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031440.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	123563	135218	13.04%	1.702%
2	1.532	146	153	170	rVB	117637	135754	13.09%	1.709%
3	2.063	308	318	332	rBV	233738	346295	33.39%	4.360%
4	2.323	397	399	400	rBV	421	179	0.02%	0.002%
5	2.449	431	438	444	rBV4	1421	2206	0.21%	0.028%
6	2.545	465	468	469	rBV	356	180	0.02%	0.002%
7	2.625	490	493	495	rBV2	337	164	0.02%	0.002%
8	2.642	495	498	500	rVV	363	216	0.02%	0.003%
9	2.706	515	518	521	rVV3	461	298	0.03%	0.004%
10	2.793	543	545	548	rBV2	398	217	0.02%	0.003%
11	2.860	564	566	572	rVB2	653	361	0.03%	0.005%
12	2.947	590	593	599	rBV2	431	376	0.04%	0.005%
13	2.979	599	603	604	rBV2	282	192	0.02%	0.002%
14	3.002	608	610	614	rVB2	560	256	0.02%	0.003%
15	3.027	614	618	620	rBV2	292	237	0.02%	0.003%
16	3.085	634	636	640	rBV2	350	284	0.03%	0.004%
17	3.195	668	670	672	rBV2	325	186	0.02%	0.002%
18	3.323	705	710	712	rBV3	502	357	0.03%	0.004%
19	3.413	734	738	739	rBV	512	276	0.03%	0.003%
20	3.471	754	756	759	rVB2	446	242	0.02%	0.003%
21	3.490	759	762	768	rBV3	273	305	0.03%	0.004%
22	3.516	768	770	777	rVB3	202	178	0.02%	0.002%
23	3.661	812	815	820	rVB3	413	368	0.04%	0.005%
24	3.693	820	825	826	rBV3	428	309	0.03%	0.004%
25	3.793	846	856	889	rBV	79337	233733	22.54%	2.943%
26	4.256	982	1000	1026	rBV2	170482	444021	42.81%	5.590%
27	4.670	1125	1129	1133	rVB2	554	405	0.04%	0.005%
28	4.696	1133	1137	1141	rBV4	538	509	0.05%	0.006%
29	4.741	1148	1151	1154	rBV3	545	412	0.04%	0.005%
30	4.783	1161	1164	1169	rBV3	398	242	0.02%	0.003%
31	4.963	1202	1220	1242	rBV2	390241	1037097	100.00%	13.057%
32	5.404	1355	1357	1359	rBV	390	214	0.02%	0.003%
33	5.497	1381	1386	1387	rBV2	369	293	0.03%	0.004%
34	5.542	1387	1400	1419	rBV	300113	627311	60.49%	7.898%
35	5.831	1480	1490	1505	rBV	28574	57371	5.53%	0.722%
36	5.995	1525	1541	1567	rBV	240362	513517	49.51%	6.465%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031440.D
 Acq On : 08 Jun 2023 11:33
 Operator : SY/MD
 Sample : 03076-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.397	1662	1666	1669	rBV3	440	329	0.03%	0.004%
38	6.436	1675	1678	1680	rBV2	332	176	0.02%	0.002%
39	6.670	1745	1751	1754	rBV3	635	582	0.06%	0.007%
40	6.683	1754	1755	1758	rVV	416	246	0.02%	0.003%
41	6.783	1784	1786	1788	rBV2	414	209	0.02%	0.003%
42	6.844	1802	1805	1807	rBV2	423	241	0.02%	0.003%
43	6.857	1807	1809	1813	rBV2	358	205	0.02%	0.003%
44	6.918	1817	1828	1849	rBV	116126	225387	21.73%	2.838%
45	7.198	1911	1915	1917	rBV3	416	314	0.03%	0.004%
46	7.249	1919	1931	1972	rBV	418261	759534	73.24%	9.562%
47	7.558	2017	2027	2050	rBV	90644	164439	15.86%	2.070%
48	7.847	2115	2117	2119	rBV2	321	205	0.02%	0.003%
49	7.857	2119	2120	2122	rBV	412	195	0.02%	0.002%
50	7.902	2132	2134	2135	rBV2	1136	381	0.04%	0.005%
51	8.034	2164	2175	2213	rBV2	222222	502646	48.47%	6.328%
52	8.413	2291	2293	2294	rBV	727	304	0.03%	0.004%
53	8.461	2306	2308	2314	rBV5	400	482	0.05%	0.006%
54	8.567	2339	2341	2346	rVB4	783	606	0.06%	0.008%
55	8.622	2354	2358	2360	rBV2	461	406	0.04%	0.005%
56	8.718	2384	2388	2390	rBV2	406	386	0.04%	0.005%
57	8.789	2398	2410	2440	rBV	486948	810220	78.12%	10.201%
58	9.098	2505	2506	2510	rBV2	756	584	0.06%	0.007%
59	9.159	2523	2525	2530	rBV4	598	391	0.04%	0.005%
60	9.204	2537	2539	2542	rBV3	366	250	0.02%	0.003%
61	9.246	2547	2552	2553	rBV	406	278	0.03%	0.003%
62	9.317	2571	2574	2576	rBV2	338	214	0.02%	0.003%
63	9.397	2595	2599	2601	rVB3	359	174	0.02%	0.002%
64	9.452	2614	2616	2619	rVB	347	185	0.02%	0.002%
65	9.474	2619	2623	2626	rBV2	565	412	0.04%	0.005%
66	9.519	2634	2637	2639	rBV	632	389	0.04%	0.005%
67	9.551	2645	2647	2649	rBV3	462	199	0.02%	0.003%
68	9.590	2657	2659	2662	rBV2	350	164	0.02%	0.002%
69	9.690	2688	2690	2693	rBV3	749	430	0.04%	0.005%
70	9.712	2693	2697	2702	rVV2	444	394	0.04%	0.005%
71	9.786	2718	2720	2723	rVB2	426	223	0.02%	0.003%
72	9.837	2732	2736	2739	rBV3	731	616	0.06%	0.008%
73	9.918	2758	2761	2763	rBV	386	255	0.02%	0.003%
74	10.034	2794	2797	2798	rBV2	624	294	0.03%	0.004%
75	10.101	2815	2818	2821	rBV2	334	239	0.02%	0.003%
76	10.159	2823	2836	2855	rBV	285092	460608	44.41%	5.799%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031440.D
 Acq On : 08 Jun 2023 11:33
 Operator : SY/MD
 Sample : 03076-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.336	2886	2891	2898	rVV4	2326	2948	0.28%	0.037%
78	10.374	2901	2903	2905	rBV4	332	174	0.02%	0.002%
79	10.529	2944	2951	2953	rBV3	515	634	0.06%	0.008%
80	10.664	2991	2993	2996	rBV2	335	163	0.02%	0.002%
81	10.706	3004	3006	3009	rBV2	503	200	0.02%	0.003%
82	10.744	3015	3018	3023	rBV3	602	293	0.03%	0.004%
83	10.927	3073	3075	3079	rVB2	454	189	0.02%	0.002%
84	11.056	3113	3115	3117	rBV	390	189	0.02%	0.002%
85	11.127	3134	3137	3141	rBV2	738	689	0.07%	0.009%
86	11.191	3145	3157	3176	rBV	476646	744116	71.75%	9.368%
87	11.384	3214	3217	3218	rBV2	414	237	0.02%	0.003%
88	11.435	3231	3233	3235	rBV2	479	314	0.03%	0.004%
89	11.567	3261	3274	3297	rBV	450206	715149	68.96%	9.004%
90	11.882	3370	3372	3375	rBV3	433	265	0.03%	0.003%
91	11.953	3392	3394	3399	rBV3	377	286	0.03%	0.004%
92	12.091	3436	3437	3441	rBV2	294	182	0.02%	0.002%
93	12.587	3588	3591	3595	rBV3	720	510	0.05%	0.006%
94	12.815	3660	3662	3665	rBV2	430	283	0.03%	0.004%
95	12.976	3709	3712	3715	rBV3	547	317	0.03%	0.004%
96	13.284	3806	3808	3812	rVB2	683	430	0.04%	0.005%
97	13.451	3856	3860	3863	rBV3	697	701	0.07%	0.009%
98	13.567	3894	3896	3898	rVB	801	310	0.03%	0.004%
99	14.088	4056	4058	4064	rVB4	689	427	0.04%	0.005%
100	14.249	4107	4108	4111	rBV4	523	293	0.03%	0.004%




Sum of corrected areas: 7942870

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031440.D
Acq On : 08 Jun 2023 11:33
Operator : SY/MD
Sample : 03076-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

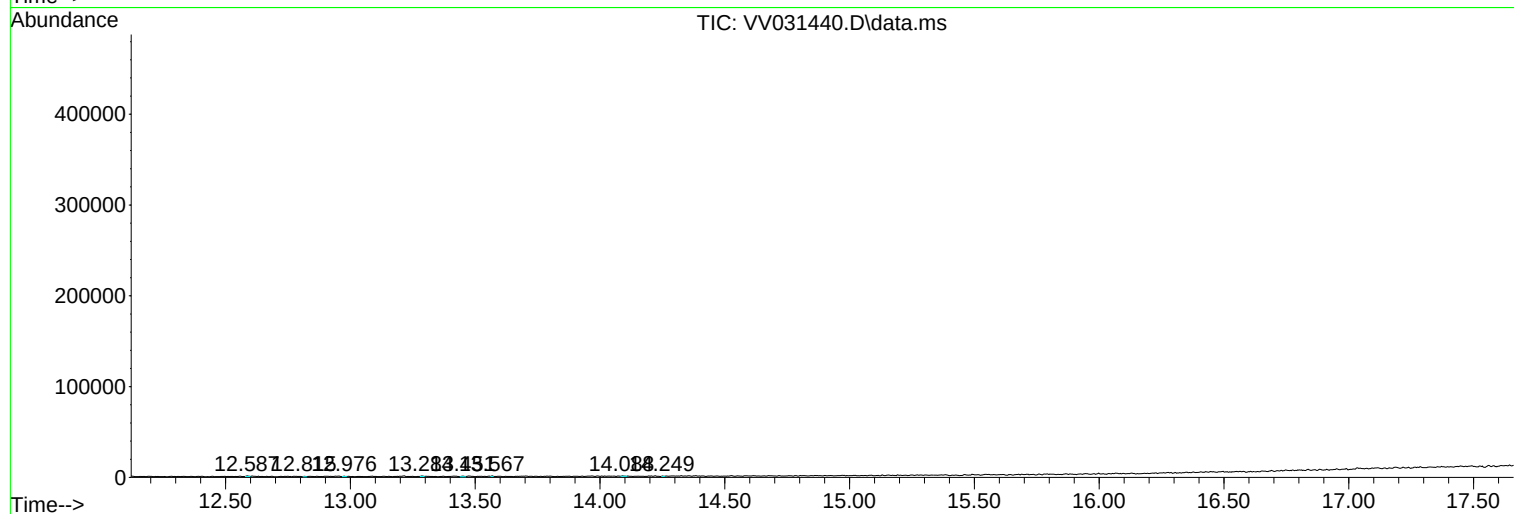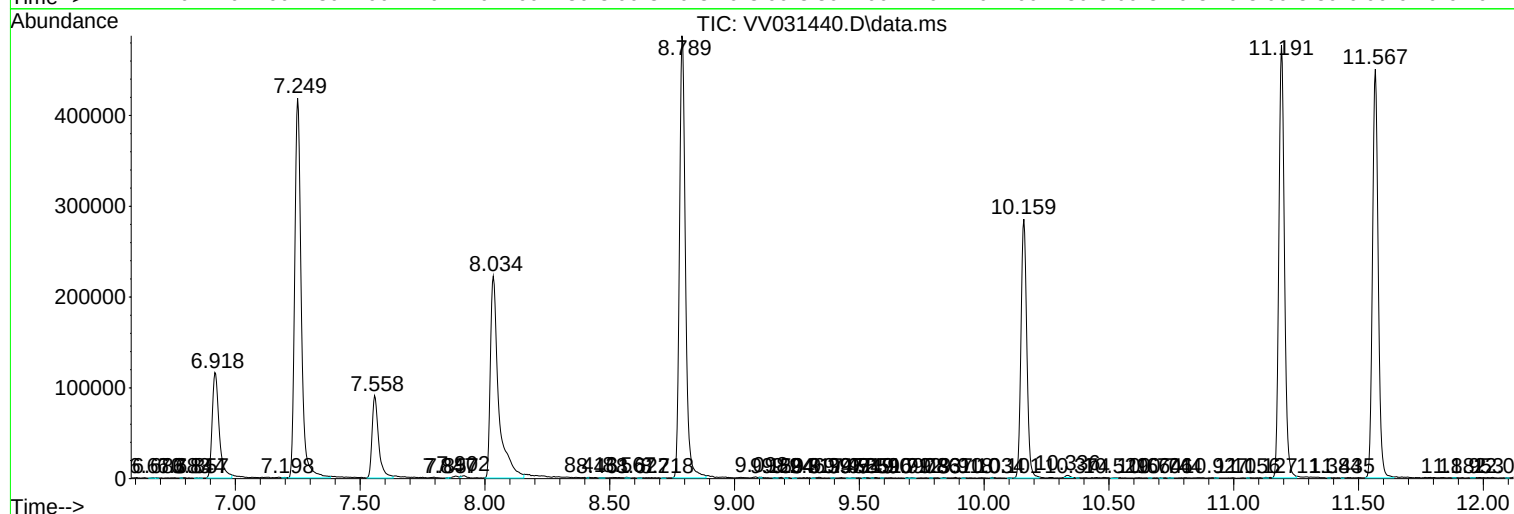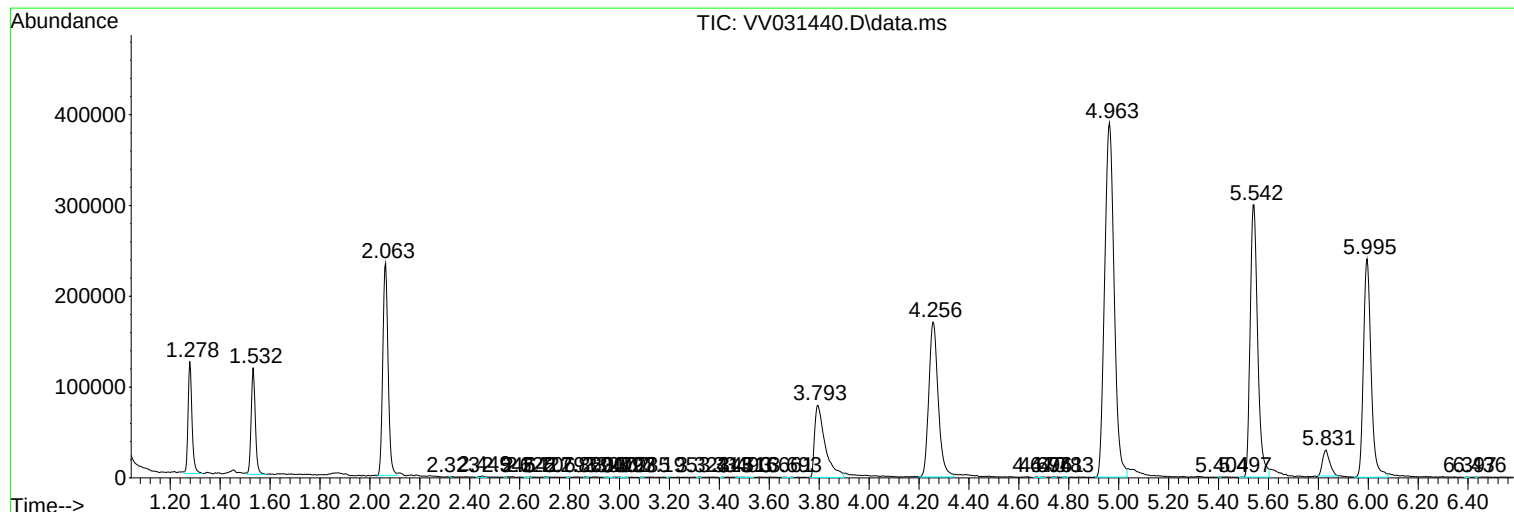

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031440.D
Acq On : 08 Jun 2023 11:33
Operator : SY/MD
Sample : 03076-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031440.D
Acq On : 08 Jun 2023 11:33
Operator : SY/MD
Sample : 03076-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc