

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031441.D
 Acq On : 08 Jun 2023 11:57
 Operator : SY/MD
 Sample : 03076-04DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F83DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	120581	133638	12.65%	1.564%
2	1.532	147	153	166	rVB	116663	139143	13.17%	1.628%
3	2.063	308	318	332	rBV2	247189	375494	35.54%	4.395%
4	2.661	501	504	508	rBV2	387	321	0.03%	0.004%
5	2.770	534	538	542	rBV4	348	280	0.03%	0.003%
6	2.857	563	565	569	rBV	266	218	0.02%	0.003%
7	2.896	572	577	580	rBV2	542	488	0.05%	0.006%
8	3.008	608	612	615	rBV4	550	450	0.04%	0.005%
9	3.043	621	623	627	rBV	229	129	0.01%	0.002%
10	3.124	642	648	651	rBV3	1114	1206	0.11%	0.014%
11	3.359	717	721	724	rBV	315	223	0.02%	0.003%
12	3.387	727	730	732	rBV	372	198	0.02%	0.002%
13	3.432	742	744	746	rBV2	255	119	0.01%	0.001%
14	3.497	758	764	766	rBV2	482	452	0.04%	0.005%
15	3.526	771	773	775	rVB2	286	113	0.01%	0.001%
16	3.564	781	785	789	rBV3	296	317	0.03%	0.004%
17	3.658	812	814	816	rBV3	180	105	0.01%	0.001%
18	3.696	823	826	828	rBV	137	95	0.01%	0.001%
19	3.799	847	858	894	rBV	82189	281687	26.66%	3.297%
20	4.256	984	1000	1028	rBV2	168581	444343	42.06%	5.200%
21	4.635	1115	1118	1120	rBV2	411	277	0.03%	0.003%
22	4.677	1129	1131	1135	rVB3	438	272	0.03%	0.003%
23	4.696	1135	1137	1140	rVB2	595	302	0.03%	0.004%
24	4.838	1175	1181	1183	rBV2	327	308	0.03%	0.004%
25	4.876	1191	1193	1194	rBV	309	113	0.01%	0.001%
26	4.963	1203	1220	1248	rBV3	392019	1056476	100.00%	12.364%
27	5.445	1369	1370	1371	rBV3	264	91	0.01%	0.001%
28	5.468	1375	1377	1378	rVV3	349	120	0.01%	0.001%
29	5.539	1387	1399	1418	rBV	299010	619921	58.68%	7.255%
30	5.838	1478	1492	1525	rBV3	290885	620873	58.77%	7.266%
31	5.995	1530	1541	1563	rVV	238828	489829	46.36%	5.733%
32	6.194	1599	1603	1609	rBV5	758	946	0.09%	0.011%
33	6.362	1652	1655	1658	rBV2	374	174	0.02%	0.002%
34	6.474	1689	1690	1691	rBV2	233	84	0.01%	0.001%
35	6.516	1700	1703	1704	rBV	255	134	0.01%	0.002%
36	6.558	1712	1716	1719	rBV3	540	372	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031441.D
 Acq On : 08 Jun 2023 11:57
 Operator : SY/MD
 Sample : 03076-04DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F83DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.667	1748	1750	1752	rVB	401	128	0.01%	0.001%
38	6.741	1768	1773	1777	rBV4	681	574	0.05%	0.007%
39	6.764	1777	1780	1782	rBV	281	132	0.01%	0.002%
40	6.809	1792	1794	1796	rVB	272	67	0.01%	0.001%
41	6.854	1805	1808	1810	rVB2	454	244	0.02%	0.003%
42	6.873	1811	1814	1815	rBV2	208	126	0.01%	0.001%
43	6.918	1817	1828	1852	rBV	118254	231074	21.87%	2.704%
44	7.188	1908	1912	1915	rBV3	1001	773	0.07%	0.009%
45	7.207	1915	1918	1919	rBV2	611	317	0.03%	0.004%
46	7.249	1919	1931	1961	rVV	422126	762133	72.14%	8.920%
47	7.558	2017	2027	2056	rBV	88914	168279	15.93%	1.969%
48	7.754	2084	2088	2095	rBV4	765	908	0.09%	0.011%
49	7.815	2104	2107	2110	rBV3	564	402	0.04%	0.005%
50	7.831	2110	2112	2115	rBV3	433	220	0.02%	0.003%
51	7.976	2153	2157	2158	rBV2	378	218	0.02%	0.003%
52	8.034	2165	2175	2212	rBV2	220712	494400	46.80%	5.786%
53	8.522	2323	2327	2331	rBV4	921	830	0.08%	0.010%
54	8.744	2393	2396	2399	rBV3	298	245	0.02%	0.003%
55	8.789	2399	2410	2438	rBV	478415	807115	76.40%	9.446%
56	9.001	2472	2476	2477	rBV3	562	463	0.04%	0.005%
57	9.037	2483	2487	2489	rBV3	484	323	0.03%	0.004%
58	9.194	2534	2536	2542	rBV3	471	332	0.03%	0.004%
59	9.291	2564	2566	2569	rBV2	535	333	0.03%	0.004%
60	9.371	2589	2591	2595	rVB3	322	111	0.01%	0.001%
61	9.445	2610	2614	2619	rBV3	460	473	0.04%	0.006%
62	9.468	2619	2621	2625	rBV3	420	180	0.02%	0.002%
63	9.558	2648	2649	2651	rVB2	305	71	0.01%	0.001%
64	9.644	2670	2676	2678	rBV4	547	512	0.05%	0.006%
65	9.673	2683	2685	2689	rBV3	212	160	0.02%	0.002%
66	9.693	2689	2691	2694	rBV3	422	265	0.03%	0.003%
67	9.841	2735	2737	2740	rVB2	308	139	0.01%	0.002%
68	9.853	2740	2741	2743	rBV	373	169	0.02%	0.002%
69	9.908	2756	2758	2759	rBV	315	121	0.01%	0.001%
70	10.062	2803	2806	2808	rBV2	410	261	0.02%	0.003%
71	10.159	2825	2836	2860	rVB	292810	467549	44.26%	5.472%
72	10.426	2916	2919	2920	rBV2	302	153	0.01%	0.002%
73	10.519	2944	2948	2949	rBV2	310	219	0.02%	0.003%
74	10.615	2976	2978	2980	rVB	416	168	0.02%	0.002%
75	10.632	2980	2983	2986	rBV3	626	387	0.04%	0.005%
76	10.696	3001	3003	3004	rBV	283	120	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031441.D
 Acq On : 08 Jun 2023 11:57
 Operator : SY/MD
 Sample : 03076-04DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F83DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.802	3033	3036	3038	rBV2	542	287	0.03%	0.003%
78	11.127	3134	3137	3142	rBV4	811	598	0.06%	0.007%
79	11.191	3146	3157	3178	rBV	465345	731929	69.28%	8.566%
80	11.567	3262	3274	3291	rBV	433722	699303	66.19%	8.184%
81	11.760	3332	3334	3335	rBV	363	155	0.01%	0.002%
82	11.841	3356	3359	3363	rBV3	510	411	0.04%	0.005%
83	12.329	3509	3511	3515	rBV2	623	346	0.03%	0.004%
84	13.766	3955	3958	3960	rBV2	534	289	0.03%	0.003%
85	13.815	3970	3973	3975	rBV2	712	400	0.04%	0.005%
86	14.355	4137	4141	4143	rBV3	1012	818	0.08%	0.010%




Sum of corrected areas: 8544541

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031441.D
Acq On : 08 Jun 2023 11:57
Operator : SY/MD
Sample : 03076-04DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F83DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

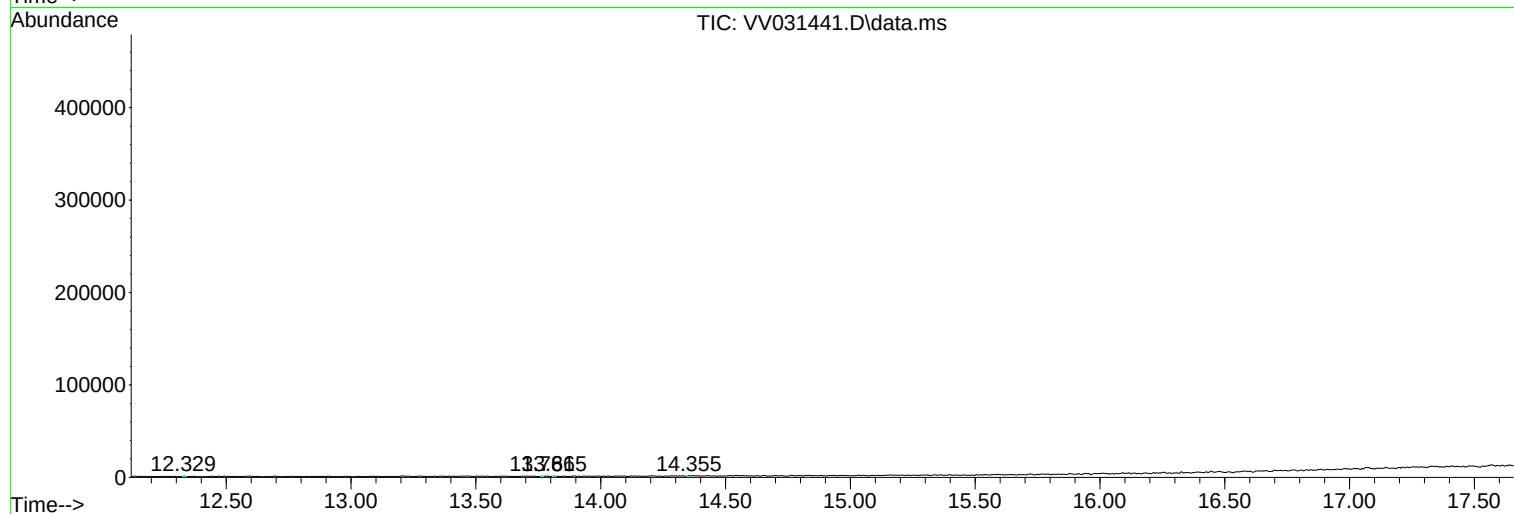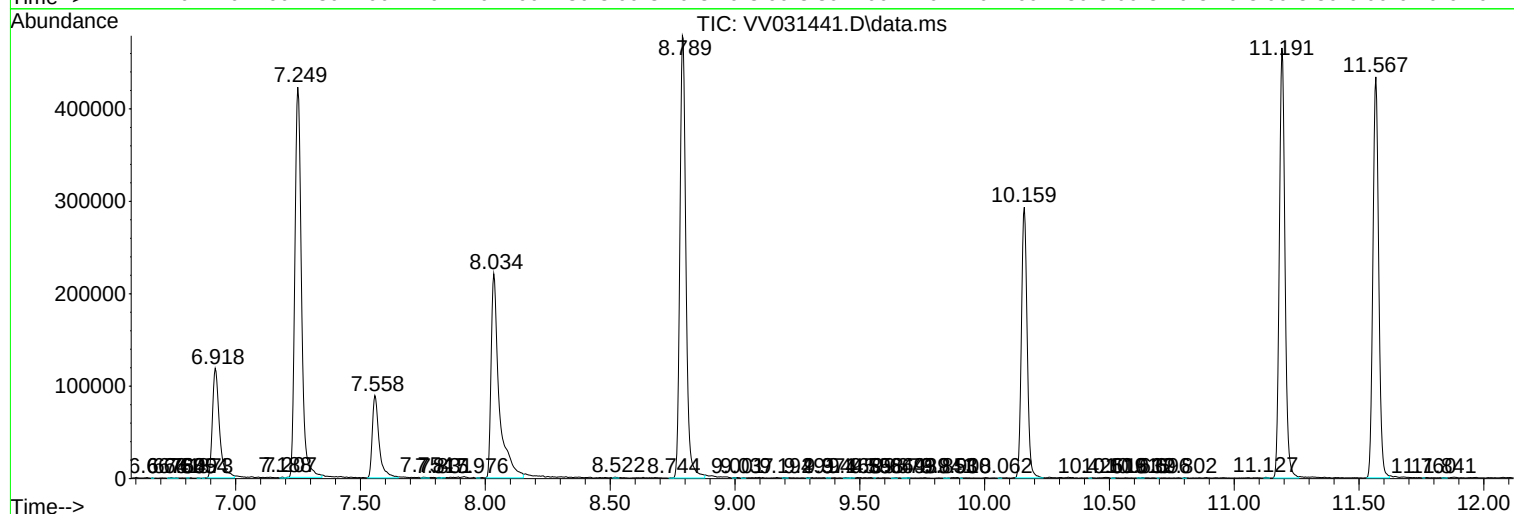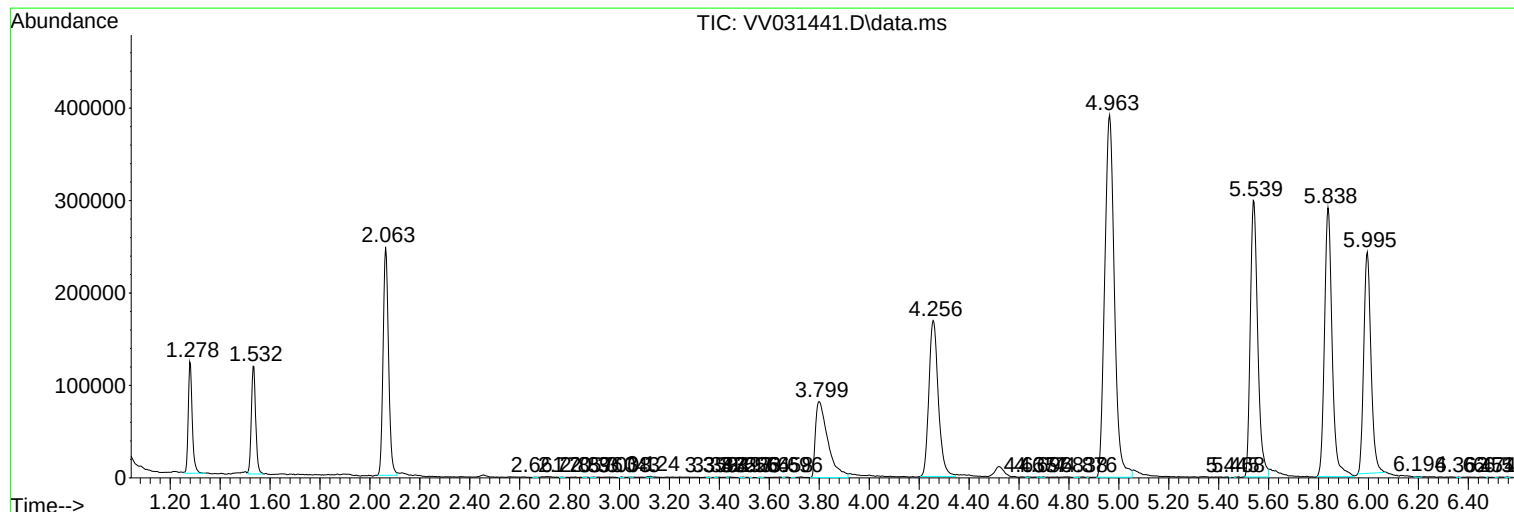

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031441.D
Acq On : 08 Jun 2023 11:57
Operator : SY/MD
Sample : 03076-04DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F83DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031441.D
Acq On : 08 Jun 2023 11:57
Operator : SY/MD
Sample : 03076-04DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F83DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------