

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031443.D
 Acq On : 08 Jun 2023 12:44
 Operator : SY/MD
 Sample : 03077-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	133191	144748	12.57%	1.723%
2	1.532	147	153	170	rVB	127572	149769	13.01%	1.783%
3	2.063	308	318	331	rBV	252050	370209	32.15%	4.406%
4	2.500	452	454	457	rBV4	646	430	0.04%	0.005%
5	2.555	467	471	473	rBV2	445	331	0.03%	0.004%
6	2.706	515	518	521	rBV4	968	860	0.07%	0.010%
7	2.896	575	577	581	rVB3	250	160	0.01%	0.002%
8	2.973	597	601	602	rBV3	560	326	0.03%	0.004%
9	2.998	606	609	611	rBV2	350	189	0.02%	0.002%
10	3.037	618	621	623	rBV	542	303	0.03%	0.004%
11	3.108	640	643	645	rBV2	528	301	0.03%	0.004%
12	3.124	645	648	649	rBV2	401	243	0.02%	0.003%
13	3.326	710	711	714	rBV2	263	161	0.01%	0.002%
14	3.416	735	739	740	rBV2	432	271	0.02%	0.003%
15	3.461	751	753	756	rBV2	266	170	0.01%	0.002%
16	3.487	756	761	762	rVV2	411	212	0.02%	0.003%
17	3.519	766	771	776	rBV2	506	529	0.05%	0.006%
18	3.568	783	786	789	rBV2	229	164	0.01%	0.002%
19	3.638	806	808	811	rBV	247	195	0.02%	0.002%
20	3.757	843	845	847	rBV2	465	241	0.02%	0.003%
21	3.796	847	857	888	rBV	80920	240240	20.86%	2.859%
22	4.256	985	1000	1026	rBV	185731	476504	41.38%	5.671%
23	4.567	1094	1097	1098	rBV2	642	294	0.03%	0.003%
24	4.667	1126	1128	1132	rBV	363	227	0.02%	0.003%
25	4.699	1136	1138	1140	rBV2	377	196	0.02%	0.002%
26	4.834	1177	1180	1185	rBV4	548	523	0.05%	0.006%
27	4.902	1199	1201	1203	rBV2	617	311	0.03%	0.004%
28	4.963	1203	1220	1268	rVV2	422351	1151613	100.00%	13.706%
29	5.265	1312	1314	1316	rBV2	580	229	0.02%	0.003%
30	5.413	1359	1360	1363	rVB2	336	176	0.02%	0.002%
31	5.539	1387	1399	1430	rBV	302470	645119	56.02%	7.678%
32	5.831	1478	1490	1509	rBV5	41178	101299	8.80%	1.206%
33	5.937	1520	1523	1527	rBV3	608	474	0.04%	0.006%
34	5.995	1527	1541	1572	rBV	257813	552023	47.93%	6.570%
35	6.284	1629	1631	1632	rBV	683	298	0.03%	0.004%
36	6.358	1652	1654	1658	rBV3	363	219	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031443.D
 Acq On : 08 Jun 2023 12:44
 Operator : SY/MD
 Sample : 03077-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.387	1661	1663	1666	rVB	628	217	0.02%	0.003%
38	6.413	1668	1671	1672	rBV	253	142	0.01%	0.002%
39	6.429	1674	1676	1677	rBV	297	159	0.01%	0.002%
40	6.506	1694	1700	1703	rVB3	560	502	0.04%	0.006%
41	6.551	1712	1714	1719	rBV2	521	382	0.03%	0.005%
42	6.664	1746	1749	1752	rBV2	401	288	0.03%	0.003%
43	6.706	1759	1762	1764	rBV	360	189	0.02%	0.002%
44	6.719	1764	1766	1769	rBV2	413	309	0.03%	0.004%
45	6.767	1779	1781	1785	rVB2	496	330	0.03%	0.004%
46	6.792	1787	1789	1791	rBV2	257	140	0.01%	0.002%
47	6.841	1801	1804	1808	rBV2	405	310	0.03%	0.004%
48	6.866	1808	1812	1817	rVB3	740	600	0.05%	0.007%
49	6.918	1817	1828	1861	rBV2	127267	248566	21.58%	2.958%
50	7.111	1886	1888	1892	rVB4	883	417	0.04%	0.005%
51	7.249	1919	1931	1951	rBV	456242	817794	71.01%	9.733%
52	7.558	2017	2027	2049	rBV	91425	176308	15.31%	2.098%
53	7.796	2097	2101	2106	rVB3	850	763	0.07%	0.009%
54	7.825	2106	2110	2111	rBV	364	258	0.02%	0.003%
55	7.857	2118	2120	2121	rBV	374	140	0.01%	0.002%
56	7.876	2122	2126	2127	rBV	1292	837	0.07%	0.010%
57	8.034	2165	2175	2212	rBV2	236592	531559	46.16%	6.326%
58	8.606	2350	2353	2354	rBV2	456	251	0.02%	0.003%
59	8.680	2374	2376	2380	rBV4	431	390	0.03%	0.005%
60	8.728	2389	2391	2394	rBV2	336	176	0.02%	0.002%
61	8.744	2394	2396	2398	rBV	433	219	0.02%	0.003%
62	8.789	2399	2410	2434	rBV	489090	810153	70.35%	9.642%
63	9.011	2477	2479	2483	rVB3	781	482	0.04%	0.006%
64	9.159	2523	2525	2526	rBV	495	220	0.02%	0.003%
65	9.316	2569	2574	2578	rBV3	460	438	0.04%	0.005%
66	9.423	2605	2607	2611	rVB2	577	325	0.03%	0.004%
67	9.448	2613	2615	2618	rVB	459	141	0.01%	0.002%
68	9.468	2618	2621	2623	rBV2	447	295	0.03%	0.004%
69	9.480	2623	2625	2628	rBV4	562	368	0.03%	0.004%
70	9.497	2628	2630	2635	rVB3	602	413	0.04%	0.005%
71	9.580	2654	2656	2657	rBV3	285	130	0.01%	0.002%
72	9.673	2683	2685	2688	rVB	387	183	0.02%	0.002%
73	9.696	2688	2692	2693	rBV	625	281	0.02%	0.003%
74	9.802	2723	2725	2732	rVB2	606	486	0.04%	0.006%
75	9.828	2732	2733	2735	rBV	361	160	0.01%	0.002%
76	9.921	2760	2762	2763	rVB	532	142	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031443.D
 Acq On : 08 Jun 2023 12:44
 Operator : SY/MD
 Sample : 03077-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	9.940	2763	2768	2772	rBV3	478	591	0.05%	0.007%
78	9.956	2772	2773	2775	rVV2	548	179	0.02%	0.002%
79	10.088	2810	2814	2817	rVB2	455	415	0.04%	0.005%
80	10.159	2825	2836	2856	rBV	309876	491607	42.69%	5.851%
81	10.336	2885	2891	2904	rVB4	3627	5930	0.51%	0.071%
82	10.387	2904	2907	2909	rVB2	280	143	0.01%	0.002%
83	10.448	2923	2926	2927	rBV2	397	226	0.02%	0.003%
84	10.480	2932	2936	2938	rBV2	351	319	0.03%	0.004%
85	10.516	2943	2947	2949	rBV3	314	233	0.02%	0.003%
86	10.632	2981	2983	2986	rBV2	279	123	0.01%	0.001%
87	10.757	3018	3022	3023	rBV2	346	241	0.02%	0.003%
88	10.812	3036	3039	3041	rBV2	386	253	0.02%	0.003%
89	11.123	3133	3136	3141	rBV4	749	842	0.07%	0.010%
90	11.191	3145	3157	3182	rBV	457637	727733	63.19%	8.661%
91	11.567	3262	3274	3295	rBV	462260	735418	63.86%	8.753%
92	11.985	3401	3404	3407	rBV3	614	366	0.03%	0.004%
93	12.818	3659	3663	3664	rBV2	391	284	0.02%	0.003%
94	12.837	3667	3669	3671	rVB2	523	187	0.02%	0.002%
95	13.242	3793	3795	3802	rVB3	795	452	0.04%	0.005%
96	13.602	3904	3907	3908	rBV	331	178	0.02%	0.002%
97	13.667	3925	3927	3930	rBV2	408	227	0.02%	0.003%
98	13.766	3956	3958	3959	rBV	683	256	0.02%	0.003%
99	13.840	3979	3981	3985	rVV2	831	325	0.03%	0.004%
100	13.856	3985	3986	3993	rVB	732	591	0.05%	0.007%




Sum of corrected areas: 8402139

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031443.D
Acq On : 08 Jun 2023 12:44
Operator : SY/MD
Sample : 03077-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

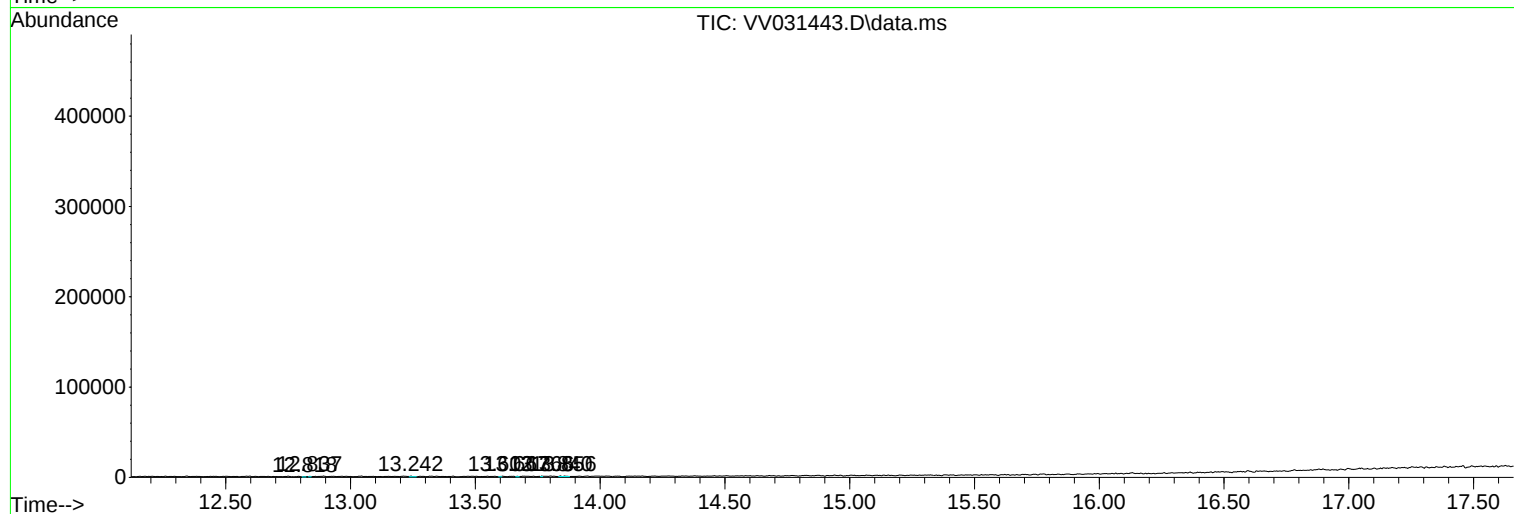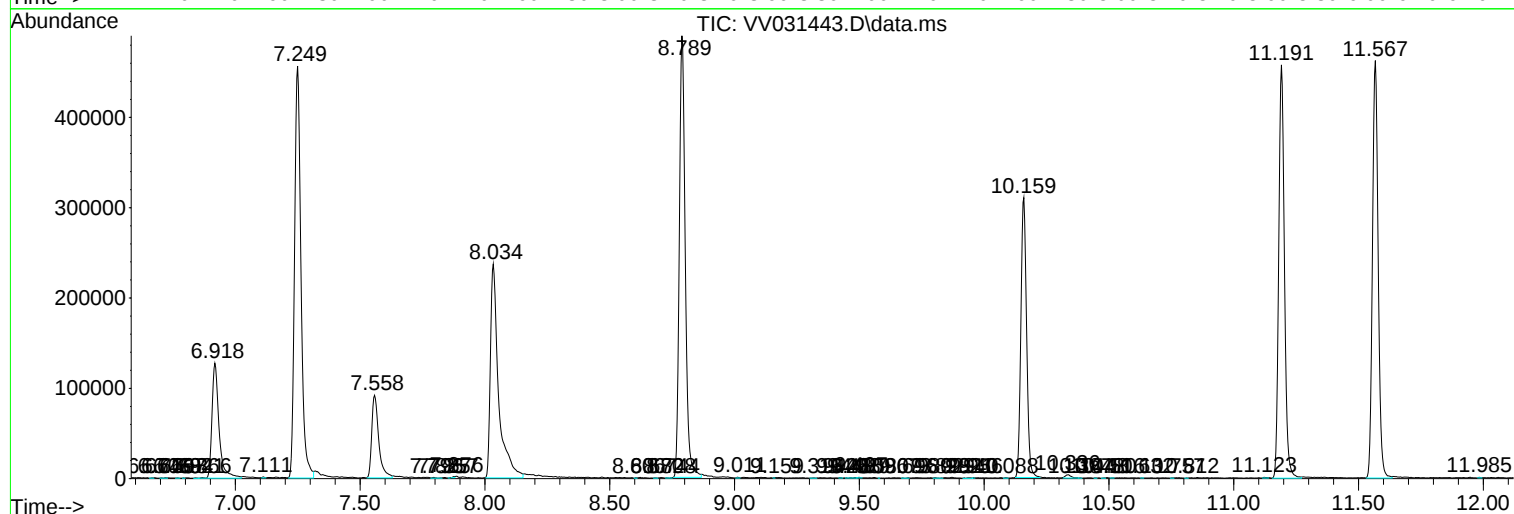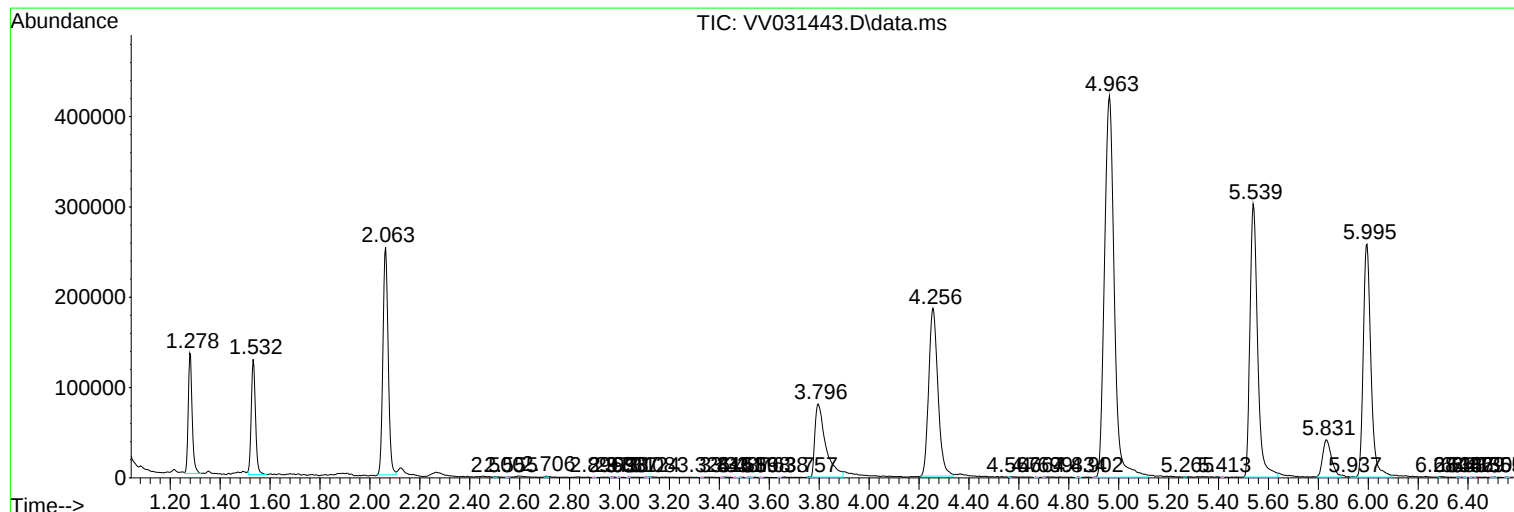

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031443.D
Acq On : 08 Jun 2023 12:44
Operator : SY/MD
Sample : 03077-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031443.D
Acq On : 08 Jun 2023 12:44
Operator : SY/MD
Sample : 03077-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
