

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031444.D
 Acq On : 08 Jun 2023 13:08
 Operator : SY/MD
 Sample : 03077-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	124207	134309	12.45%	1.685%
2	1.532	146	153	166	rVB	120649	139461	12.93%	1.749%
3	2.063	308	318	330	rBV	243404	356205	33.02%	4.468%
4	2.497	451	453	455	rBV2	466	202	0.02%	0.003%
5	2.632	493	495	498	rVB3	828	346	0.03%	0.004%
6	2.651	498	501	504	rVB	476	254	0.02%	0.003%
7	2.674	506	508	511	rVB	370	195	0.02%	0.002%
8	2.709	515	519	520	rBV2	374	296	0.03%	0.004%
9	2.767	535	537	539	rBV2	294	157	0.01%	0.002%
10	2.928	586	587	589	rBV	297	131	0.01%	0.002%
11	3.114	642	645	649	rVB2	343	219	0.02%	0.003%
12	3.134	649	651	657	rBV3	525	354	0.03%	0.004%
13	3.208	668	674	677	rBV2	449	511	0.05%	0.006%
14	3.262	689	691	695	rBV2	251	163	0.02%	0.002%
15	3.288	696	699	701	rVV	329	166	0.02%	0.002%
16	3.365	720	723	724	rBV	308	139	0.01%	0.002%
17	3.378	724	727	734	rVB3	327	246	0.02%	0.003%
18	3.433	741	744	746	rBV	354	159	0.01%	0.002%
19	3.600	794	796	799	rBV2	263	152	0.01%	0.002%
20	3.680	819	821	823	rBV	298	129	0.01%	0.002%
21	3.706	827	829	831	rVB	262	118	0.01%	0.001%
22	3.719	831	833	836	rVB2	361	159	0.01%	0.002%
23	3.738	836	839	841	rBV	278	158	0.01%	0.002%
24	3.796	847	857	886	rBV	76596	224727	20.83%	2.819%
25	4.256	985	1000	1024	rBV	176094	455872	42.25%	5.718%
26	4.580	1099	1101	1103	rBV	433	148	0.01%	0.002%
27	4.693	1132	1136	1142	rVB2	575	605	0.06%	0.008%
28	4.719	1142	1144	1147	rBV2	599	420	0.04%	0.005%
29	4.744	1149	1152	1154	rBV2	720	419	0.04%	0.005%
30	4.812	1171	1173	1175	rBV	475	214	0.02%	0.003%
31	4.851	1182	1185	1189	rVB5	530	321	0.03%	0.004%
32	4.870	1189	1191	1194	rBV3	430	314	0.03%	0.004%
33	4.963	1203	1220	1243	rBV2	400135	1078903	100.00%	13.533%
34	5.269	1311	1315	1319	rVB3	938	752	0.07%	0.009%
35	5.416	1359	1361	1365	rBV	510	222	0.02%	0.003%
36	5.539	1382	1399	1423	rBV	283955	607147	56.27%	7.616%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031444.D
 Acq On : 08 Jun 2023 13:08
 Operator : SY/MD
 Sample : 03077-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.831	1478	1490	1509	rBV5	30490	70171	6.50%	0.880%
38	5.944	1523	1525	1526	rBV5	607	234	0.02%	0.003%
39	5.995	1528	1541	1566	rVV	248085	522972	48.47%	6.560%
40	6.281	1628	1630	1632	rBV2	381	156	0.01%	0.002%
41	6.297	1632	1635	1636	rBV2	411	214	0.02%	0.003%
42	6.333	1644	1646	1651	rBV4	387	358	0.03%	0.004%
43	6.375	1657	1659	1663	rVB2	457	250	0.02%	0.003%
44	6.397	1663	1666	1668	rBV2	489	294	0.03%	0.004%
45	6.506	1698	1700	1702	rVB2	385	169	0.02%	0.002%
46	6.529	1702	1707	1709	rBV2	634	499	0.05%	0.006%
47	6.555	1712	1715	1717	rBV	461	283	0.03%	0.004%
48	6.567	1717	1719	1721	rVB2	313	124	0.01%	0.002%
49	6.616	1728	1734	1738	rBV4	730	656	0.06%	0.008%
50	6.812	1792	1795	1796	rBV	296	128	0.01%	0.002%
51	6.828	1796	1800	1804	rBV2	321	247	0.02%	0.003%
52	6.850	1804	1807	1810	rBV2	597	353	0.03%	0.004%
53	6.918	1817	1828	1853	rBV	124310	239215	22.17%	3.001%
54	7.149	1896	1900	1903	rBV3	481	510	0.05%	0.006%
55	7.204	1915	1917	1919	rBV	351	170	0.02%	0.002%
56	7.249	1919	1931	1965	rBV	439652	789799	73.20%	9.907%
57	7.558	2017	2027	2049	rBV	92471	167045	15.48%	2.095%
58	7.818	2106	2108	2110	rBV	349	129	0.01%	0.002%
59	7.876	2122	2126	2127	rBV2	2839	1942	0.18%	0.024%
60	7.957	2148	2151	2154	rBV2	289	173	0.02%	0.002%
61	7.979	2154	2158	2159	rBV2	354	303	0.03%	0.004%
62	8.034	2165	2175	2212	rBV2	220103	500250	46.37%	6.275%
63	8.432	2297	2299	2301	rBV2	538	323	0.03%	0.004%
64	8.516	2322	2325	2328	rBV3	666	468	0.04%	0.006%
65	8.709	2383	2385	2387	rVB2	620	234	0.02%	0.003%
66	8.789	2399	2410	2437	rBV	454868	772407	71.59%	9.689%
67	9.095	2501	2505	2507	rBV4	594	504	0.05%	0.006%
68	9.239	2545	2550	2551	rBV	411	272	0.03%	0.003%
69	9.355	2582	2586	2590	rVV3	497	377	0.03%	0.005%
70	9.490	2624	2628	2631	rBV3	638	592	0.05%	0.007%
71	9.628	2666	2671	2673	rBV2	638	604	0.06%	0.008%
72	9.680	2685	2687	2689	rBV3	335	200	0.02%	0.003%
73	9.921	2759	2762	2765	rVV3	389	177	0.02%	0.002%
74	9.995	2781	2785	2787	rBV2	621	428	0.04%	0.005%
75	10.075	2806	2810	2811	rBV	340	214	0.02%	0.003%
76	10.114	2817	2822	2823	rBV	308	256	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031444.D
 Acq On : 08 Jun 2023 13:08
 Operator : SY/MD
 Sample : 03077-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.159	2824	2836	2860	rVB	296887	473717	43.91%	5.942%
78	10.243	2860	2862	2865	rVB	435	165	0.02%	0.002%
79	10.259	2865	2867	2868	rBV	450	205	0.02%	0.003%
80	10.333	2883	2890	2901	rVB	8579	13918	1.29%	0.175%
81	10.519	2946	2948	2953	rBV4	482	447	0.04%	0.006%
82	10.670	2993	2995	2997	rBV	362	198	0.02%	0.002%
83	10.702	3003	3005	3007	rBV	242	129	0.01%	0.002%
84	10.725	3010	3012	3018	rVB3	239	177	0.02%	0.002%
85	10.754	3019	3021	3024	rVV2	447	147	0.01%	0.002%
86	10.866	3052	3056	3058	rBV3	596	551	0.05%	0.007%
87	11.001	3097	3098	3102	rBV2	284	176	0.02%	0.002%
88	11.191	3145	3157	3176	rBV	437212	692362	64.17%	8.685%
89	11.416	3226	3227	3231	rBV	372	126	0.01%	0.002%
90	11.567	3262	3274	3298	rBV	448978	708594	65.68%	8.888%
91	12.024	3414	3416	3418	rVB2	794	359	0.03%	0.005%
92	12.037	3418	3420	3423	rBV2	466	239	0.02%	0.003%
93	12.088	3434	3436	3437	rBV	435	149	0.01%	0.002%
94	13.037	3729	3731	3734	rVB	444	250	0.02%	0.003%
95	13.291	3807	3810	3812	rBV3	584	359	0.03%	0.005%
96	13.513	3877	3879	3882	rVB2	745	295	0.03%	0.004%
97	13.603	3905	3907	3908	rBV2	452	178	0.02%	0.002%
98	13.796	3964	3967	3969	rBV3	760	541	0.05%	0.007%
99	13.866	3986	3989	3990	rBV2	435	293	0.03%	0.004%
100	14.654	4232	4234	4240	rBV5	745	587	0.05%	0.007%




Sum of corrected areas: 7972155

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031444.D
Acq On : 08 Jun 2023 13:08
Operator : SY/MD
Sample : 03077-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

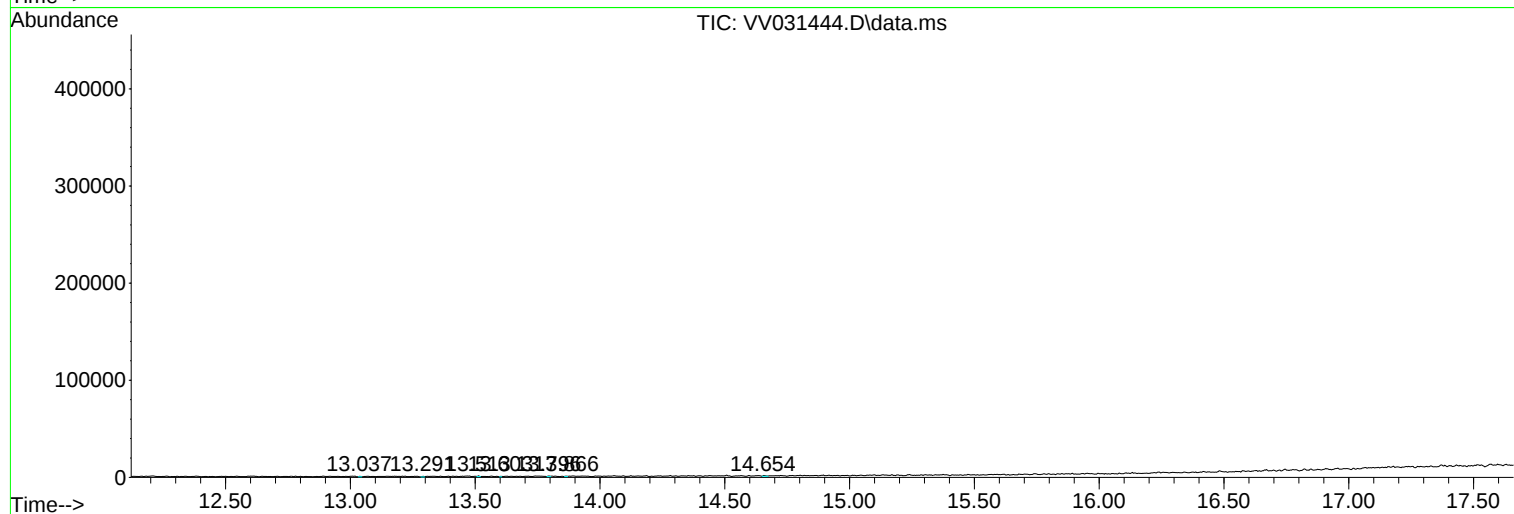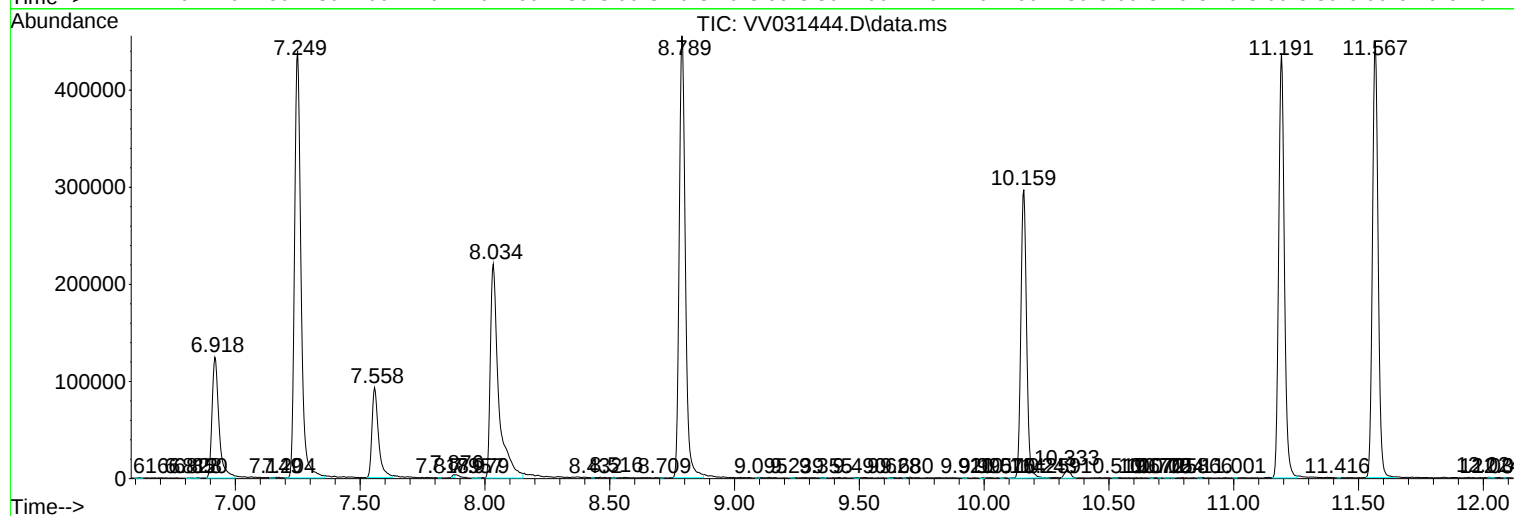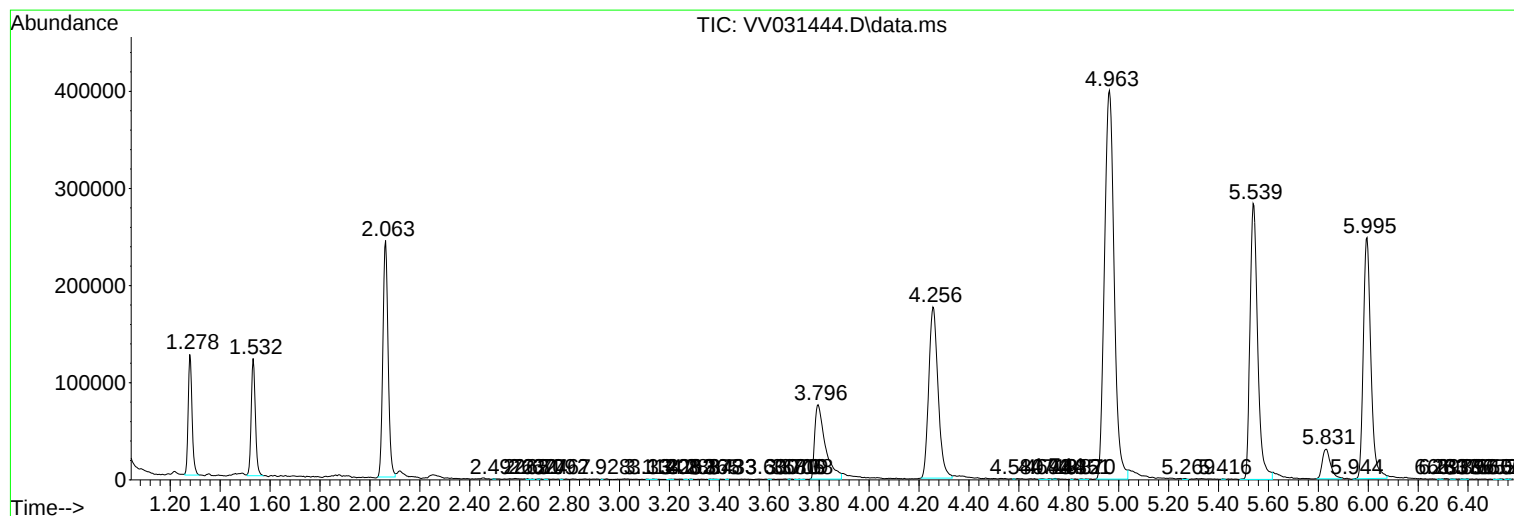

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031444.D
Acq On : 08 Jun 2023 13:08
Operator : SY/MD
Sample : 03077-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031444.D
Acq On : 08 Jun 2023 13:08
Operator : SY/MD
Sample : 03077-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------