

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031445.D
 Acq On : 08 Jun 2023 13:31
 Operator : SY/MD
 Sample : 03077-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	127095	138942	12.82%	1.703%
2	1.532	146	153	169	rVB	119085	142035	13.10%	1.741%
3	2.063	307	318	330	rBV	239704	355492	32.80%	4.358%
4	2.700	511	516	519	rBV3	987	891	0.08%	0.011%
5	2.774	537	539	541	rBV	473	254	0.02%	0.003%
6	2.912	579	582	587	rVB4	650	620	0.06%	0.008%
7	2.941	587	591	593	rBV	510	332	0.03%	0.004%
8	2.973	599	601	602	rBV	373	160	0.01%	0.002%
9	3.069	627	631	633	rBV	485	299	0.03%	0.004%
10	3.092	635	638	639	rVV2	306	172	0.02%	0.002%
11	3.105	639	642	645	rVV3	374	297	0.03%	0.004%
12	3.163	657	660	663	rBV3	439	265	0.02%	0.003%
13	3.214	673	676	678	rBV2	381	229	0.02%	0.003%
14	3.253	685	688	690	rBV2	424	259	0.02%	0.003%
15	3.417	732	739	743	rBV2	404	407	0.04%	0.005%
16	3.446	746	748	752	rVB3	359	197	0.02%	0.002%
17	3.497	763	764	768	rVB	477	170	0.02%	0.002%
18	3.519	768	771	774	rBV2	355	236	0.02%	0.003%
19	3.536	774	776	779	rBV	292	161	0.01%	0.002%
20	3.600	795	796	799	rBV	243	180	0.02%	0.002%
21	3.629	803	805	809	rVB2	317	206	0.02%	0.003%
22	3.706	826	829	831	rBV	331	185	0.02%	0.002%
23	3.735	837	838	845	rVB3	255	220	0.02%	0.003%
24	3.793	846	856	883	rBV	81080	232285	21.43%	2.847%
25	4.256	983	1000	1026	rBV	175021	459079	42.36%	5.627%
26	4.558	1092	1094	1096	rBV2	596	275	0.03%	0.003%
27	4.696	1131	1137	1139	rBV3	524	460	0.04%	0.006%
28	4.744	1150	1152	1153	rBV	551	232	0.02%	0.003%
29	4.796	1166	1168	1170	rBV2	322	164	0.02%	0.002%
30	4.838	1177	1181	1184	rBV2	301	224	0.02%	0.003%
31	4.863	1185	1189	1190	rBV3	415	323	0.03%	0.004%
32	4.963	1202	1220	1246	rBV2	403075	1083851	100.00%	13.286%
33	5.291	1319	1322	1326	rBV3	616	464	0.04%	0.006%
34	5.320	1329	1331	1333	rVB2	658	278	0.03%	0.003%
35	5.339	1334	1337	1340	rBV2	906	527	0.05%	0.006%
36	5.539	1387	1399	1431	rBV	306252	652902	60.24%	8.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031445.D
 Acq On : 08 Jun 2023 13:31
 Operator : SY/MD
 Sample : 03077-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.777	1471	1473	1476	rBV3	653	469	0.04%	0.006%
38	5.828	1480	1489	1512	rVB3	29686	65808	6.07%	0.807%
39	5.995	1527	1541	1566	rBV2	246684	528661	48.78%	6.480%
40	6.272	1624	1627	1632	rBV4	529	537	0.05%	0.007%
41	6.416	1668	1672	1674	rBV2	517	359	0.03%	0.004%
42	6.494	1694	1696	1698	rVB2	621	189	0.02%	0.002%
43	6.564	1715	1718	1721	rBV	240	218	0.02%	0.003%
44	6.584	1721	1724	1727	rVB3	467	347	0.03%	0.004%
45	6.635	1736	1740	1742	rBV3	708	548	0.05%	0.007%
46	6.664	1746	1749	1753	rBV	368	294	0.03%	0.004%
47	6.783	1783	1786	1792	rBV2	340	372	0.03%	0.005%
48	6.918	1814	1828	1855	rBV	123776	237521	21.91%	2.912%
49	7.249	1919	1931	1954	rBV	437768	778638	71.84%	9.544%
50	7.558	2017	2027	2054	rBV	91664	171391	15.81%	2.101%
51	7.786	2096	2098	2100	rVB2	558	218	0.02%	0.003%
52	7.979	2156	2158	2164	rVB	595	437	0.04%	0.005%
53	8.034	2164	2175	2207	rBV2	228944	505972	46.68%	6.202%
54	8.513	2321	2324	2326	rBV2	628	426	0.04%	0.005%
55	8.616	2354	2356	2360	rBV3	441	292	0.03%	0.004%
56	8.696	2378	2381	2383	rBV2	645	303	0.03%	0.004%
57	8.789	2396	2410	2436	rBV	490605	828656	76.45%	10.158%
58	9.137	2514	2518	2519	rBV	342	227	0.02%	0.003%
59	9.146	2519	2521	2526	rVV2	475	412	0.04%	0.005%
60	9.211	2539	2541	2545	rBV2	319	262	0.02%	0.003%
61	9.265	2552	2558	2562	rBV4	798	797	0.07%	0.010%
62	9.362	2582	2588	2589	rBV2	539	468	0.04%	0.006%
63	9.387	2594	2596	2598	rBV3	280	175	0.02%	0.002%
64	9.455	2614	2617	2620	rVB2	396	233	0.02%	0.003%
65	9.481	2620	2625	2626	rBV3	493	397	0.04%	0.005%
66	9.539	2640	2643	2645	rBV2	330	172	0.02%	0.002%
67	9.593	2657	2660	2662	rBV2	448	261	0.02%	0.003%
68	9.619	2665	2668	2671	rVB3	655	338	0.03%	0.004%
69	9.638	2671	2674	2677	rBV	385	218	0.02%	0.003%
70	9.677	2684	2686	2687	rBV	415	168	0.02%	0.002%
71	9.731	2699	2703	2705	rBV2	372	241	0.02%	0.003%
72	9.764	2708	2713	2717	rVV4	554	567	0.05%	0.007%
73	9.944	2766	2769	2771	rVB2	581	276	0.03%	0.003%
74	9.982	2778	2781	2784	rVV3	510	310	0.03%	0.004%
75	10.066	2804	2807	2812	rBV4	560	598	0.06%	0.007%
76	10.159	2824	2836	2863	rVB	296054	479645	44.25%	5.879%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031445.D
 Acq On : 08 Jun 2023 13:31
 Operator : SY/MD
 Sample : 03077-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.259	2863	2867	2870	rVB2	450	348	0.03%	0.004%
78	10.278	2871	2873	2875	rVV	449	189	0.02%	0.002%
79	10.336	2884	2891	2898	rVB4	3506	5278	0.49%	0.065%
80	10.587	2967	2969	2973	rVB2	468	388	0.04%	0.005%
81	10.619	2973	2979	2981	rBV2	632	552	0.05%	0.007%
82	11.133	3135	3139	3140	rBV2	461	228	0.02%	0.003%
83	11.191	3146	3157	3178	rBV	461068	742769	68.53%	9.105%
84	11.387	3216	3218	3221	rVB3	783	411	0.04%	0.005%
85	11.468	3240	3243	3246	rBV4	467	369	0.03%	0.005%
86	11.567	3262	3274	3298	rBV	458177	720965	66.52%	8.838%
87	11.731	3322	3325	3326	rBV2	539	303	0.03%	0.004%
88	11.927	3384	3386	3390	rBV2	377	257	0.02%	0.003%
89	11.982	3401	3403	3408	rVB4	592	258	0.02%	0.003%
90	12.140	3448	3452	3457	rBV3	543	528	0.05%	0.006%
91	12.165	3457	3460	3463	rBV2	713	490	0.05%	0.006%
92	12.291	3493	3499	3502	rBV2	290	380	0.04%	0.005%
93	12.879	3675	3682	3685	rBV3	538	783	0.07%	0.010%
94	13.008	3720	3722	3724	rBV2	409	217	0.02%	0.003%
95	13.127	3756	3759	3760	rBV3	509	309	0.03%	0.004%
96	13.339	3822	3825	3827	rBV2	512	273	0.03%	0.003%
97	13.435	3853	3855	3857	rBV	325	182	0.02%	0.002%
98	13.525	3881	3883	3884	rBV	388	179	0.02%	0.002%
99	13.535	3884	3886	3889	rVB3	691	353	0.03%	0.004%
100	13.635	3911	3917	3923	rBV7	827	1283	0.12%	0.016%



Sum of corrected areas: 8157986

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031445.D
Acq On : 08 Jun 2023 13:31
Operator : SY/MD
Sample : 03077-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

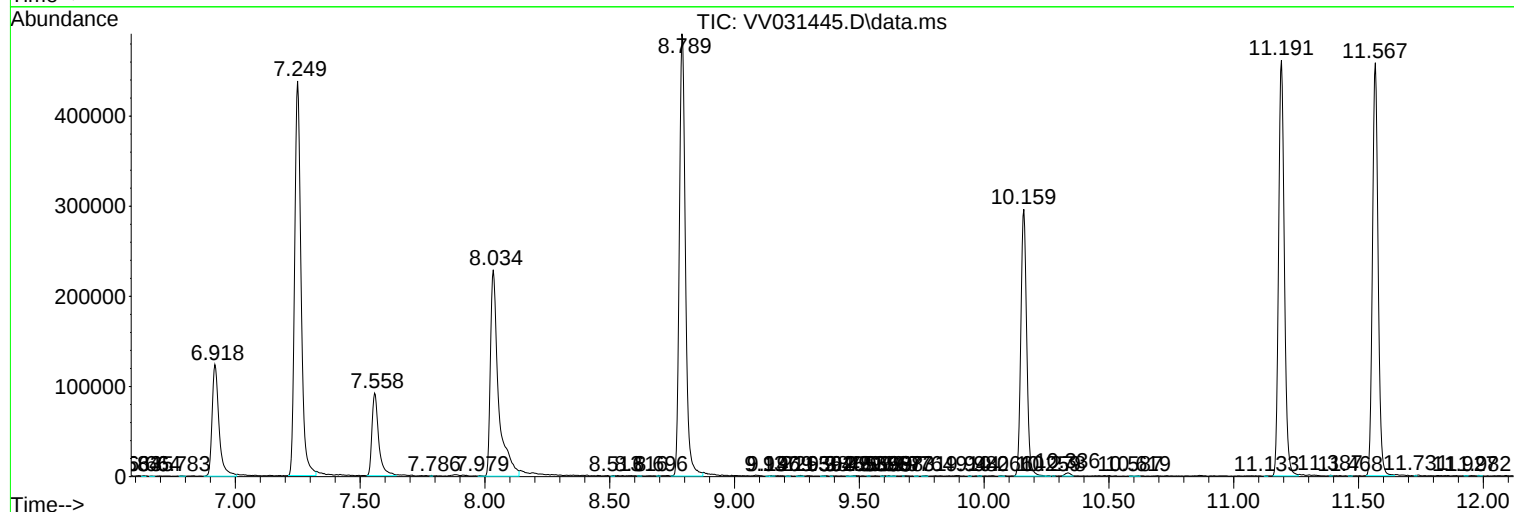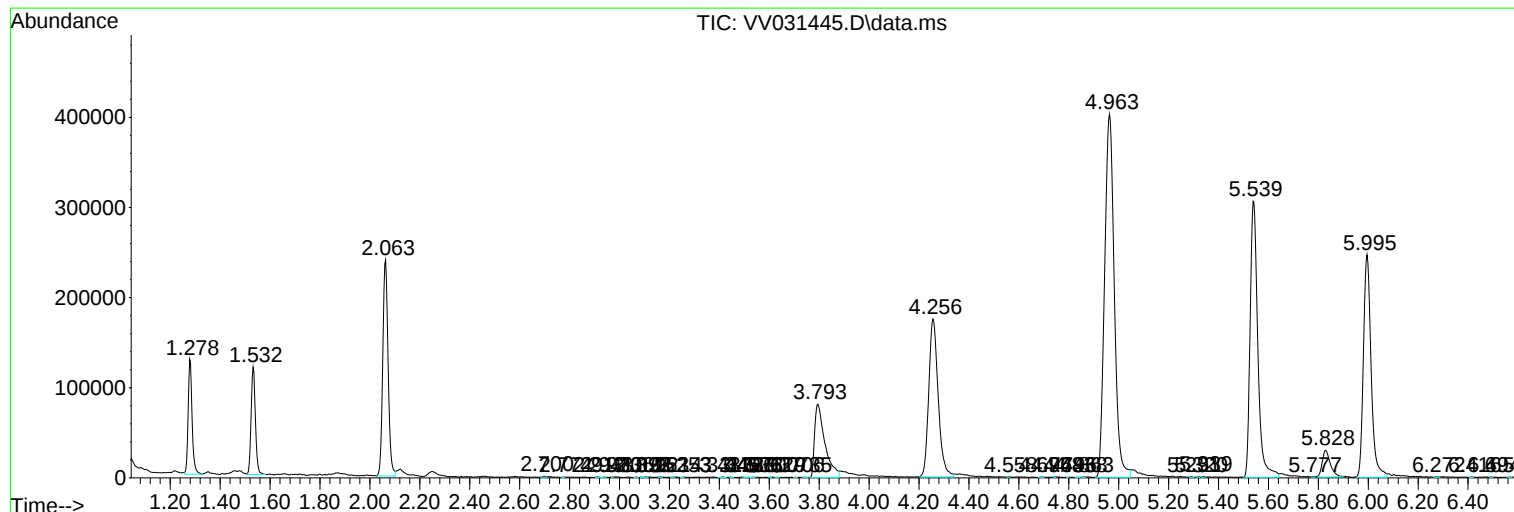

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031445.D
Acq On : 08 Jun 2023 13:31
Operator : SY/MD
Sample : 03077-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031445.D
Acq On : 08 Jun 2023 13:31
Operator : SY/MD
Sample : 03077-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------