

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031447.D
 Acq On : 08 Jun 2023 14:19
 Operator : SY/MD
 Sample : 03077-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

Signal : TIC: VV031447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	112163	123864	12.88%	1.648%
2	1.532	147	153	164	rVB	106701	123758	12.87%	1.647%
3	2.063	308	318	331	rBV	212894	314421	32.70%	4.184%
4	2.561	471	473	477	rVB3	503	287	0.03%	0.004%
5	2.587	477	481	485	rVB3	463	432	0.04%	0.006%
6	2.622	489	492	494	rBV2	511	336	0.03%	0.004%
7	2.709	513	519	520	rBV3	1106	839	0.09%	0.011%
8	2.802	544	548	550	rBV	579	422	0.04%	0.006%
9	2.889	573	575	577	rBV2	398	243	0.03%	0.003%
10	2.947	591	593	595	rBV	419	179	0.02%	0.002%
11	2.979	601	603	608	rBV2	344	224	0.02%	0.003%
12	3.008	609	612	615	rVB2	544	295	0.03%	0.004%
13	3.050	623	625	628	rBV2	389	179	0.02%	0.002%
14	3.105	638	642	644	rBV2	594	420	0.04%	0.006%
15	3.121	645	647	650	rBV2	603	349	0.04%	0.005%
16	3.178	663	665	666	rBV	289	161	0.02%	0.002%
17	3.246	682	686	687	rBV	551	225	0.02%	0.003%
18	3.301	700	703	709	rVB3	252	216	0.02%	0.003%
19	3.330	709	712	717	rBV2	441	459	0.05%	0.006%
20	3.362	719	722	725	rVV	439	283	0.03%	0.004%
21	3.391	728	731	733	rVV2	461	256	0.03%	0.003%
22	3.416	737	739	743	rVV3	441	255	0.03%	0.003%
23	3.436	743	745	746	rVV3	275	141	0.01%	0.002%
24	3.449	747	749	752	rVB2	686	362	0.04%	0.005%
25	3.490	759	762	764	rBV2	347	235	0.02%	0.003%
26	3.587	790	792	797	rBV3	381	305	0.03%	0.004%
27	3.670	815	818	823	rBV	540	507	0.05%	0.007%
28	3.744	838	841	843	rVB	480	194	0.02%	0.003%
29	3.796	848	857	889	rBV	74958	221993	23.09%	2.954%
30	4.256	984	1000	1024	rBV2	160363	416524	43.32%	5.542%
31	4.632	1113	1117	1118	rBV	494	302	0.03%	0.004%
32	4.728	1144	1147	1149	rBV3	413	287	0.03%	0.004%
33	4.812	1171	1173	1176	rVB2	500	289	0.03%	0.004%
34	4.828	1176	1178	1179	rBV2	253	127	0.01%	0.002%
35	4.963	1202	1220	1243	rBV2	361899	961509	100.00%	12.794%
36	5.333	1331	1335	1338	rBV3	527	459	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031447.D
 Acq On : 08 Jun 2023 14:19
 Operator : SY/MD
 Sample : 03077-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.368	1344	1346	1350	rVB2	281	199	0.02%	0.003%
38	5.403	1353	1357	1360	rBV3	617	495	0.05%	0.007%
39	5.423	1360	1363	1366	rVB	762	420	0.04%	0.006%
40	5.458	1371	1374	1378	rVB2	462	297	0.03%	0.004%
41	5.481	1378	1381	1382	rBV2	499	212	0.02%	0.003%
42	5.542	1387	1400	1441	rBV	295920	642641	66.84%	8.551%
43	5.831	1480	1490	1509	rBV3	26197	55436	5.77%	0.738%
44	5.995	1527	1541	1566	rBV2	222381	477996	49.71%	6.360%
45	6.436	1675	1678	1680	rBV	344	225	0.02%	0.003%
46	6.448	1680	1682	1685	rBV3	357	223	0.02%	0.003%
47	6.500	1696	1698	1702	rVB2	322	219	0.02%	0.003%
48	6.519	1702	1704	1706	rBV2	329	127	0.01%	0.002%
49	6.571	1716	1720	1723	rBV2	677	494	0.05%	0.007%
50	6.657	1742	1747	1751	rBV3	477	486	0.05%	0.006%
51	6.715	1762	1765	1770	rVB2	430	289	0.03%	0.004%
52	6.738	1770	1772	1776	rBV2	444	257	0.03%	0.003%
53	6.860	1808	1810	1815	rVB3	464	369	0.04%	0.005%
54	6.918	1817	1828	1857	rBV	107515	215943	22.46%	2.873%
55	7.249	1919	1931	1959	rBV	380124	681642	70.89%	9.070%
56	7.513	2011	2013	2016	rBV2	521	266	0.03%	0.004%
57	7.558	2018	2027	2052	rBV	81933	151845	15.79%	2.020%
58	7.767	2090	2092	2095	rBV2	404	209	0.02%	0.003%
59	7.854	2116	2119	2120	rBV2	369	226	0.02%	0.003%
60	7.966	2152	2154	2156	rBV2	446	203	0.02%	0.003%
61	7.989	2156	2161	2163	rBV3	587	377	0.04%	0.005%
62	8.034	2165	2175	2210	rBV3	209589	468701	48.75%	6.236%
63	8.368	2277	2279	2280	rBV	693	249	0.03%	0.003%
64	8.432	2296	2299	2301	rBV2	656	411	0.04%	0.005%
65	8.474	2309	2312	2315	rBV2	442	285	0.03%	0.004%
66	8.497	2315	2319	2322	rVV5	763	519	0.05%	0.007%
67	8.542	2331	2333	2335	rBV	322	182	0.02%	0.002%
68	8.574	2341	2343	2346	rVB2	642	321	0.03%	0.004%
69	8.789	2398	2410	2432	rBV	486763	802035	83.41%	10.672%
70	8.989	2471	2472	2475	rVB3	673	318	0.03%	0.004%
71	9.358	2585	2587	2591	rBV3	396	253	0.03%	0.003%
72	9.468	2617	2621	2622	rBV	271	145	0.02%	0.002%
73	9.487	2625	2627	2628	rBV	717	305	0.03%	0.004%
74	9.525	2637	2639	2642	rVB2	689	379	0.04%	0.005%
75	9.606	2660	2664	2667	rBV2	417	322	0.03%	0.004%
76	9.686	2687	2689	2692	rVB	317	187	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031447.D
 Acq On : 08 Jun 2023 14:19
 Operator : SY/MD
 Sample : 03077-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	9.706	2692	2695	2696	rBV2	336	177	0.02%	0.002%
78	9.815	2726	2729	2731	rBV	296	212	0.02%	0.003%
79	9.870	2742	2746	2748	rBV2	979	721	0.07%	0.010%
80	9.911	2757	2759	2762	rVB2	498	226	0.02%	0.003%
81	9.985	2779	2782	2784	rBV	384	191	0.02%	0.003%
82	10.159	2822	2836	2862	rBV	279004	448612	46.66%	5.969%
83	10.320	2877	2886	2887	rBV5	578	681	0.07%	0.009%
84	10.448	2922	2926	2929	rBV2	456	467	0.05%	0.006%
85	10.689	2999	3001	3004	rBV	303	209	0.02%	0.003%
86	10.857	3048	3053	3057	rBV2	839	1082	0.11%	0.014%
87	10.943	3077	3080	3082	rBV2	453	234	0.02%	0.003%
88	11.133	3133	3139	3143	rBV2	1240	1463	0.15%	0.019%
89	11.191	3146	3157	3181	rBV	459847	731521	76.08%	9.733%
90	11.493	3249	3251	3253	rBV	407	218	0.02%	0.003%
91	11.567	3262	3274	3297	rBV	406252	650161	67.62%	8.651%
92	12.095	3436	3438	3440	rBV	374	131	0.01%	0.002%
93	12.394	3528	3531	3532	rBV	343	203	0.02%	0.003%
94	12.641	3606	3608	3612	rVB2	887	477	0.05%	0.006%
95	12.667	3612	3616	3617	rBV2	584	383	0.04%	0.005%
96	12.931	3696	3698	3699	rBV	326	172	0.02%	0.002%
97	13.043	3731	3733	3736	rBV3	667	462	0.05%	0.006%
98	13.111	3752	3754	3755	rBV3	290	125	0.01%	0.002%
99	13.377	3835	3837	3840	rVB2	635	208	0.02%	0.003%
100	13.400	3842	3844	3847	rBV2	345	129	0.01%	0.002%




Sum of corrected areas: 7515510

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031447.D
Acq On : 08 Jun 2023 14:19
Operator : SY/MD
Sample : 03077-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

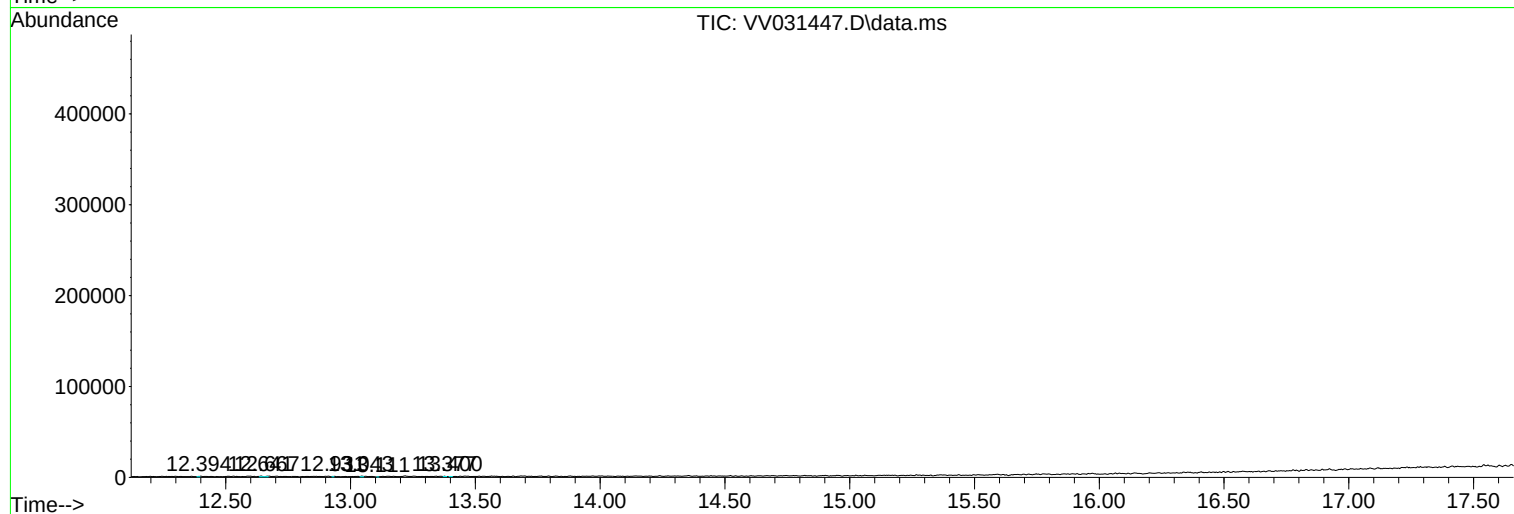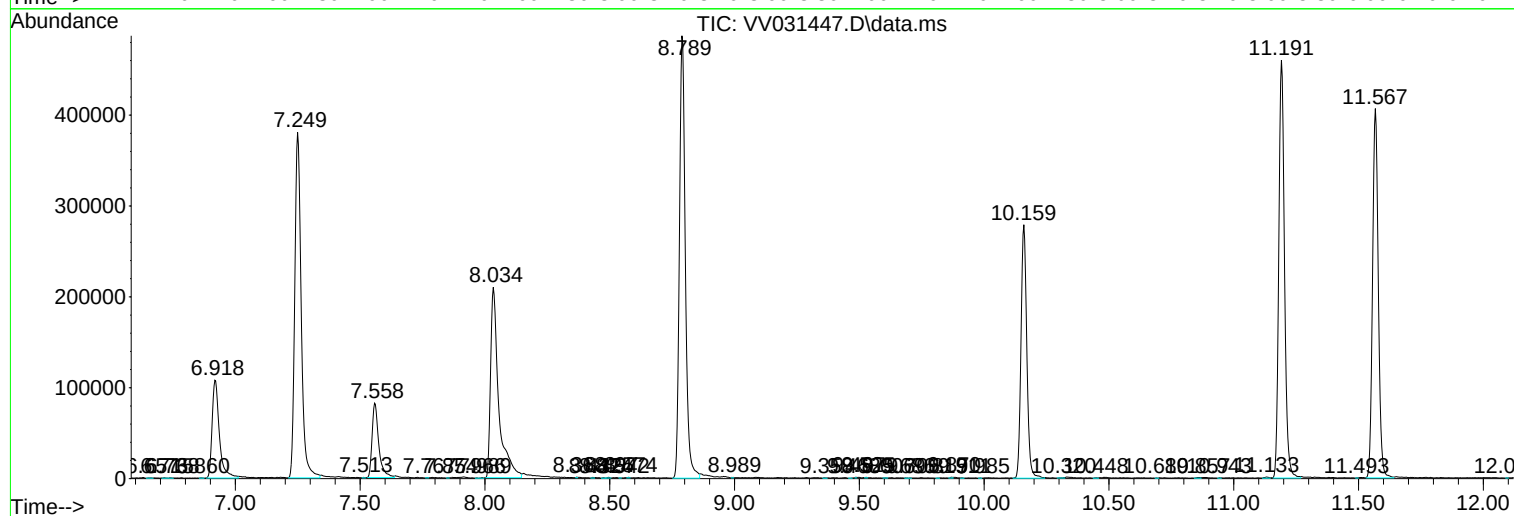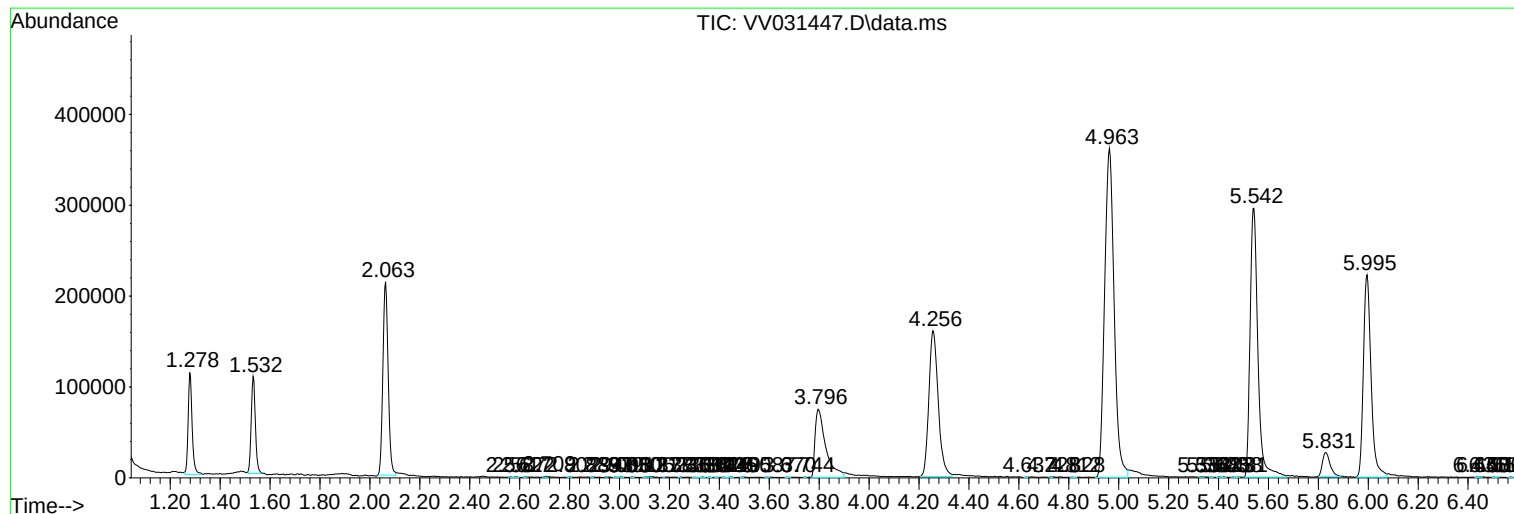

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031447.D
Acq On : 08 Jun 2023 14:19
Operator : SY/MD
Sample : 03077-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031447.D
Acq On : 08 Jun 2023 14:19
Operator : SY/MD
Sample : 03077-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc