

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031448.D
 Acq On : 08 Jun 2023 14:42
 Operator : SY/MD
 Sample : 03077-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	112599	122468	12.09%	1.420%
2	1.532	146	153	168	rVB	109454	130762	12.90%	1.516%
3	2.063	308	318	333	rBV2	241071	369462	36.46%	4.284%
4	2.220	365	367	369	rBV2	660	355	0.04%	0.004%
5	2.433	431	433	434	rBV	417	223	0.02%	0.003%
6	2.491	448	451	452	rBV	500	279	0.03%	0.003%
7	2.712	517	520	522	rVB3	512	264	0.03%	0.003%
8	2.864	565	567	571	rVV3	324	257	0.03%	0.003%
9	2.976	600	602	607	rVB3	315	228	0.02%	0.003%
10	3.034	617	620	622	rBV2	274	180	0.02%	0.002%
11	3.092	636	638	641	rBV3	605	435	0.04%	0.005%
12	3.214	673	676	679	rBV3	315	225	0.02%	0.003%
13	3.259	687	690	696	rBV4	404	452	0.04%	0.005%
14	3.307	704	705	711	rVB3	463	393	0.04%	0.005%
15	3.346	712	717	719	rBV	265	198	0.02%	0.002%
16	3.439	742	746	751	rVB2	396	370	0.04%	0.004%
17	3.503	763	766	770	rVB2	391	230	0.02%	0.003%
18	3.542	776	778	780	rBV	402	209	0.02%	0.002%
19	3.577	786	789	795	rVB3	361	287	0.03%	0.003%
20	3.638	803	808	809	rBV	291	225	0.02%	0.003%
21	3.667	815	817	824	rVB3	476	275	0.03%	0.003%
22	3.716	830	832	834	rBV2	563	286	0.03%	0.003%
23	3.751	839	843	847	rVB2	270	209	0.02%	0.002%
24	3.796	847	857	895	rBV	81519	274288	27.07%	3.180%
25	4.191	977	980	983	rBV3	856	638	0.06%	0.007%
26	4.256	985	1000	1024	rVV2	162851	428721	42.31%	4.971%
27	4.606	1107	1109	1110	rBV	410	176	0.02%	0.002%
28	4.642	1117	1120	1123	rBV4	466	329	0.03%	0.004%
29	4.658	1123	1125	1127	rVB	536	189	0.02%	0.002%
30	4.693	1132	1136	1141	rBV4	350	300	0.03%	0.003%
31	4.716	1141	1143	1147	rBV2	325	221	0.02%	0.003%
32	4.738	1147	1150	1152	rBV4	436	204	0.02%	0.002%
33	4.799	1167	1169	1175	rBV2	284	233	0.02%	0.003%
34	4.889	1195	1197	1203	rBV7	485	484	0.05%	0.006%
35	4.963	1203	1220	1260	rBV2	375515	1013271	100.00%	11.748%
36	5.281	1318	1319	1323	rVB2	578	275	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031448.D
 Acq On : 08 Jun 2023 14:42
 Operator : SY/MD
 Sample : 03077-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.413	1357	1360	1362	rBV3	425	252	0.02%	0.003%
38	5.539	1387	1399	1430	rBV2	304919	646257	63.78%	7.493%
39	5.767	1468	1470	1473	rVB2	1048	545	0.05%	0.006%
40	5.838	1478	1492	1523	rBV2	406269	850331	83.92%	9.859%
41	5.995	1529	1541	1571	rVB	230721	487303	48.09%	5.650%
42	6.275	1627	1628	1631	rVB2	694	236	0.02%	0.003%
43	6.355	1650	1653	1658	rVB3	836	554	0.05%	0.006%
44	6.397	1662	1666	1667	rBV3	434	275	0.03%	0.003%
45	6.561	1712	1717	1718	rBV	362	249	0.02%	0.003%
46	6.613	1730	1733	1736	rBV3	722	512	0.05%	0.006%
47	6.764	1777	1780	1781	rBV	362	171	0.02%	0.002%
48	6.918	1818	1828	1854	rBV	112749	218069	21.52%	2.528%
49	7.249	1919	1931	1967	rBV	396809	717534	70.81%	8.319%
50	7.558	2018	2027	2055	rBV	83456	156117	15.41%	1.810%
51	7.760	2086	2090	2091	rBV3	431	245	0.02%	0.003%
52	8.034	2165	2175	2209	rBV2	220360	491472	48.50%	5.698%
53	8.519	2324	2326	2330	rBV	371	229	0.02%	0.003%
54	8.545	2330	2334	2335	rBV2	483	304	0.03%	0.004%
55	8.629	2358	2360	2362	rBV2	354	188	0.02%	0.002%
56	8.645	2363	2365	2368	rVV2	549	327	0.03%	0.004%
57	8.789	2398	2410	2438	rBV	491485	814890	80.42%	9.448%
58	8.995	2472	2474	2477	rBV2	655	386	0.04%	0.004%
59	9.133	2514	2517	2519	rBV2	430	275	0.03%	0.003%
60	9.201	2535	2538	2541	rBV3	371	185	0.02%	0.002%
61	9.336	2576	2580	2581	rBV	368	281	0.03%	0.003%
62	9.394	2592	2598	2604	rBV5	556	728	0.07%	0.008%
63	9.484	2622	2626	2636	rBV6	1037	1233	0.12%	0.014%
64	9.526	2636	2639	2642	rBV	440	289	0.03%	0.003%
65	9.619	2664	2668	2673	rBV3	500	432	0.04%	0.005%
66	9.670	2682	2684	2688	rVB2	487	227	0.02%	0.003%
67	9.741	2704	2706	2707	rBV	544	219	0.02%	0.003%
68	9.776	2715	2717	2721	rBV2	457	242	0.02%	0.003%
69	9.825	2727	2732	2737	rBV3	520	578	0.06%	0.007%
70	9.918	2759	2761	2762	rBV2	393	178	0.02%	0.002%
71	9.976	2777	2779	2781	rBV	507	235	0.02%	0.003%
72	9.995	2781	2785	2786	rBV2	341	224	0.02%	0.003%
73	10.159	2824	2836	2863	rVV	291713	462252	45.62%	5.359%
74	10.391	2903	2908	2911	rBV3	368	326	0.03%	0.004%
75	10.410	2911	2914	2915	rVV2	417	218	0.02%	0.003%
76	10.529	2947	2951	2952	rBV2	271	168	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031448.D
 Acq On : 08 Jun 2023 14:42
 Operator : SY/MD
 Sample : 03077-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.564	2958	2962	2964	rBV2	345	250	0.02%	0.003%
78	10.760	3021	3023	3026	rBV	316	207	0.02%	0.002%
79	10.863	3049	3055	3058	rBV4	880	993	0.10%	0.012%
80	10.944	3077	3080	3082	rBV3	373	209	0.02%	0.002%
81	10.969	3086	3088	3092	rVB2	450	271	0.03%	0.003%
82	10.992	3092	3095	3101	rBV3	620	487	0.05%	0.006%
83	11.117	3132	3134	3136	rBV2	395	240	0.02%	0.003%
84	11.191	3145	3157	3183	rBV	468911	739710	73.00%	8.576%
85	11.567	3262	3274	3296	rBV	425509	674211	66.54%	7.817%
86	11.767	3335	3336	3341	rVB3	406	228	0.02%	0.003%
87	11.841	3356	3359	3361	rBV2	551	372	0.04%	0.004%
88	12.037	3418	3420	3422	rBV2	450	238	0.02%	0.003%
89	12.149	3451	3455	3458	rBV3	732	596	0.06%	0.007%
90	12.342	3513	3515	3517	rBV	429	182	0.02%	0.002%
91	12.455	3547	3550	3557	rBV3	651	787	0.08%	0.009%
92	12.841	3669	3670	3677	rVB	511	362	0.04%	0.004%
93	13.014	3722	3724	3728	rBV3	578	341	0.03%	0.004%
94	13.050	3733	3735	3739	rVB	789	465	0.05%	0.005%
95	13.075	3739	3743	3747	rBV4	508	536	0.05%	0.006%
96	13.181	3773	3776	3777	rBV2	469	245	0.02%	0.003%
97	13.400	3840	3844	3845	rBV	327	253	0.02%	0.003%
98	13.464	3862	3864	3867	rBV2	802	436	0.04%	0.005%
99	13.522	3876	3882	3884	rVB3	608	590	0.06%	0.007%
100	13.673	3926	3929	3932	rBV4	636	559	0.06%	0.006%




Sum of corrected areas: 8625105

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031448.D
Acq On : 08 Jun 2023 14:42
Operator : SY/MD
Sample : 03077-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

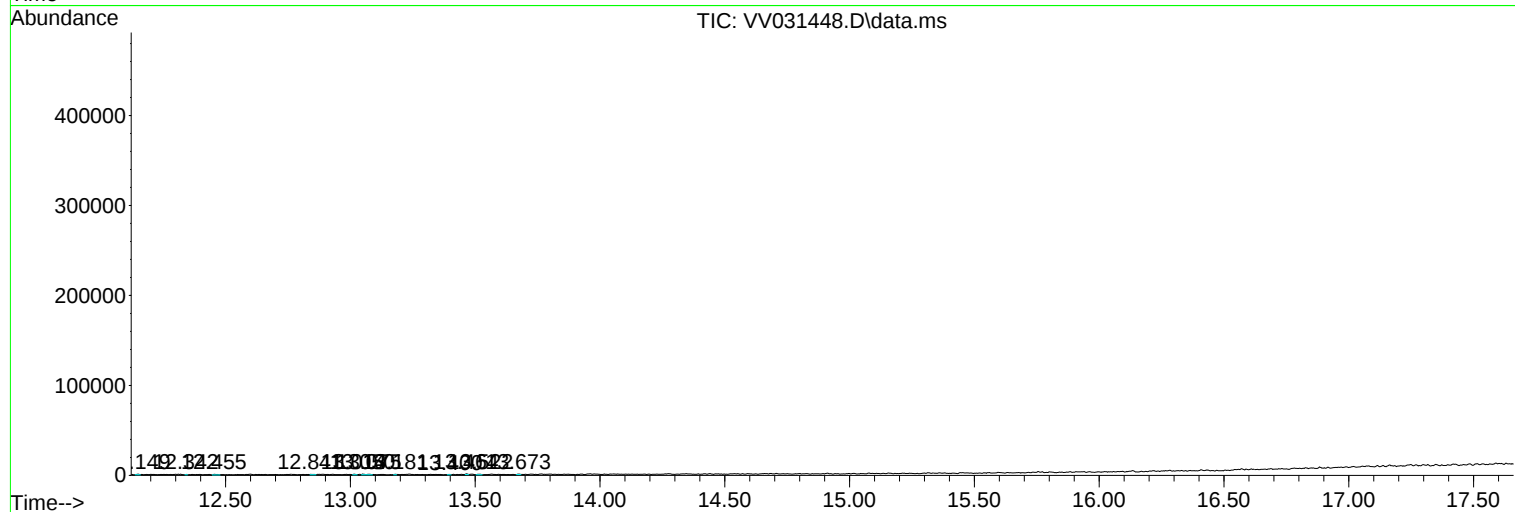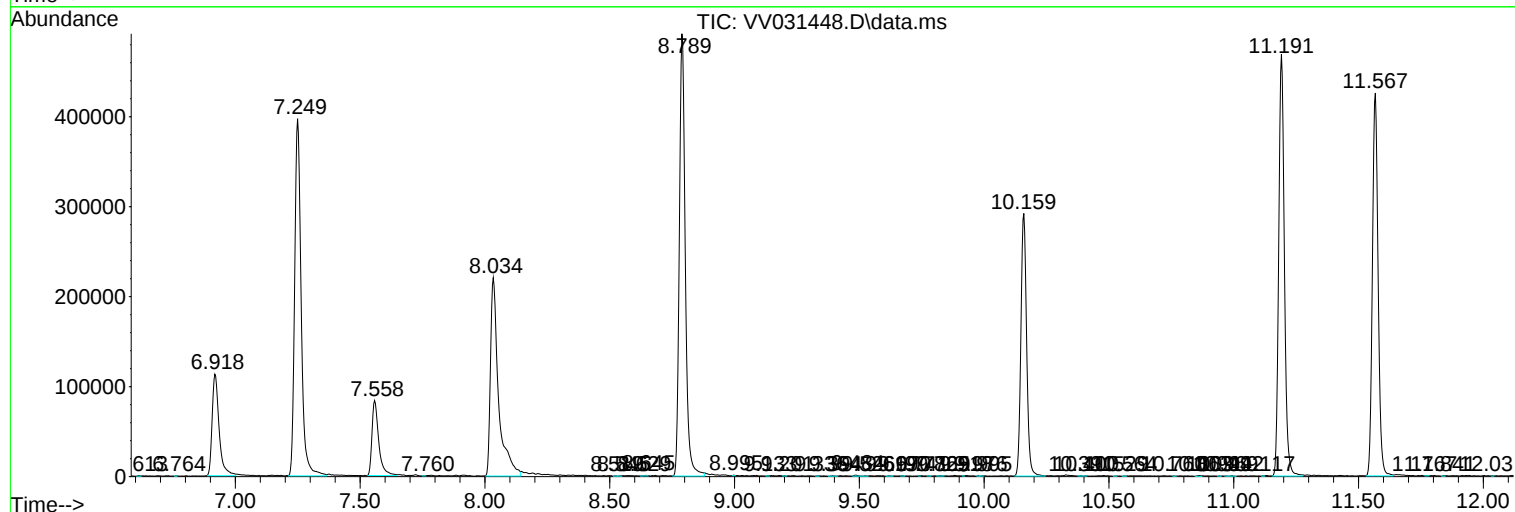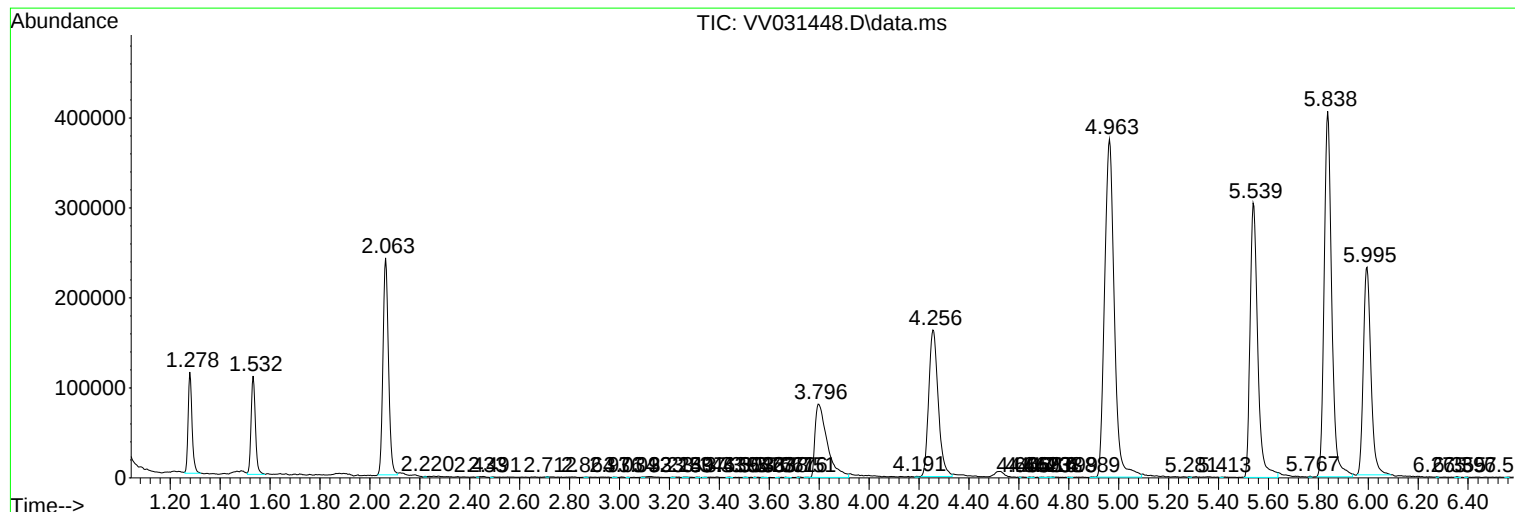

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031448.D
Acq On : 08 Jun 2023 14:42
Operator : SY/MD
Sample : 03077-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031448.D
Acq On : 08 Jun 2023 14:42
Operator : SY/MD
Sample : 03077-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FC3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------