

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031454.D
 Acq On : 08 Jun 2023 17:26
 Operator : SY/MD
 Sample : 03098-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZES4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	98057	105919	12.25%	1.589%
2	1.532	147	153	167	rVB	95398	113789	13.16%	1.707%
3	2.063	308	318	330	rBV	182705	267786	30.97%	4.017%
4	2.449	434	438	448	rVB5	1490	1979	0.23%	0.030%
5	2.677	506	509	511	rBV3	489	302	0.03%	0.005%
6	2.700	511	516	519	rBV4	1223	959	0.11%	0.014%
7	2.809	547	550	553	rBV	507	345	0.04%	0.005%
8	2.934	581	589	590	rBV	381	370	0.04%	0.006%
9	2.986	601	605	606	rBV2	443	284	0.03%	0.004%
10	3.034	617	620	622	rBV2	301	258	0.03%	0.004%
11	3.153	654	657	658	rBV	371	209	0.02%	0.003%
12	3.349	713	718	720	rBV4	526	438	0.05%	0.007%
13	3.388	729	730	735	rBV2	370	326	0.04%	0.005%
14	3.581	783	790	795	rBV3	524	603	0.07%	0.009%
15	3.732	833	837	843	rVB3	536	591	0.07%	0.009%
16	3.799	848	858	889	rBV	69379	209340	24.21%	3.141%
17	4.256	983	1000	1030	rBV	142038	380945	44.06%	5.715%
18	4.574	1097	1099	1102	rVB3	607	321	0.04%	0.005%
19	4.609	1106	1110	1113	rBV2	714	497	0.06%	0.007%
20	4.658	1124	1125	1129	rVB	678	262	0.03%	0.004%
21	4.677	1129	1131	1136	rVB3	387	241	0.03%	0.004%
22	4.709	1138	1141	1146	rBV3	253	247	0.03%	0.004%
23	4.764	1155	1158	1160	rBV2	382	271	0.03%	0.004%
24	4.870	1188	1191	1194	rBV4	454	356	0.04%	0.005%
25	4.963	1202	1220	1247	rBV3	322935	864623	100.00%	12.971%
26	5.159	1279	1281	1285	rVB4	929	356	0.04%	0.005%
27	5.404	1355	1357	1360	rVB2	383	198	0.02%	0.003%
28	5.420	1360	1362	1365	rBV	378	259	0.03%	0.004%
29	5.449	1369	1371	1372	rBV	391	196	0.02%	0.003%
30	5.458	1372	1374	1377	rVB	671	270	0.03%	0.004%
31	5.478	1377	1380	1382	rBV2	601	382	0.04%	0.006%
32	5.542	1387	1400	1423	rBV	254273	539415	62.39%	8.092%
33	5.760	1466	1468	1470	rBV	743	444	0.05%	0.007%
34	5.828	1477	1489	1507	rBV2	47379	100814	11.66%	1.512%
35	5.995	1528	1541	1568	rBV	205809	435648	50.39%	6.536%
36	6.246	1618	1619	1623	rVB2	648	290	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060823\
 Data File : VW031454.D
 Acq On : 08 Jun 2023 17:26
 Operator : SY/MD
 Sample : 03098-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZES4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.275	1623	1628	1630	rBV2	851	587	0.07%	0.009%
38	6.330	1642	1645	1653	rVB5	655	598	0.07%	0.009%
39	6.500	1695	1698	1700	rBV	528	357	0.04%	0.005%
40	6.635	1738	1740	1745	rVB4	563	434	0.05%	0.007%
41	6.683	1753	1755	1760	rBV3	483	395	0.05%	0.006%
42	6.789	1786	1788	1791	rVV	433	218	0.03%	0.003%
43	6.918	1818	1828	1859	rBV	98390	190089	21.99%	2.852%
44	7.143	1894	1898	1899	rBV2	400	266	0.03%	0.004%
45	7.249	1919	1931	1961	rBV	322790	589526	68.18%	8.844%
46	7.503	2007	2010	2013	rBV2	874	635	0.07%	0.010%
47	7.558	2018	2027	2053	rVV	71111	134984	15.61%	2.025%
48	7.834	2109	2113	2115	rVB2	435	324	0.04%	0.005%
49	7.850	2115	2118	2119	rBV	416	194	0.02%	0.003%
50	7.944	2143	2147	2148	rBV	504	304	0.04%	0.005%
51	7.982	2157	2159	2162	rBV3	439	221	0.03%	0.003%
52	8.034	2166	2175	2222	rVV2	179094	442076	51.13%	6.632%
53	8.439	2298	2301	2304	rBV3	495	360	0.04%	0.005%
54	8.468	2308	2310	2316	rVV4	723	633	0.07%	0.009%
55	8.516	2322	2325	2326	rBV2	728	490	0.06%	0.007%
56	8.580	2342	2345	2348	rVB3	699	307	0.04%	0.005%
57	8.670	2368	2373	2375	rBV3	491	401	0.05%	0.006%
58	8.725	2388	2390	2391	rBV	504	256	0.03%	0.004%
59	8.789	2398	2410	2433	rBV	402522	683976	79.11%	10.261%
60	9.143	2516	2520	2523	rBV2	521	475	0.05%	0.007%
61	9.368	2584	2590	2593	rBV2	473	366	0.04%	0.005%
62	9.458	2616	2618	2622	rBV	277	232	0.03%	0.003%
63	9.519	2634	2637	2639	rBV2	621	405	0.05%	0.006%
64	9.561	2646	2650	2654	rBV2	840	664	0.08%	0.010%
65	9.580	2654	2656	2659	rBV2	426	256	0.03%	0.004%
66	9.616	2664	2667	2671	rBV4	501	409	0.05%	0.006%
67	9.635	2671	2673	2678	rBV3	302	227	0.03%	0.003%
68	9.693	2688	2691	2694	rBV3	522	351	0.04%	0.005%
69	9.844	2736	2738	2743	rBV3	385	327	0.04%	0.005%
70	9.944	2767	2769	2772	rBV2	560	361	0.04%	0.005%
71	9.960	2772	2774	2777	rVB2	572	290	0.03%	0.004%
72	10.018	2789	2792	2793	rBV2	440	265	0.03%	0.004%
73	10.159	2824	2836	2859	rBV	219605	355232	41.09%	5.329%
74	10.333	2884	2890	2900	rVB3	2260	3282	0.38%	0.049%
75	10.641	2983	2986	2988	rBV2	426	256	0.03%	0.004%
76	10.683	2996	2999	3001	rBV2	425	222	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031454.D
 Acq On : 08 Jun 2023 17:26
 Operator : SY/MD
 Sample : 03098-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZES4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.712	3006	3008	3012	rVB2	757	347	0.04%	0.005%
78	10.757	3018	3022	3024	rBV2	263	215	0.02%	0.003%
79	10.837	3044	3047	3051	rBV2	495	372	0.04%	0.006%
80	10.963	3084	3086	3089	rBV3	375	203	0.02%	0.003%
81	11.191	3146	3157	3182	rBV	396746	626597	72.47%	9.400%
82	11.509	3247	3256	3262	rBV8	5210	9348	1.08%	0.140%
83	11.567	3264	3274	3293	rVB	367894	582617	67.38%	8.741%
84	11.944	3389	3391	3393	rBV2	513	290	0.03%	0.004%
85	12.130	3446	3449	3450	rBV2	460	189	0.02%	0.003%
86	12.288	3496	3498	3501	rBV2	305	195	0.02%	0.003%
87	12.413	3532	3537	3540	rBV4	607	614	0.07%	0.009%
88	12.857	3673	3675	3678	rBV2	502	278	0.03%	0.004%
89	13.056	3734	3737	3738	rBV2	374	233	0.03%	0.003%
90	13.066	3738	3740	3745	rVV4	824	463	0.05%	0.007%
91	13.159	3766	3769	3770	rVB2	437	192	0.02%	0.003%
92	13.175	3770	3774	3775	rBV	471	287	0.03%	0.004%
93	13.339	3823	3825	3831	rVB3	595	551	0.06%	0.008%
94	13.365	3831	3833	3834	rBV2	526	226	0.03%	0.003%
95	13.445	3855	3858	3859	rBV3	692	345	0.04%	0.005%
96	13.644	3919	3920	3924	rVB3	525	249	0.03%	0.004%
97	13.664	3924	3926	3927	rBV	449	210	0.02%	0.003%
98	13.908	4000	4002	4005	rBV3	492	351	0.04%	0.005%
99	14.053	4045	4047	4049	rBV2	485	228	0.03%	0.003%
100	14.468	4174	4176	4177	rBV2	882	321	0.04%	0.005%




Sum of corrected areas: 6665705

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031454.D
Acq On : 08 Jun 2023 17:26
Operator : SY/MD
Sample : 03098-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZES4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

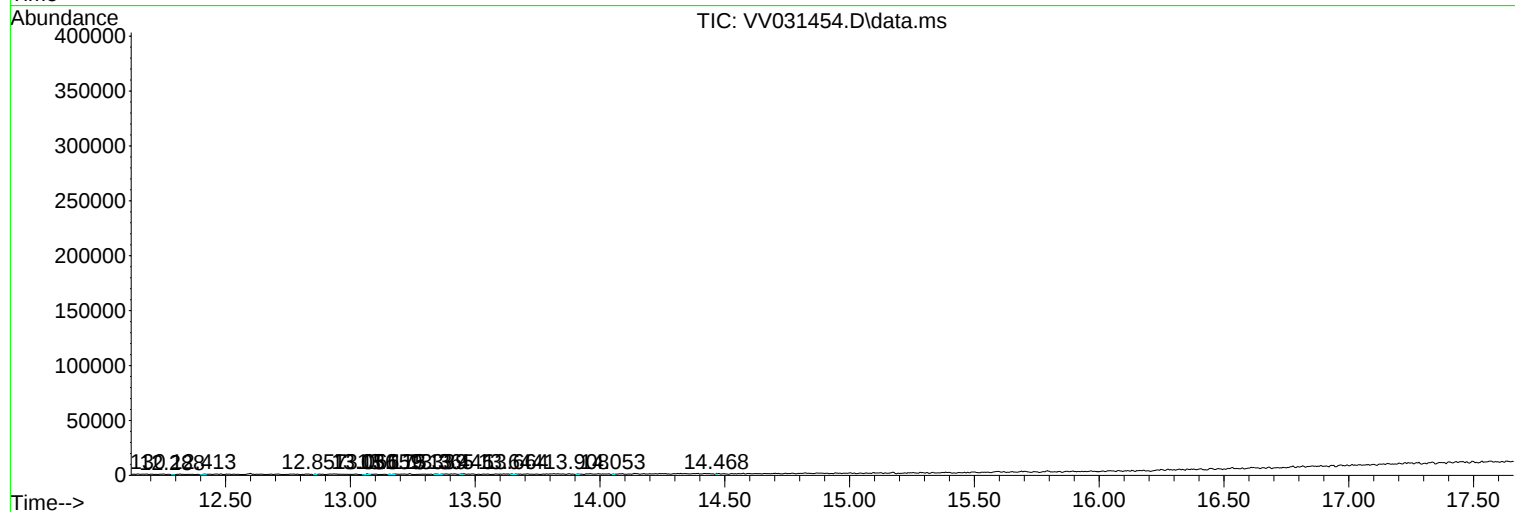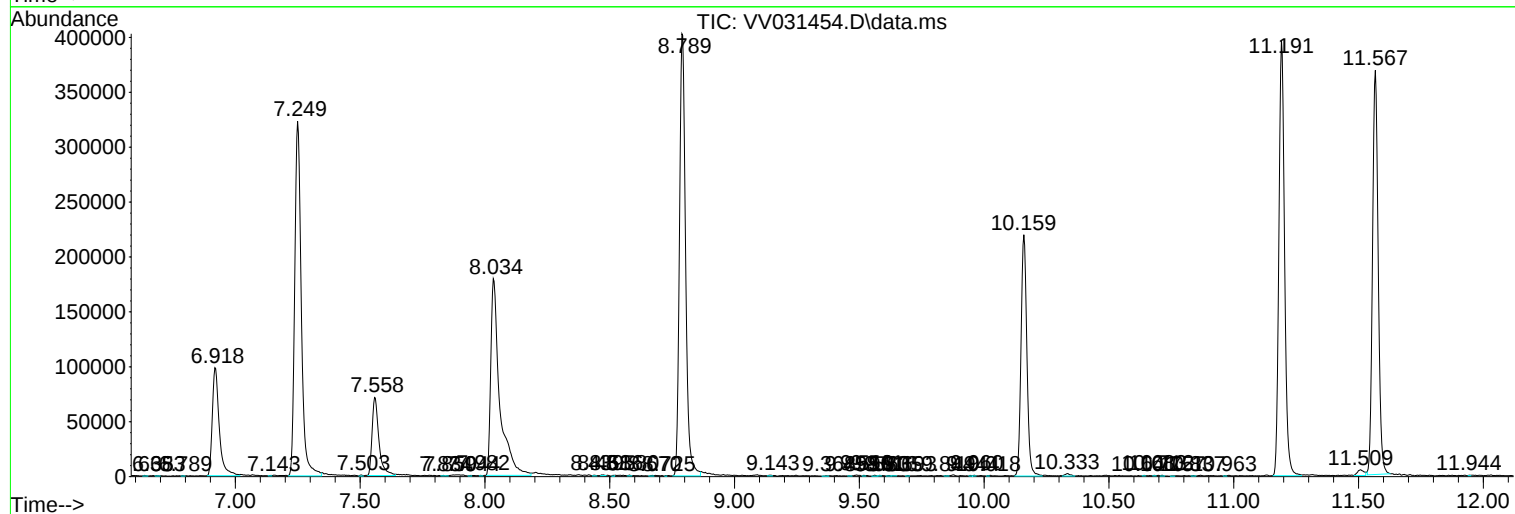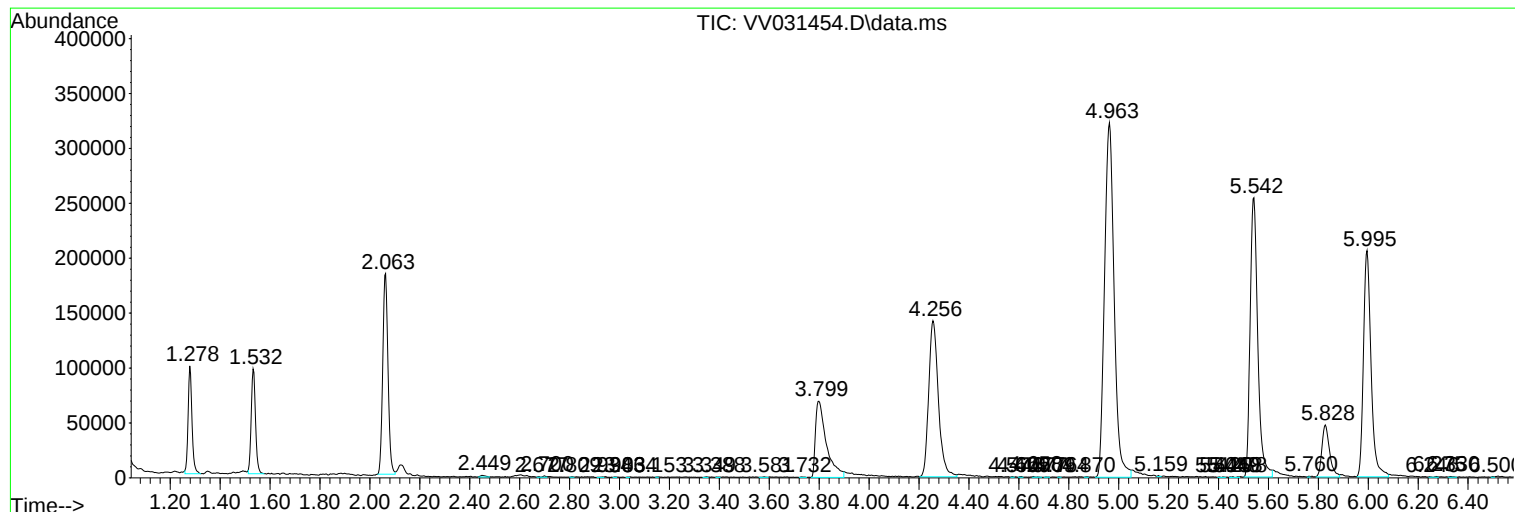

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031454.D
Acq On : 08 Jun 2023 17:26
Operator : SY/MD
Sample : 03098-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZES4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031454.D
Acq On : 08 Jun 2023 17:26
Operator : SY/MD
Sample : 03098-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZES4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------