

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031455.D
 Acq On : 08 Jun 2023 17:50
 Operator : SY/MD
 Sample : 03098-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZES3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	93665	104804	12.59%	1.605%
2	1.532	147	153	166	rVB	92785	107684	12.94%	1.649%
3	2.063	308	318	331	rBV	180278	264722	31.81%	4.053%
4	2.590	472	482	484	rBV5	1726	2378	0.29%	0.036%
5	2.674	504	508	509	rBV2	513	363	0.04%	0.006%
6	2.687	509	512	517	rVV5	740	635	0.08%	0.010%
7	2.754	529	533	534	rBV2	518	348	0.04%	0.005%
8	2.831	553	557	559	rBV3	438	366	0.04%	0.006%
9	2.931	586	588	591	rBV2	446	245	0.03%	0.004%
10	3.095	637	639	642	rVB3	431	212	0.03%	0.003%
11	3.220	676	678	682	rVB3	374	279	0.03%	0.004%
12	3.301	700	703	706	rBV2	232	221	0.03%	0.003%
13	3.368	719	724	726	rBV2	289	304	0.04%	0.005%
14	3.423	737	741	747	rBV3	342	397	0.05%	0.006%
15	3.609	797	799	802	rVV2	389	228	0.03%	0.003%
16	3.735	836	838	841	rBV2	591	405	0.05%	0.006%
17	3.799	848	858	897	rBV	67218	206575	24.82%	3.163%
18	4.256	986	1000	1027	rBV	135796	356971	42.90%	5.466%
19	4.760	1152	1157	1159	rBV2	533	386	0.05%	0.006%
20	4.883	1193	1195	1200	rVB2	523	306	0.04%	0.005%
21	4.963	1203	1220	1243	rBV2	312363	832132	100.00%	12.741%
22	5.423	1361	1363	1365	rBV2	478	224	0.03%	0.003%
23	5.494	1380	1385	1387	rBV3	718	563	0.07%	0.009%
24	5.542	1387	1400	1426	rBV2	254442	544273	65.41%	8.334%
25	5.731	1457	1459	1461	rBV2	649	292	0.04%	0.004%
26	5.780	1471	1474	1475	rBV2	799	421	0.05%	0.006%
27	5.828	1479	1489	1519	rVB3	44288	96495	11.60%	1.477%
28	5.931	1519	1521	1523	rBV2	559	243	0.03%	0.004%
29	5.995	1528	1541	1567	rBV	197325	419169	50.37%	6.418%
30	6.185	1598	1600	1603	rBV3	599	425	0.05%	0.007%
31	6.329	1641	1645	1647	rBV3	469	410	0.05%	0.006%
32	6.362	1653	1655	1658	rBV2	527	337	0.04%	0.005%
33	6.429	1670	1676	1679	rBV3	758	658	0.08%	0.010%
34	6.516	1700	1703	1709	rBV4	654	757	0.09%	0.012%
35	6.722	1763	1767	1769	rBV2	767	540	0.06%	0.008%
36	6.799	1787	1791	1793	rBV3	427	275	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031455.D
 Acq On : 08 Jun 2023 17:50
 Operator : SY/MD
 Sample : 03098-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZES3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.828	1796	1800	1803	rBV2	431	281	0.03%	0.004%
38	6.844	1803	1805	1807	rBV2	447	224	0.03%	0.003%
39	6.870	1810	1813	1817	rBV2	476	393	0.05%	0.006%
40	6.918	1817	1828	1859	rBV	93493	187809	22.57%	2.876%
41	7.140	1894	1897	1900	rVB3	528	294	0.04%	0.005%
42	7.207	1916	1918	1920	rBV2	434	198	0.02%	0.003%
43	7.249	1920	1931	1952	rBV	313234	561848	67.52%	8.603%
44	7.522	2014	2016	2018	rBV	708	368	0.04%	0.006%
45	7.561	2018	2028	2054	rVV	70885	133323	16.02%	2.041%
46	7.738	2081	2083	2086	rBV3	506	269	0.03%	0.004%
47	7.783	2094	2097	2100	rBV3	370	259	0.03%	0.004%
48	7.882	2122	2128	2135	rBV6	1836	2352	0.28%	0.036%
49	7.944	2144	2147	2151	rBV3	816	526	0.06%	0.008%
50	8.034	2165	2175	2213	rBV2	175890	429453	51.61%	6.576%
51	8.439	2296	2301	2303	rBV4	839	724	0.09%	0.011%
52	8.461	2307	2308	2313	rVB2	544	391	0.05%	0.006%
53	8.490	2313	2317	2318	rBV2	720	396	0.05%	0.006%
54	8.693	2379	2380	2382	rBV2	738	261	0.03%	0.004%
55	8.789	2398	2410	2435	rBV	412634	700071	84.13%	10.719%
56	9.069	2495	2497	2500	rBV4	632	496	0.06%	0.008%
57	9.156	2521	2524	2527	rVV2	438	320	0.04%	0.005%
58	9.214	2540	2542	2547	rVV2	338	292	0.04%	0.004%
59	9.249	2551	2553	2556	rBV2	396	196	0.02%	0.003%
60	9.333	2576	2579	2581	rBV	573	266	0.03%	0.004%
61	9.403	2598	2601	2606	rBV3	751	600	0.07%	0.009%
62	9.493	2623	2629	2630	rBV	604	516	0.06%	0.008%
63	9.709	2694	2696	2700	rVB2	579	325	0.04%	0.005%
64	9.731	2700	2703	2707	rBV3	485	394	0.05%	0.006%
65	9.796	2721	2723	2729	rBB2	566	419	0.05%	0.006%
66	9.866	2742	2745	2746	rBV	567	270	0.03%	0.004%
67	9.915	2757	2760	2762	rBV2	746	456	0.05%	0.007%
68	9.947	2769	2770	2776	rVB3	526	396	0.05%	0.006%
69	9.979	2776	2780	2783	rBV4	322	281	0.03%	0.004%
70	10.043	2796	2800	2803	rBV2	464	399	0.05%	0.006%
71	10.075	2809	2810	2815	rVB3	425	320	0.04%	0.005%
72	10.159	2824	2836	2859	rVV	217585	351828	42.28%	5.387%
73	10.333	2884	2890	2901	rVB4	3845	6277	0.75%	0.096%
74	10.381	2901	2905	2907	rBV2	396	238	0.03%	0.004%
75	10.426	2917	2919	2921	rBV2	481	223	0.03%	0.003%
76	10.452	2924	2927	2933	rBV3	455	477	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031455.D
 Acq On : 08 Jun 2023 17:50
 Operator : SY/MD
 Sample : 03098-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZES3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.477	2933	2935	2938	rBV3	343	265	0.03%	0.004%
78	10.641	2984	2986	2990	rVB4	427	280	0.03%	0.004%
79	10.670	2993	2995	3000	rVV3	526	385	0.05%	0.006%
80	10.796	3031	3034	3036	rBV2	675	460	0.06%	0.007%
81	10.911	3067	3070	3071	rBV2	441	235	0.03%	0.004%
82	11.082	3120	3123	3125	rBV	515	243	0.03%	0.004%
83	11.098	3125	3128	3130	rBV	321	222	0.03%	0.003%
84	11.191	3143	3157	3180	rBV	399208	631448	75.88%	9.669%
85	11.416	3223	3227	3228	rBV2	415	245	0.03%	0.004%
86	11.567	3263	3274	3295	rBV	356897	562998	67.66%	8.620%
87	11.744	3327	3329	3336	rVB3	568	450	0.05%	0.007%
88	12.001	3407	3409	3414	rBV	481	412	0.05%	0.006%
89	12.233	3479	3481	3484	rVB2	500	218	0.03%	0.003%
90	12.406	3531	3535	3536	rBV2	455	358	0.04%	0.005%
91	12.477	3555	3557	3559	rBV2	399	248	0.03%	0.004%
92	12.596	3591	3594	3597	rBV2	554	442	0.05%	0.007%
93	12.699	3624	3626	3629	rBV2	374	235	0.03%	0.004%
94	12.747	3637	3641	3644	rBV3	355	332	0.04%	0.005%
95	12.892	3684	3686	3689	rVB3	625	280	0.03%	0.004%
96	13.004	3718	3721	3723	rBV3	508	391	0.05%	0.006%
97	13.059	3734	3738	3742	rBV5	516	424	0.05%	0.006%
98	13.580	3898	3900	3903	rBV2	406	214	0.03%	0.003%
99	13.934	4008	4010	4013	rBV	508	347	0.04%	0.005%
100	14.207	4092	4095	4096	rBV2	678	365	0.04%	0.006%


Sum of corrected areas: 6530969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031455.D
Acq On : 08 Jun 2023 17:50
Operator : SY/MD
Sample : 03098-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZES3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

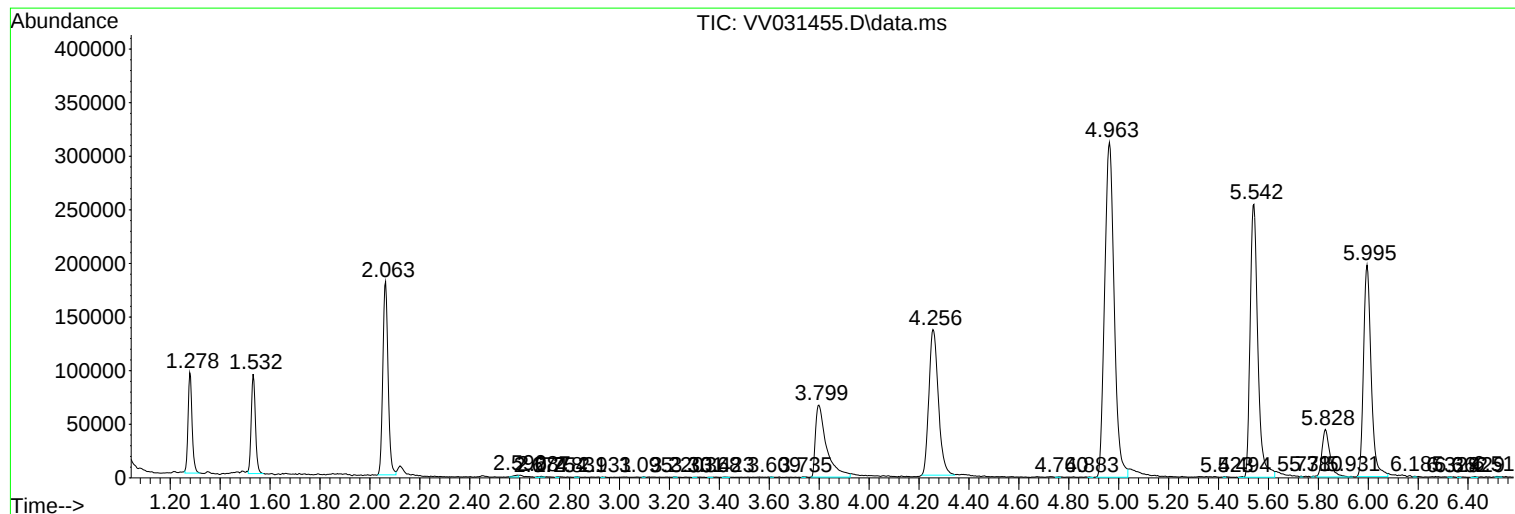

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031455.D
Acq On : 08 Jun 2023 17:50
Operator : SY/MD
Sample : 03098-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZES3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031455.D
Acq On : 08 Jun 2023 17:50
Operator : SY/MD
Sample : 03098-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZES3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------