

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031457.D
 Acq On : 08 Jun 2023 18:37
 Operator : SY/MD
 Sample : 02992-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	120987	132655	12.27%	1.684%
2	1.532	146	153	169	rVB	121973	149164	13.79%	1.894%
3	2.063	308	318	334	rBV	230323	340138	31.45%	4.319%
4	2.401	420	423	425	rVV2	499	266	0.02%	0.003%
5	2.413	425	427	429	rVB	663	268	0.02%	0.003%
6	2.452	429	439	450	rBV2	8079	13760	1.27%	0.175%
7	2.526	459	462	463	rBV2	432	274	0.03%	0.003%
8	2.558	470	472	474	rBV2	586	230	0.02%	0.003%
9	2.700	513	516	518	rBV2	746	451	0.04%	0.006%
10	2.774	537	539	545	rVB3	342	285	0.03%	0.004%
11	2.899	576	578	581	rVB2	419	228	0.02%	0.003%
12	2.915	581	583	586	rBV2	578	401	0.04%	0.005%
13	2.950	590	594	598	rBV3	342	264	0.02%	0.003%
14	3.159	655	659	660	rBV	563	240	0.02%	0.003%
15	3.220	676	678	681	rBV3	406	249	0.02%	0.003%
16	3.265	688	692	695	rBV3	468	324	0.03%	0.004%
17	3.317	704	708	710	rBV3	325	248	0.02%	0.003%
18	3.433	740	744	747	rBV	319	219	0.02%	0.003%
19	3.510	764	768	769	rBV	374	249	0.02%	0.003%
20	3.600	792	796	798	rBV	377	271	0.03%	0.003%
21	3.635	804	807	814	rVB4	520	661	0.06%	0.008%
22	3.674	814	819	826	rBV2	473	575	0.05%	0.007%
23	3.741	837	840	843	rBV2	354	217	0.02%	0.003%
24	3.799	847	858	888	rBV	82041	247015	22.84%	3.137%
25	4.105	951	953	958	rVB4	658	406	0.04%	0.005%
26	4.198	980	982	983	rBV2	631	252	0.02%	0.003%
27	4.256	984	1000	1028	rVV	176102	460763	42.61%	5.851%
28	4.590	1101	1104	1109	rVB3	671	479	0.04%	0.006%
29	4.683	1131	1133	1136	rBV2	395	243	0.02%	0.003%
30	4.822	1172	1176	1177	rBV2	346	245	0.02%	0.003%
31	4.902	1196	1201	1203	rBV	252	239	0.02%	0.003%
32	4.963	1203	1220	1248	rBV2	400437	1081450	100.00%	13.732%
33	5.375	1344	1348	1350	rBV5	473	338	0.03%	0.004%
34	5.384	1350	1351	1355	rVB	541	239	0.02%	0.003%
35	5.407	1356	1358	1362	rVB3	599	286	0.03%	0.004%
36	5.433	1362	1366	1367	rBV2	408	252	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060823\
 Data File : VW031457.D
 Acq On : 08 Jun 2023 18:37
 Operator : SY/MD
 Sample : 02992-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.542	1388	1400	1419	rBV	272694	561482	51.92%	7.130%
38	5.828	1477	1489	1503	rBV2	34685	77951	7.21%	0.990%
39	5.937	1520	1523	1526	rBV2	724	362	0.03%	0.005%
40	5.995	1526	1541	1567	rBV2	246312	528706	48.89%	6.714%
41	6.317	1640	1641	1647	rVB3	603	357	0.03%	0.005%
42	6.452	1679	1683	1684	rVB	506	278	0.03%	0.004%
43	6.571	1711	1720	1724	rBV5	1666	2615	0.24%	0.033%
44	6.831	1795	1801	1804	rBV2	388	397	0.04%	0.005%
45	6.860	1808	1810	1813	rVB2	436	196	0.02%	0.002%
46	6.918	1817	1828	1852	rBV2	112867	222952	20.62%	2.831%
47	7.249	1919	1931	1963	rBV	411689	761167	70.38%	9.665%
48	7.558	2018	2027	2052	rBV	84509	157989	14.61%	2.006%
49	7.757	2085	2089	2091	rBV2	530	489	0.05%	0.006%
50	7.953	2146	2150	2151	rBV2	388	249	0.02%	0.003%
51	8.034	2165	2175	2213	rBV2	232271	522804	48.34%	6.639%
52	8.461	2303	2308	2311	rBV3	674	686	0.06%	0.009%
53	8.580	2342	2345	2348	rBV3	622	499	0.05%	0.006%
54	8.651	2365	2367	2370	rVB4	851	460	0.04%	0.006%
55	8.674	2370	2374	2378	rBV2	686	607	0.06%	0.008%
56	8.709	2383	2385	2387	rBV	296	203	0.02%	0.003%
57	8.789	2399	2410	2438	rBV	436014	733886	67.86%	9.319%
58	9.133	2515	2517	2519	rBV	433	228	0.02%	0.003%
59	9.272	2558	2560	2561	rBV2	421	209	0.02%	0.003%
60	9.297	2565	2568	2570	rBV2	417	256	0.02%	0.003%
61	9.358	2585	2587	2591	rBV2	334	218	0.02%	0.003%
62	9.410	2601	2603	2605	rBV	461	263	0.02%	0.003%
63	9.686	2684	2689	2692	rBV3	444	418	0.04%	0.005%
64	9.751	2706	2709	2714	rVV3	455	438	0.04%	0.006%
65	9.802	2722	2725	2727	rBV2	447	265	0.02%	0.003%
66	9.944	2767	2769	2774	rVB2	578	345	0.03%	0.004%
67	10.079	2808	2811	2813	rBV2	434	316	0.03%	0.004%
68	10.111	2819	2821	2823	rBV2	326	210	0.02%	0.003%
69	10.159	2824	2836	2858	rVV	291353	470799	43.53%	5.978%
70	10.323	2885	2887	2889	rBV3	522	234	0.02%	0.003%
71	10.358	2895	2898	2902	rVB3	566	386	0.04%	0.005%
72	10.448	2923	2926	2928	rVB2	457	219	0.02%	0.003%
73	10.484	2934	2937	2944	rVB4	592	616	0.06%	0.008%
74	10.516	2944	2947	2950	rBV	392	305	0.03%	0.004%
75	10.693	3000	3002	3004	rBV	404	196	0.02%	0.002%
76	10.712	3004	3008	3009	rBV2	405	234	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031457.D
 Acq On : 08 Jun 2023 18:37
 Operator : SY/MD
 Sample : 02992-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.854	3050	3052	3053	rBV2	532	245	0.02%	0.003%
78	10.953	3081	3083	3088	rVB2	292	241	0.02%	0.003%
79	11.047	3108	3112	3113	rBV2	549	289	0.03%	0.004%
80	11.075	3118	3121	3123	rBV	537	294	0.03%	0.004%
81	11.092	3124	3126	3131	rVB3	559	348	0.03%	0.004%
82	11.124	3135	3136	3141	rBV2	429	300	0.03%	0.004%
83	11.191	3145	3157	3180	rBV	426739	664459	61.44%	8.437%
84	11.567	3261	3274	3294	rBV	453582	719559	66.54%	9.137%
85	11.982	3400	3403	3404	rBV2	527	247	0.02%	0.003%
86	12.005	3408	3410	3411	rBV	551	230	0.02%	0.003%
87	12.120	3444	3446	3447	rBV	675	302	0.03%	0.004%
88	12.159	3454	3458	3460	rBV3	650	413	0.04%	0.005%
89	12.194	3466	3469	3471	rBV2	454	268	0.02%	0.003%
90	12.345	3514	3516	3519	rVB3	582	282	0.03%	0.004%
91	12.374	3519	3525	3527	rBV	536	473	0.04%	0.006%
92	12.741	3636	3639	3640	rBV2	496	262	0.02%	0.003%
93	13.043	3731	3733	3736	rBV3	609	400	0.04%	0.005%
94	13.091	3743	3748	3749	rBV2	445	314	0.03%	0.004%
95	13.153	3764	3767	3772	rVB2	546	458	0.04%	0.006%
96	13.175	3772	3774	3775	rBV	430	216	0.02%	0.003%
97	13.397	3841	3843	3846	rVB	505	309	0.03%	0.004%
98	13.439	3855	3856	3858	rBV2	502	289	0.03%	0.004%
99	13.847	3981	3983	3986	rBV3	529	302	0.03%	0.004%
100	14.288	4118	4120	4122	rBV3	684	357	0.03%	0.005%




Sum of corrected areas: 7875191

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031457.D
Acq On : 08 Jun 2023 18:37
Operator : SY/MD
Sample : 02992-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

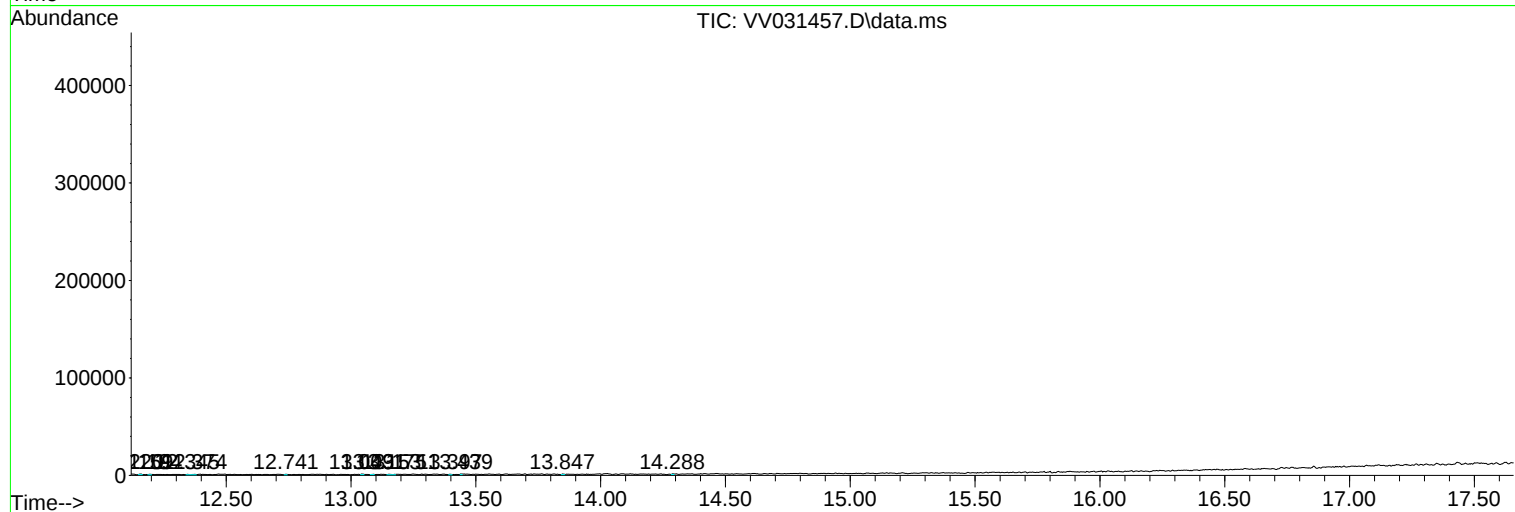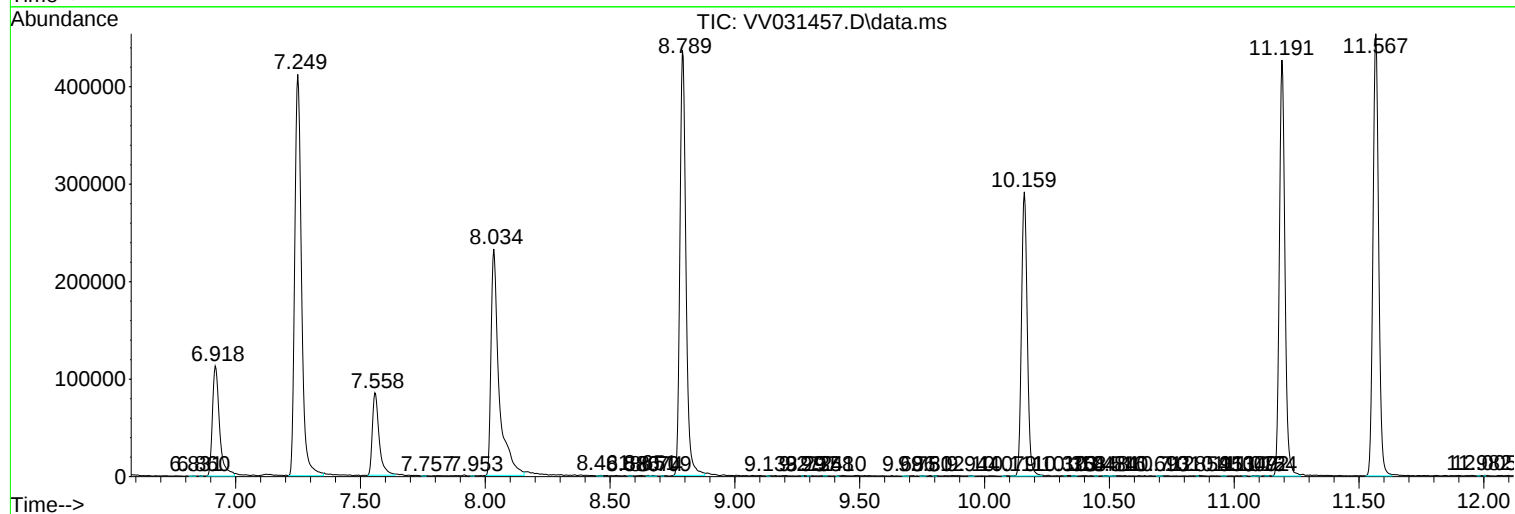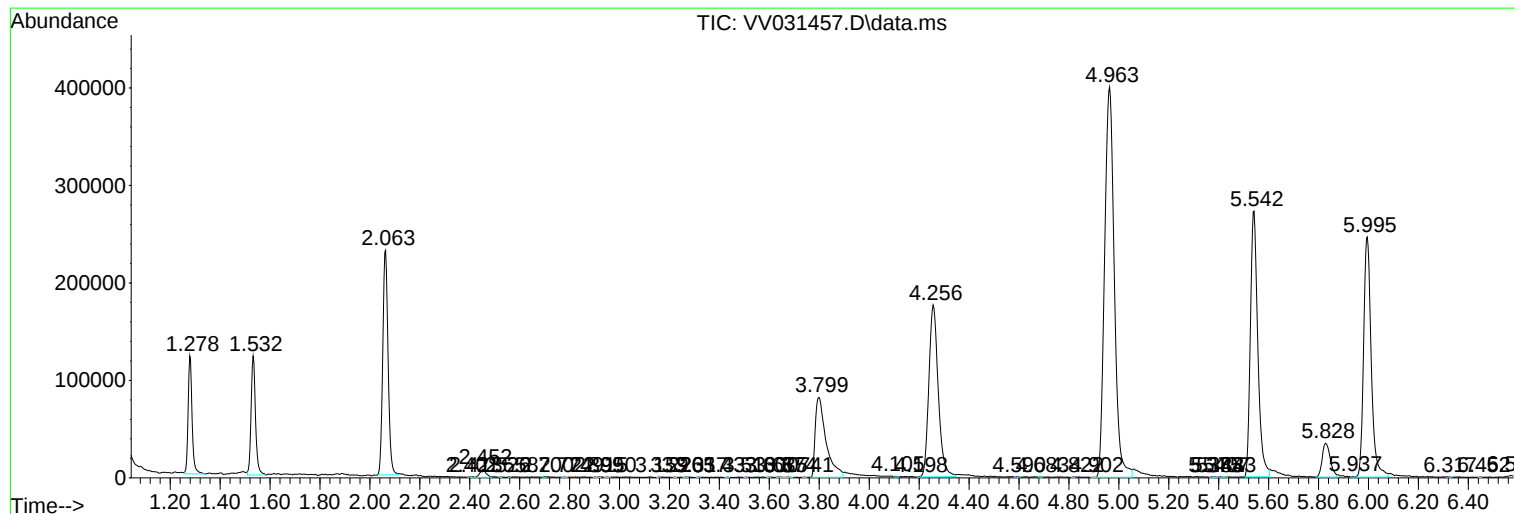

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031457.D
Acq On : 08 Jun 2023 18:37
Operator : SY/MD
Sample : 02992-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031457.D
Acq On : 08 Jun 2023 18:37
Operator : SY/MD
Sample : 02992-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------