

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031460.D
 Acq On : 08 Jun 2023 20:18
 Operator : SY/MD
 Sample : VV0608WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK352

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	128290	141325	12.42%	1.682%
2	1.532	147	153	169	rVB	129677	152649	13.42%	1.817%
3	2.063	308	318	336	rBV	247968	367933	32.34%	4.380%
4	2.452	432	439	449	rVB7	2524	4299	0.38%	0.051%
5	2.648	498	500	502	rBV2	269	140	0.01%	0.002%
6	2.693	509	514	518	rBV4	982	929	0.08%	0.011%
7	2.786	541	543	547	rVB	297	163	0.01%	0.002%
8	2.812	547	551	553	rBV2	420	306	0.03%	0.004%
9	2.908	579	581	583	rBV2	304	168	0.01%	0.002%
10	3.150	652	656	659	rBV3	490	385	0.03%	0.005%
11	3.188	665	668	673	rBV3	389	321	0.03%	0.004%
12	3.233	680	682	686	rVB2	465	219	0.02%	0.003%
13	3.256	686	689	692	rBV3	245	184	0.02%	0.002%
14	3.323	702	710	713	rBV3	561	620	0.05%	0.007%
15	3.391	729	731	734	rVB2	567	299	0.03%	0.004%
16	3.426	739	742	748	rVB4	558	539	0.05%	0.006%
17	3.462	748	753	756	rBV4	418	398	0.03%	0.005%
18	3.516	767	770	772	rBV2	452	189	0.02%	0.002%
19	3.535	772	776	780	rVB2	448	385	0.03%	0.005%
20	3.555	780	782	785	rBV	303	174	0.02%	0.002%
21	3.580	785	790	793	rBV3	326	220	0.02%	0.003%
22	3.609	795	799	800	rBV	418	226	0.02%	0.003%
23	3.725	831	835	838	rVV2	377	311	0.03%	0.004%
24	3.799	848	858	892	rBV	87206	263216	23.14%	3.133%
25	4.256	985	1000	1025	rBV	184324	474007	41.66%	5.642%
26	4.500	1074	1076	1078	rBV	649	336	0.03%	0.004%
27	4.593	1101	1105	1108	rBV4	648	591	0.05%	0.007%
28	4.629	1114	1116	1119	rBB2	531	214	0.02%	0.003%
29	4.648	1120	1122	1124	rVV2	487	167	0.01%	0.002%
30	4.738	1148	1150	1152	rBV2	417	204	0.02%	0.002%
31	4.757	1154	1156	1158	rVB2	447	150	0.01%	0.002%
32	4.822	1174	1176	1180	rBV3	378	265	0.02%	0.003%
33	4.963	1202	1220	1245	rBV2	430317	1137737	100.00%	13.543%
34	5.291	1320	1322	1325	rBV2	471	188	0.02%	0.002%
35	5.330	1332	1334	1337	rBV	528	348	0.03%	0.004%
36	5.346	1337	1339	1342	rVV3	518	272	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031460.D
 Acq On : 08 Jun 2023 20:18
 Operator : SY/MD
 Sample : VV0608WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK352

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.539	1387	1399	1423	rBV	295864	619980	54.49%	7.380%
38	5.828	1478	1489	1511	rBV	33739	74949	6.59%	0.892%
39	5.995	1526	1541	1563	rBV	261463	550838	48.42%	6.557%
40	6.265	1622	1625	1626	rBV2	605	306	0.03%	0.004%
41	6.297	1633	1635	1638	rVB2	404	199	0.02%	0.002%
42	6.317	1638	1641	1643	rBV2	382	260	0.02%	0.003%
43	6.384	1658	1662	1666	rBV	427	313	0.03%	0.004%
44	6.436	1675	1678	1679	rBV2	264	144	0.01%	0.002%
45	6.465	1685	1687	1690	rVB3	812	391	0.03%	0.005%
46	6.497	1690	1697	1699	rBV4	424	461	0.04%	0.005%
47	6.526	1704	1706	1710	rVB3	489	254	0.02%	0.003%
48	6.567	1710	1719	1721	rBV6	1820	2422	0.21%	0.029%
49	6.670	1749	1751	1754	rBV2	313	213	0.02%	0.003%
50	6.735	1770	1771	1775	rVB2	544	321	0.03%	0.004%
51	6.757	1775	1778	1783	rBB3	561	533	0.05%	0.006%
52	6.825	1797	1799	1802	rBV2	209	147	0.01%	0.002%
53	6.918	1816	1828	1847	rBV	118404	229937	20.21%	2.737%
54	7.249	1919	1931	1956	rBV	453206	812253	71.39%	9.669%
55	7.558	2018	2027	2055	rBV	88701	164558	14.46%	1.959%
56	7.809	2103	2105	2108	rBV2	573	278	0.02%	0.003%
57	7.918	2133	2139	2146	rBV9	1564	1828	0.16%	0.022%
58	7.960	2148	2152	2154	rBV3	544	336	0.03%	0.004%
59	8.034	2165	2175	2214	rBV2	246498	564993	49.66%	6.725%
60	8.625	2357	2359	2362	rBV2	330	208	0.02%	0.002%
61	8.741	2393	2395	2398	rVB2	445	258	0.02%	0.003%
62	8.789	2398	2410	2435	rBV	469772	794944	69.87%	9.462%
63	9.040	2485	2488	2493	rBV4	446	332	0.03%	0.004%
64	9.117	2510	2512	2516	rVB2	410	204	0.02%	0.002%
65	9.252	2552	2554	2556	rBV3	268	196	0.02%	0.002%
66	9.445	2611	2614	2617	rBV2	403	332	0.03%	0.004%
67	9.461	2617	2619	2621	rBV2	402	186	0.02%	0.002%
68	9.538	2641	2643	2644	rBV2	437	164	0.01%	0.002%
69	9.696	2688	2692	2694	rBV2	265	216	0.02%	0.003%
70	9.882	2743	2750	2752	rBV4	1105	1244	0.11%	0.015%
71	9.908	2756	2758	2759	rBV2	383	174	0.02%	0.002%
72	9.963	2772	2775	2776	rBV	470	263	0.02%	0.003%
73	10.159	2824	2836	2860	rBV	314206	504894	44.38%	6.010%
74	10.323	2884	2887	2889	rBV3	580	366	0.03%	0.004%
75	10.432	2919	2921	2924	rBV2	292	190	0.02%	0.002%
76	10.474	2930	2934	2936	rBV4	1000	699	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031460.D
 Acq On : 08 Jun 2023 20:18
 Operator : SY/MD
 Sample : VV0608WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK352

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.526	2947	2950	2951	rBV2	271	147	0.01%	0.002%
78	10.564	2960	2962	2966	rBV3	369	227	0.02%	0.003%
79	10.673	2994	2996	3001	rVB2	435	304	0.03%	0.004%
80	10.747	3016	3019	3020	rBV2	375	159	0.01%	0.002%
81	10.789	3030	3032	3033	rBV	458	199	0.02%	0.002%
82	11.082	3121	3123	3128	rBV2	425	306	0.03%	0.004%
83	11.133	3136	3139	3144	rVB4	1509	1508	0.13%	0.018%
84	11.191	3144	3157	3176	rBV	462294	728052	63.99%	8.666%
85	11.432	3230	3232	3235	rBV2	363	222	0.02%	0.003%
86	11.500	3250	3253	3255	rBV2	542	419	0.04%	0.005%
87	11.567	3262	3274	3300	rBV	484873	772155	67.87%	9.191%
88	11.866	3365	3367	3370	rVB	493	155	0.01%	0.002%
89	11.969	3394	3399	3406	rBV4	772	1047	0.09%	0.012%
90	12.358	3517	3520	3521	rBV	434	254	0.02%	0.003%
91	12.561	3581	3583	3585	rBV2	381	195	0.02%	0.002%
92	12.590	3590	3592	3602	rVB6	1700	2161	0.19%	0.026%
93	12.632	3602	3605	3608	rBV2	436	315	0.03%	0.004%
94	12.908	3688	3691	3693	rBV3	508	326	0.03%	0.004%
95	13.204	3779	3783	3784	rBV2	1467	925	0.08%	0.011%
96	13.451	3853	3860	3867	rBV2	4855	7309	0.64%	0.087%
97	13.622	3911	3913	3916	rBV2	374	192	0.02%	0.002%
98	13.696	3929	3936	3940	rBV6	2002	2686	0.24%	0.032%
99	13.905	3997	4001	4002	rBV3	814	544	0.05%	0.006%
100	13.969	4018	4021	4023	rBV3	522	353	0.03%	0.004%




Sum of corrected areas: 8401021

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031460.D
Acq On : 08 Jun 2023 20:18
Operator : SY/MD
Sample : VV0608WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK352

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

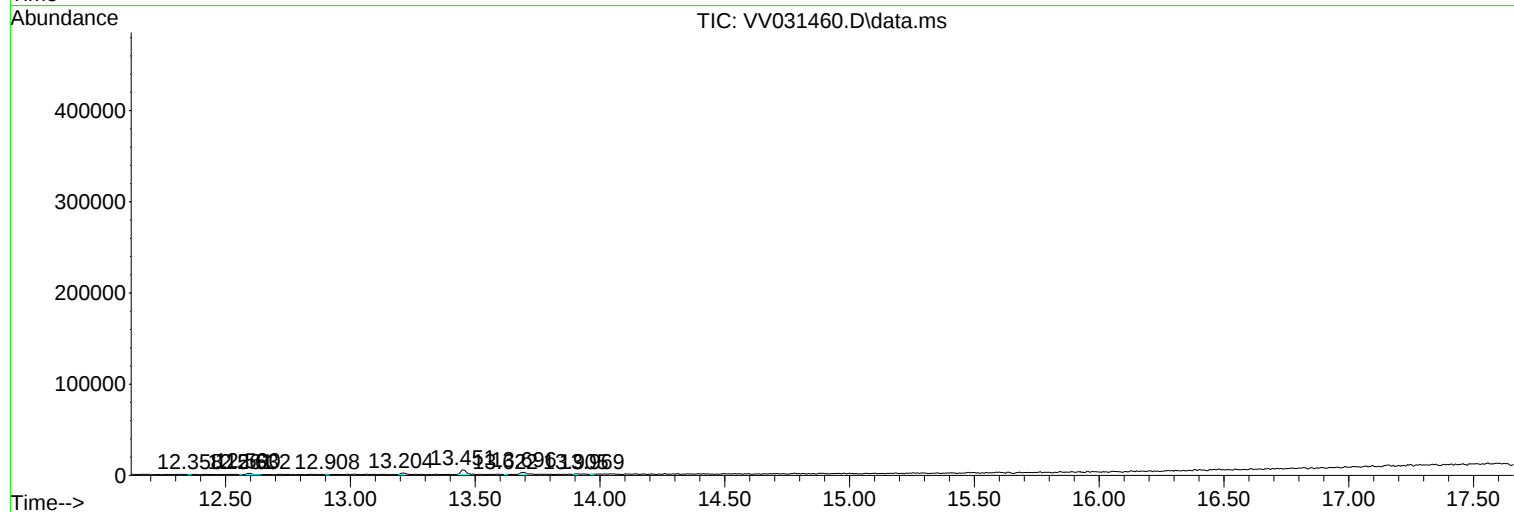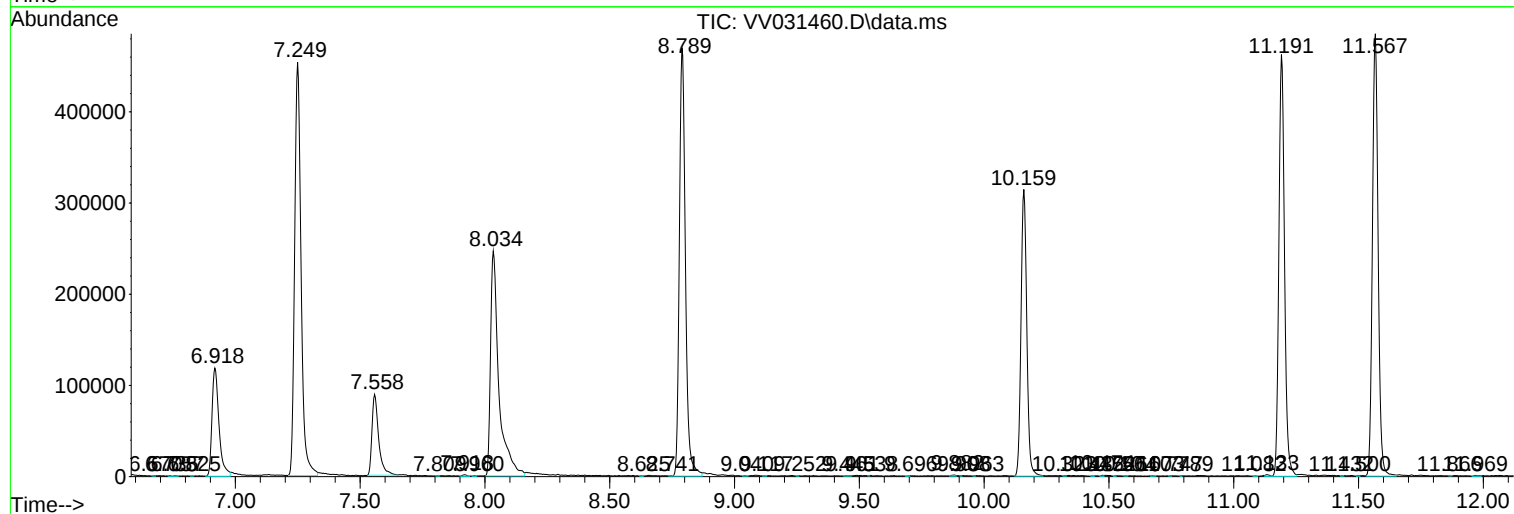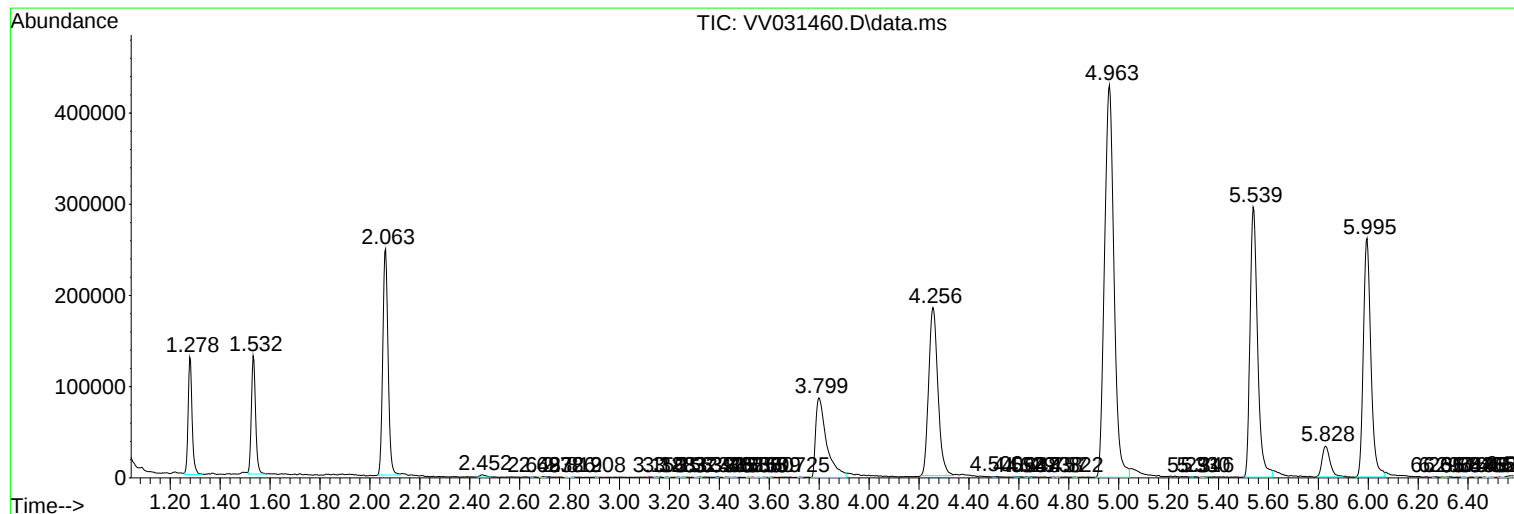

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031460.D
Acq On : 08 Jun 2023 20:18
Operator : SY/MD
Sample : VV0608WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK352

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031460.D
Acq On : 08 Jun 2023 20:18
Operator : SY/MD
Sample : VV0608WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK352

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------