

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031462.D
 Acq On : 08 Jun 2023 21:17
 Operator : SY/MD
 Sample : 03106-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031462.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	118786	125226	11.54%	1.536%
2	1.532	147	153	170	rVB	122434	142542	13.14%	1.748%
3	2.063	308	318	332	rBV	237483	342572	31.57%	4.201%
4	2.442	434	436	437	rBV	522	222	0.02%	0.003%
5	2.645	496	499	500	rBV2	556	281	0.03%	0.003%
6	2.703	512	517	520	rBV3	1222	1144	0.11%	0.014%
7	2.860	564	566	571	rBV2	429	206	0.02%	0.003%
8	2.982	599	604	605	rBV3	529	323	0.03%	0.004%
9	3.050	623	625	627	rBV	736	376	0.03%	0.005%
10	3.076	630	633	635	rBV	333	210	0.02%	0.003%
11	3.169	661	662	668	rVV2	466	305	0.03%	0.004%
12	3.230	678	681	683	rVB2	375	235	0.02%	0.003%
13	3.333	710	713	716	rVB3	434	237	0.02%	0.003%
14	3.497	759	764	768	rVB2	370	325	0.03%	0.004%
15	3.551	778	781	784	rBV3	405	303	0.03%	0.004%
16	3.590	790	793	799	rVB3	363	261	0.02%	0.003%
17	3.796	843	857	887	rBV	77977	233460	21.52%	2.863%
18	4.256	983	1000	1027	rBV	180313	468199	43.15%	5.742%
19	4.706	1135	1140	1144	rVB4	448	371	0.03%	0.005%
20	4.744	1144	1152	1154	rBV5	696	854	0.08%	0.010%
21	4.757	1154	1156	1159	rVB2	542	239	0.02%	0.003%
22	4.786	1161	1165	1167	rBV2	324	251	0.02%	0.003%
23	4.860	1185	1188	1190	rBV	447	218	0.02%	0.003%
24	4.963	1200	1220	1246	rBV2	406213	1084958	100.00%	13.305%
25	5.400	1350	1356	1361	rBV3	819	1035	0.10%	0.013%
26	5.439	1364	1368	1372	rBV2	452	470	0.04%	0.006%
27	5.538	1387	1399	1428	rBV	290979	613345	56.53%	7.522%
28	5.837	1478	1492	1516	rBV5	74985	182734	16.84%	2.241%
29	5.995	1526	1541	1580	rBV	252663	542992	50.05%	6.659%
30	6.217	1608	1610	1612	rBV2	479	230	0.02%	0.003%
31	6.426	1672	1675	1679	rBV4	464	292	0.03%	0.004%
32	6.509	1698	1701	1703	rBV3	630	408	0.04%	0.005%
33	6.558	1710	1716	1720	rBV5	2081	2513	0.23%	0.031%
34	6.661	1744	1748	1750	rBV3	480	408	0.04%	0.005%
35	6.709	1757	1763	1765	rBV3	451	305	0.03%	0.004%
36	6.760	1777	1779	1785	rVB3	449	313	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031462.D
 Acq On : 08 Jun 2023 21:17
 Operator : SY/MD
 Sample : 03106-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.789	1785	1788	1791	rBV2	676	436	0.04%	0.005%
38	6.863	1806	1811	1812	rBV2	352	272	0.03%	0.003%
39	6.918	1816	1828	1848	rBV2	113683	219972	20.27%	2.698%
40	7.181	1908	1910	1911	rBV	533	222	0.02%	0.003%
41	7.249	1919	1931	1963	rBV	424597	773720	71.31%	9.489%
42	7.558	2017	2027	2048	rBV	85036	159816	14.73%	1.960%
43	7.780	2092	2096	2097	rBV2	458	303	0.03%	0.004%
44	7.882	2123	2128	2136	rVB4	2469	3024	0.28%	0.037%
45	8.034	2164	2175	2214	rBV2	226669	516249	47.58%	6.331%
46	8.596	2348	2350	2355	rBV3	365	223	0.02%	0.003%
47	8.696	2379	2381	2383	rBV2	326	225	0.02%	0.003%
48	8.747	2394	2397	2399	rVB2	438	269	0.02%	0.003%
49	8.789	2399	2410	2441	rBV	465590	780149	71.91%	9.567%
50	9.130	2514	2516	2521	rVB2	712	558	0.05%	0.007%
51	9.191	2533	2535	2545	rBV2	478	533	0.05%	0.007%
52	9.310	2566	2572	2575	rBV3	668	710	0.07%	0.009%
53	9.355	2584	2586	2589	rBV2	505	355	0.03%	0.004%
54	9.416	2600	2605	2608	rVV3	574	504	0.05%	0.006%
55	9.455	2614	2617	2620	rBV	339	280	0.03%	0.003%
56	9.509	2632	2634	2637	rBV2	397	303	0.03%	0.004%
57	9.564	2647	2651	2655	rVB3	523	441	0.04%	0.005%
58	9.590	2655	2659	2661	rBV2	429	327	0.03%	0.004%
59	9.625	2668	2670	2676	rVB2	602	439	0.04%	0.005%
60	9.651	2676	2678	2680	rVB2	485	210	0.02%	0.003%
61	9.779	2716	2718	2722	rVB3	537	387	0.04%	0.005%
62	9.799	2722	2724	2727	rVB2	354	228	0.02%	0.003%
63	9.818	2727	2730	2731	rBV2	366	235	0.02%	0.003%
64	9.876	2742	2748	2753	rBV4	760	844	0.08%	0.010%
65	9.947	2768	2770	2773	rBV3	611	313	0.03%	0.004%
66	10.053	2801	2803	2807	rBV2	463	256	0.02%	0.003%
67	10.159	2823	2836	2856	rBV	296254	483515	44.57%	5.930%
68	10.332	2883	2890	2901	rVB3	4934	7790	0.72%	0.096%
69	10.435	2918	2922	2927	rVB3	681	522	0.05%	0.006%
70	10.596	2969	2972	2975	rBV2	474	372	0.03%	0.005%
71	10.641	2984	2986	2989	rVB	570	245	0.02%	0.003%
72	10.689	2998	3001	3002	rBV	391	226	0.02%	0.003%
73	10.712	3006	3008	3012	rVB2	490	290	0.03%	0.004%
74	10.744	3015	3018	3019	rBV2	371	237	0.02%	0.003%
75	10.792	3030	3033	3037	rBV4	660	475	0.04%	0.006%
76	10.837	3042	3047	3048	rBV2	560	458	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031462.D
 Acq On : 08 Jun 2023 21:17
 Operator : SY/MD
 Sample : 03106-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.866	3051	3056	3061	rVB5	960	976	0.09%	0.012%
78	10.895	3061	3065	3071	rBB3	565	584	0.05%	0.007%
79	10.972	3086	3089	3093	rBV2	428	307	0.03%	0.004%
80	10.992	3093	3095	3100	rVB3	441	253	0.02%	0.003%
81	11.043	3108	3111	3113	rBV	298	245	0.02%	0.003%
82	11.111	3128	3132	3134	rBV3	595	406	0.04%	0.005%
83	11.191	3146	3157	3180	rBV	445990	702215	64.72%	8.612%
84	11.467	3240	3243	3250	rVB4	442	370	0.03%	0.005%
85	11.567	3262	3274	3297	rBV	472296	738206	68.04%	9.053%
86	12.024	3414	3416	3419	rVB3	606	251	0.02%	0.003%
87	12.059	3419	3427	3429	rBV4	554	660	0.06%	0.008%
88	12.107	3439	3442	3445	rBV2	387	285	0.03%	0.003%
89	12.242	3479	3484	3487	rBV3	639	583	0.05%	0.007%
90	12.352	3517	3518	3522	rBV2	395	308	0.03%	0.004%
91	12.596	3590	3594	3600	rVB5	952	1129	0.10%	0.014%
92	12.721	3628	3633	3634	rBV2	516	382	0.04%	0.005%
93	12.802	3655	3658	3660	rBV2	496	285	0.03%	0.003%
94	12.972	3709	3711	3713	rBV	403	214	0.02%	0.003%
95	13.098	3748	3750	3752	rVB3	550	207	0.02%	0.003%
96	13.139	3761	3763	3767	rBV2	469	364	0.03%	0.004%
97	13.262	3798	3801	3805	rBV3	559	313	0.03%	0.004%
98	13.403	3839	3845	3849	rBV4	717	676	0.06%	0.008%
99	13.426	3849	3852	3855	rBV4	420	375	0.03%	0.005%
100	14.358	4140	4142	4144	rBV2	496	321	0.03%	0.004%




Sum of corrected areas: 8154211

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031462.D
Acq On : 08 Jun 2023 21:17
Operator : SY/MD
Sample : 03106-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

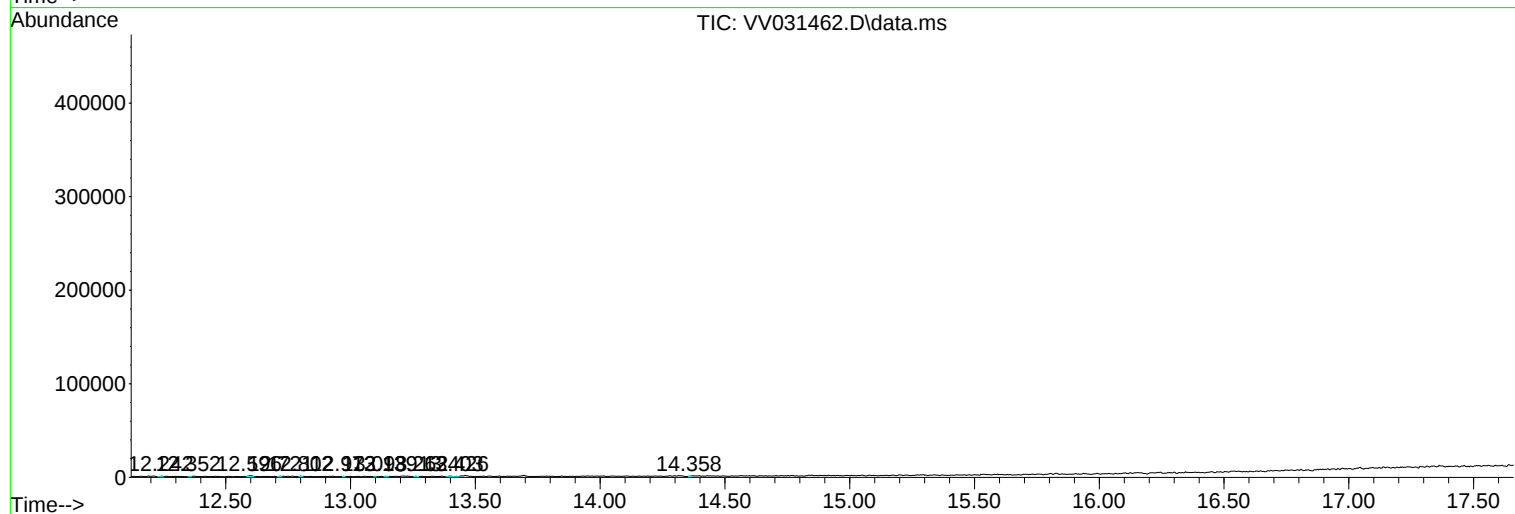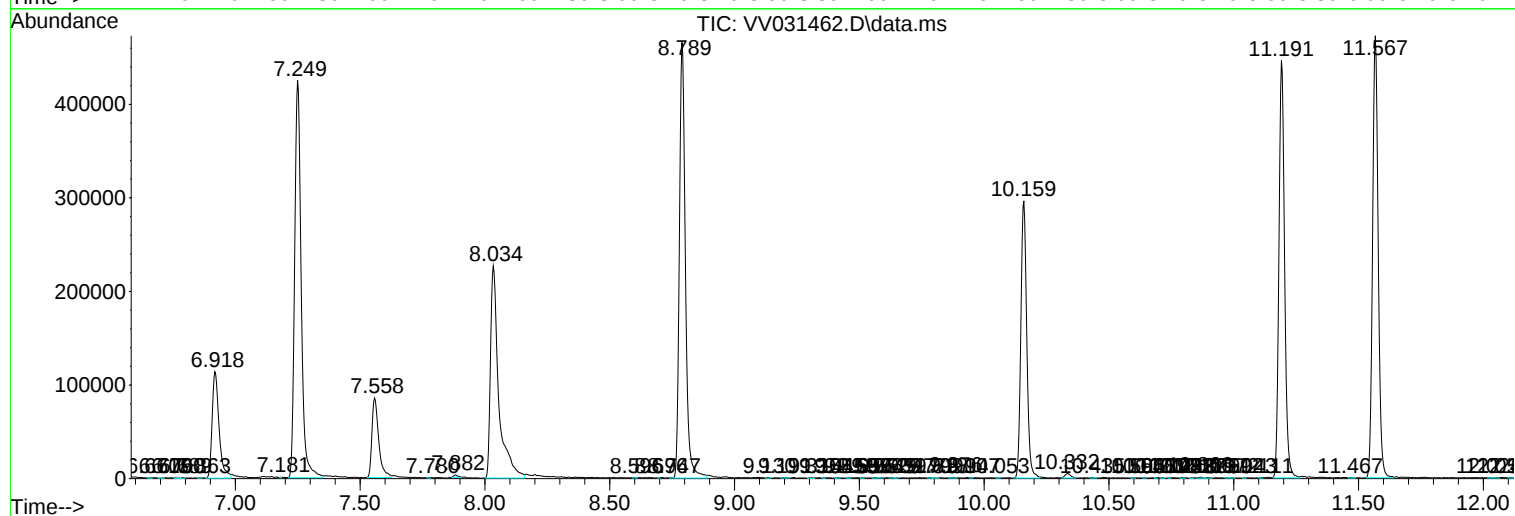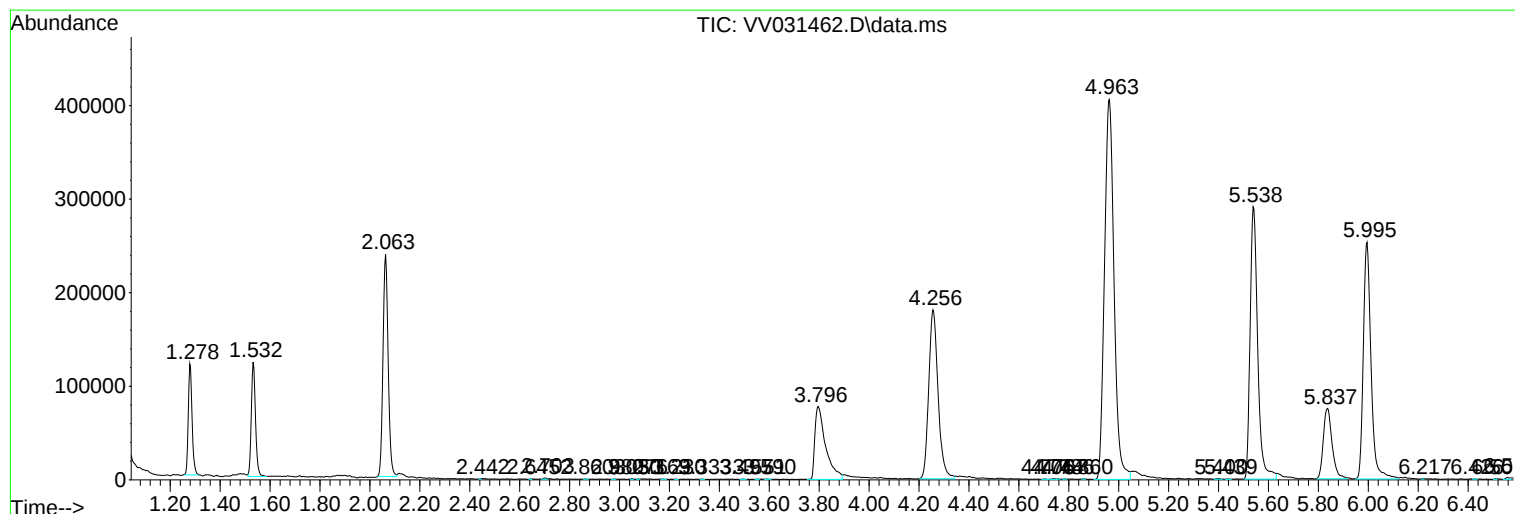

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031462.D
Acq On : 08 Jun 2023 21:17
Operator : SY/MD
Sample : 03106-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031462.D
Acq On : 08 Jun 2023 21:17
Operator : SY/MD
Sample : 03106-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------