

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031463.D
 Acq On : 08 Jun 2023 21:41
 Operator : SY/MD
 Sample : 03106-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031463.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	102323	112354	12.55%	1.685%
2	1.532	147	153	166	rVB	104166	122286	13.66%	1.834%
3	2.063	308	318	335	rBV2	195971	290505	32.45%	4.357%
4	2.751	530	532	534	rBV2	420	217	0.02%	0.003%
5	2.825	550	555	558	rBV3	315	265	0.03%	0.004%
6	2.863	565	567	568	rBV	458	198	0.02%	0.003%
7	3.005	608	611	615	rBV2	422	302	0.03%	0.005%
8	3.127	644	649	652	rVV3	582	428	0.05%	0.006%
9	3.143	652	654	658	rVB2	319	173	0.02%	0.003%
10	3.220	674	678	682	rBV3	349	250	0.03%	0.004%
11	3.240	682	684	687	rVB	510	255	0.03%	0.004%
12	3.262	687	691	695	rVB3	458	422	0.05%	0.006%
13	3.294	698	701	704	rBV2	364	267	0.03%	0.004%
14	3.323	707	710	711	rBV2	343	185	0.02%	0.003%
15	3.400	730	734	735	rBV2	259	207	0.02%	0.003%
16	3.500	763	765	768	rBV2	384	232	0.03%	0.003%
17	3.542	773	778	782	rVB3	450	421	0.05%	0.006%
18	3.580	784	790	795	rBV2	484	489	0.05%	0.007%
19	3.619	798	802	805	rBV3	249	257	0.03%	0.004%
20	3.731	834	837	839	rBV3	384	226	0.03%	0.003%
21	3.744	839	841	849	rBV3	232	274	0.03%	0.004%
22	3.799	849	858	890	rBV2	65381	198748	22.20%	2.981%
23	4.256	985	1000	1028	rBV2	143486	379882	42.43%	5.697%
24	4.500	1073	1076	1078	rBV4	817	602	0.07%	0.009%
25	4.632	1113	1117	1120	rBV4	768	589	0.07%	0.009%
26	4.735	1142	1149	1155	rBV5	596	837	0.09%	0.013%
27	4.786	1161	1165	1166	rBV	439	248	0.03%	0.004%
28	4.831	1176	1179	1181	rBV2	506	296	0.03%	0.004%
29	4.963	1203	1220	1242	rBV2	330597	895216	100.00%	13.426%
30	5.352	1340	1341	1342	rBV2	491	180	0.02%	0.003%
31	5.407	1356	1358	1361	rBV2	432	240	0.03%	0.004%
32	5.429	1362	1365	1370	rVV4	647	557	0.06%	0.008%
33	5.538	1387	1399	1424	rBV	243732	514777	57.50%	7.720%
34	5.731	1457	1459	1462	rBV2	739	402	0.04%	0.006%
35	5.770	1469	1471	1475	rVB3	447	233	0.03%	0.003%
36	5.828	1478	1489	1510	rVV2	29289	63963	7.14%	0.959%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031463.D
 Acq On : 08 Jun 2023 21:41
 Operator : SY/MD
 Sample : 03106-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.950	1525	1527	1528	rBV2	437	228	0.03%	0.003%
38	5.995	1528	1541	1563	rBV	206693	436697	48.78%	6.549%
39	6.233	1611	1615	1616	rBV2	438	331	0.04%	0.005%
40	6.278	1627	1629	1633	rBV2	359	175	0.02%	0.003%
41	6.329	1642	1645	1649	rBV3	353	242	0.03%	0.004%
42	6.410	1667	1670	1672	rBV	413	249	0.03%	0.004%
43	6.442	1678	1680	1684	rVB4	488	336	0.04%	0.005%
44	6.535	1705	1709	1710	rBV4	307	205	0.02%	0.003%
45	6.574	1715	1721	1726	rVV5	1230	1590	0.18%	0.024%
46	6.677	1750	1753	1755	rBV3	667	330	0.04%	0.005%
47	6.728	1767	1769	1772	rVB3	653	322	0.04%	0.005%
48	6.751	1773	1776	1778	rBV3	417	233	0.03%	0.003%
49	6.921	1816	1829	1861	rBV	93689	189043	21.12%	2.835%
50	7.249	1919	1931	1961	rBV	341801	622441	69.53%	9.335%
51	7.561	2018	2028	2051	rBV	67882	130023	14.52%	1.950%
52	7.831	2109	2112	2117	rBV4	363	356	0.04%	0.005%
53	7.905	2132	2135	2138	rBV2	709	358	0.04%	0.005%
54	7.921	2138	2140	2142	rVB3	551	196	0.02%	0.003%
55	8.034	2166	2175	2210	rBV2	178173	419973	46.91%	6.298%
56	8.448	2302	2304	2305	rBV	547	237	0.03%	0.004%
57	8.542	2331	2333	2336	rBV2	479	240	0.03%	0.004%
58	8.677	2373	2375	2379	rBV2	323	191	0.02%	0.003%
59	8.722	2386	2389	2392	rBV	541	379	0.04%	0.006%
60	8.789	2399	2410	2437	rBV	388598	665709	74.36%	9.984%
61	9.050	2488	2491	2495	rVB3	466	389	0.04%	0.006%
62	9.098	2504	2506	2509	rBV2	541	240	0.03%	0.004%
63	9.191	2534	2535	2539	rBV2	309	210	0.02%	0.003%
64	9.284	2561	2564	2567	rBV2	344	274	0.03%	0.004%
65	9.329	2574	2578	2580	rBV	262	191	0.02%	0.003%
66	9.368	2587	2590	2592	rBV2	387	259	0.03%	0.004%
67	9.445	2612	2614	2616	rBV2	343	174	0.02%	0.003%
68	9.535	2639	2642	2647	rBV2	504	437	0.05%	0.007%
69	9.632	2671	2672	2676	rBV2	328	176	0.02%	0.003%
70	9.873	2743	2747	2755	rBV4	678	683	0.08%	0.010%
71	9.979	2777	2780	2784	rBV	282	213	0.02%	0.003%
72	10.046	2799	2801	2804	rBV2	278	179	0.02%	0.003%
73	10.095	2812	2816	2818	rBV	280	227	0.03%	0.003%
74	10.159	2823	2836	2854	rVV	244039	394685	44.09%	5.919%
75	10.233	2857	2859	2863	rVB	597	368	0.04%	0.006%
76	10.390	2906	2908	2909	rBV	478	224	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031463.D
 Acq On : 08 Jun 2023 21:41
 Operator : SY/MD
 Sample : 03106-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.525	2947	2950	2954	rVB2	459	230	0.03%	0.003%
78	10.548	2954	2957	2959	rBV2	470	292	0.03%	0.004%
79	10.564	2960	2962	2970	rVB2	509	531	0.06%	0.008%
80	10.789	3030	3032	3035	rBV3	295	187	0.02%	0.003%
81	10.808	3035	3038	3039	rBV2	351	184	0.02%	0.003%
82	10.985	3091	3093	3098	rVB2	693	408	0.05%	0.006%
83	11.033	3100	3108	3113	rBV3	624	925	0.10%	0.014%
84	11.191	3146	3157	3182	rBV	375602	603800	67.45%	9.055%
85	11.368	3210	3212	3218	rVB3	871	517	0.06%	0.008%
86	11.397	3218	3221	3222	rBV	349	210	0.02%	0.003%
87	11.567	3262	3274	3299	rBV	373473	599843	67.01%	8.996%
88	11.750	3328	3331	3334	rBV2	506	439	0.05%	0.007%
89	11.959	3393	3396	3397	rBV	472	246	0.03%	0.004%
90	12.075	3429	3432	3434	rBV2	562	325	0.04%	0.005%
91	12.162	3457	3459	3461	rBV	426	251	0.03%	0.004%
92	12.631	3602	3605	3606	rBV	513	220	0.02%	0.003%
93	12.715	3629	3631	3632	rBV	452	235	0.03%	0.004%
94	13.210	3781	3785	3788	rBV3	541	418	0.05%	0.006%
95	13.390	3838	3841	3842	rBV2	396	279	0.03%	0.004%
96	13.432	3851	3854	3857	rBV3	618	471	0.05%	0.007%
97	13.860	3984	3987	3991	rBV3	635	459	0.05%	0.007%
98	13.882	3991	3994	3997	rBV3	646	411	0.05%	0.006%
99	14.053	4045	4047	4053	rVB3	869	586	0.07%	0.009%
100	14.737	4258	4260	4263	rBV	597	405	0.05%	0.006%




Sum of corrected areas: 6667868

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031463.D
Acq On : 08 Jun 2023 21:41
Operator : SY/MD
Sample : 03106-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

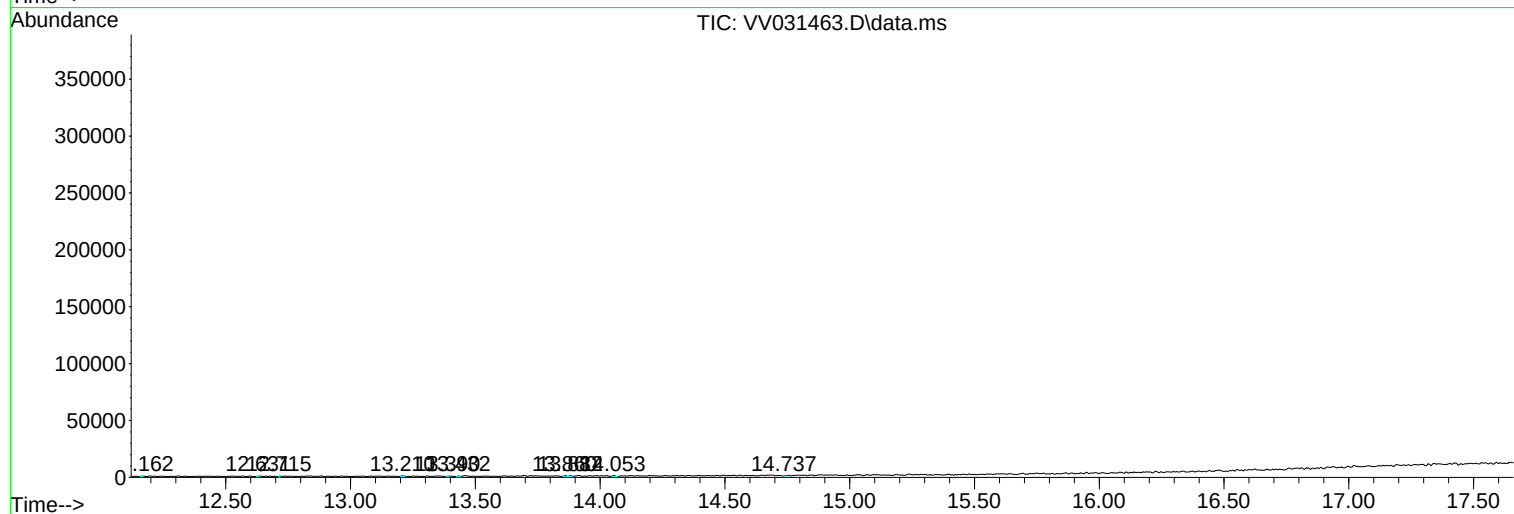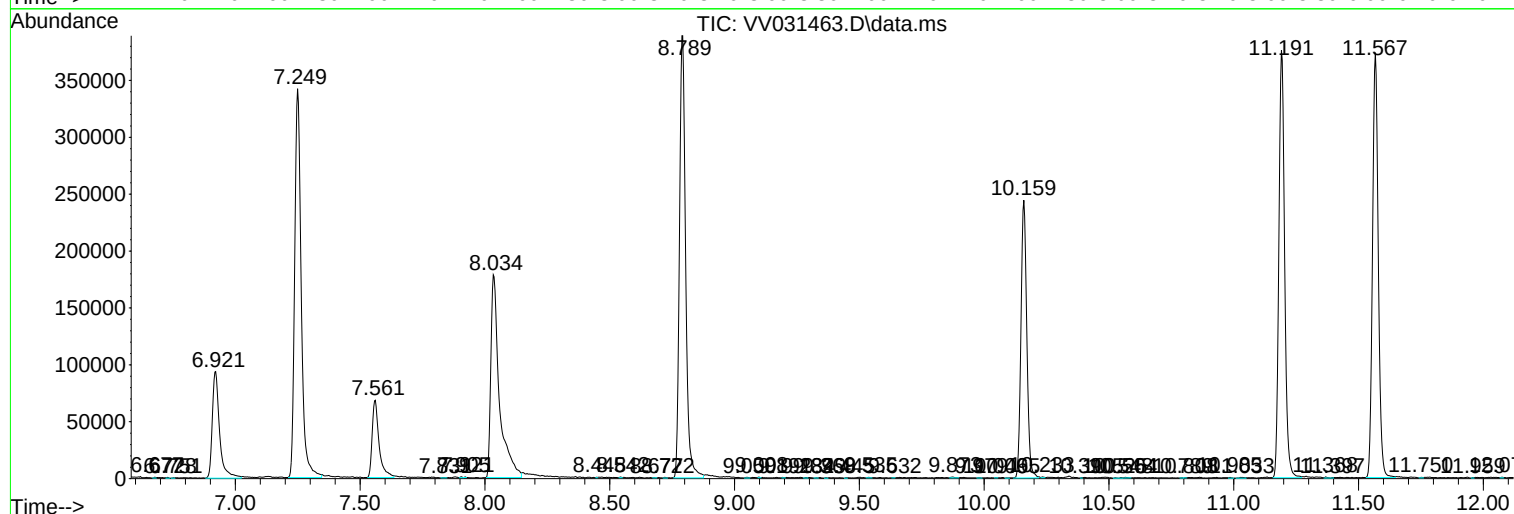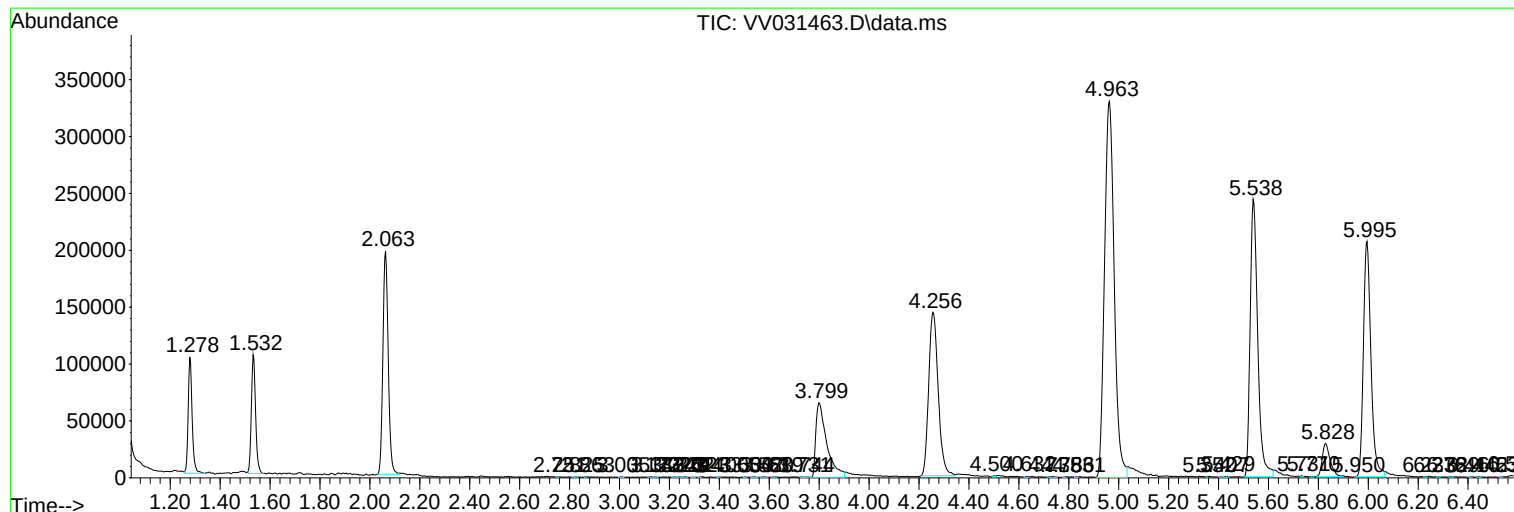

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031463.D
Acq On : 08 Jun 2023 21:41
Operator : SY/MD
Sample : 03106-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031463.D
Acq On : 08 Jun 2023 21:41
Operator : SY/MD
Sample : 03106-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc