

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031464.D
 Acq On : 08 Jun 2023 22:05
 Operator : SY/MD
 Sample : 03106-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031464.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	116617	128080	11.94%	1.583%
2	1.532	147	153	168	rVB	121425	144433	13.46%	1.785%
3	2.063	308	318	332	rBV	233863	343513	32.02%	4.245%
4	2.449	435	438	443	rBV4	671	735	0.07%	0.009%
5	2.564	471	474	475	rBV	348	196	0.02%	0.002%
6	2.609	486	488	493	rVB3	416	255	0.02%	0.003%
7	2.693	508	514	515	rBV3	951	712	0.07%	0.009%
8	2.796	543	546	550	rVB3	420	218	0.02%	0.003%
9	2.857	563	565	569	rBV	357	235	0.02%	0.003%
10	2.915	580	583	587	rBV2	516	388	0.04%	0.005%
11	2.960	594	597	601	rVB2	413	355	0.03%	0.004%
12	3.031	616	619	621	rVV2	604	308	0.03%	0.004%
13	3.111	642	644	645	rBV	343	163	0.02%	0.002%
14	3.227	677	680	682	rBV2	332	157	0.01%	0.002%
15	3.256	684	689	692	rVV3	704	447	0.04%	0.006%
16	3.281	695	697	701	rVB2	474	288	0.03%	0.004%
17	3.307	701	705	708	rBV2	307	257	0.02%	0.003%
18	3.381	724	728	729	rBV2	213	175	0.02%	0.002%
19	3.513	764	769	771	rVB2	456	353	0.03%	0.004%
20	3.535	773	776	778	rVV	571	335	0.03%	0.004%
21	3.561	782	784	786	rBV	287	160	0.01%	0.002%
22	3.606	793	798	800	rBV3	396	416	0.04%	0.005%
23	3.712	826	831	838	rVB4	458	533	0.05%	0.007%
24	3.741	838	840	844	rBV2	371	227	0.02%	0.003%
25	3.764	844	847	848	rBV2	403	243	0.02%	0.003%
26	3.796	848	857	882	rBV	83761	241349	22.50%	2.982%
27	4.256	984	1000	1025	rBV	178377	460138	42.89%	5.686%
28	4.500	1073	1076	1077	rBV2	906	496	0.05%	0.006%
29	4.664	1124	1127	1129	rBV3	451	265	0.02%	0.003%
30	4.963	1203	1220	1244	rBV2	402126	1072882	100.00%	13.258%
31	5.333	1333	1335	1339	rBV3	534	300	0.03%	0.004%
32	5.391	1351	1353	1357	rVB2	681	381	0.04%	0.005%
33	5.448	1369	1371	1373	rVB3	336	143	0.01%	0.002%
34	5.481	1378	1381	1385	rBV4	485	462	0.04%	0.006%
35	5.539	1387	1399	1421	rBV	289365	597365	55.68%	7.382%
36	5.786	1474	1476	1477	rBV	401	176	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031464.D
 Acq On : 08 Jun 2023 22:05
 Operator : SY/MD
 Sample : 03106-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.838	1477	1492	1511	rVV5	101484	240971	22.46%	2.978%
38	5.995	1528	1541	1572	rBV	250068	526402	49.06%	6.505%
39	6.243	1614	1618	1620	rBV4	601	432	0.04%	0.005%
40	6.384	1658	1662	1664	rBV3	310	277	0.03%	0.003%
41	6.403	1664	1668	1671	rVB2	701	479	0.04%	0.006%
42	6.445	1679	1681	1685	rVB2	525	231	0.02%	0.003%
43	6.497	1694	1697	1699	rBV2	373	257	0.02%	0.003%
44	6.535	1705	1709	1712	rBV2	500	335	0.03%	0.004%
45	6.564	1712	1718	1720	rBV3	1685	2061	0.19%	0.025%
46	6.629	1735	1738	1741	rBV3	684	485	0.05%	0.006%
47	6.731	1768	1770	1774	rVB2	413	234	0.02%	0.003%
48	6.918	1818	1828	1855	rBV	111635	221138	20.61%	2.733%
49	7.249	1919	1931	1957	rBV	423264	757791	70.63%	9.364%
50	7.558	2015	2027	2055	rBV	81693	158778	14.80%	1.962%
51	7.760	2088	2090	2092	rBV	461	284	0.03%	0.004%
52	7.812	2104	2106	2110	rBV2	641	347	0.03%	0.004%
53	7.863	2119	2122	2125	rBV2	367	316	0.03%	0.004%
54	7.882	2125	2128	2130	rBV2	504	391	0.04%	0.005%
55	7.940	2144	2146	2147	rBV	344	159	0.01%	0.002%
56	7.985	2157	2160	2162	rBV3	485	276	0.03%	0.003%
57	8.034	2164	2175	2210	rBV2	234277	533641	49.74%	6.594%
58	8.387	2282	2285	2288	rBV2	911	654	0.06%	0.008%
59	8.693	2378	2380	2383	rVB2	470	235	0.02%	0.003%
60	8.741	2393	2395	2399	rVB3	649	430	0.04%	0.005%
61	8.789	2399	2410	2434	rBV	457308	762992	71.12%	9.428%
62	9.124	2509	2514	2516	rBV2	598	471	0.04%	0.006%
63	9.271	2557	2560	2563	rBV2	388	209	0.02%	0.003%
64	9.300	2567	2569	2572	rVB	574	323	0.03%	0.004%
65	9.342	2577	2582	2586	rBV	409	322	0.03%	0.004%
66	9.368	2586	2590	2593	rBV3	360	370	0.03%	0.005%
67	9.751	2704	2709	2711	rBV4	462	428	0.04%	0.005%
68	9.834	2728	2735	2739	rBV4	780	663	0.06%	0.008%
69	9.876	2739	2748	2753	rBV5	994	1212	0.11%	0.015%
70	9.960	2772	2774	2778	rVB2	393	211	0.02%	0.003%
71	10.024	2791	2794	2798	rBV4	374	306	0.03%	0.004%
72	10.159	2825	2836	2854	rBV	291729	467130	43.54%	5.772%
73	10.390	2906	2908	2912	rVB	298	191	0.02%	0.002%
74	10.452	2922	2927	2929	rBV2	639	521	0.05%	0.006%
75	10.545	2951	2956	2960	rVB2	803	626	0.06%	0.008%
76	10.567	2960	2963	2965	rBV2	291	176	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
 Data File : VV031464.D
 Acq On : 08 Jun 2023 22:05
 Operator : SY/MD
 Sample : 03106-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.583	2966	2968	2973	rVB3	490	299	0.03%	0.004%
78	10.808	3036	3038	3043	rVB3	490	244	0.02%	0.003%
79	10.860	3049	3054	3059	rBV4	680	825	0.08%	0.010%
80	10.915	3070	3071	3078	rBV2	313	317	0.03%	0.004%
81	11.021	3102	3104	3110	rVB3	390	333	0.03%	0.004%
82	11.059	3110	3116	3118	rBV4	619	678	0.06%	0.008%
83	11.078	3120	3122	3126	rVB2	596	344	0.03%	0.004%
84	11.133	3134	3139	3143	rBV4	761	837	0.08%	0.010%
85	11.191	3145	3157	3176	rBV	436026	685889	63.93%	8.476%
86	11.455	3237	3239	3243	rBV2	640	385	0.04%	0.005%
87	11.567	3262	3274	3303	rBV	450711	717858	66.91%	8.871%
88	11.760	3332	3334	3339	rBV3	567	417	0.04%	0.005%
89	12.181	3463	3465	3470	rBV3	590	435	0.04%	0.005%
90	12.213	3473	3475	3479	rBV3	302	253	0.02%	0.003%
91	12.374	3523	3525	3527	rBV2	554	279	0.03%	0.003%
92	12.493	3560	3562	3564	rBV2	473	283	0.03%	0.003%
93	12.619	3599	3601	3610	rVB3	498	298	0.03%	0.004%
94	12.734	3636	3637	3640	rVB2	417	150	0.01%	0.002%
95	12.931	3694	3698	3703	rBV	601	575	0.05%	0.007%
96	13.040	3729	3732	3735	rBV3	510	308	0.03%	0.004%
97	13.111	3753	3754	3757	rBV	290	187	0.02%	0.002%
98	13.159	3766	3769	3772	rBV	459	316	0.03%	0.004%
99	13.696	3933	3936	3940	rBV2	937	519	0.05%	0.006%
100	13.763	3954	3957	3961	rVB3	616	505	0.05%	0.006%




Sum of corrected areas: 8092428

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031464.D
Acq On : 08 Jun 2023 22:05
Operator : SY/MD
Sample : 03106-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

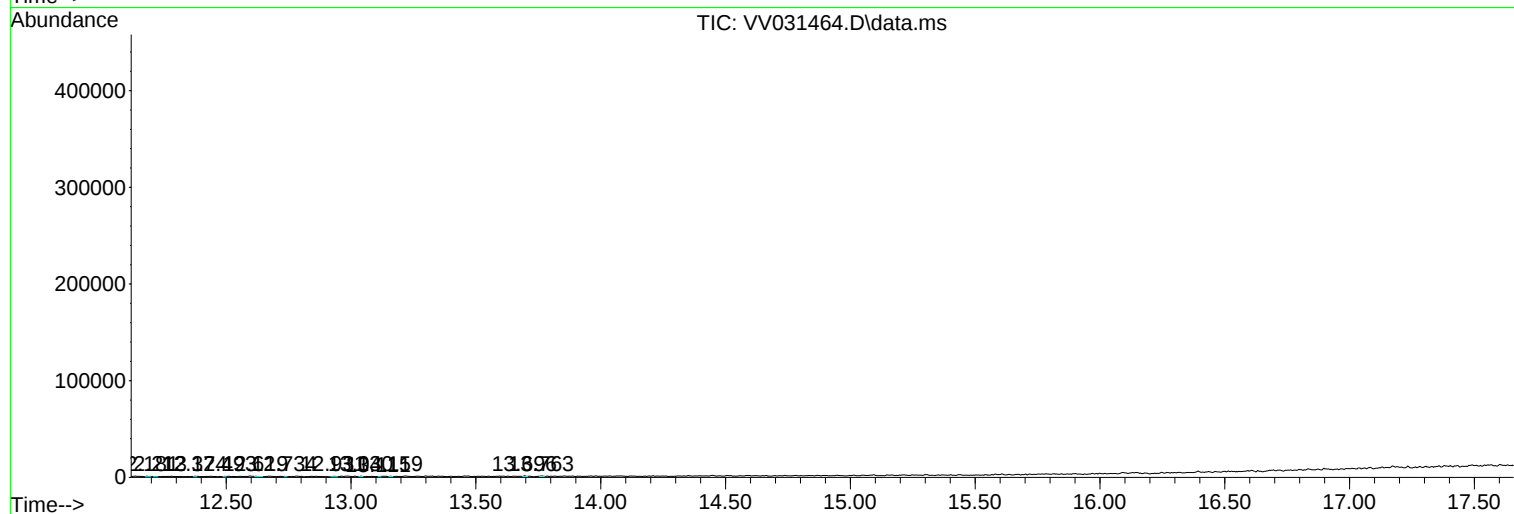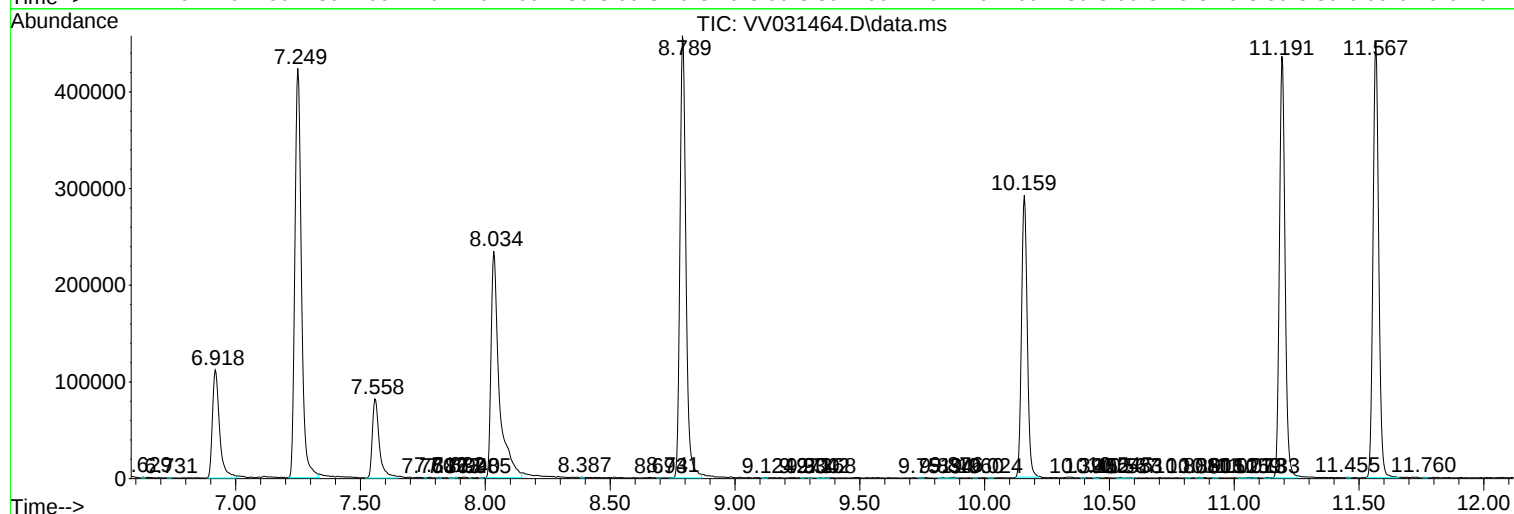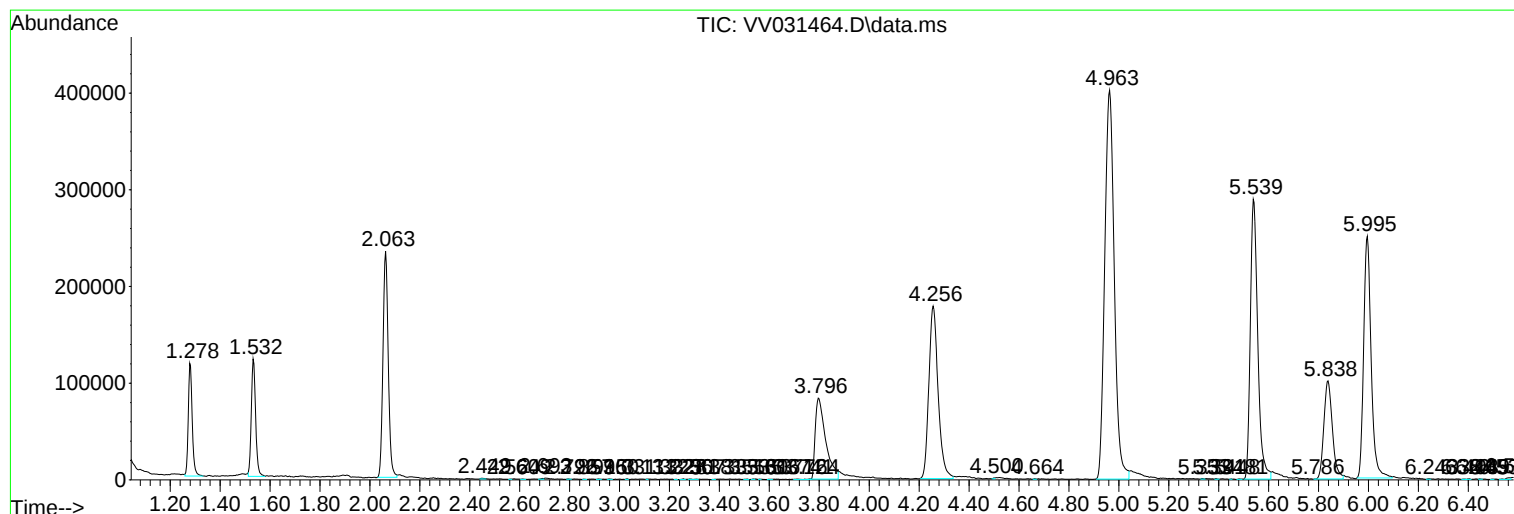

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031464.D
Acq On : 08 Jun 2023 22:05
Operator : SY/MD
Sample : 03106-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060823\
Data File : VV031464.D
Acq On : 08 Jun 2023 22:05
Operator : SY/MD
Sample : 03106-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc